
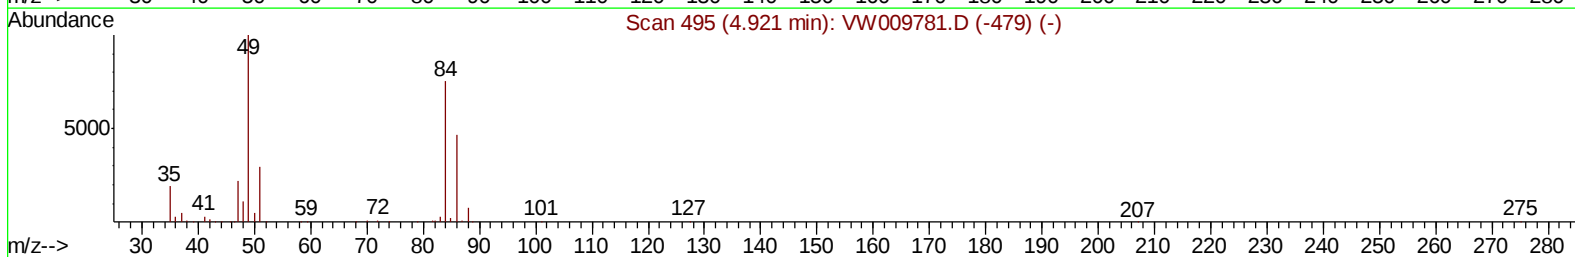
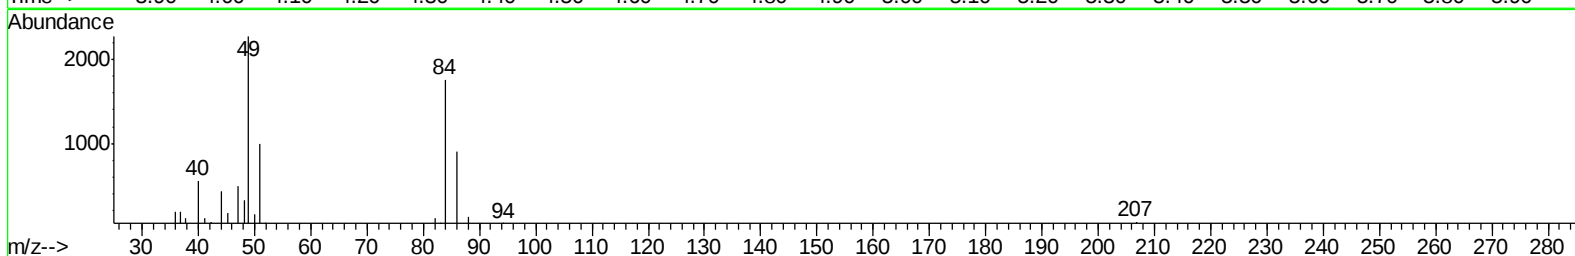


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009772.D
 Acq On : 06 Apr 2019 15:01
 Operator : SY/VA
 Sample : K2327-05
 Misc : 5.75G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 04:00:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 03:56:20 2019
 Response via : Initial Calibration

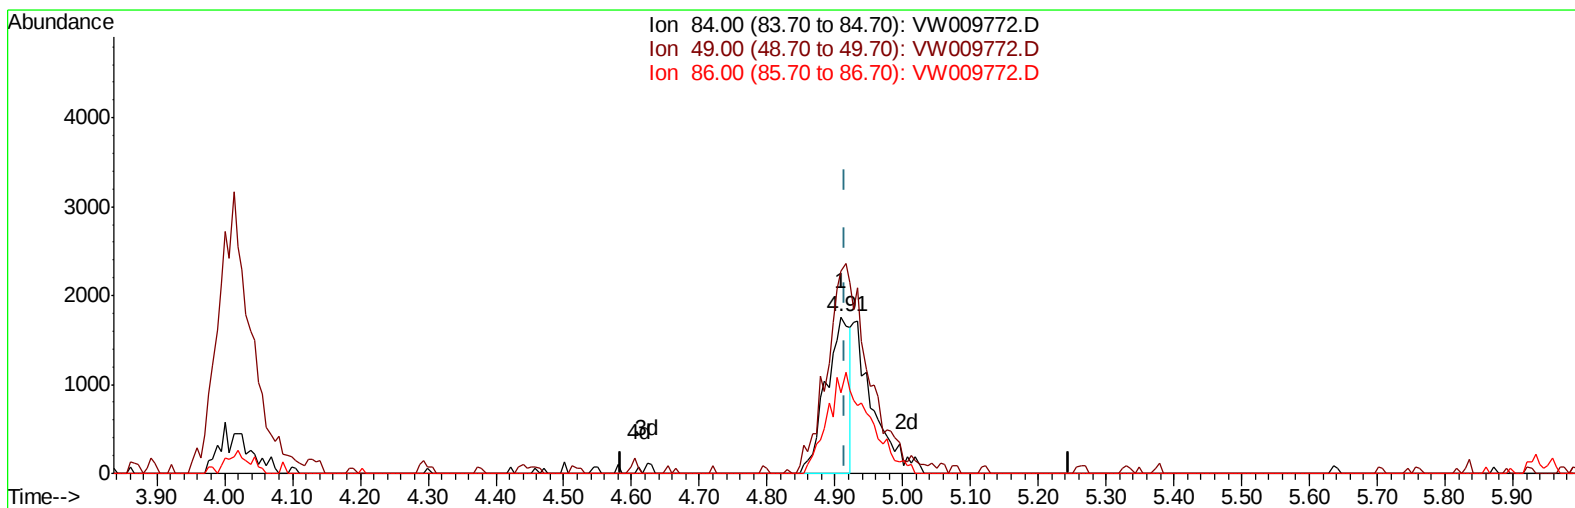

TIC: VW009772.D

(16) Methylene chloride (T)




4.909min (-0.006) 0.48ug/L

response 4238

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	128.97
86.00	66.30	51.36
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009772.D
Acq On : 06 Apr 2019 15:01
Operator : SY/VA
Sample : K2327-05
Misc : 5.75G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 04:00:40 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

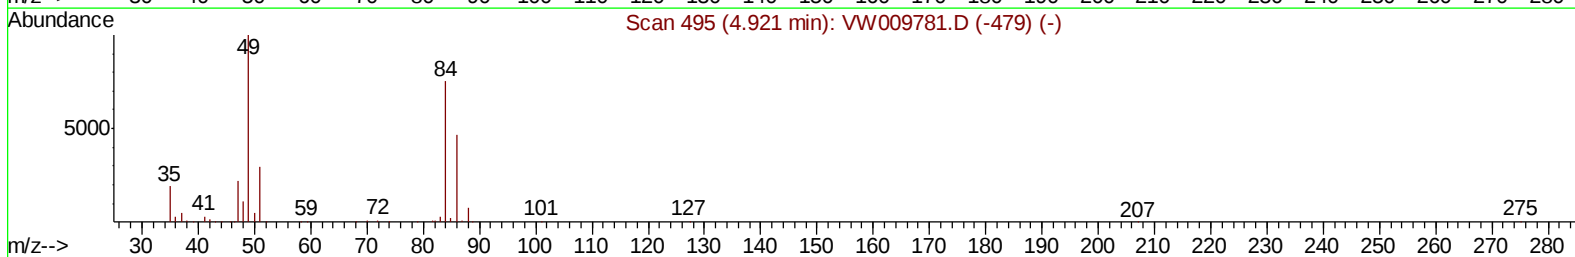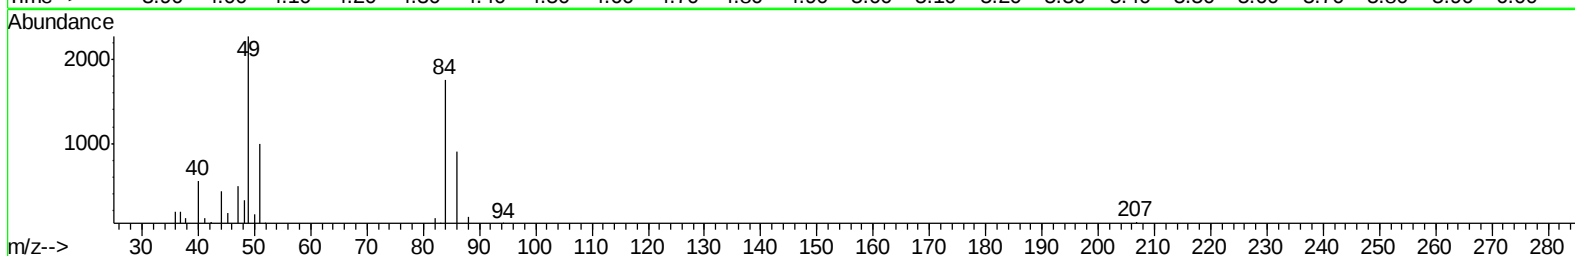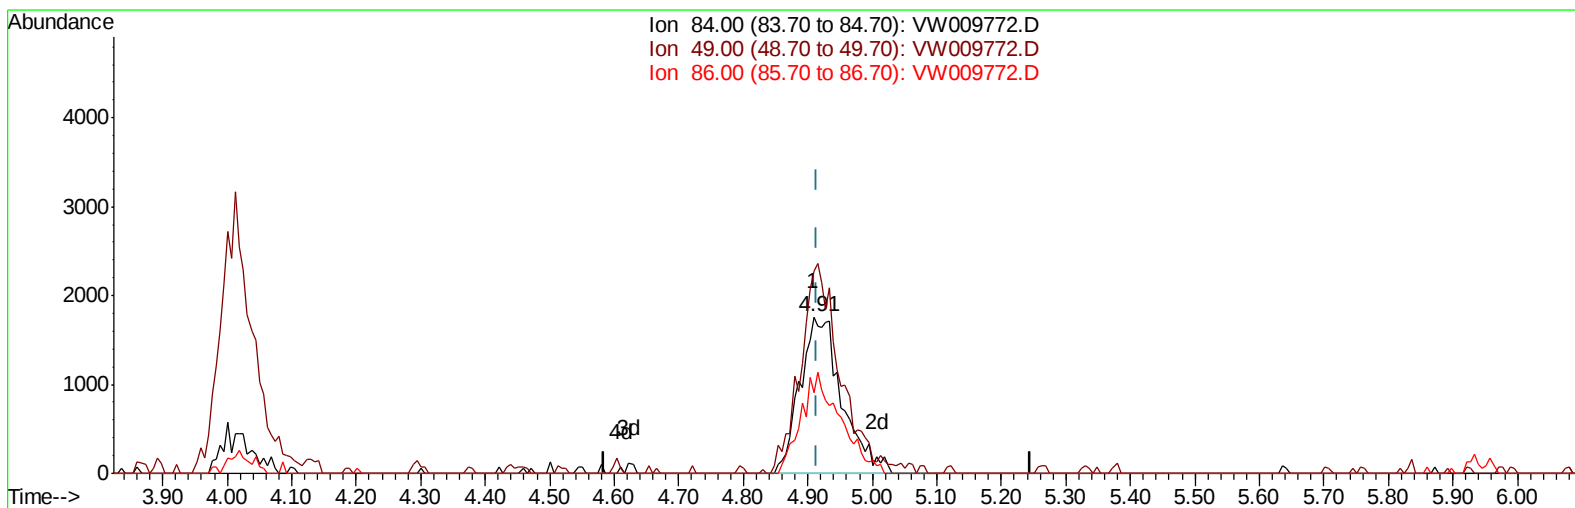

TIC: VW009772.D

(16) Methylene chloride (T)

4.909min (-0.006) 0.90ug/L m

response 7956

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	128.97
86.00	66.30	51.36
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009772.D
 Acq On : 06 Apr 2019 15:01
 Operator : SY/VA
 Sample : K2327-05
 Misc : 5.75G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 06:09:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 03:56:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	501632	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	483557	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	205250	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	165827	25.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.04%
7) Chloroethane-d5	2.89	69	152491	25.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.44%
10) 1,1-Dichloroethene-d2	4.01	63	288753	20.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.80%
20) 2-Butanone-d5	7.07	46	105667	49.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.16%
24) Chloroform-d	7.65	84	367663	26.86	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	107.44%
26) 1,2-Dichloroethane-d4	8.31	65	229269	27.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.12%
29) Benzene-d6	8.27	84	701577	27.64	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.56%
33) 1,2-Dichloropropane-d6	9.27	67	214795	27.40	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.60%
37) Toluene-d8	10.32	98	635469	27.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.32%
38) trans-1,3-Dichloropropene-	10.57	79	93734	25.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.28%
39) 2-Hexanone-d5	10.93	63	75654	51.19	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.38%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	177987	24.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.68%
61) 1,2-Dichlorobenzene-d4	13.85	152	217537	30.20	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	120.80%#

Target Compounds					Qvalue
22) cis-1,2-Dichloroethene	7.17	96	5264	0.710 ug/L	87
35) Trichloroethene	9.09	95	21385	2.809 ug/L	97
47) Tetrachloroethene	10.86	164	10434	1.740 ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009772.D
Acq On : 06 Apr 2019 15:01
Operator : SY/VA
Sample : K2327-05
Misc : 5.75G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 06:09:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

