


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009776.D
Acq On : 06 Apr 2019 16:51
Operator : SY/VA
Sample : K2277-21
Misc : 5.88G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF2R5

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:09 AM

Quant Time: Apr 07 06:34:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

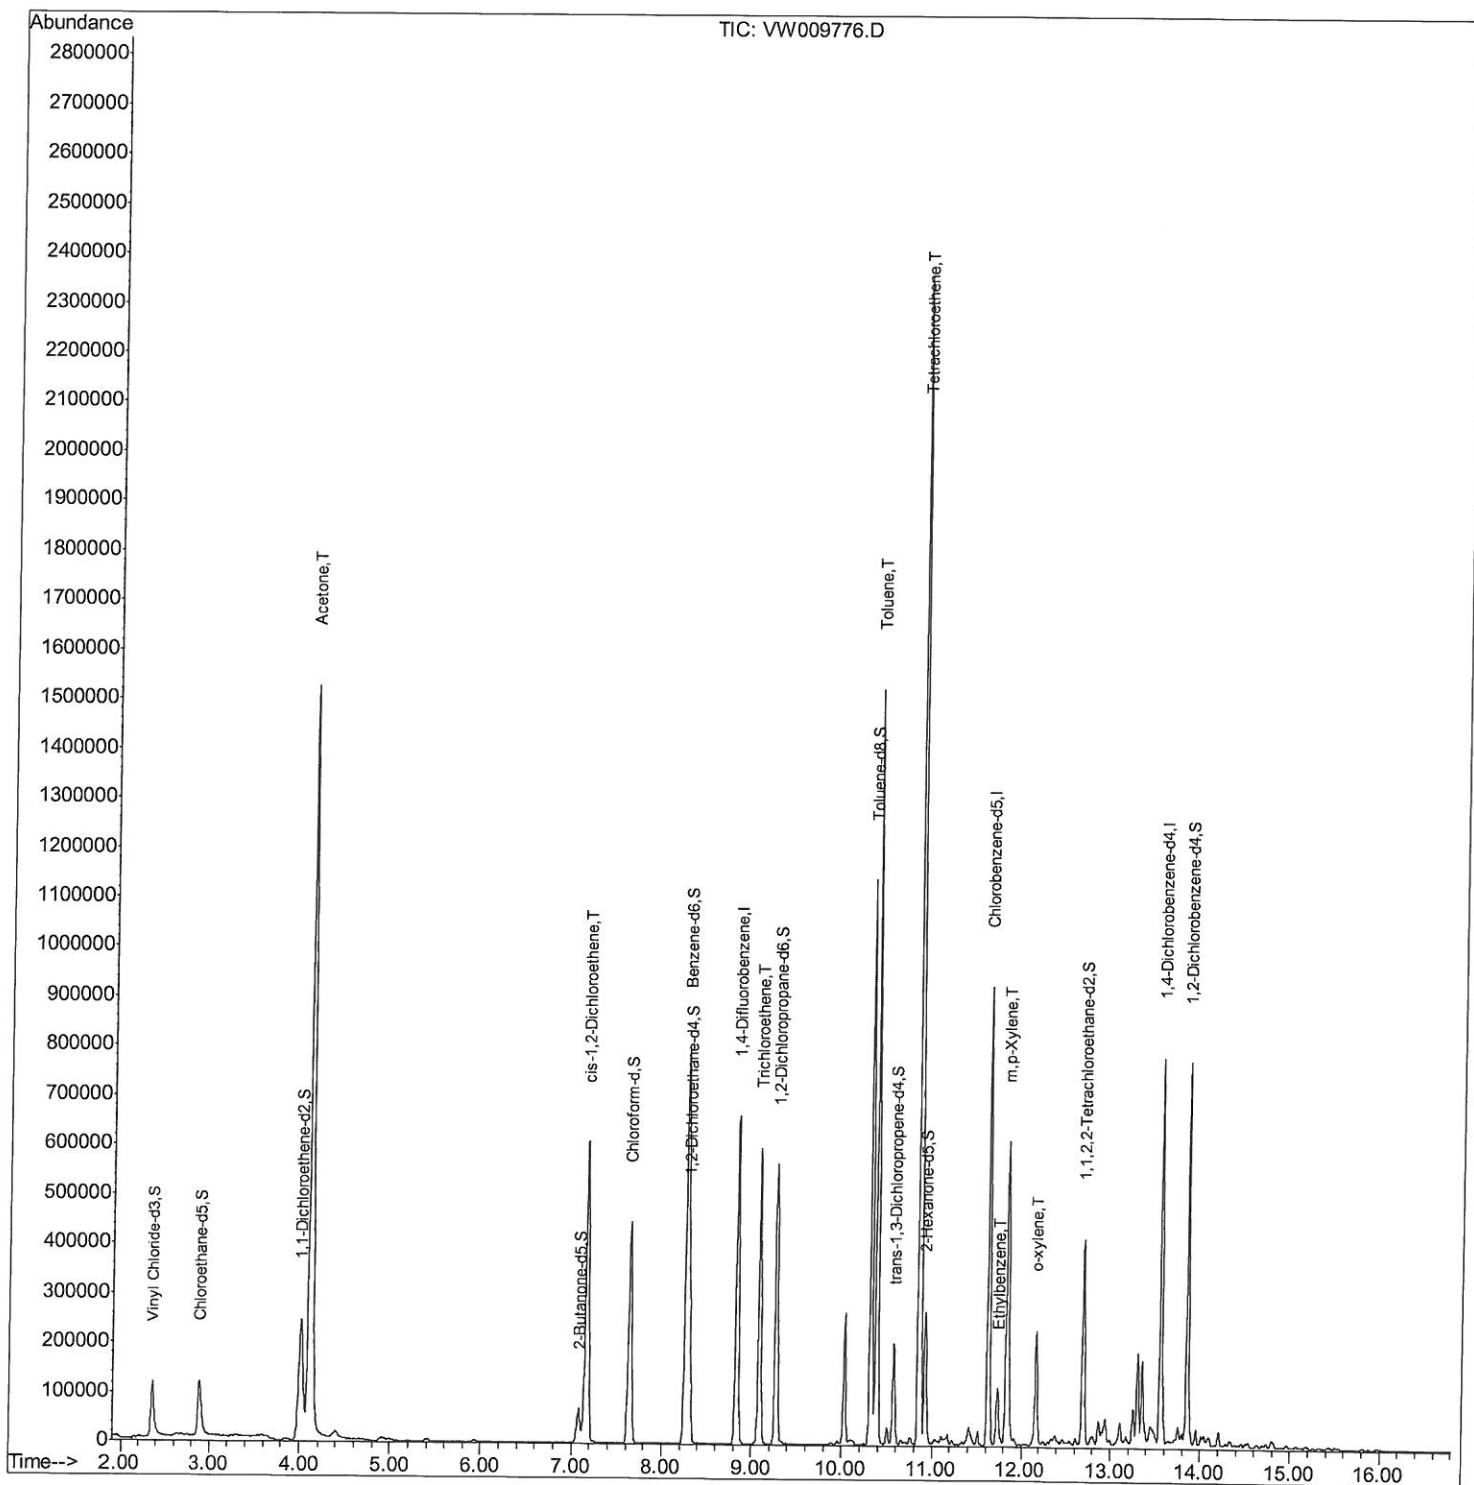

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009776.D
Acq On : 06 Apr 2019 16:51
Operator : SY/VA
Sample : K2277-21
Misc : 5.88G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF2R5

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:09 AM

Quant Time: Apr 07 04:01:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

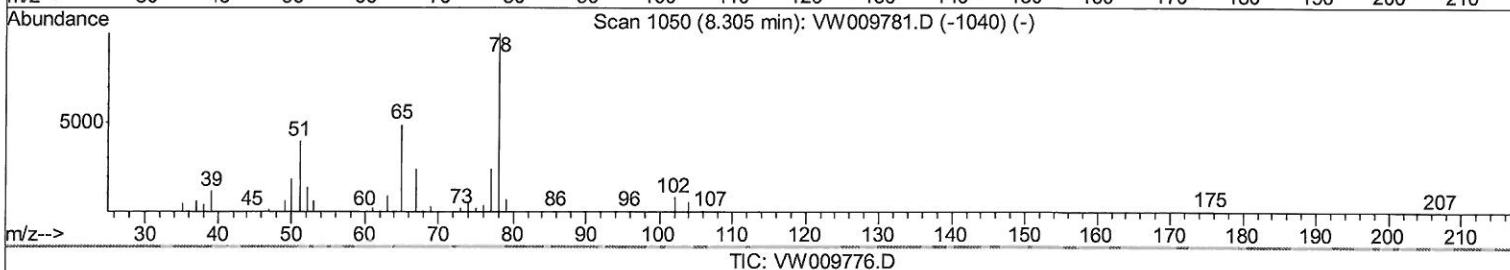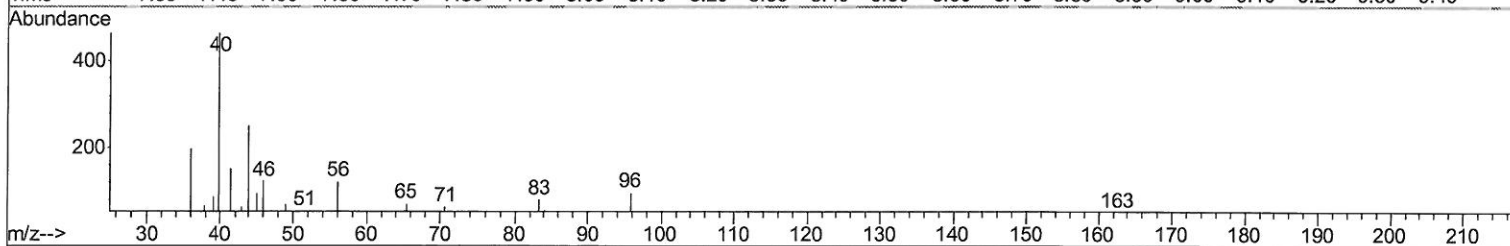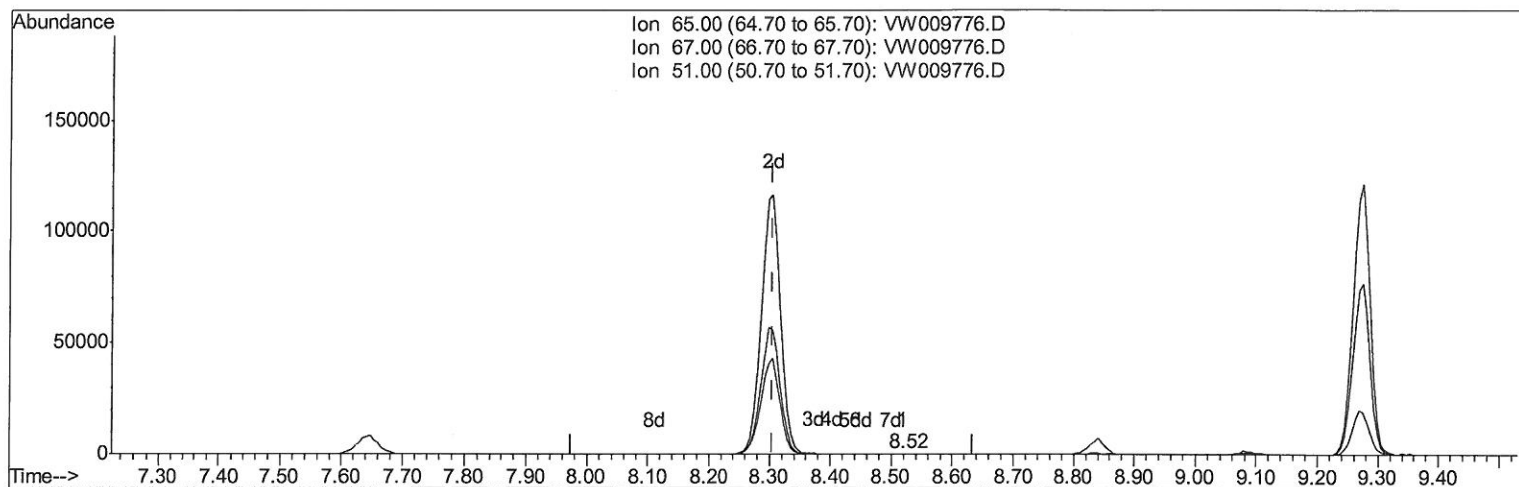

(26) 1,2-Dichloroethane-d4 (S)

8.519min (+0.214) 0.01ug/L

response 51

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	37.25
51.00	109.90	107.84
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009776.D
Acq On : 06 Apr 2019 16:51
Operator : SY/VA
Sample : K2277-21
Misc : 5.88G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF2R5

Manual Integrations

MMDadoda
4/11/2019 11:43:09 AM

Quant Time: Apr 07 04:01:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

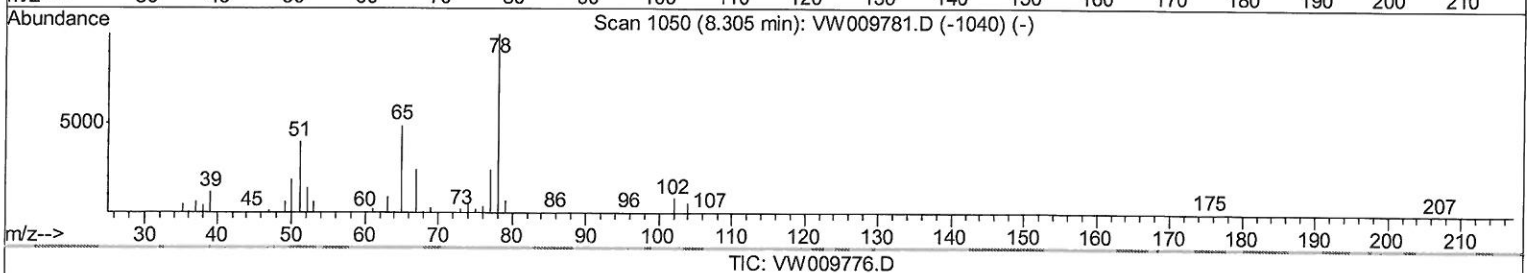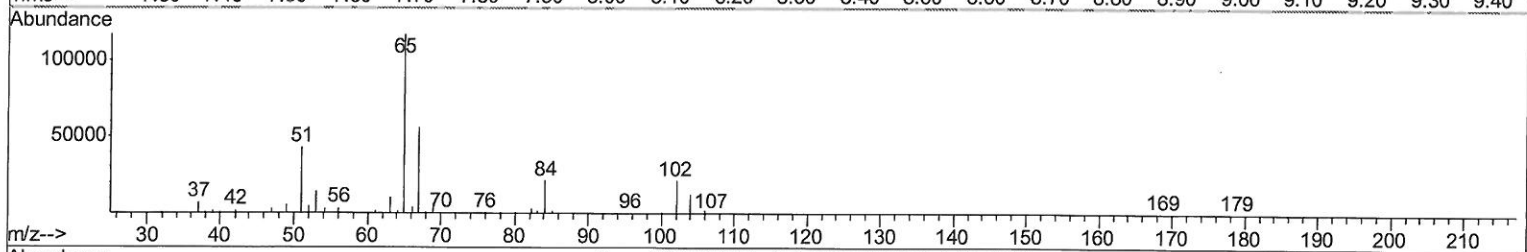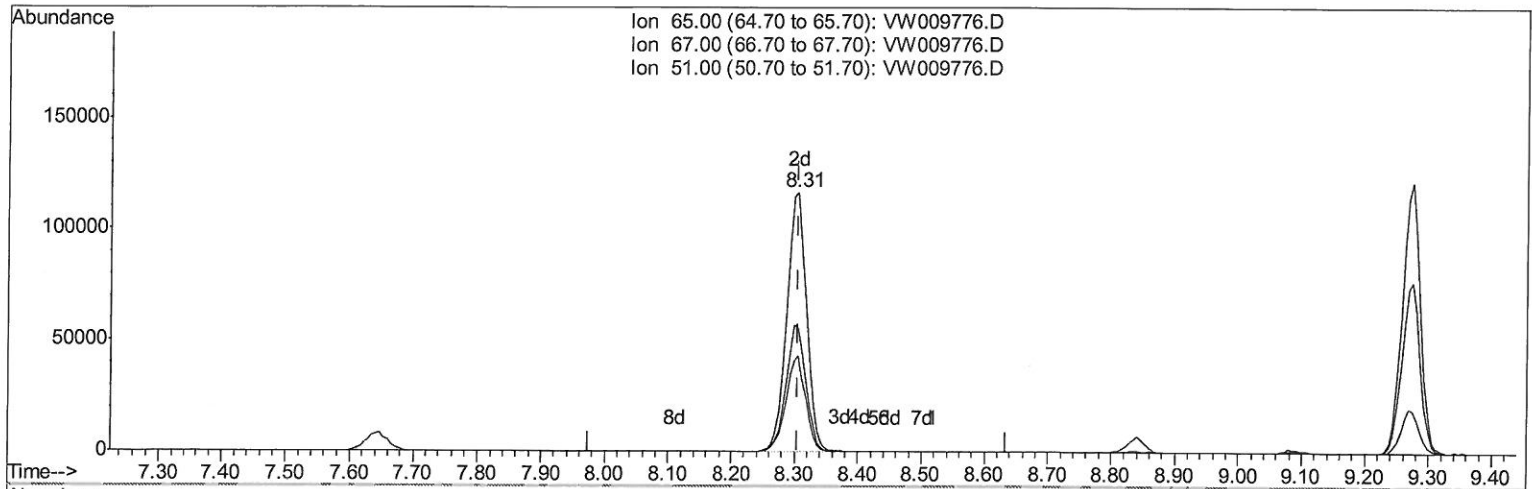

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.000) 29.36ug/L m

response 252676

Ion	Exp%	Act%
-----	------	------

65.00	100	100
67.00	50.90	0.01#
51.00	109.90	0.02#
0.00	0.00	0.00

$$\frac{7m\theta}{419119}$$

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009776.D
 Acq On : 06 Apr 2019 16:51
 Operator : SY/VA
 Sample : K2277-21
 Misc : 5.88G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF2R5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:09 AM

Quant Time: Apr 07 06:34:01 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Sun Apr 07 03:56:20 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	513670	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	470834	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	186355	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	181160	26.95	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	107.80%		
7) Chloroethane-d5	2.89	69	167158	27.14	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	108.56%		
10) 1,1-Dichloroethene-d2	4.01	63	310303	21.47	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	85.88%		
20) 2-Butanone-d5	7.07	46	115667	53.00	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.00%		
24) Chloroform-d	7.64	84	408672	29.16	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	116.64%		
26) 1,2-Dichloroethane-d4	8.31	65	252676m	29.36	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	117.44%		
29) Benzene-d6	8.27	84	770731	31.18	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	124.72%		
33) 1,2-Dichloropropane-d6	9.27	67	238695	31.27	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	125.08%#		
37) Toluene-d8	10.32	98	683944	29.93	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	119.72%		
38) trans-1,3-Dichloropropene-	10.57	79	97150	26.68	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	106.72%		
39) 2-Hexanone-d5	10.93	63	83325	57.91	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	115.82%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	186045	26.21	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	104.84%		
61) 1,2-Dichlorobenzene-d4	13.85	152	186551	28.53	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	114.12%		

7 MQ
 4/9/19

Target Compounds

					Qvalue
13) Acetone	4.12	43	2657982	1136.674	ug/L 100
22) cis-1,2-Dichloroethene	7.17	96	327372	43.139	ug/L 99
35) Trichloroethene	9.09	95	189344	25.540	ug/L 99
44) Toluene	10.38	91	1038477	34.606	ug/L 99
47) Tetrachloroethene	10.86	164	473430	81.083	ug/L 98
53) Ethylbenzene	11.73	91	76755	2.245	ug/L 97
54) m,p-Xylene	11.84	106	161446	12.769	ug/L 100
55) o-xylene	12.16	106	53499	4.443	ug/L 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed