




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
 Data File : VW009797.D
 Acq On : 07 Apr 2019 03:58
 Operator : SY/VA
 Sample : K2217-20
 Misc : 5.38G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF610

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 05:36:41 2019
 Response via : Initial Calibration

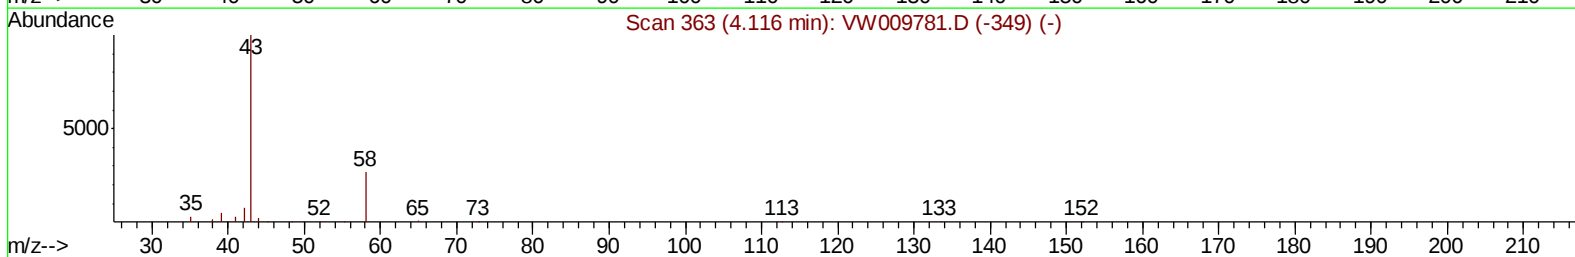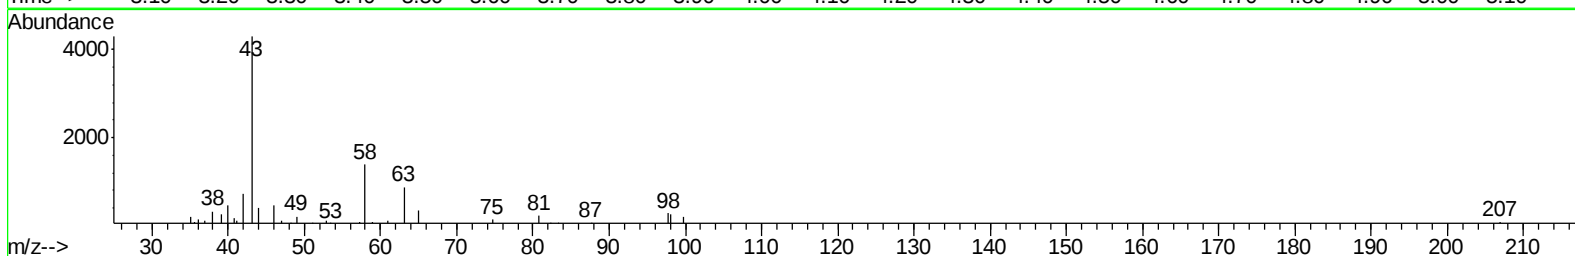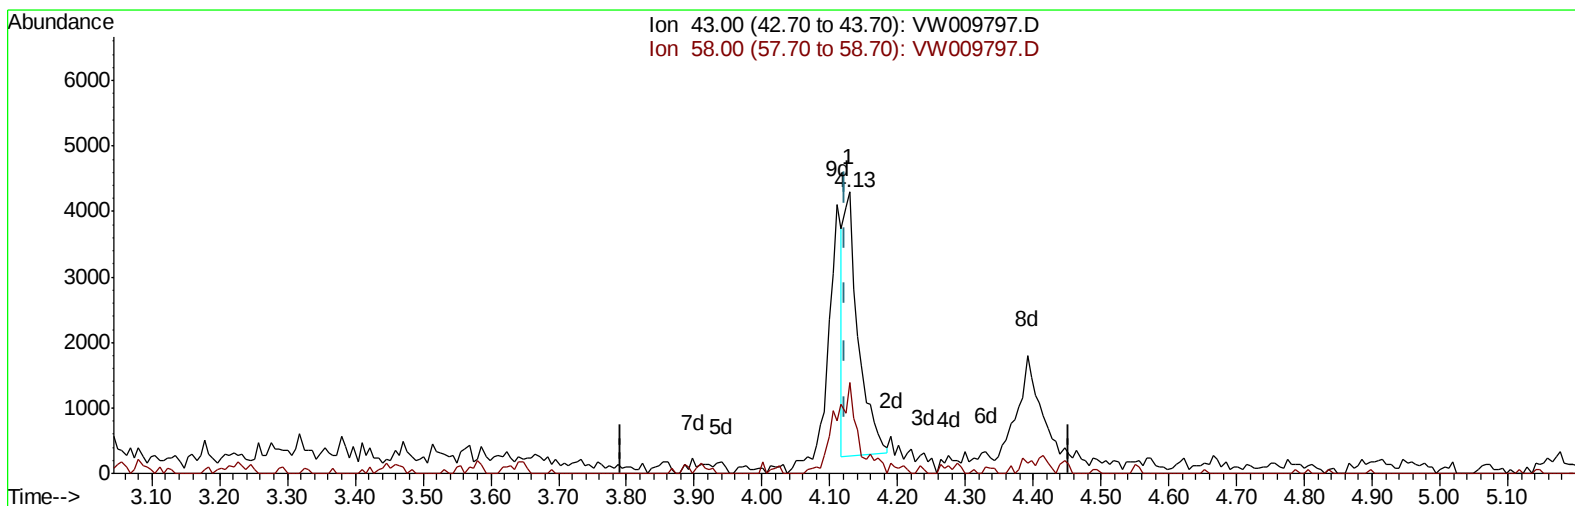

TIC: VW009797.D

(13) Acetone (T)

4.129min (+0.006) 3.46ug/L

response 5870

Ion	Exp%	Act%
43.00	100	100
58.00	26.50	47.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
 Data File : VW009797.D
 Acq On : 07 Apr 2019 03:58
 Operator : SY/VA
 Sample : K2217-20
 Misc : 5.38G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF610

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 05:36:41 2019
 Response via : Initial Calibration

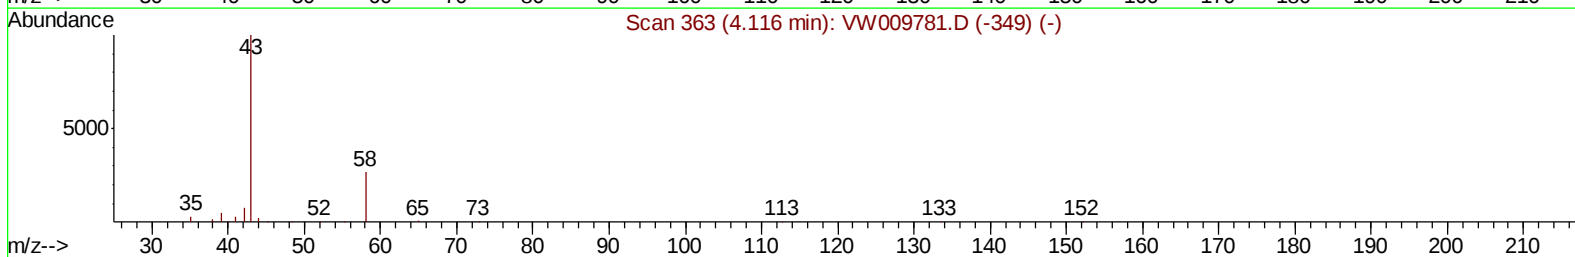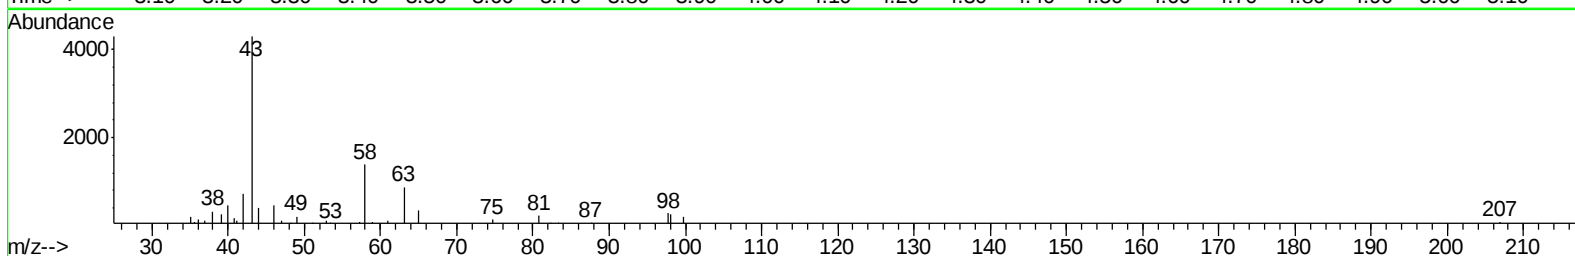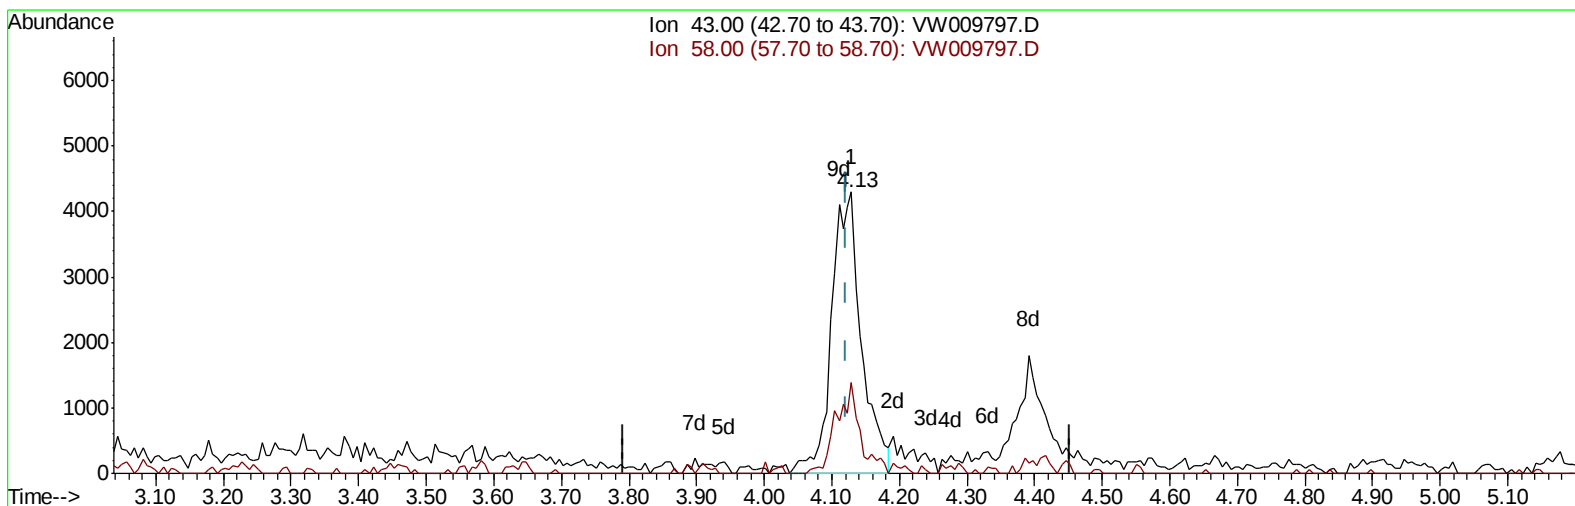

TIC: VW009797.D

(13) Acetone (T)

4.129min (+0.006) 7.70ug/L m

response 13069

Ion	Exp%	Act%
43.00	100	100
58.00	26.50	21.48
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009797.D
Acq On : 07 Apr 2019 03:58
Operator : SY/VA
Sample : K2217-20
Misc : 5.38G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF610

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 05:36:41 2019
Response via : Initial Calibration

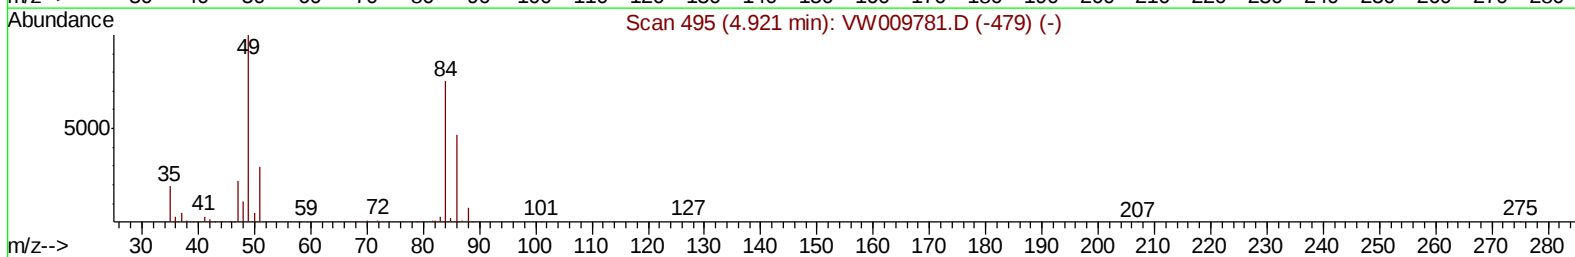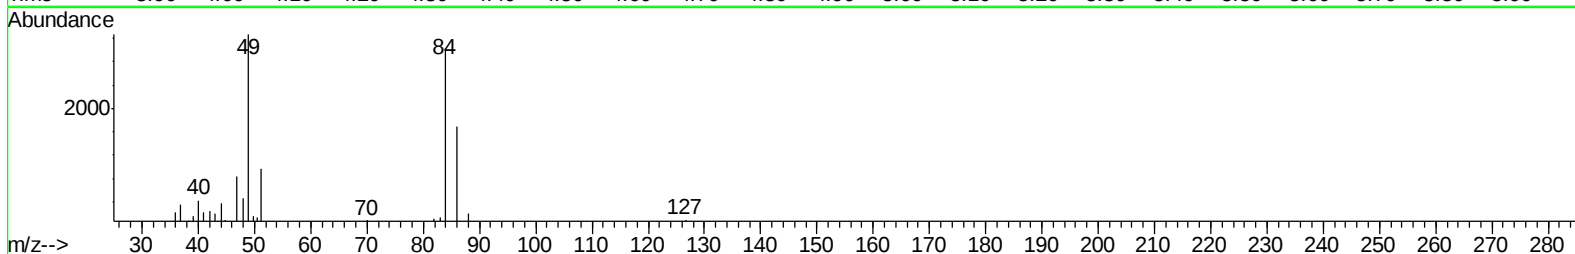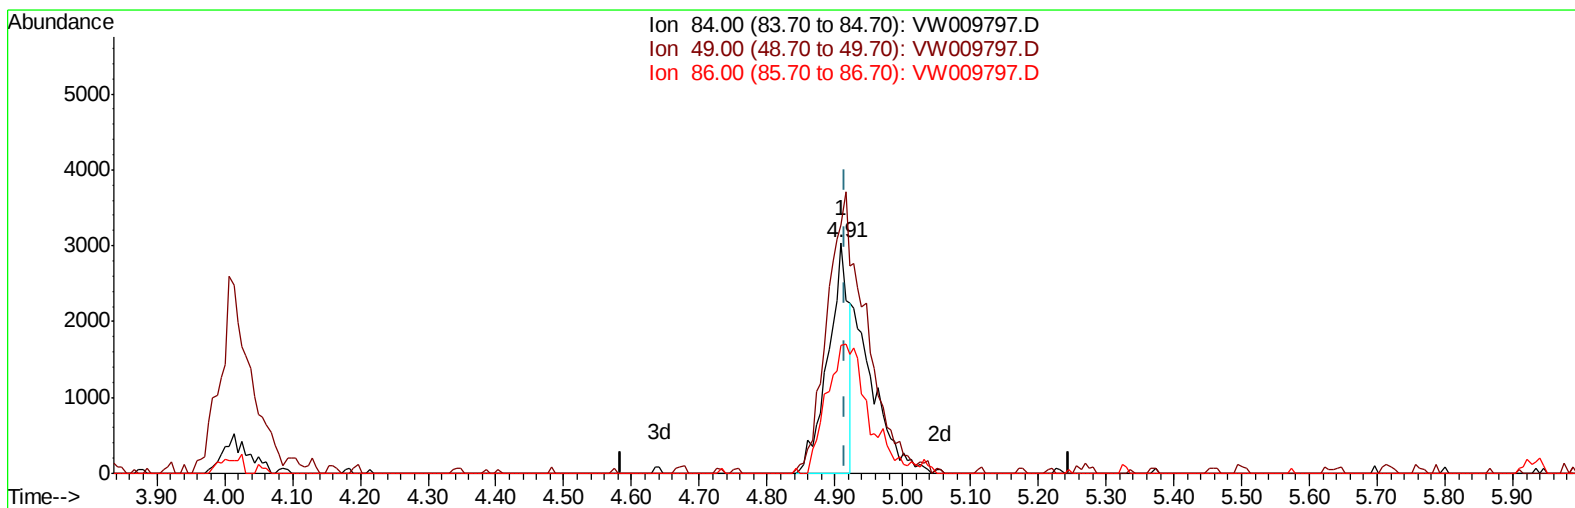

TIC: VW009797.D

(16) Methylene chloride (T)

4.909min (-0.006) 0.96ug/L

response 6282

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	107.67
86.00	66.30	55.38
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
 Data File : VW009797.D
 Acq On : 07 Apr 2019 03:58
 Operator : SY/VA
 Sample : K2217-20
 Misc : 5.38G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF610

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 05:36:41 2019
 Response via : Initial Calibration

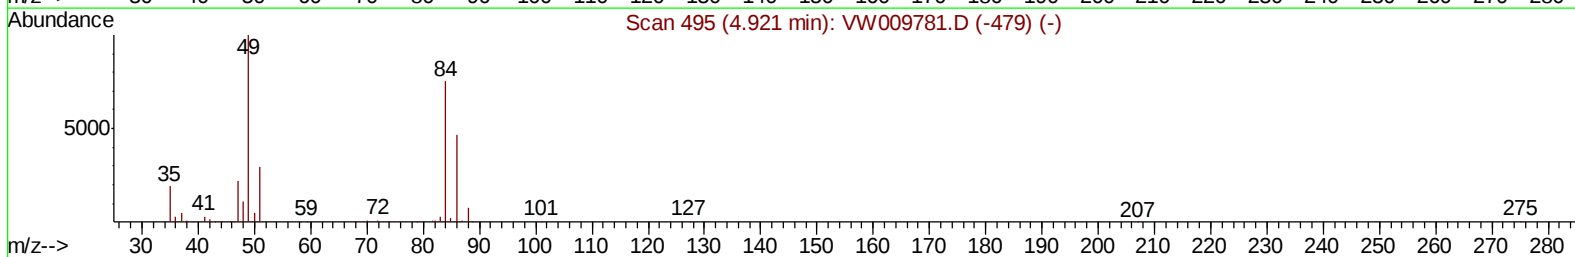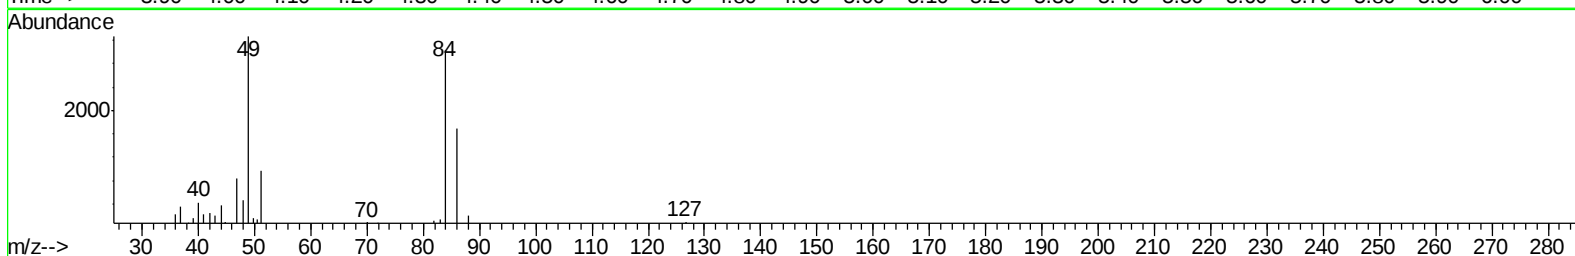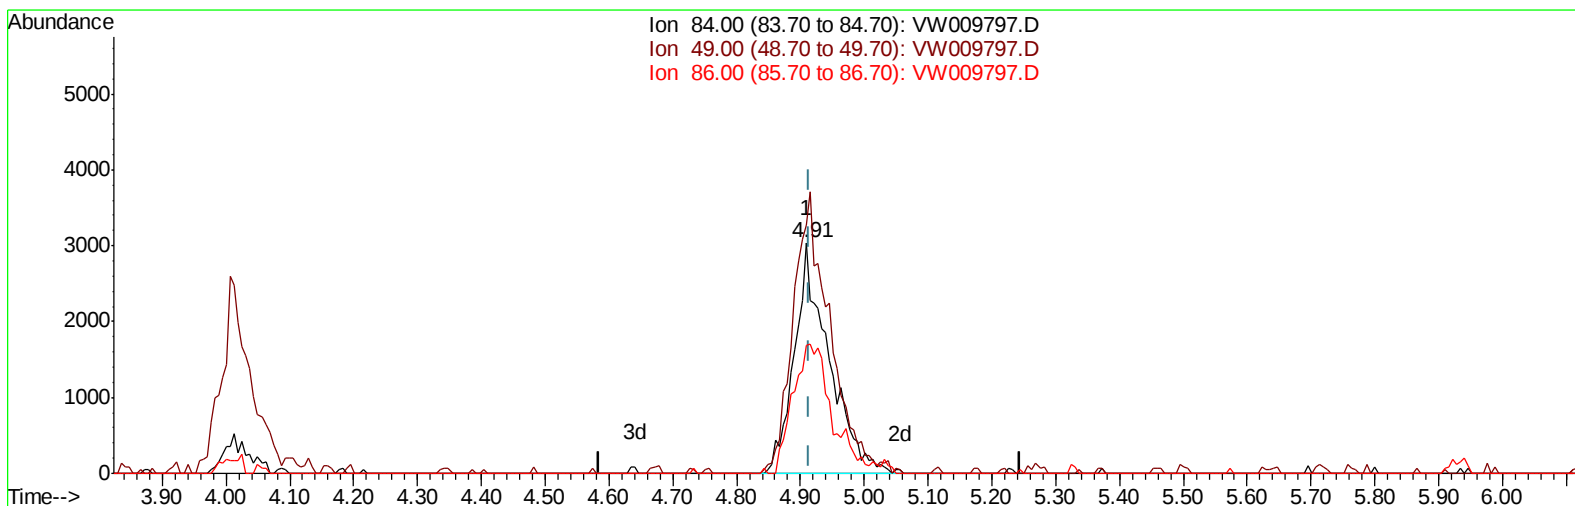

TIC: VW009797.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.75ug/L m

response 11482

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	107.67
86.00	66.30	55.38
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
 Data File : VW009798.D
 Acq On : 07 Apr 2019 04:25
 Operator : SY/VA
 Sample : K2217-19
 Misc : 4.70G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF610

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 05:36:41 2019
 Response via : Initial Calibration

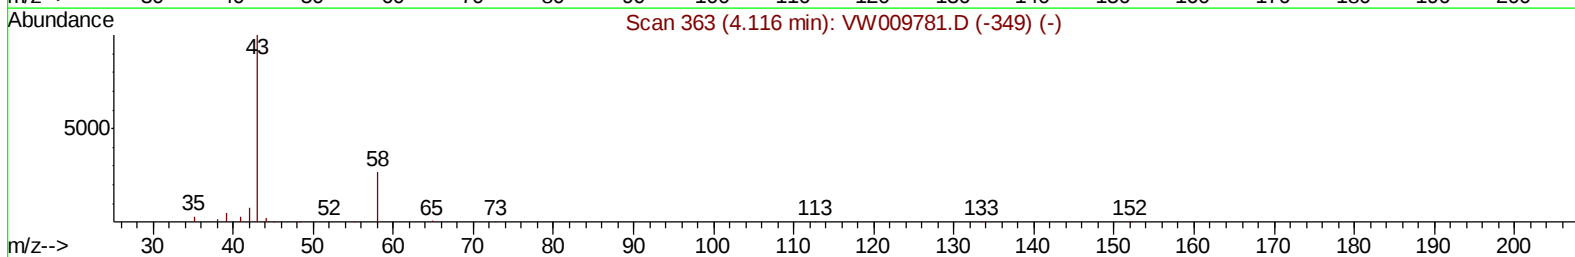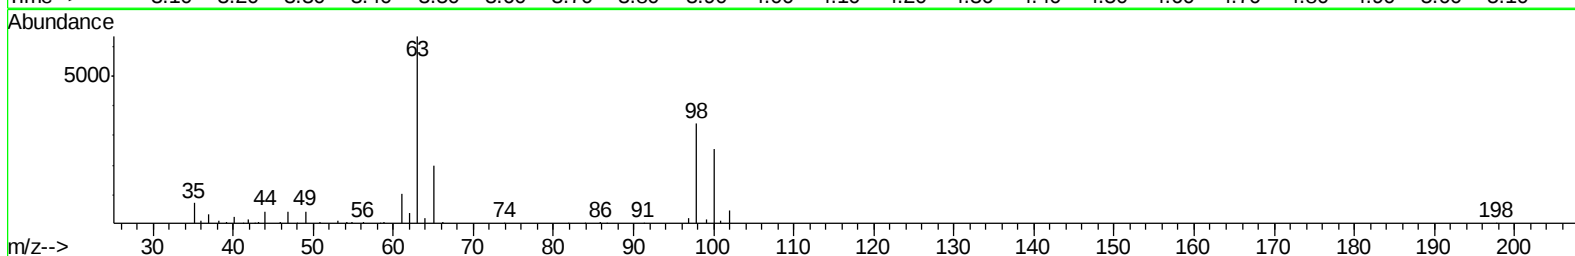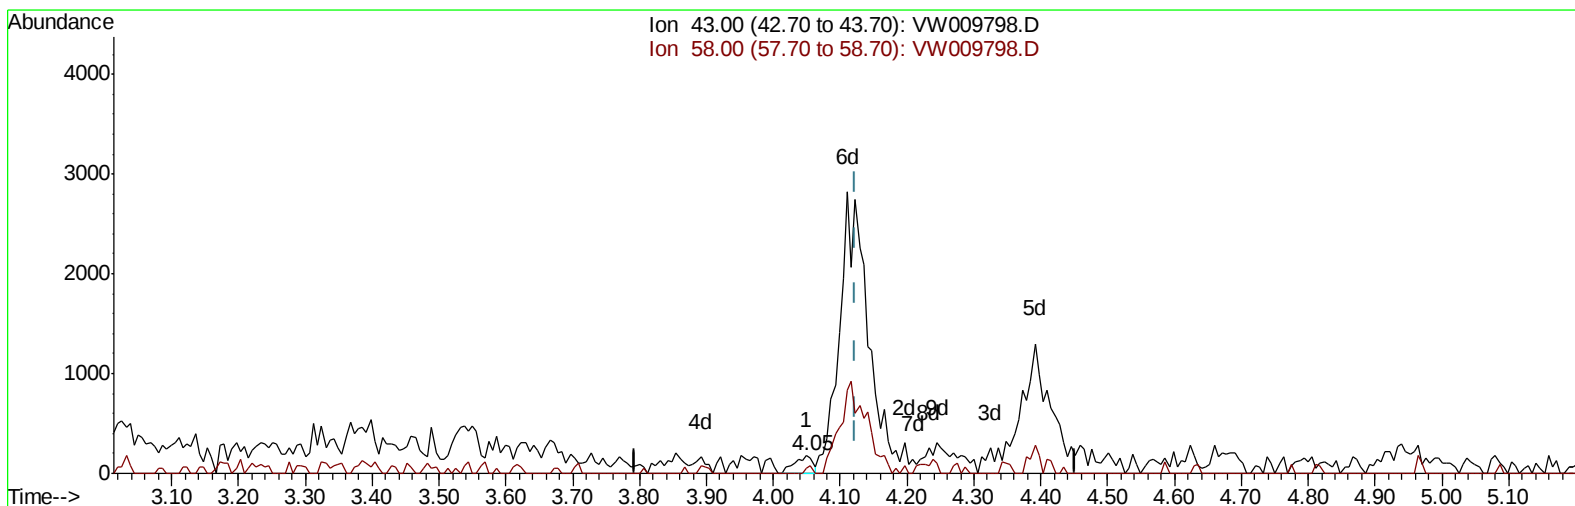

TIC: VW009798.D

(13) Acetone (T)

4.050min (-0.073) 1.07ug/L

response 335

Ion	Exp%	Act%
43.00	100	100
58.00	26.50	13.43
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
 Data File : VW009798.D
 Acq On : 07 Apr 2019 04:25
 Operator : SY/VA
 Sample : K2217-19
 Misc : 4.70G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF610

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 05:36:41 2019
 Response via : Initial Calibration

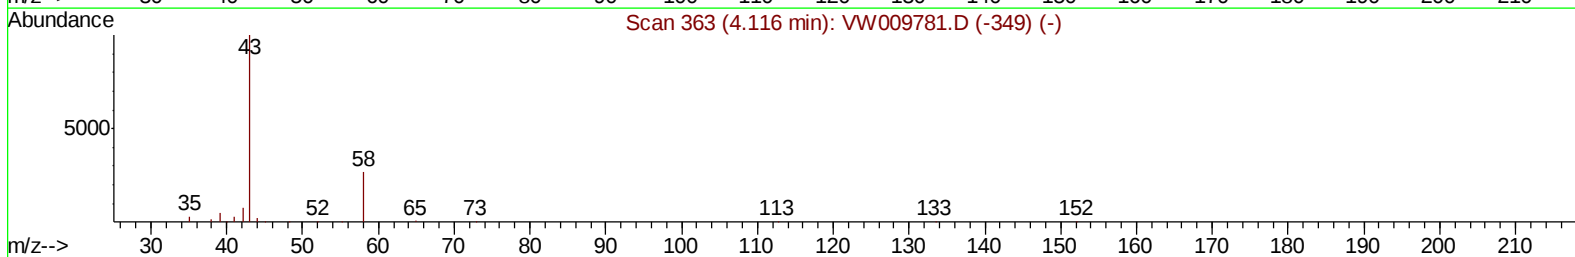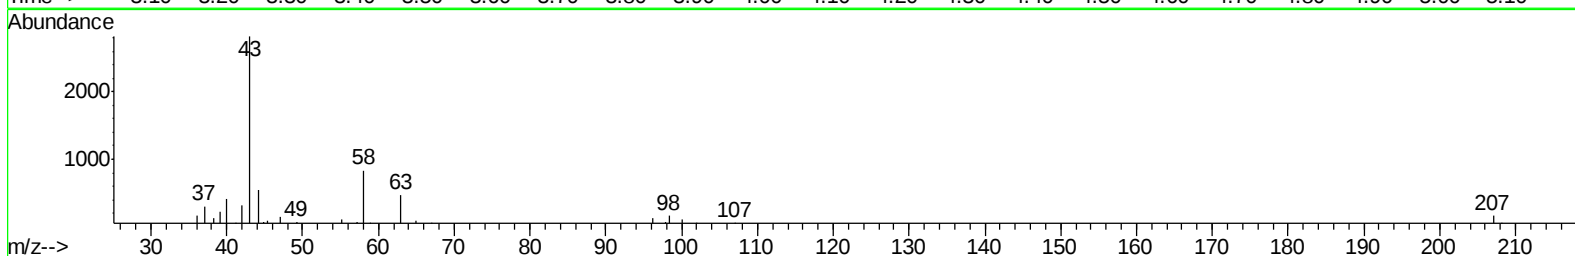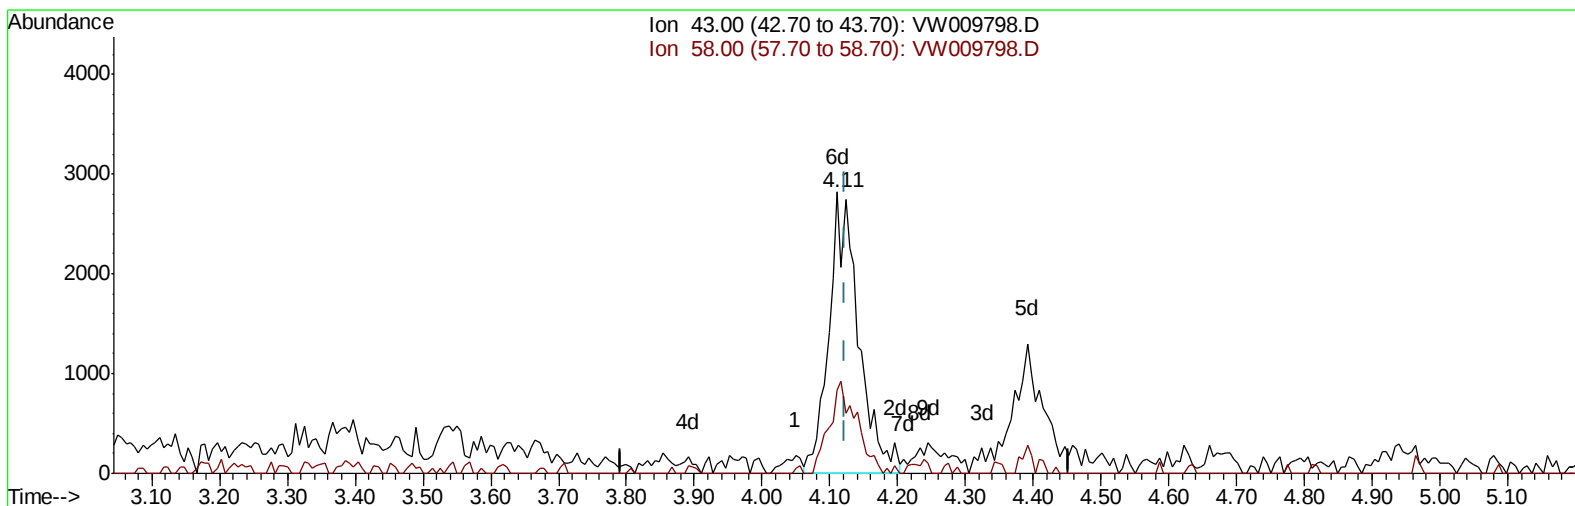

TIC: VW009798.D

(13) Acetone (T)

4.111min (-0.012) 27.19ug/L m

response 8538

Ion	Exp%	Act%
43.00	100	100
58.00	26.50	0.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009798.D
Acq On : 07 Apr 2019 04:25
Operator : SY/VA
Sample : K2217-19
Misc : 4.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF610

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 05:36:41 2019
Response via : Initial Calibration

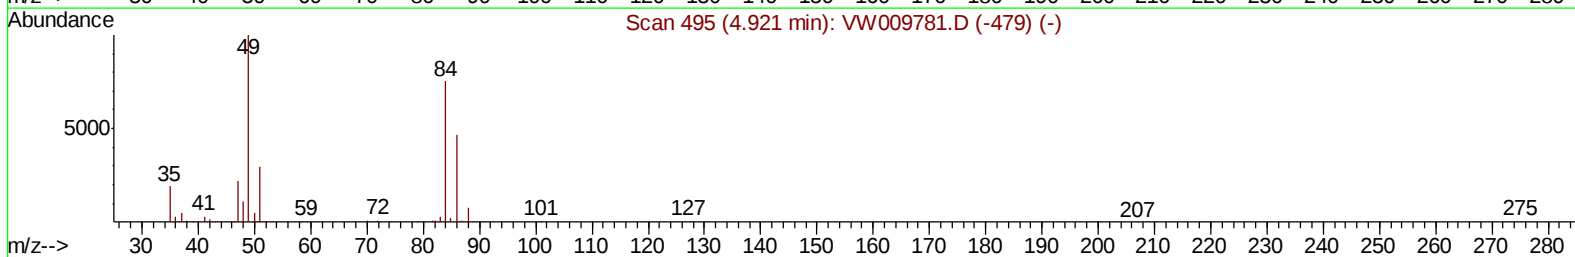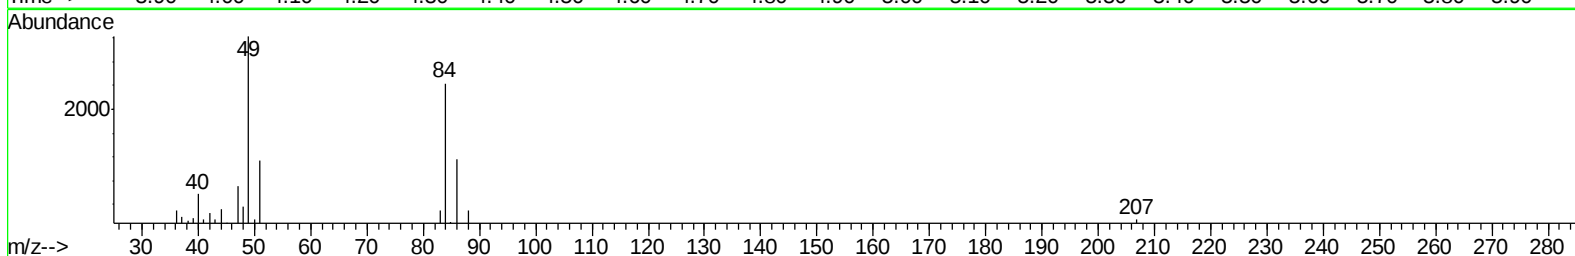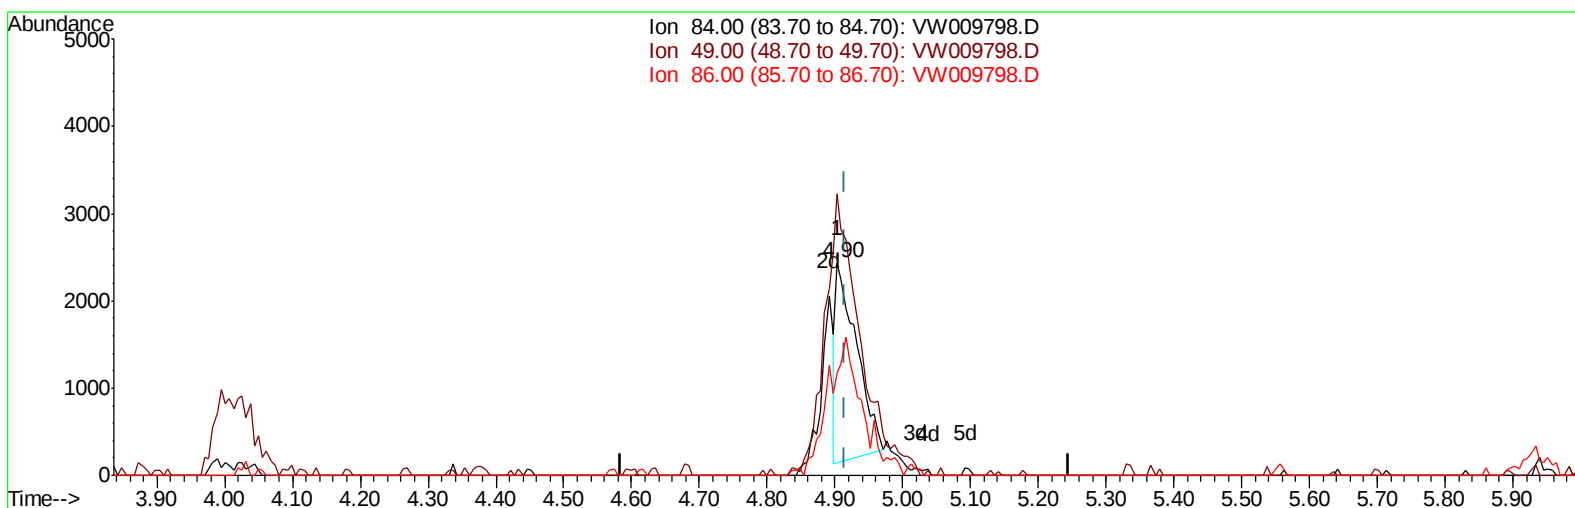

TIC: VW009798.D

(16) Methylene chloride (T)

4.903min (-0.012) 3.99ug/L

response 4853

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	132.51
86.00	66.30	47.95
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009798.D
Acq On : 07 Apr 2019 04:25
Operator : SY/VA
Sample : K2217-19
Misc : 4.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF610

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 05:36:41 2019
Response via : Initial Calibration

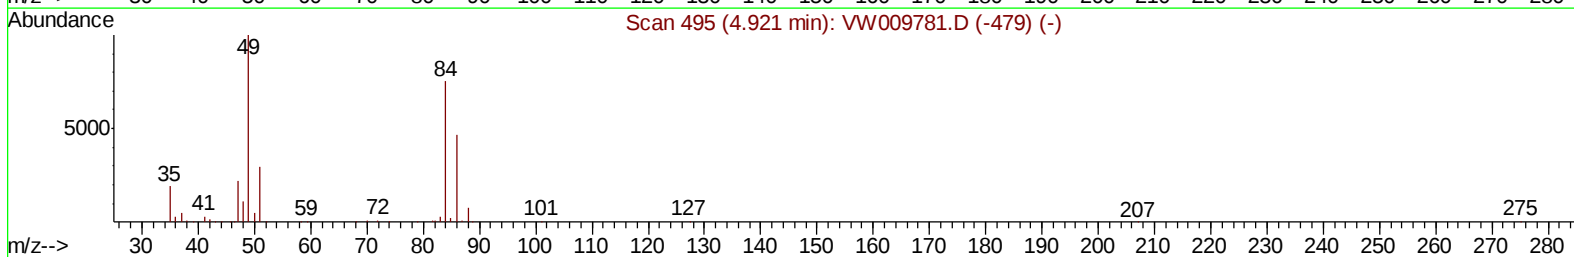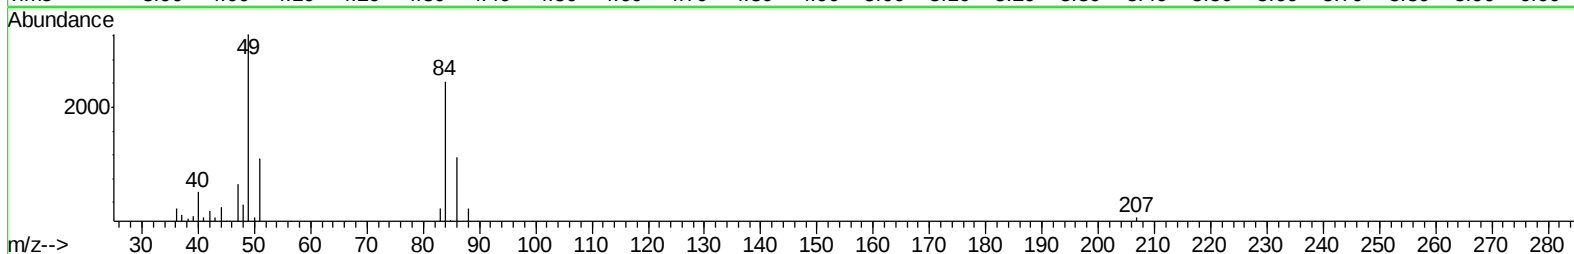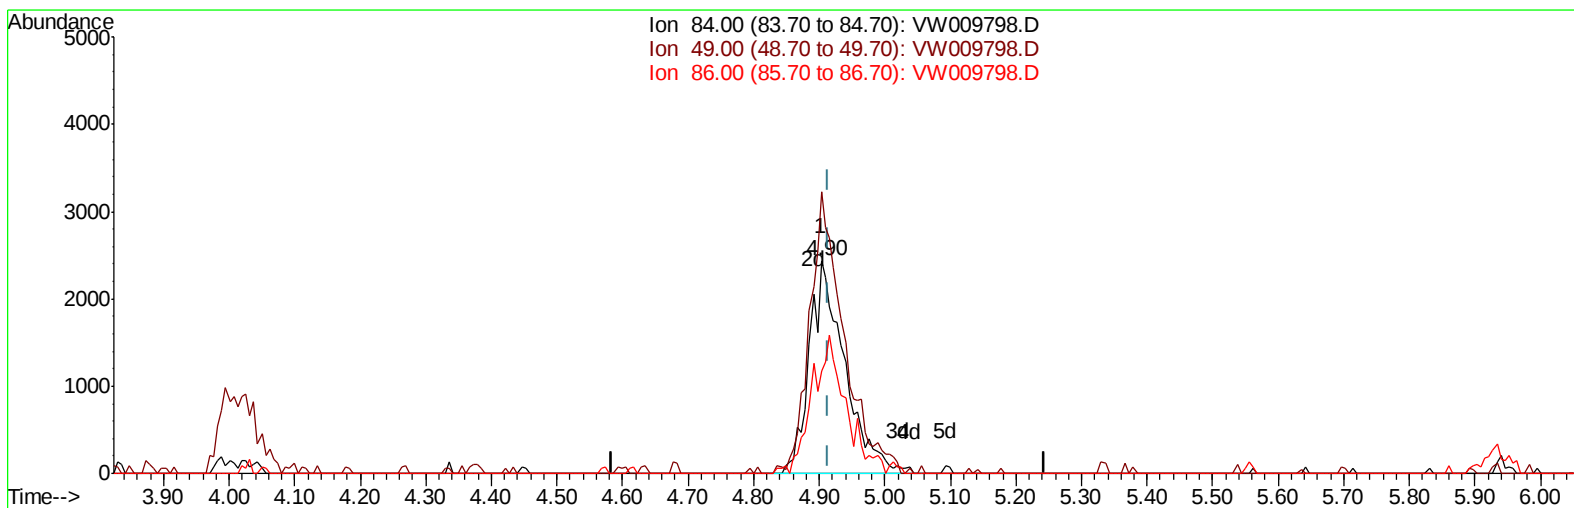

TIC: VW009798.D

(16) Methylene chloride (T)

4.903min (-0.012) 7.46ug/L m

response 9073

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	132.51
86.00	66.30	47.95
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009798.D
Acq On : 07 Apr 2019 04:25
Operator : SY/VA
Sample : K2217-19
Misc : 4.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF610

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:27 AM

Quant Time: Apr 07 05:40:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 05:36:41 2019
Response via : Initial Calibration

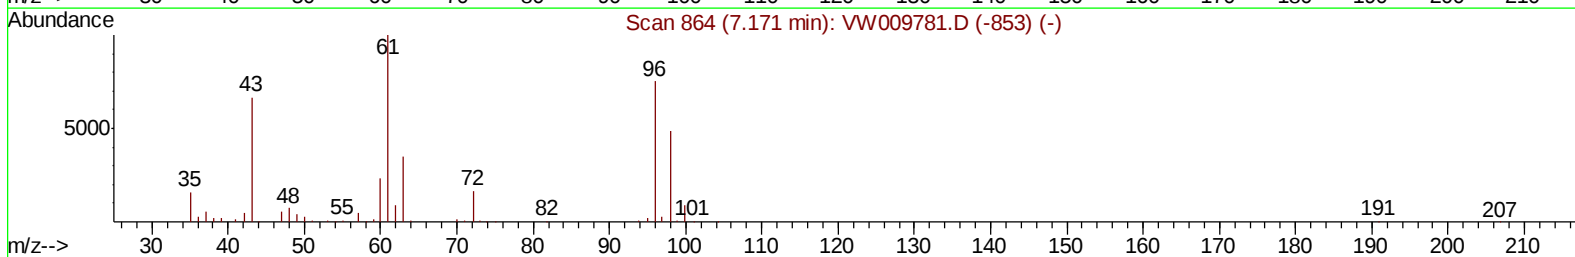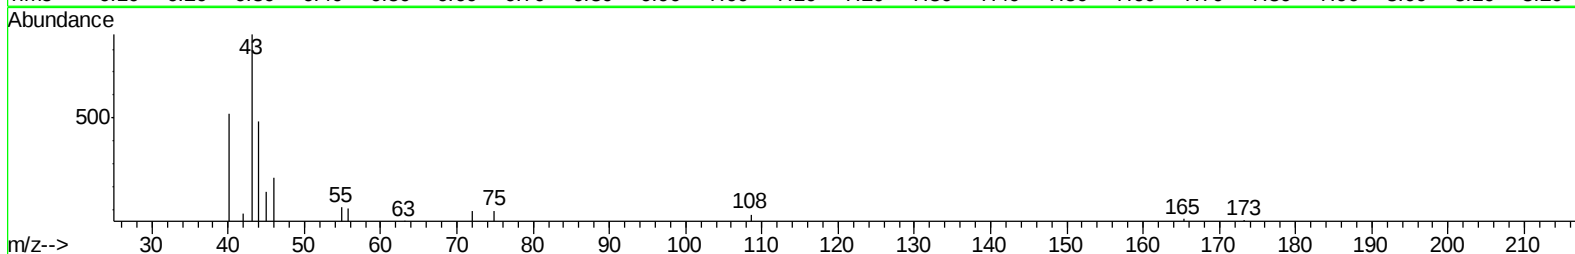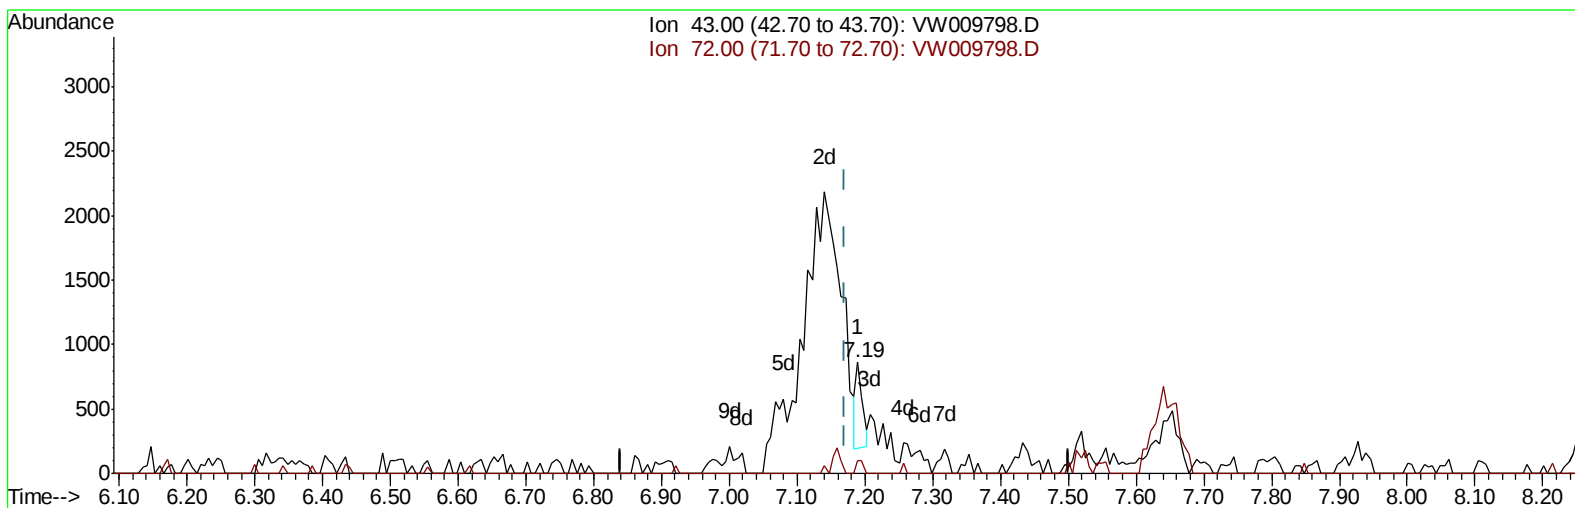

TIC: VW009798.D

(21) 2-Butanone

7.189min (+0.018) 1.10ug/L

response 441

Ion	Exp%	Act%
43.00	100	100
72.00	24.10	16.33
0.00	0.00	0.00
0.00	0.00	0.00