

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW040619\

Data File : VW009801.D

Acq On : 07 Apr 2019 11:13

Operator : SY/VA

Sample : K2168-18

Misc : 4.89G/10ML/MSVOA W/SOIL

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 17 04:08:48 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis


QLast Update : Mon Apr 08 00:51:56 2019

Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
BF675

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:29 AM

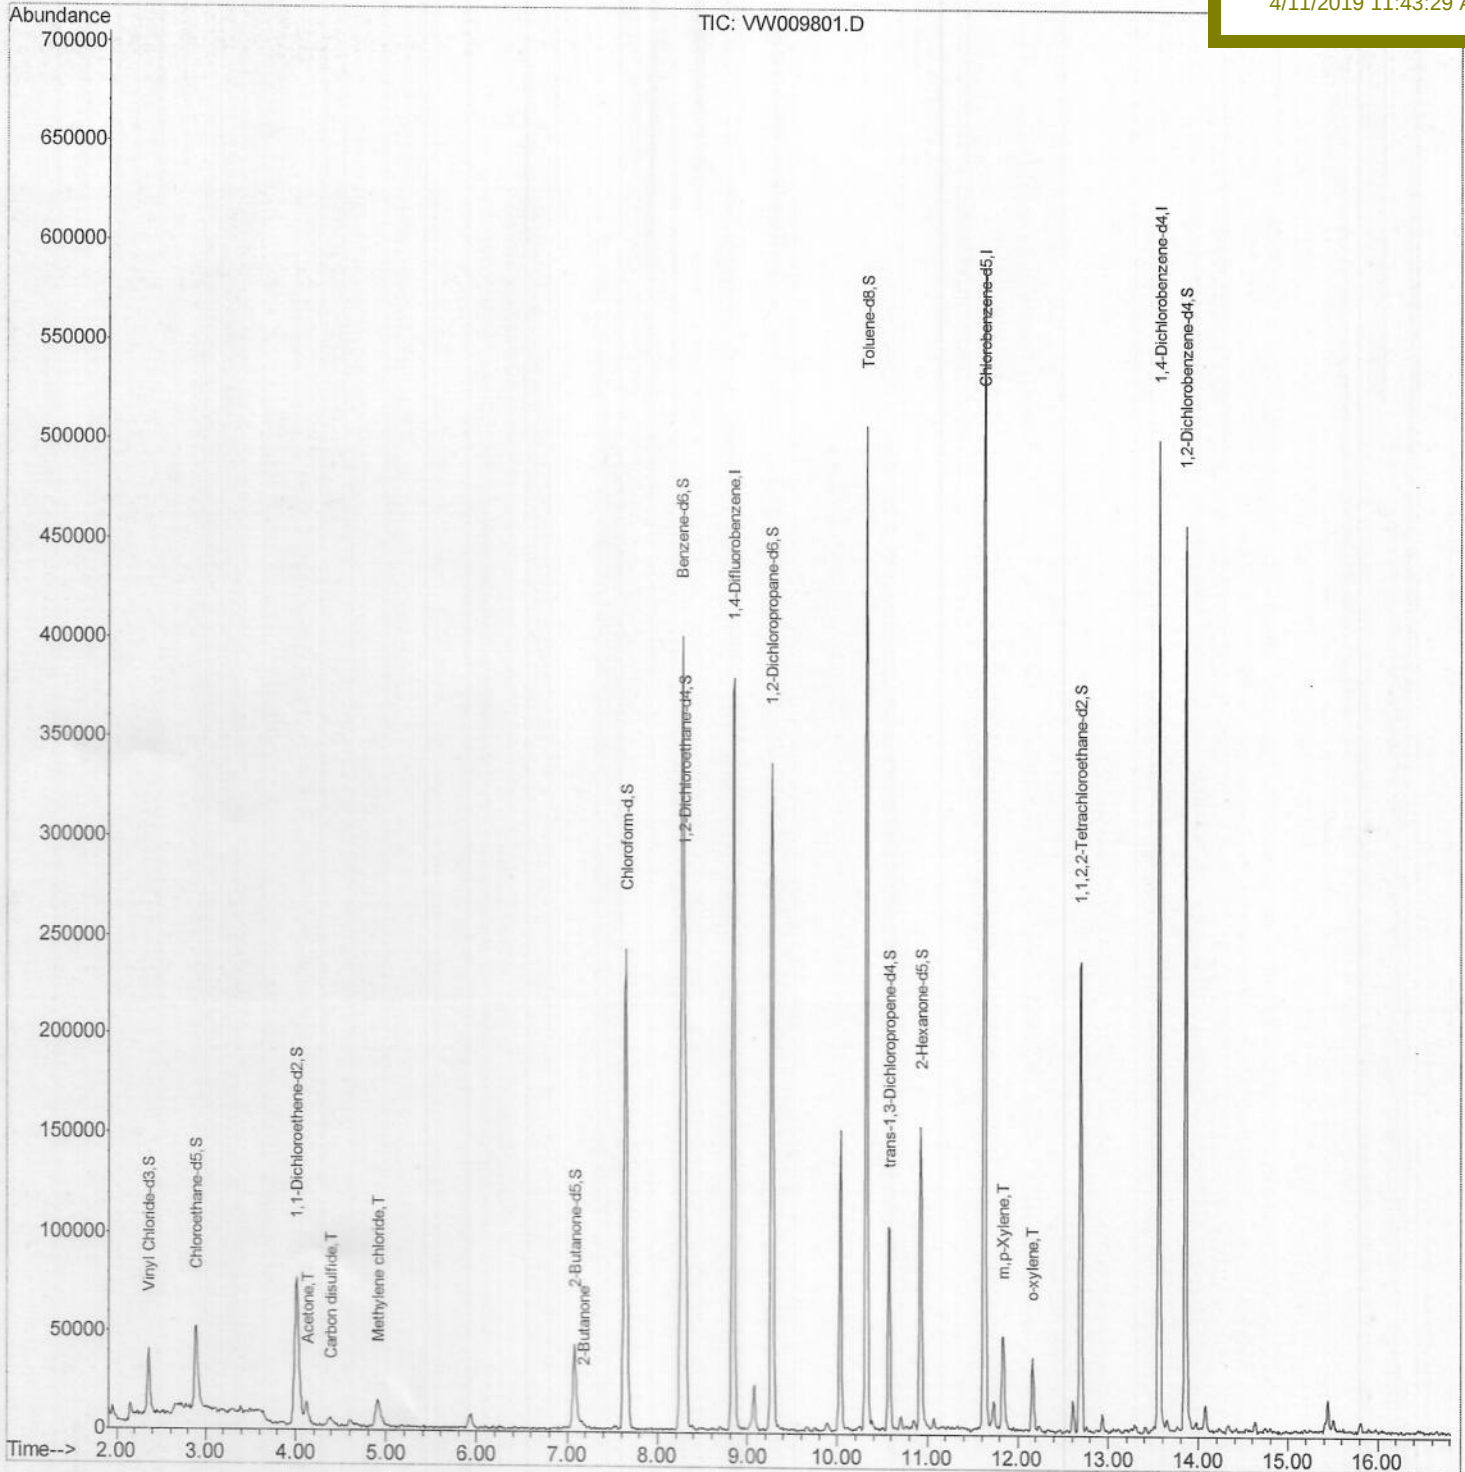

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009801.D
 Acq On : 07 Apr 2019 11:13
 Operator : SY/VA
 Sample : K2168-18
 Misc : 4.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF675

Quant Time: Apr 08 00:54:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Apr 08 00:51:56 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:29 AM

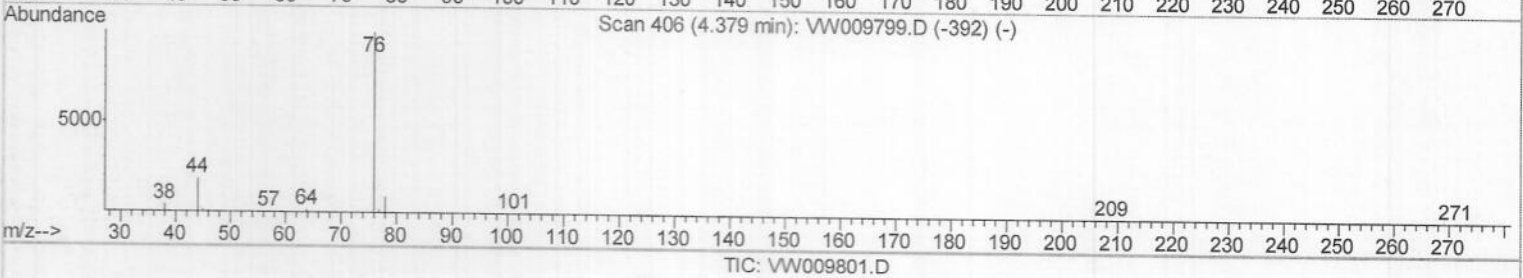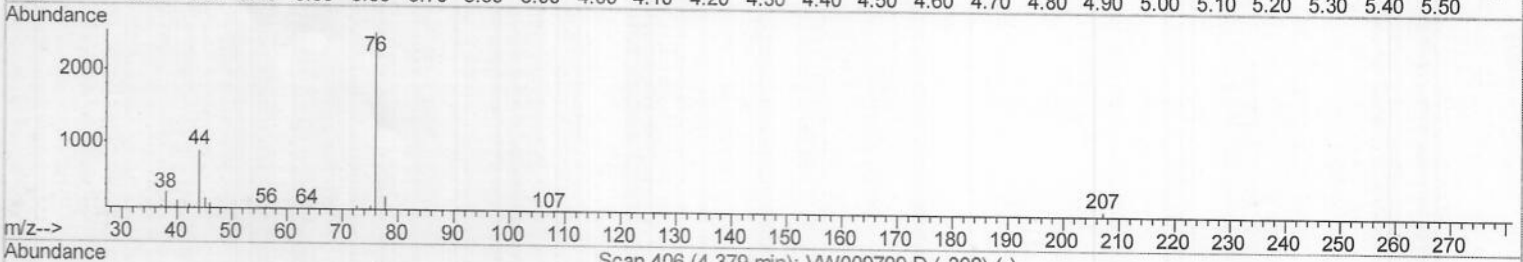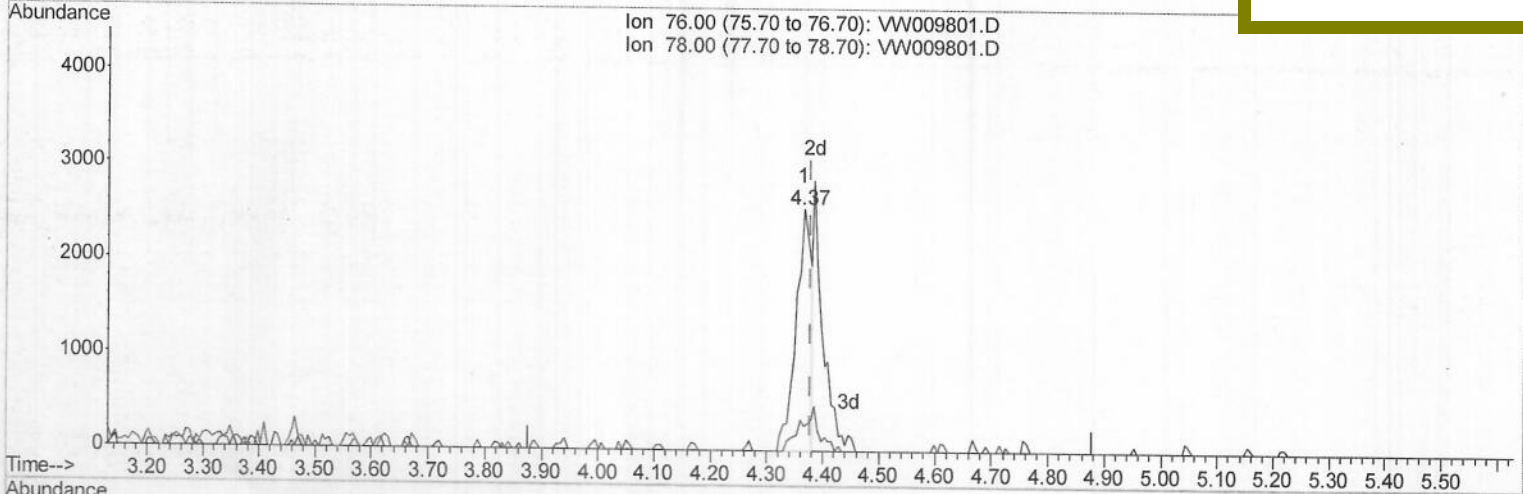

(14) Carbon disulfide (T)

4.367min (-0.012) 0.39ug/L

response 4644

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	10.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\

Data File : VW009801.D

Acq On : 07 Apr 2019 11:13

Operator : SY/VA

Sample : K2168-18

Misc : 4.89G/10ML/MSVOA_W/SOIL

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 08 00:54:39 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Mon Apr 08 00:51:56 2019




Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :

BF675

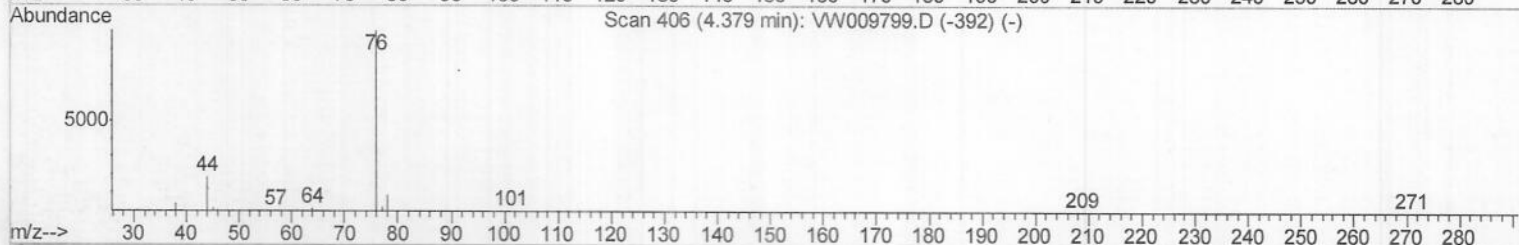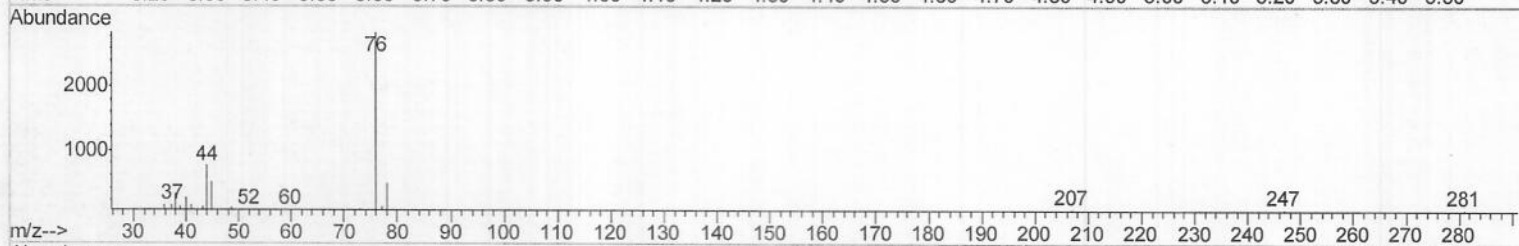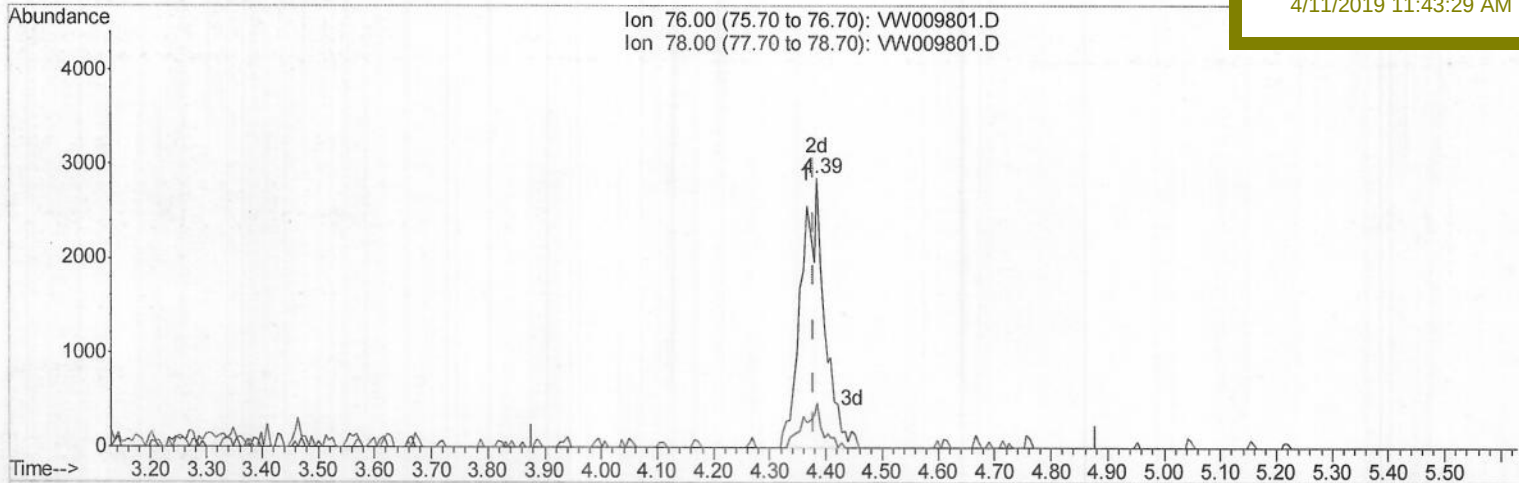Manual Integrations
APPROVEDMMDadoda
4/11/2019 11:43:29 AM

TIC: VW009801.D

(14) Carbon disulfide (T)

4.385min (+0.006) 0.68ug/L m

response 8114

3 M.D.
04/11/19

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	16.50#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009801.D
 Acq On : 07 Apr 2019 11:13
 Operator : SY/VA
 Sample : K2168-18
 Misc : 4.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 BF675

Quant Time: Apr 08 00:54:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Apr 08 00:51:56 2019
 Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
 4/11/2019 11:43:29 AM

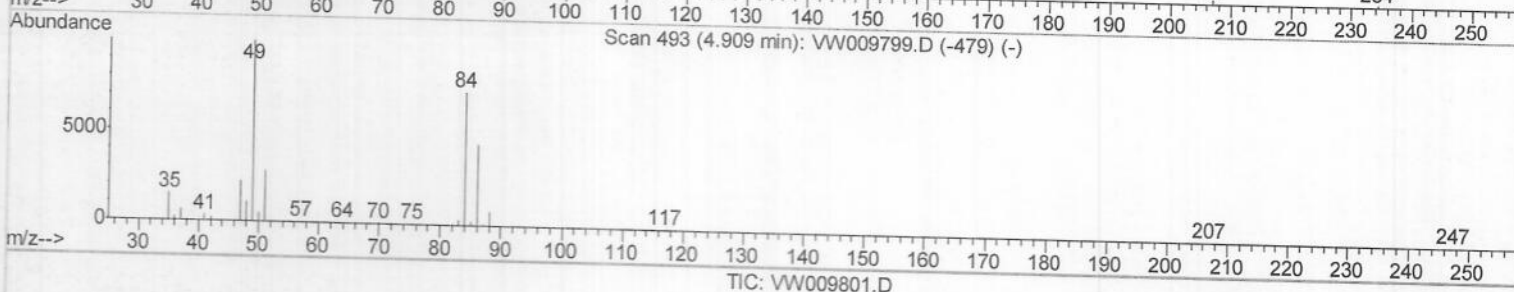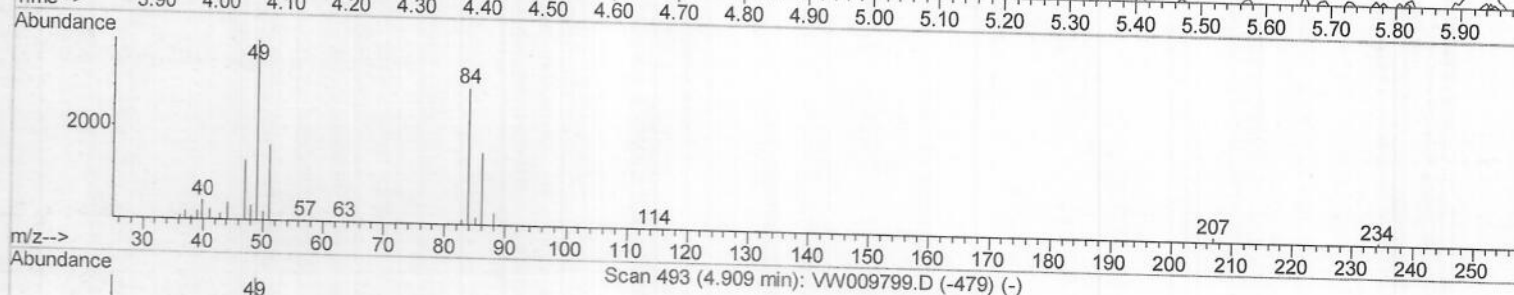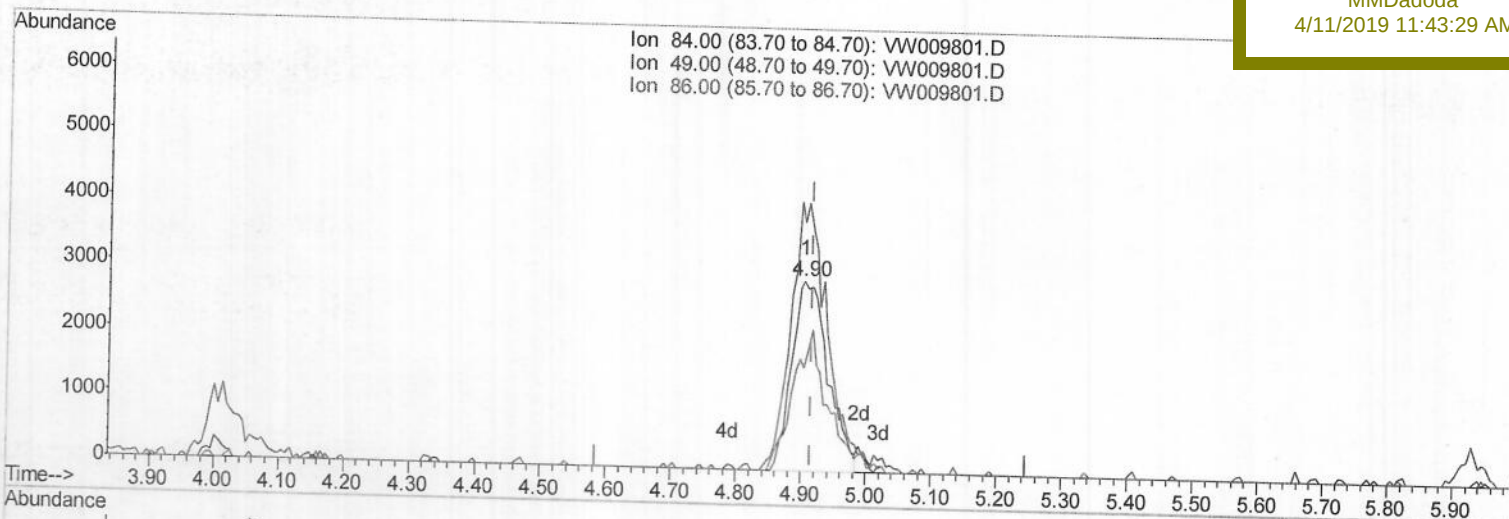

(16) Methylene chloride (T)

4.903min (-0.012) 2.20ug/L

response 11197

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	130.45
86.00	66.30	54.15
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009801.D
 Acq On : 07 Apr 2019 11:13
 Operator : SY/VA
 Sample : K2168-18
 Misc : 4.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF675

Quant Time: Apr 08 00:54:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Apr 08 00:51:56 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:29 AM

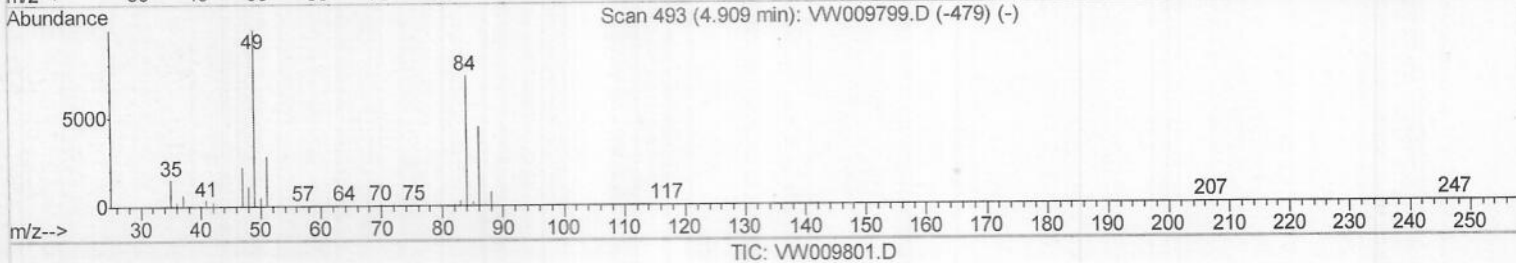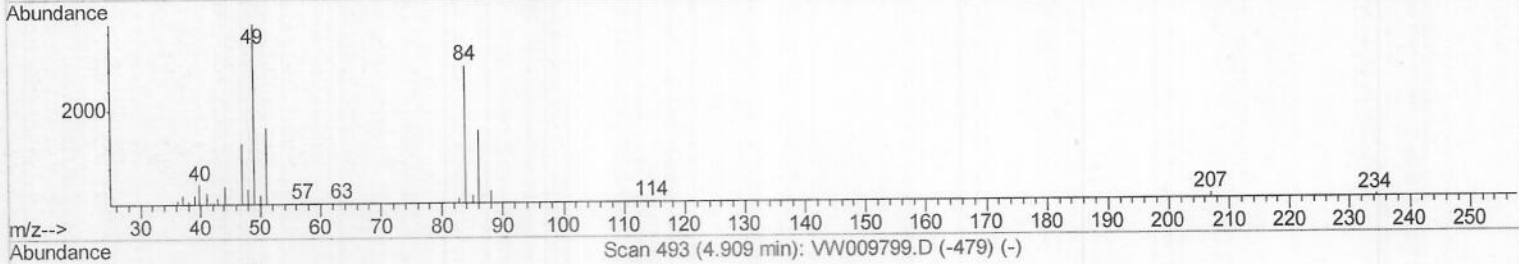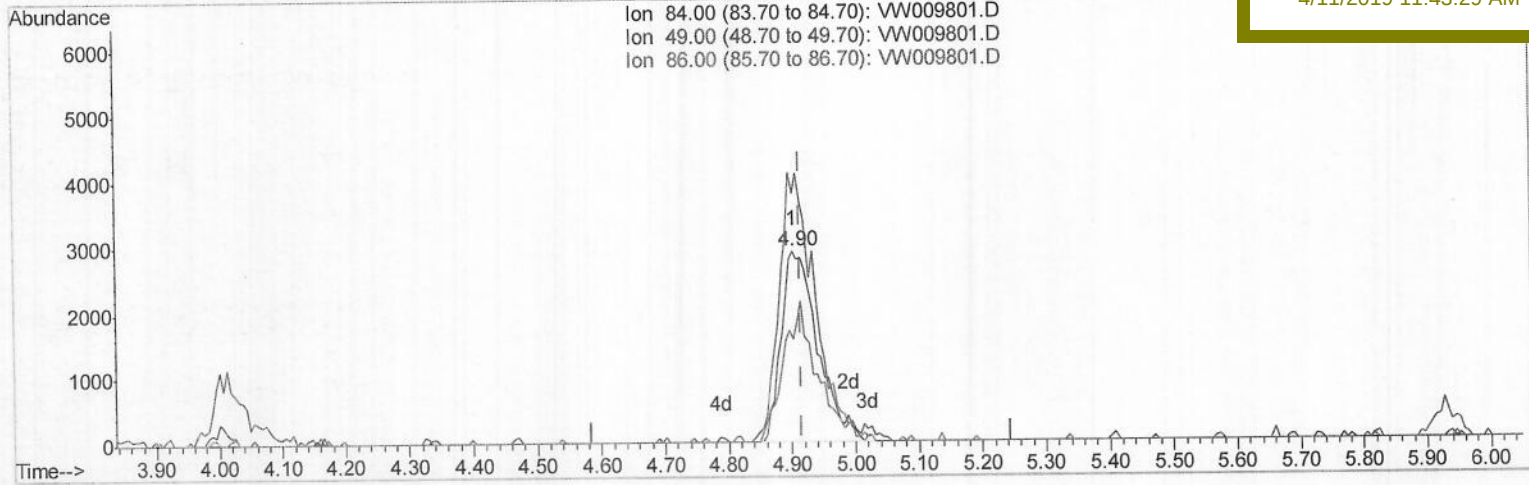

(16) Methylene chloride (T)

4.903min (-0.012) 2.27ug/L m

response 11569

Ion Exp% Act%

84.00 100 100

49.00 140.40 130.45

86.00 66.30 54.15

0.00 0.00 0.00

3 M.D.
 04/11/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW040619\
 Data File : VW009801.D
 Acq On : 07 Apr 2019 11:13
 Operator : SY/VA
 Sample : K2168-18
 Misc : 4.89G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF675

Quant Time: Apr 17 04:08:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Apr 08 00:51:56 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:29 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	288508	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	303369	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	114150	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.35	65	40348	10.69	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	42.76%		
7) Chloroethane-d5	2.89	69	59868	17.31	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.24%		
10) 1,1-Dichloroethene-d2	4.01	63	90374	11.13	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	44.52%#		
20) 2-Butanone-d5	7.07	46	72389	59.05	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	118.10%		
24) Chloroform-d	7.64	84	224068	28.46	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	113.84%		
26) 1,2-Dichloroethane-d4	8.30	65	155834	32.24	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	128.96%		
29) Benzene-d6	8.27	84	372011	23.36	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	93.44%		
33) 1,2-Dichloropropane-d6	9.27	67	140866	28.64	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	114.56%		
37) Toluene-d8	10.32	98	314749	21.38	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.52%		
38) trans-1,3-Dichloropropene-	10.57	79	51456	21.93	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	87.72%		
39) 2-Hexanone-d5	10.93	63	44145	47.61	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.22%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	109934	24.04	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	96.16%		
61) 1,2-Dichlorobenzene-d4	13.85	152	110579	27.61	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	110.44%		
Target Compounds						
13) Acetone	4.12	43	18369	13.986	ug/L	99
14) Carbon disulfide	4.39	76	8114m	0.681	ug/L	
16) Methylene chloride	4.90	84	11569m	2.274	ug/L	
21) 2-Butanone	7.18	43	3373	2.019	ug/L	92
54) m,p-Xylene	11.83	106	13463	1.653	ug/L	98
55) o-xylene	12.16	106	7530	0.971	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

M.D.
 04/11/19