

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040619\
 Data File : VW009758.D
 Acq On : 06 Apr 2019 05:41
 Operator : SY/VA
 Sample : K2188-09
 Misc : 5.22G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF653

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:42:55 AM

Quant Time: Apr 06 07:17:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 06 05:36:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	382662	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	367252	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	150388	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	116133	23.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.76%
7) Chloroethane-d5	2.89	69	110377	24.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.24%
10) 1,1-Dichloroethene-d2	4.01	63	197599	18.35	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.40%
20) 2-Butanone-d5	7.08	46	79212	48.72	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.44%
24) Chloroform-d	7.65	84	262180	25.11	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.44%
26) 1,2-Dichloroethane-d4	8.31	65	171109	26.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.76%
29) Benzene-d6	8.27	84	502794	26.08	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.32%
33) 1,2-Dichloropropane-d6	9.27	67	158613	26.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.56%
37) Toluene-d8	10.32	98	436920	24.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.04%
38) trans-1,3-Dichloropropene-	10.58	79	58038	20.44	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.76%
39) 2-Hexanone-d5	10.93	63	51624	46.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.00%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	123078	22.23	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.92%
61) 1,2-Dichlorobenzene-d4	13.86	152	138000	26.15	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.60%

Target Compounds

					Ovalue
13) Acetone	4.12	43	42875	24.613 ug/L	96
14) Carbon disulfide	4.37	76	6942m	0.439 ug/L	
16) Methylene chloride	4.91	84	18857	2.794 ug/L	92
21) 2-Butanone	7.17	43	11163	5.039 ug/L	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW040619\
Data File : VW009758.D
Acq On : 06 Apr 2019 05:41
Operator : SY/VA
Sample : K2188-09
Misc : 5.22G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BF653

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:55 AM

Quant Time: Apr 06 07:17:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 05:36:42 2019
Response via : Initial Calibration

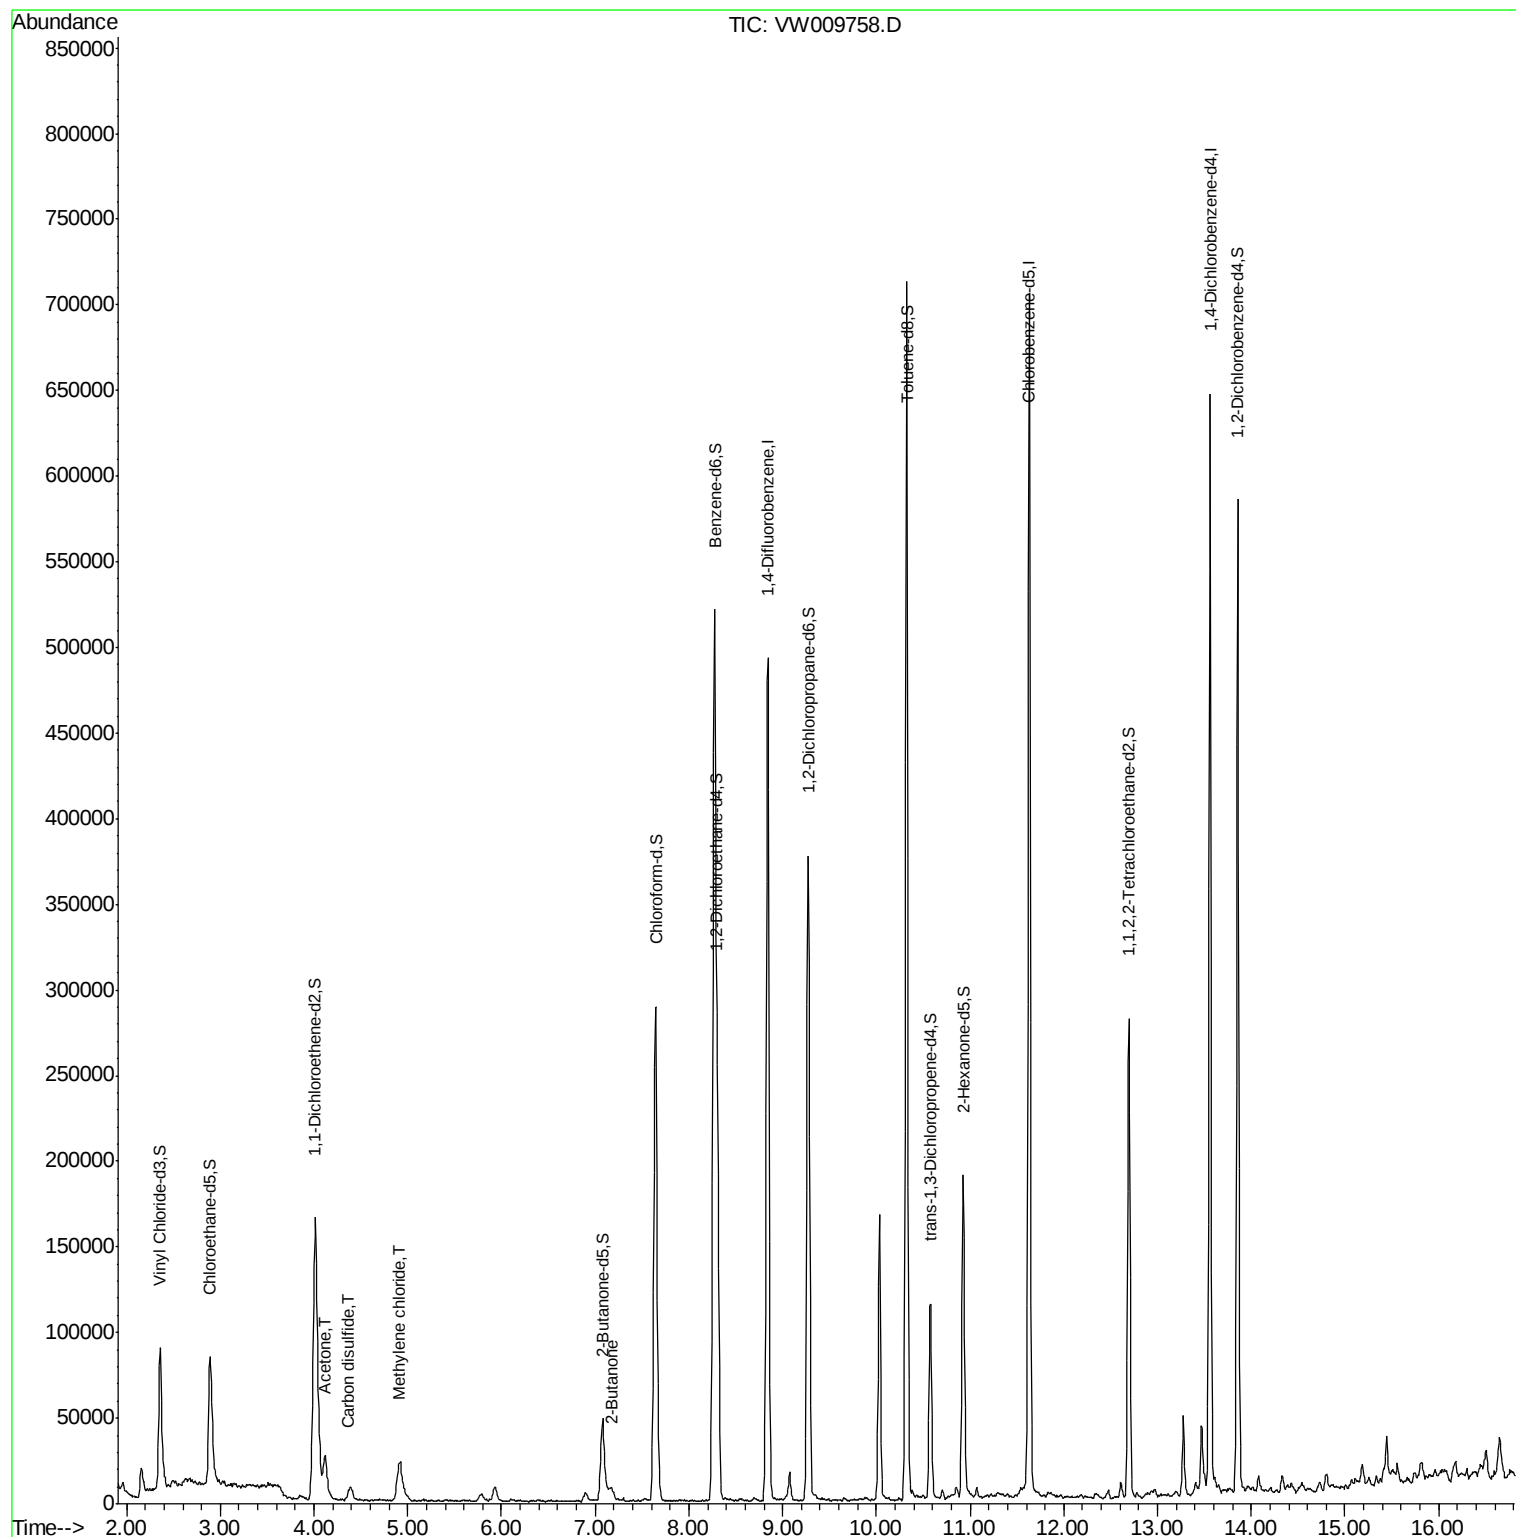

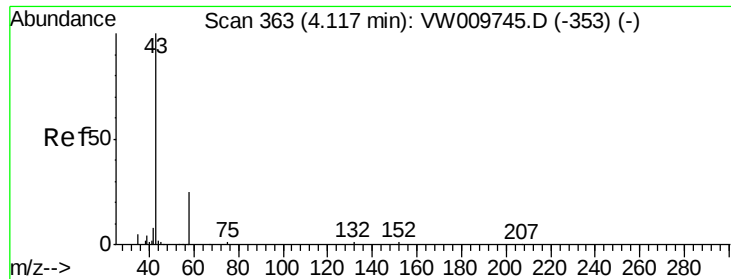





#13
Acetone
Concen: 24.613 ug/L
RT: 4.12 min Scan# 363
Delta R.T. -0.01 min
Lab File: VW009758.D
Acq: 06 Apr 2019 05:41

Instrument :
MSVOA_W
ClientSampleId :
BF653

Tot Ion	43	Resp	42875
Ion Ratio	100	Lower	Upper
58	28.7	0.0	53.0




Manual Integrations
APPROVED


MMDadoda
4/11/2019 11:42:55 AM

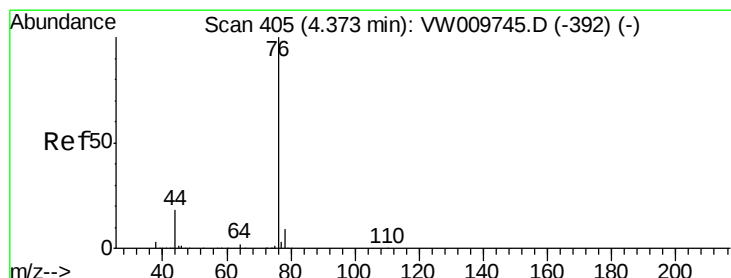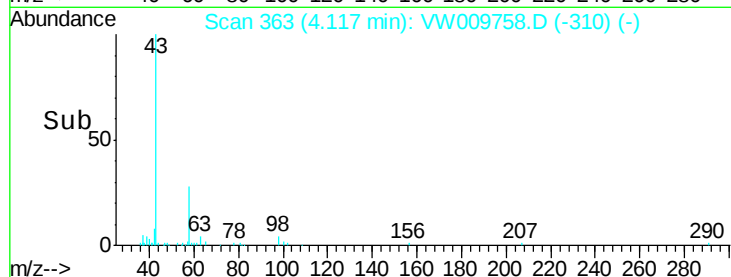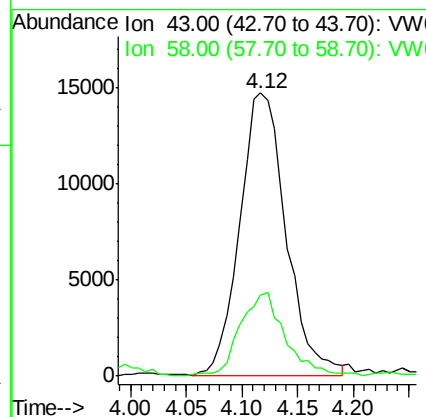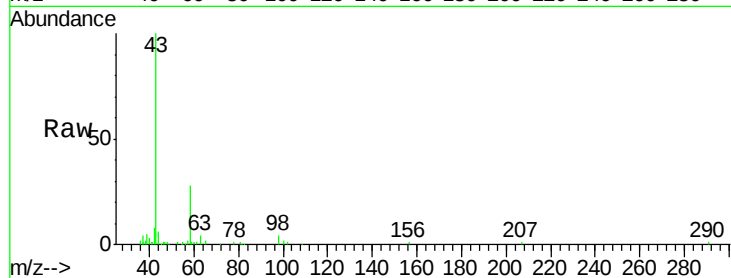

#14
Carbon disulfide
Concen: 0.439 ug/L m
RT: 4.37 min Scan# 404
Delta R.T. -0.01 min
Lab File: VW009758.D
Acq: 06 Apr 2019 05:41

Tgt Ion	76	Resp	6942
Ion Ratio	100	Lower	Upper
78	14.9	7.3	10.9#

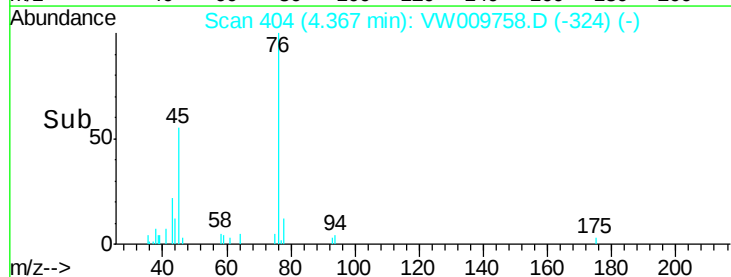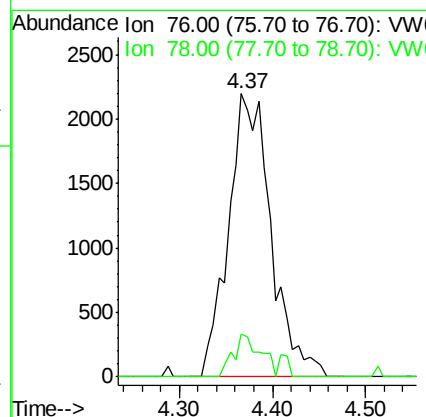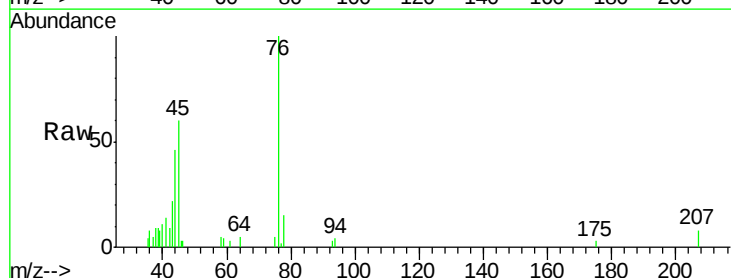

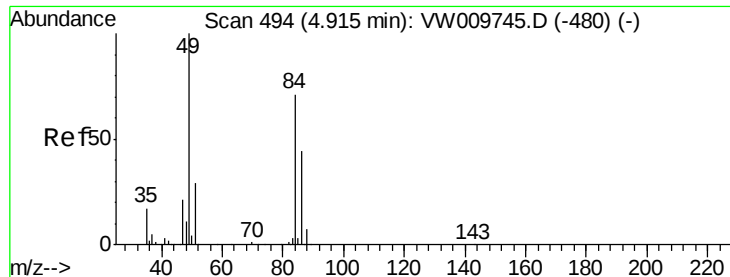





#16
Methvlene chloride
Concen: 2.794 ug/L
RT: 4.91 min Scan# 493
Delta R.T. -0.01 min
Lab File: VW009758.D
Acq: 06 Apr 2019 05:41

Instrument :
MSVOA_W
ClientSampleId :
BF653

Tot Ion	84	Resp	18857
Ion Ratio	Lower	Upper	
84	100		
49	152.3	98.3	182.5
86	62.8	46.4	86.2

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:55 AM

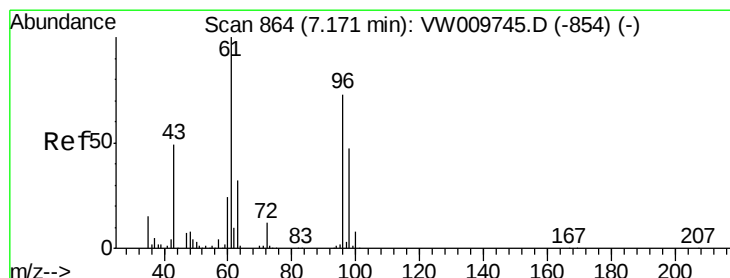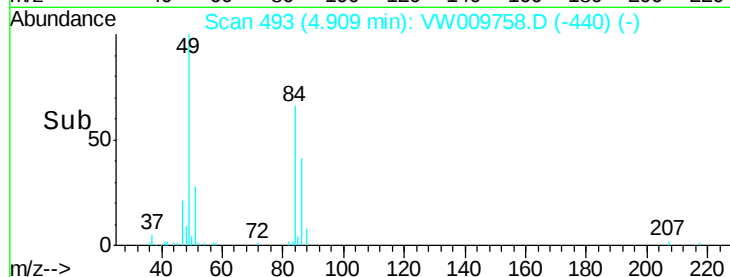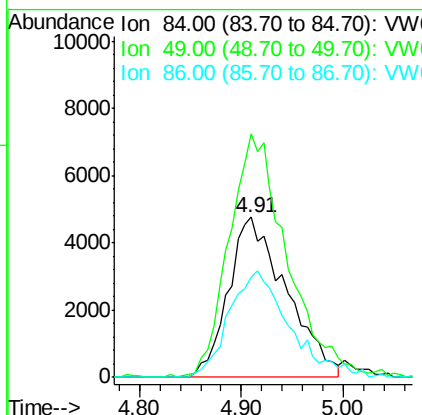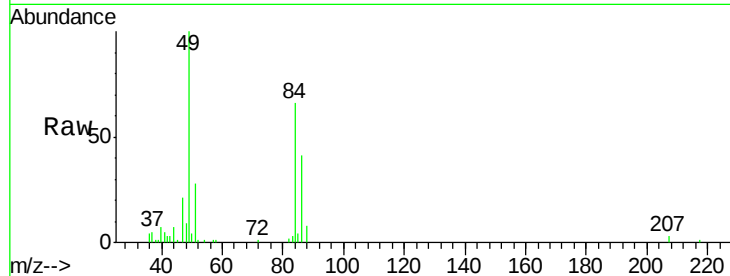

#21
2-Butanone
Concen: 5.039 ug/L
RT: 7.17 min Scan# 864
Delta R.T. 0.00 min
Lab File: VW009758.D
Acq: 06 Apr 2019 05:41

Tgt Ion	43	Resp	11163
Ion Ratio	Lower	Upper	
43	100		
72	12.9	12.0	36.1

