

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040619\
 Data File : VW009762.D
 Acq On : 06 Apr 2019 10:17
 Operator : SY/VA
 Sample : VW0406SBL02
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK25

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:42:58 AM

Quant Time: Apr 07 04:09:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 03:56:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	493518	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	468904	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	208133	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	128621	19.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.68%
7) Chloroethane-d5	2.89	69	122220	20.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.64%
10) 1,1-Dichloroethene-d2	4.01	63	234461	16.88	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.52%
20) 2-Butanone-d5	7.07	46	98088	46.78	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.56%
24) Chloroform-d	7.64	84	303807	22.56	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.24%
26) 1,2-Dichloroethane-d4	8.30	65	185551m	22.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.76%
29) Benzene-d6	8.27	84	566763	23.03	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.12%
33) 1,2-Dichloropropane-d6	9.27	67	174880	23.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.00%
37) Toluene-d8	10.32	98	512962	22.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.16%
38) trans-1,3-Dichloropropene-	10.57	79	77459	21.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.44%
39) 2-Hexanone-d5	10.93	63	67001	46.76	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.52%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	150539	21.30	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.20%
61) 1,2-Dichlorobenzene-d4	13.85	152	177144	24.25	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.00%

Target Compounds					Ovalue
16) Methylene chloride	4.91	84	9587m	1.101	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW040619\
Data File : VW009762.D
Acq On : 06 Apr 2019 10:17
Operator : SY/VA
Sample : VW0406SBL02
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VBLK25

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:58 AM

Quant Time: Apr 07 04:09:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

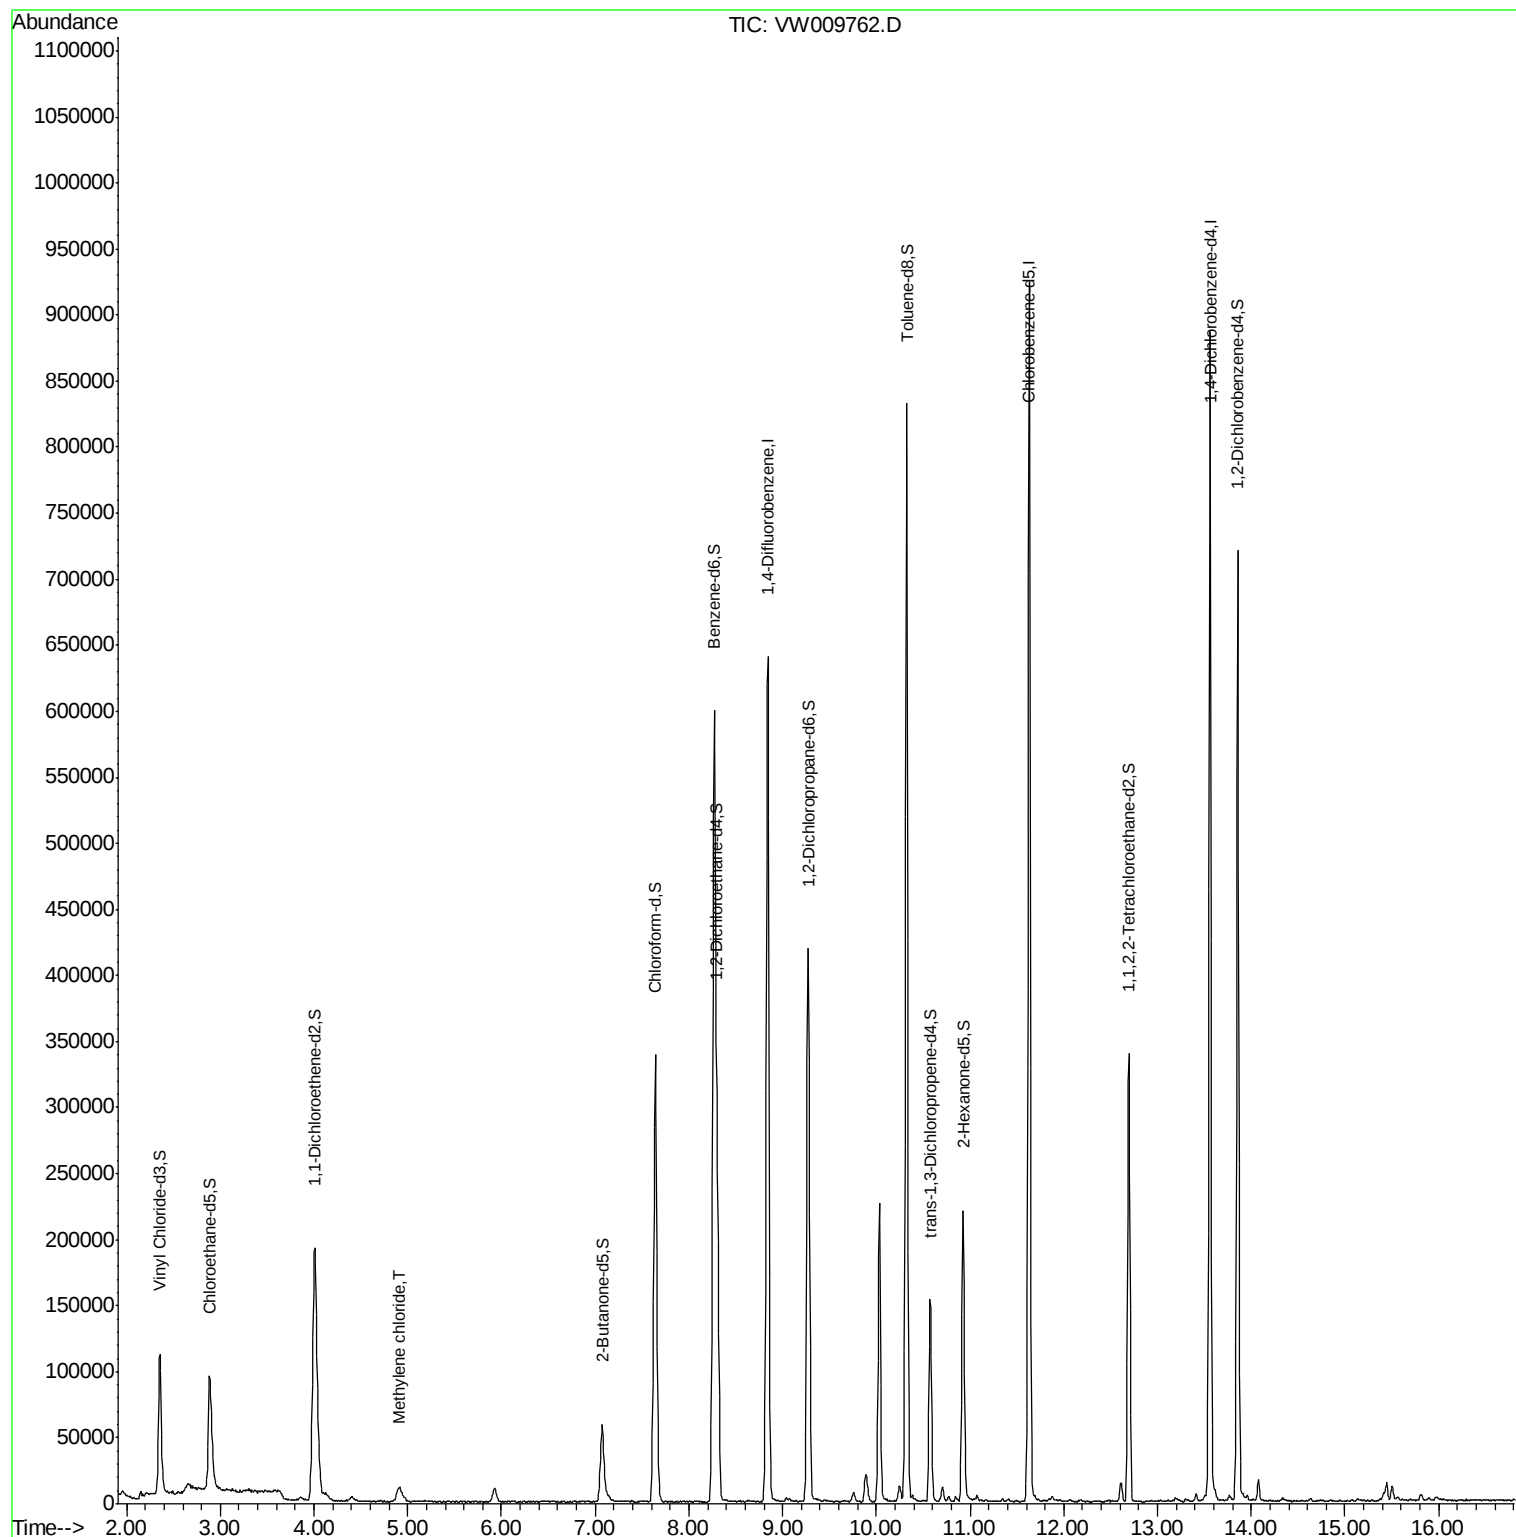

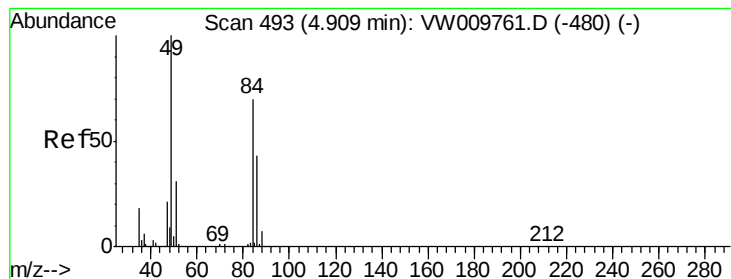

#16

Methylene chloride

Concen: 1.101 ug/L m

RT: 4.91 min Scan# 493

Delta R.T. -0.01 min

Lab File: VW009762.D

Acq: 06 Apr 2019 10:17

Tot Ion:	84	Resp:	9587
Ion Ratio	Lower	Upper	
84	100		
49	131.2	98.3	182.5
86	77.3	46.4	86.2

Instrument :
MSVOA_W
ClientSampleId :
VBLK25

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:58 AM

