

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040621\
 Data File : VW018562.D
 Acq On : 06 Apr 2021 13:30
 Operator : SY/VA
 Sample : M1896-15
 Misc : 5.68G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG587

Manual Integrations
 APPROVED

MMDadoda
 4/7/2021 5:17:25 PM

Quant Time: Apr 07 01:14:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 07 01:12:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	563511	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	513138	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	248075	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	168340	21.47	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.88%		
7) Chloroethane-d5	2.885	69	128096	18.66	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.64%		
10) 1,1-Dichloroethene-d2	4.019	63	184992m	13.66	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	54.64%		
20) 2-Butanone-d5	7.074	46	75438	43.21	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.42%		
24) Chloroform-d	7.647	84	277926	19.36	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	77.44%		
26) 1,2-Dichloroethane-d4	8.305	65	171299	20.45	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	81.80%		
29) Benzene-d6	8.275	84	544897	19.97	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	79.88%		
33) 1,2-Dichloropropane-d6	9.274	67	160465	20.39	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	81.56%		
37) Toluene-d8	10.323	98	527950	20.10	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.40%		
38) trans-1,3-Dichloroprop...	10.579	79	71439	17.60	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	70.40%		
39) 2-Hexanone-d5	10.921	63	58777	38.17	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	76.34%		
48) 1,1,2,2-Tetrachloroeth...	12.695	84	140598	19.97	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	79.88%		
61) 1,2-Dichlorobenzene-d4	13.853	152	173827	19.71	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	78.84%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	4380m	3.49	ug/L	
16) Methylene chloride	4.909	84	6898m	0.75	ug/L	
44) Toluene	10.390	91	8578	0.25	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040621\
Data File : VW018562.D
Acq On : 06 Apr 2021 13:30
Operator : SY/VA
Sample : M1896-15
Misc : 5.68G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BG587

Manual Integrations
APPROVED


MMDadoda
4/7/2021 5:17:25 PM

Quant Time: Apr 07 01:14:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 07 01:12:48 2021
Response via : Initial Calibration


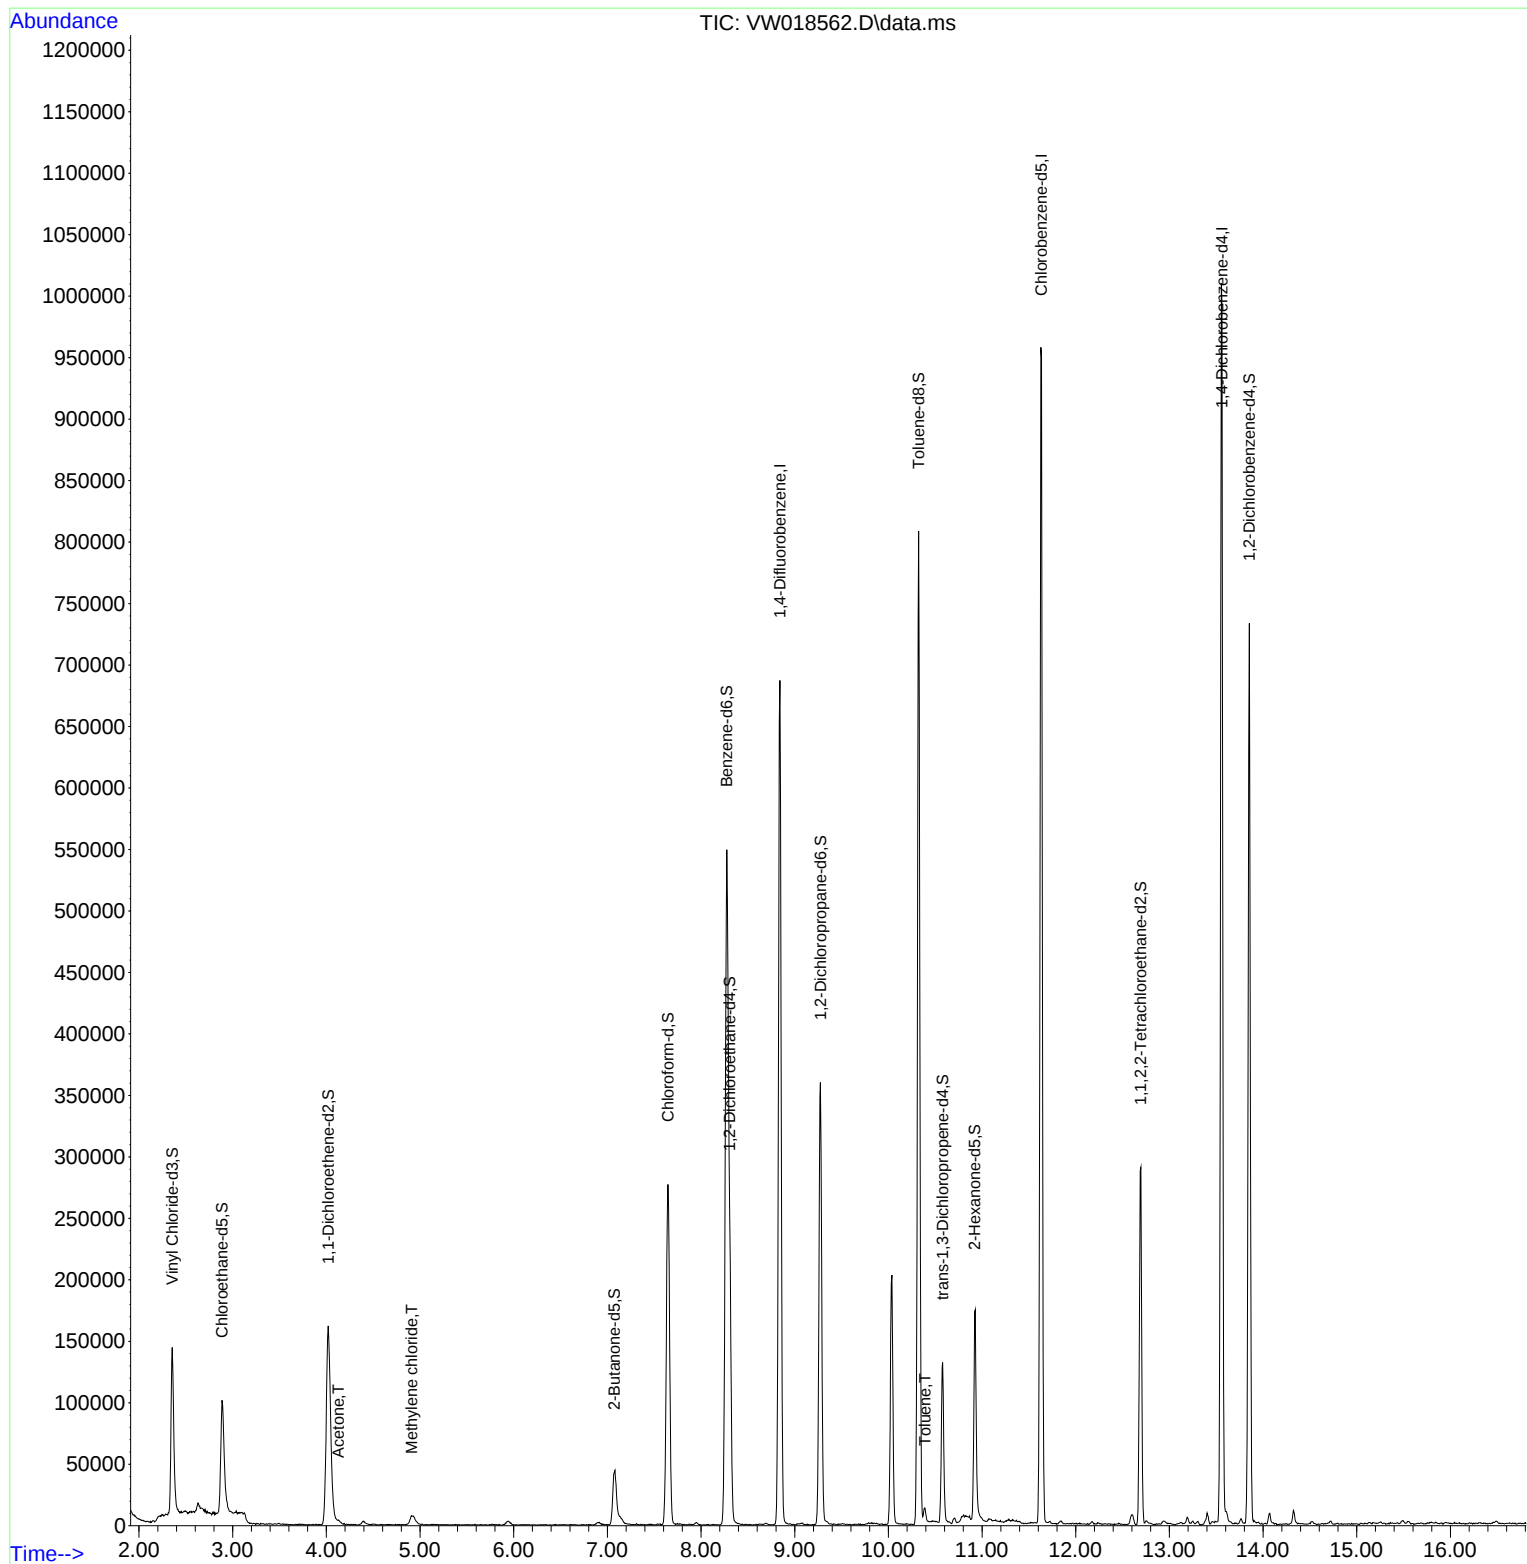


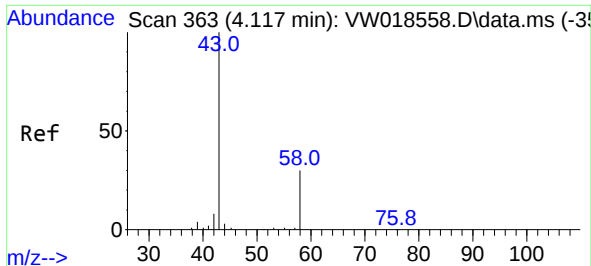

#13
Acetone
Concen: 3.49 ug/L m
RT: 4.129 min Scan# 365
Delta R.T. 0.012 min
Lab File: VW018562.D
Acq: 06 Apr 2021 13:30

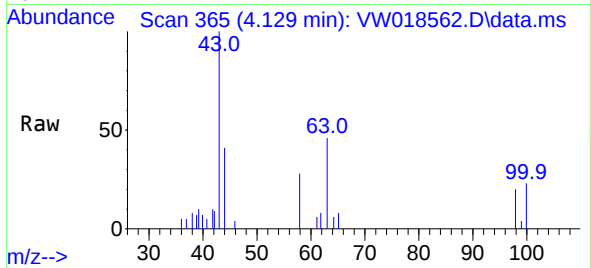


Tgt Ion: 43 Resp: 4380
Ion Ratio Lower Upper
43 100
58 12.5 0.0 62.2

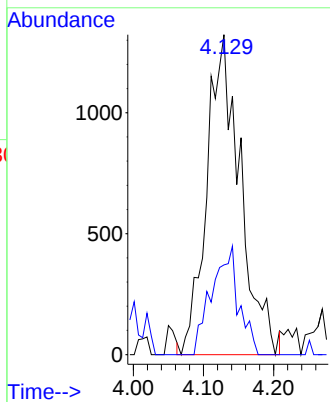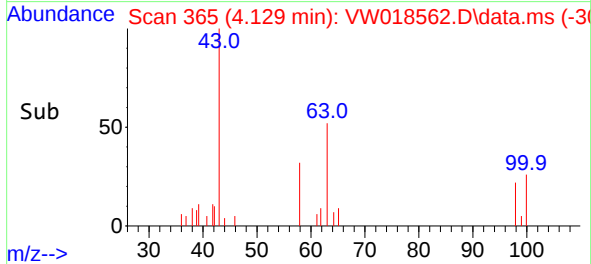


Instrument :
MSVOA_W
ClientSampled :
BG587

Manual Integrations
APPROVED



MMDadoda
4/7/2021 5:17:25 PM

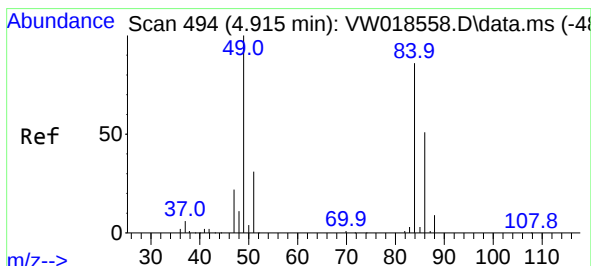


#16
Methylene chloride
Concen: 0.75 ug/L m
RT: 4.909 min Scan# 493
Delta R.T. -0.006 min
Lab File: VW018562.D
Acq: 06 Apr 2021 13:30

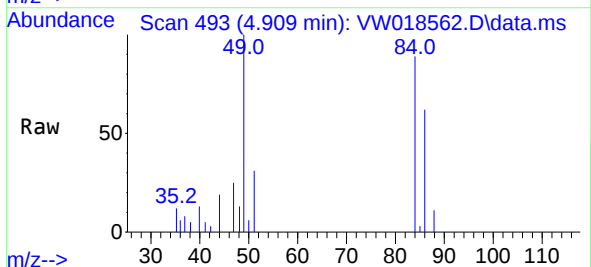


Tgt Ion: 84 Resp: 6898
Ion Ratio Lower Upper
84 100
49 112.4 74.4 138.2
86 69.3 46.1 85.7

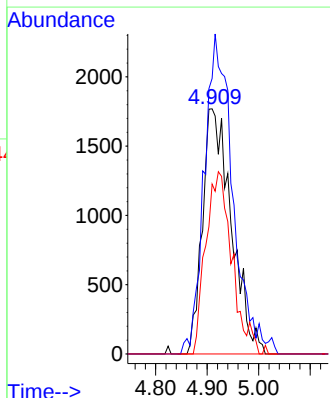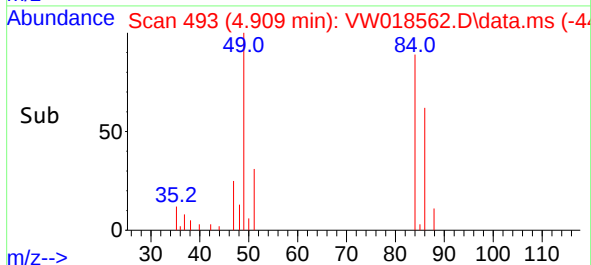

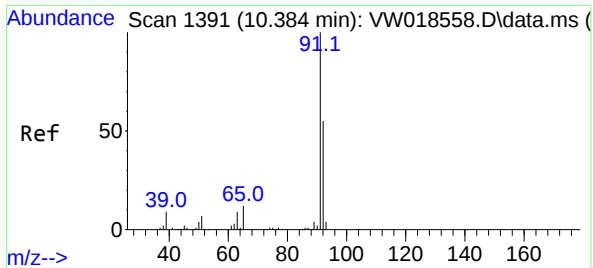

#44
Toluene
Concen: 0.25 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.006 min
Lab File: VW018562.D
Acq: 06 Apr 2021 13:30

Instrument :
MSVOA_W
ClientSampled :
BG587

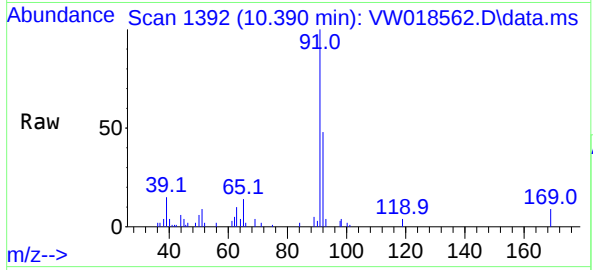

Tgt Ion: 91 Resp: 8578
Ion Ratio Lower Upper
91 100
92 48.1 42.3 78.5

Manual Integrations
APPROVED

MMDadoda
4/7/2021 5:17:25 PM

