

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040720\
Data File : VW015160.D
Acq On : 07 Apr 2020 13:54
Operator : SY/VA
Sample : L2176-02
Misc : 4.09G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG2H9

Manual Integrations
APPROVED

MMDadoda
4/8/2020 3:50:15 PM

Quant Time: Apr 08 06:12:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 08 06:10:31 2020
Response via : Initial Calibration

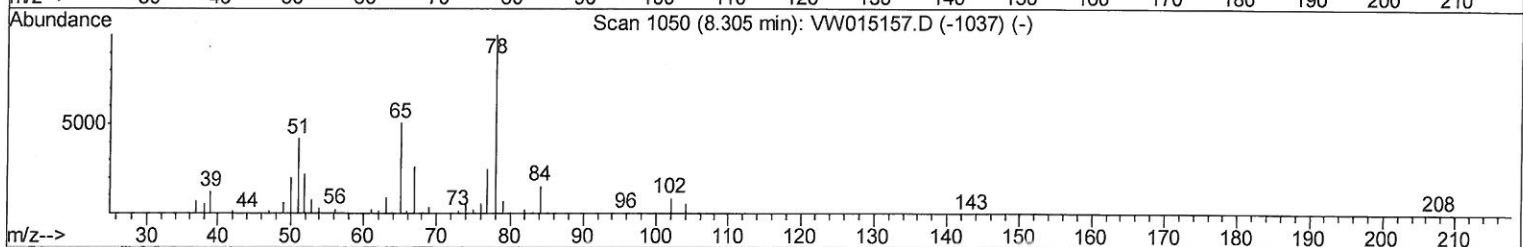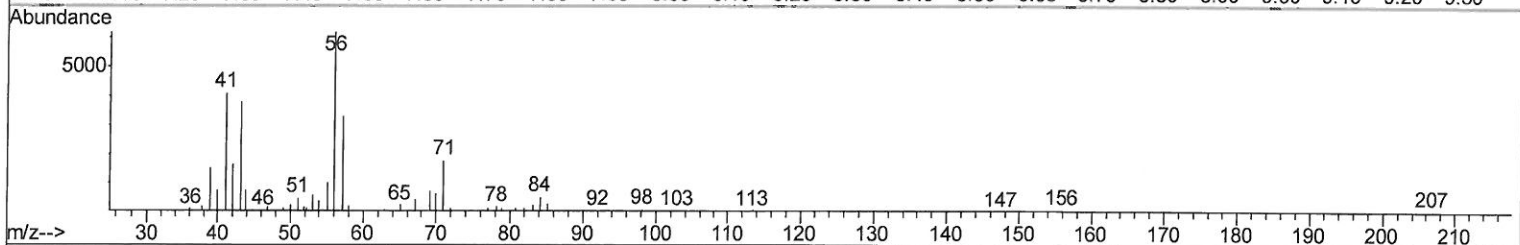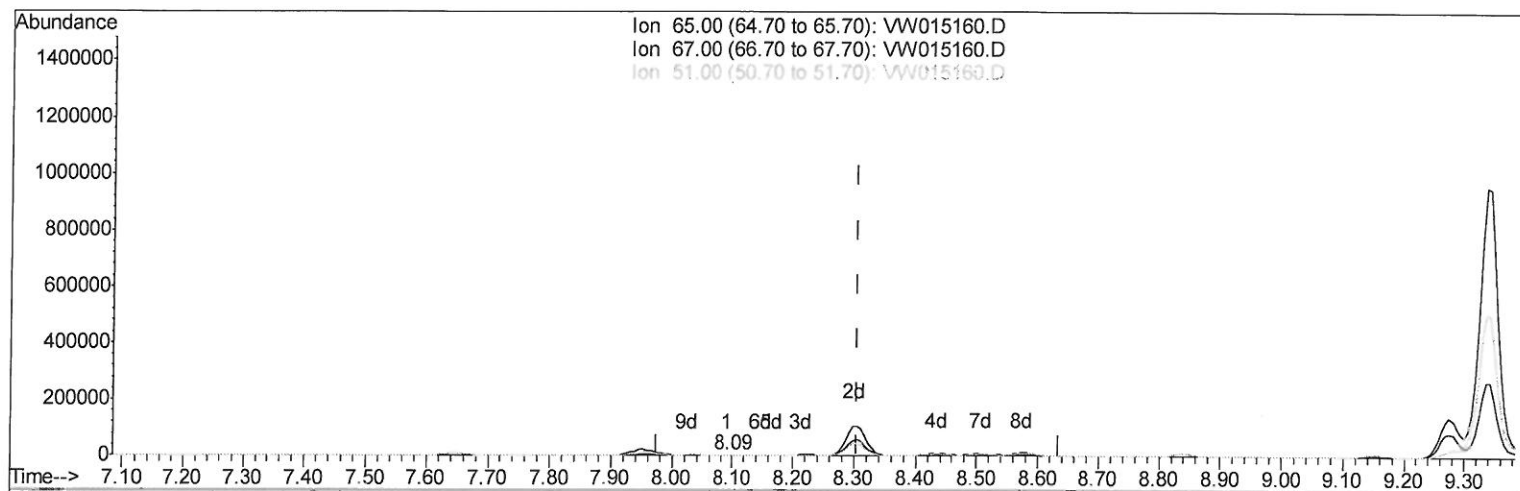

TIC: VW015160.D

(26) 1,2-Dichloroethane-d4 (S)

8.092min (-0.214) 0.01ug/L

response 144

Ion	Exp%	Act%
65.00	100	100
67.00	52.70	50.00
51.00	140.40	136.81
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040720\
 Data File : VW015160.D
 Acq On : 07 Apr 2020 13:54
 Operator : SY/VA
 Sample : L2176-02
 Misc : 4.09G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BG2H9

Manual Integrations
APPROVED

MMDadoda
 4/8/2020 3:50:15 PM

Quant Time: Apr 08 06:12:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 08 06:10:31 2020
 Response via : Initial Calibration

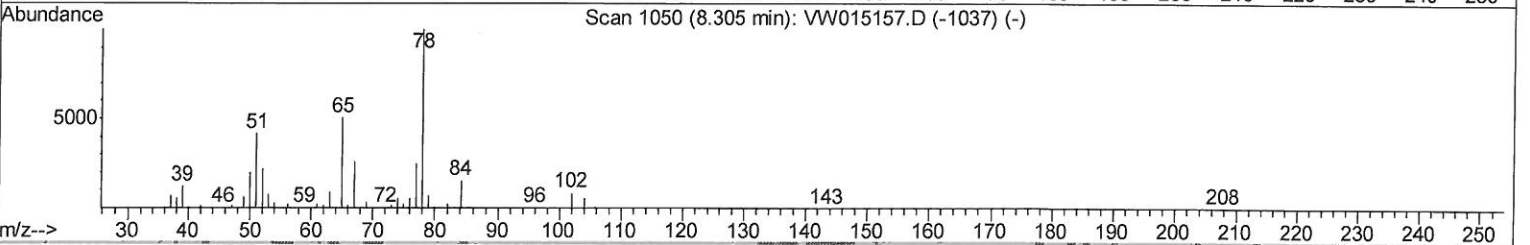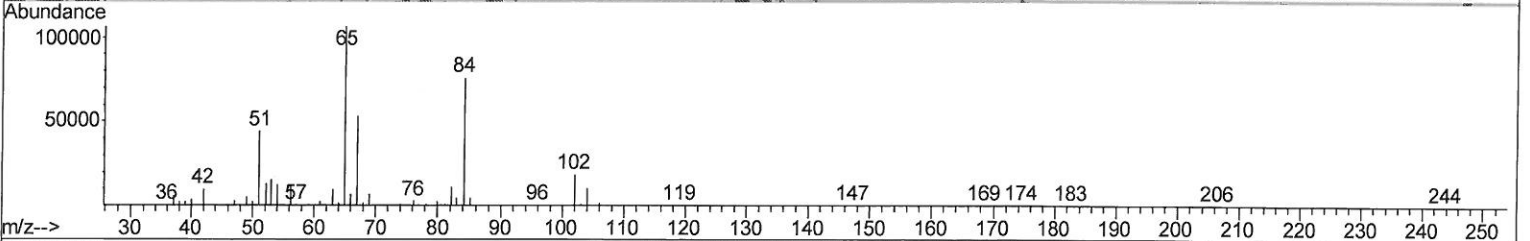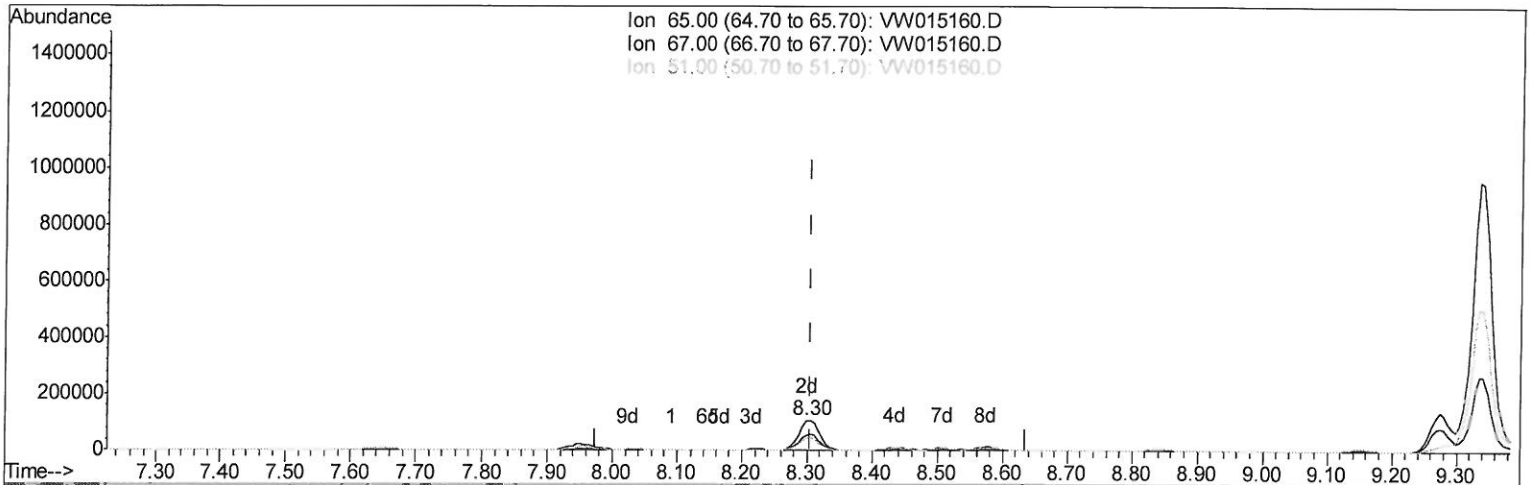

TIC: VW015160.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 22.03ug/L m

response 237187

Ion	Exp%	Act%
65.00	100	100
67.00	52.70	0.03#
51.00	140.40	0.08#
0.00	0.00	0.00

204/08/2020

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040720\
 Data File : VW015160.D
 Acq On : 07 Apr 2020 13:54
 Operator : SY/VA
 Sample : L2176-02
 Misc : 4.09G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 BG2H9

Manual Integrations
APPROVED

MMDadoda
 4/8/2020 3:50:15 PM

Quant Time: Apr 08 06:12:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 08 06:10:31 2020
 Response via : Initial Calibration

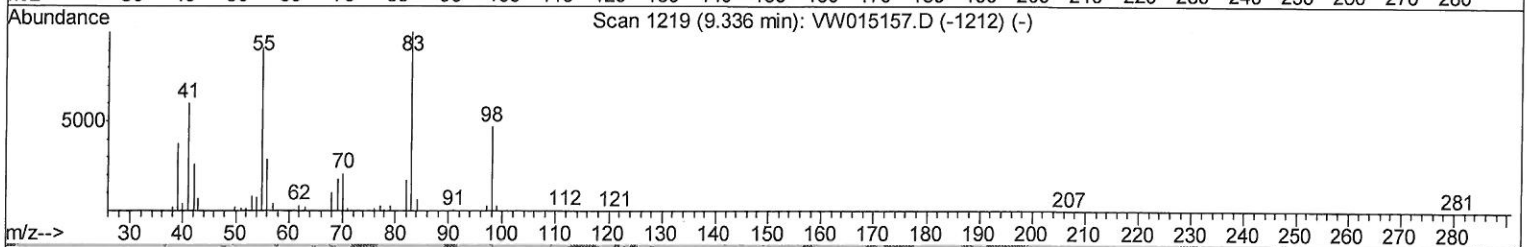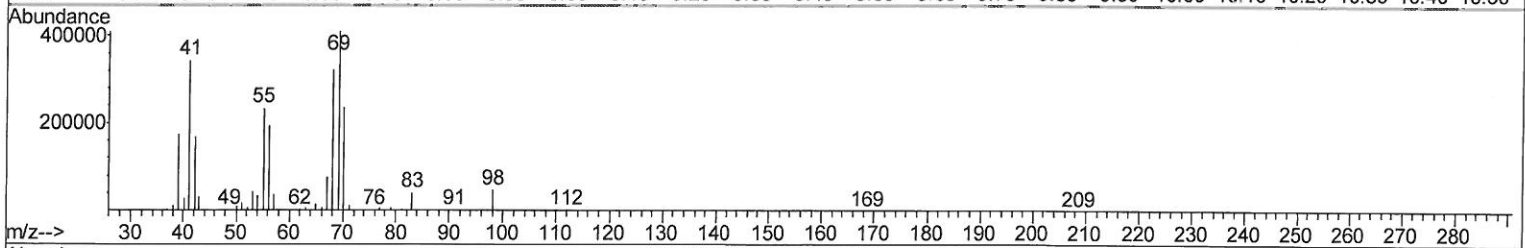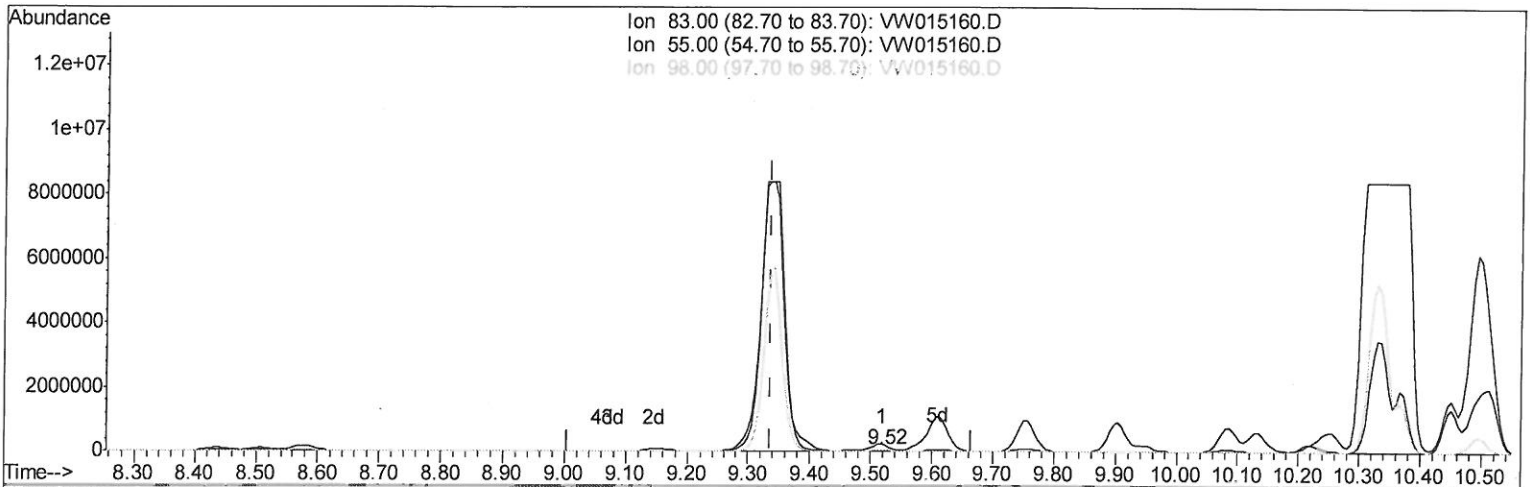

TIC: VW015160.D

(36) Methylcyclohexane (T)

9.518min (+0.183) 3.82ug/L

response 70721

Ion	Exp%	Act%
83.00	100	100
55.00	91.80	532.23#
98.00	45.80	123.05#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040720\
Data File : VW015160.D
Acq On : 07 Apr 2020 13:54
Operator : SY/VA
Sample : L2176-02
Misc : 4.09G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BG2H9

Manual Integrations
APPROVED

MMDadoda
4/8/2020 3:50:15 PM

Quant Time: Apr 08 06:12:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 08 06:10:31 2020
Response via : Initial Calibration

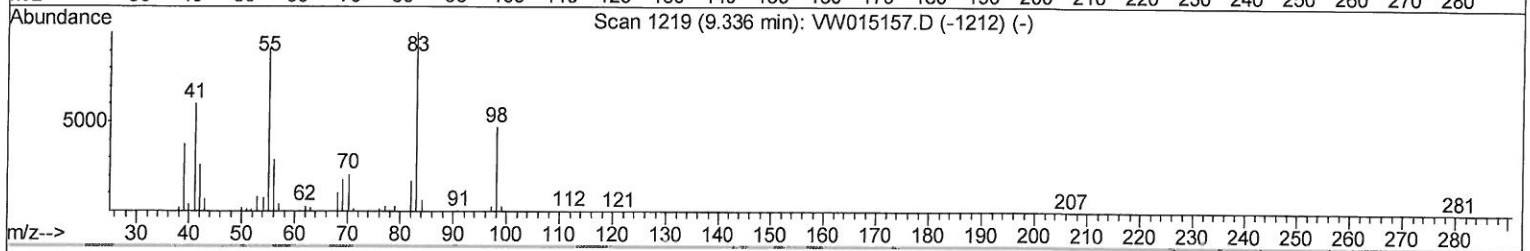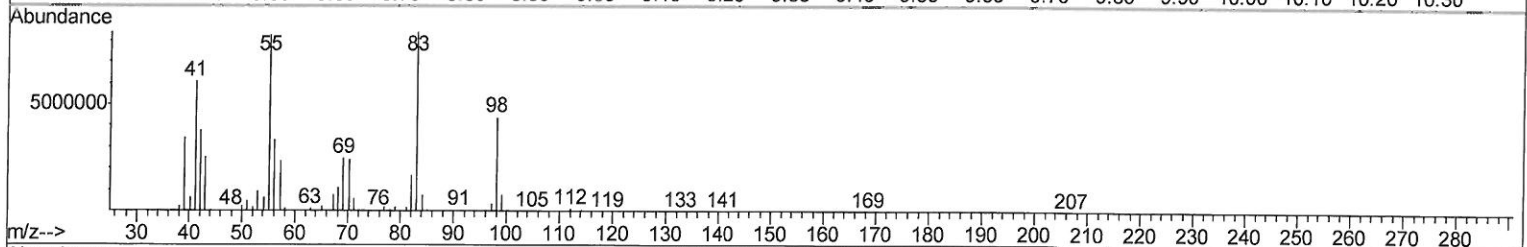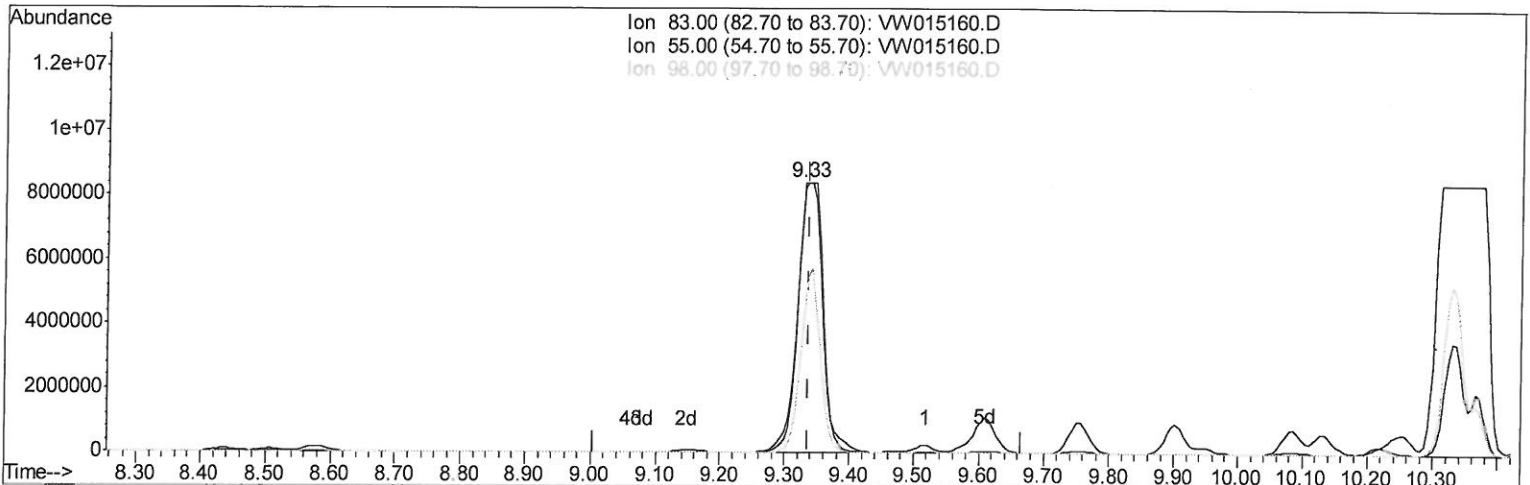

TIC: VW015160.D

(36) Methylcyclohexane (T)

9.329min (-0.006) 1197.09ug/L m

response 22168127

Ion	Exp%	Act%
83.00	100	100
55.00	91.80	1.70#
98.00	45.80	0.39#
0.00	0.00	0.00

504/08/2024

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040720\
 Data File : VW015160.D
 Acq On : 07 Apr 2020 13:54
 Operator : SY/VA
 Sample : L2176-02
 Misc : 4.09G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 BG2H9

Manual Integrations
APPROVED

MMDadoda
 4/8/2020 3:50:15 PM

Quant Time: Apr 08 06:12:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 08 06:10:31 2020
 Response via : Initial Calibration

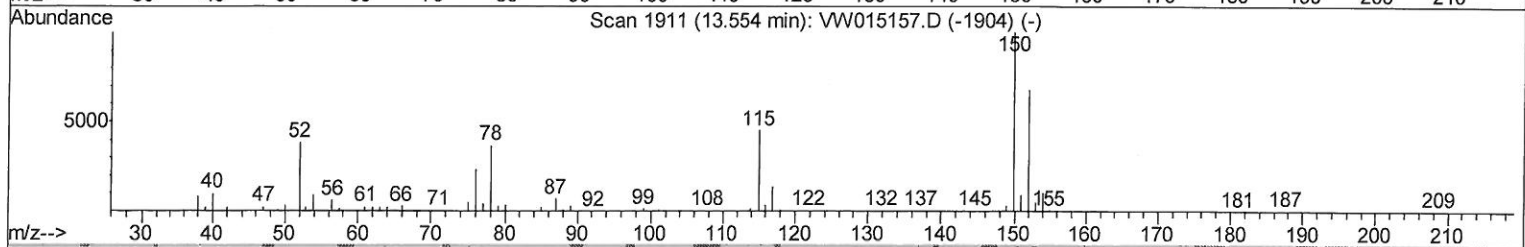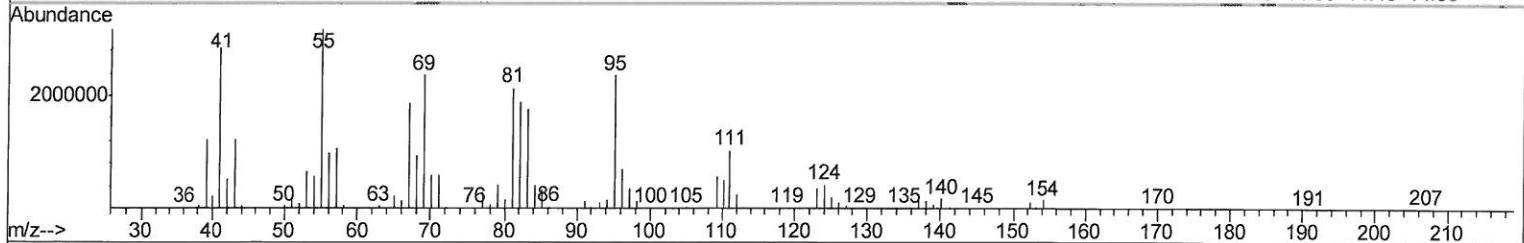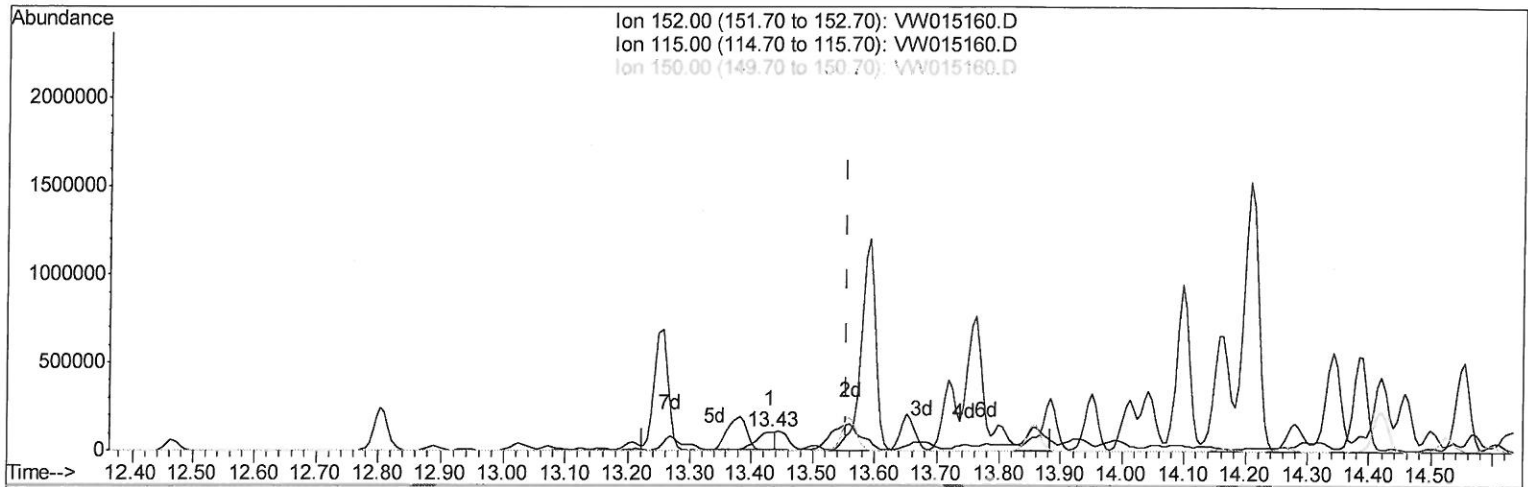

TIC: VW015160.D

(60) 1,4-Dichlorobenzene-d4 (I)

13.432min (-0.122) 25.00ug/L

response 204068

Ion	Exp%	Act%
152.00	100	100
115.00	66.50	3.92
150.00	174.80	3.26
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040720\
 Data File : VW015160.D
 Acq On : 07 Apr 2020 13:54
 Operator : SY/VA
 Sample : L2176-02
 Misc : 4.09G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG2H9

Manual Integrations
 APPROVED

MMDadoda
 4/8/2020 3:50:15 PM

Quant Time: Apr 08 06:12:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 08 06:10:31 2020
 Response via : Initial Calibration

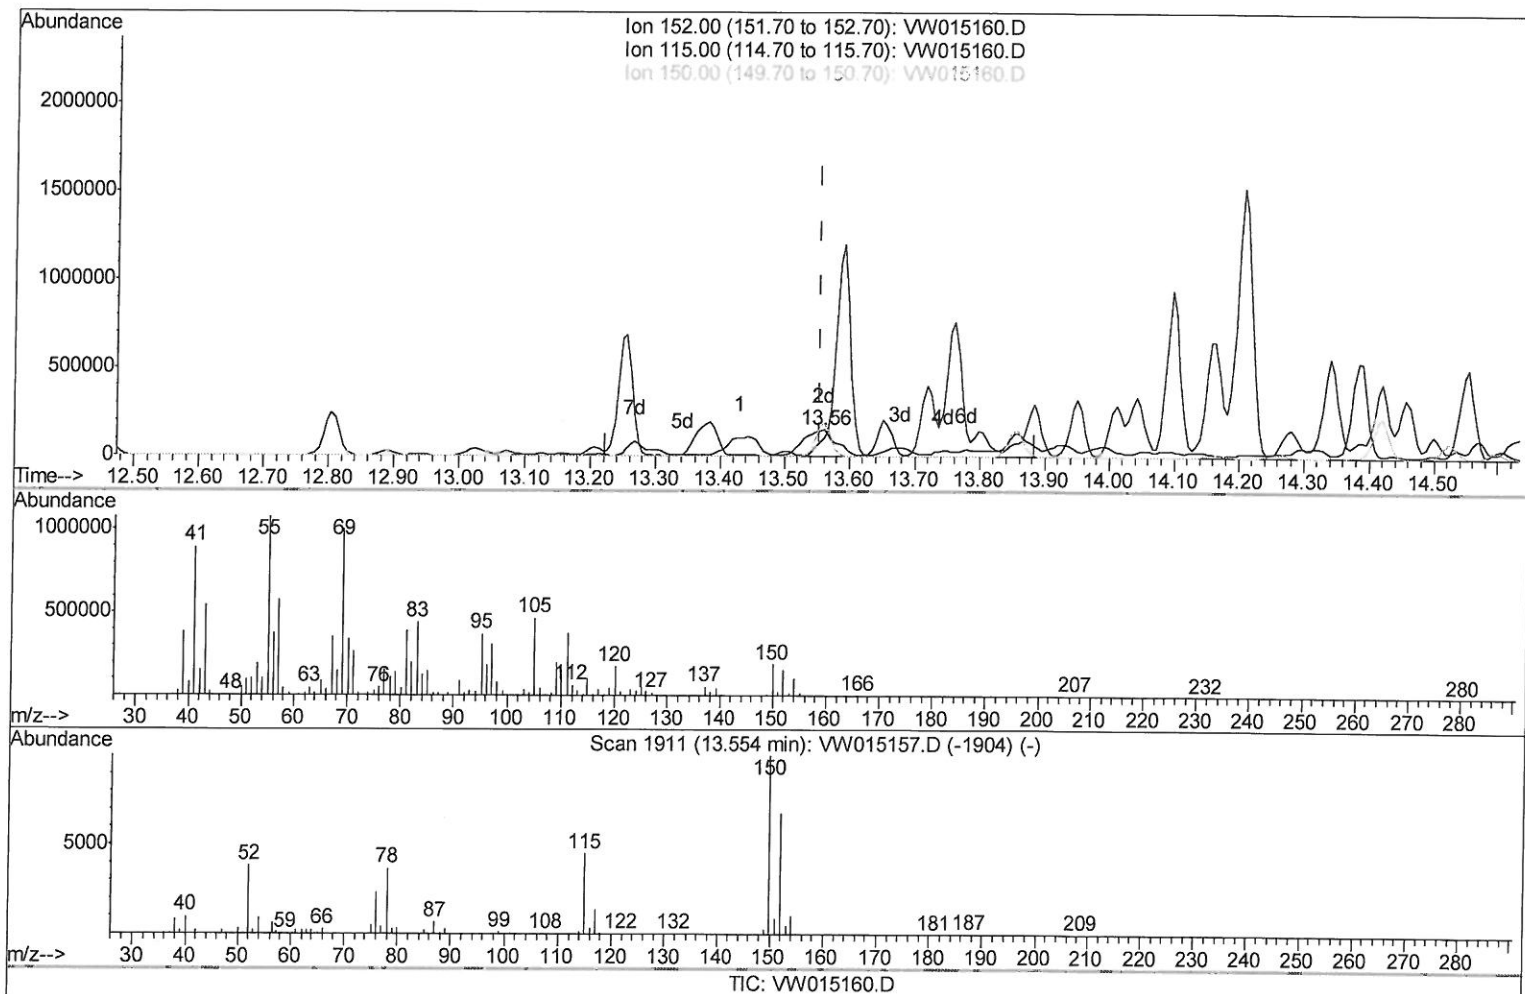

(60) 1,4-Dichlorobenzene-d4 (I)

13.560min (+0.006) 25.00ug/L m

response 526014

Ion	Exp%	Act%
152.00	100	100
115.00	66.50	1.52
150.00	174.80	1.26
0.00	0.00	0.00

04/08/2020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040720\
Quantitation Report (LSC Reviewed)

Data File : VW015160.D
Acq On : 07 Apr 2020 13:54
Operator : SY/VA
Sample : L2176-02
Misc : 4.09G/10ML/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG2H9

Manual Integrations
APPROVED

MMDadoda
4/8/2020 3:50:15 PM

Quant Time: Apr 08 13:53:44 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 08 06:10:31 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	622254	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	598537	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	526014m	25.00	ug/L	0.00

04/08/20 Sy

System Monitoring Compounds						
4) Vinyl Chloride-d3	2.35	65	207844	19.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.36%
7) Chloroethane-d5	2.89	69	195644	22.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.32%
10) 1,1-Dichloroethene-d2	4.02	63	316349	14.65	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.60%
20) 2-Butanone-d5	7.07	46	119789	48.97	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.94%
24) Chloroform-d	7.65	84	399875	21.51	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.04%
26) 1,2-Dichloroethane-d4	8.30	65	237187m	22.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.12%
29) Benzene-d6	8.27	84	810368	21.15	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.60%
33) 1,2-Dichloropropane-d6	9.27	67	301279	23.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.68%
37) Toluene-d8	10.33	98	11190572	342.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	1370.88%#
38) trans-1,3-Dichloropropene-	10.58	79	123308	25.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.28%
39) 2-Hexanone-d5	10.93	63	157082	83.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	167.14%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	503322	57.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	231.32%#
61) 1,2-Dichlorobenzene-d4	13.86	152	257284	14.06	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	56.24%#

04/08/20 Sy

Target Compounds					Qvalue
13) Acetone	4.13	43	28754	13.171	ug/L 97
16) Methylene chloride	4.91	84	23170	2.179	ug/L 93
30) Cyclohexane	7.96	56	583655	29.886	ug/L 96
36) Methylcyclohexane	9.33	83	22168127m	1197.090	ug/L 96
57) Isopropylbenzene	12.46	105	7887317	184.178	ug/L 96

04/08/20 Sy

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040720\
Quantitation Report (LSC Reviewed)

Data File : VW015160.D
Acq On : 07 Apr 2020 13:54
Operator : SY/VA
Sample : L2176-02
Misc : 4.09G/10ML/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG2H9

Manual Integrations
APPROVED

MMDadoda
4/8/2020 3:50:15 PM

Quant Time: Apr 08 13:53:44 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 08 06:10:31 2020
Response via : Initial Calibration

