


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040721\
 Data File : VW018569.D
 Acq On : 07 Apr 2021 09:38
 Operator : SY/VA
 Sample : BFB30
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB30

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Title : VOC Analysis
 Last Update : Fri Apr 09 03:11:49 2021

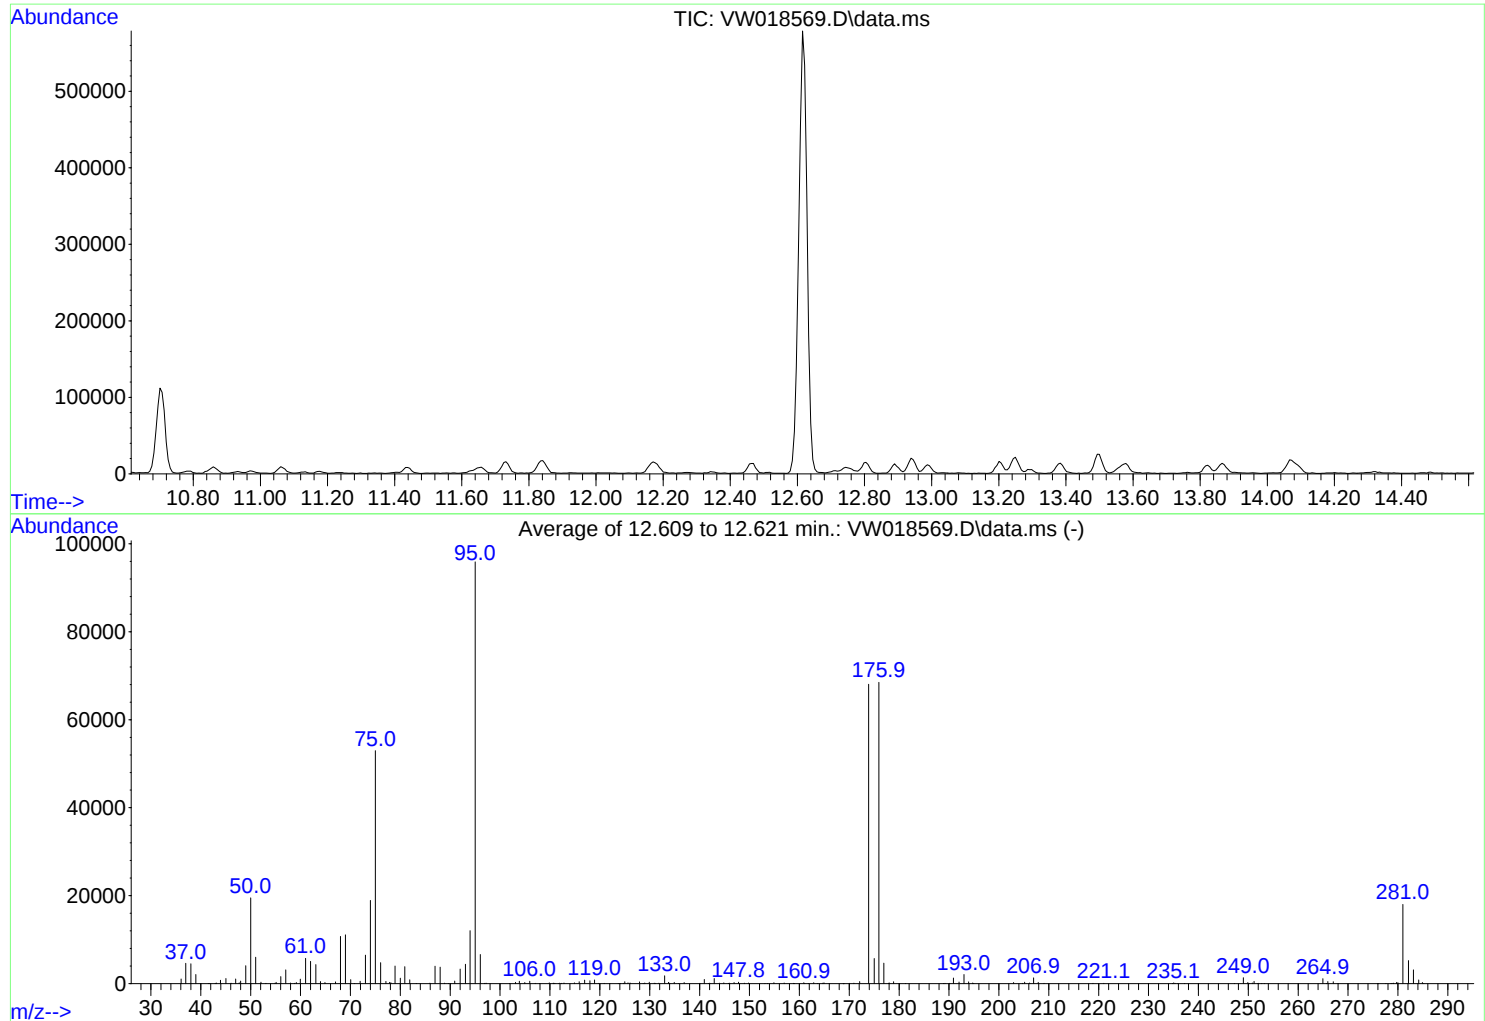

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	19493	PASS
75	95	30	80	55.2	52957	PASS
95	95	100	100	100.0	95899	PASS
96	95	5	9	6.9	6631	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.0	68072	PASS
175	174	5	9	8.4	5719	PASS
176	174	95	101	100.6	68512	PASS
177	176	5	9	6.8	4651	PASS

m/z	Abundance
36.00	739.0
37.00	3989.0
38.00	3792.0
39.10	1773.0
39.90	284.0
41.80	64.0
42.90	269.0
44.00	857.0
45.10	1210.0
46.10	92.0
47.00	1016.0
48.00	470.0
49.00	3545.0
50.00	18168.0
51.00	5015.0
52.00	302.0
53.00	111.0
54.90	307.0
56.10	1397.0
57.00	3316.0
58.00	129.0
59.20	551.0
60.00	968.0
61.00	4880.0
62.00	4521.0
63.10	3699.0
64.10	338.0
64.90	279.0
67.00	495.0
68.00	8977.0
69.00	10463.0
70.00	869.0
72.00	471.0
73.00	6931.0
74.00	16234.0
75.00	46168.0
76.10	4073.0
77.00	474.0
77.90	305.0
78.90	3468.0
80.00	987.0
80.90	3515.0
81.90	826.0
86.00	222.0
87.00	3463.0
88.00	3463.0
88.90	288.0
89.70	89.0
90.90	451.0
92.00	2907.0
93.10	3658.0
94.00	10642.0
95.00	82000.0
96.10	5610.0
97.20	299.0
103.10	412.0
103.80	527.0
104.90	178.0
105.90	534.0
109.80	182.0
110.70	165.0
111.80	124.0
112.30	175.0
112.80	95.0
115.00	210.0
115.90	507.0
116.90	815.0
118.00	662.0
119.00	703.0
119.80	107.0
120.80	129.0
123.70	92.0
125.00	744.0
125.70	305.0
126.00	315.0
127.90	243.0
129.00	141.0
130.00	298.0
130.90	163.0
131.90	189.0
133.00	2600.0
133.70	627.0
134.90	249.0
135.80	84.0
136.80	162.0
140.10	95.0
141.00	697.0
141.80	145.0
142.90	814.0
144.90	217.0
145.80	202.0
146.90	236.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

147.80	277.0
149.00	113.0
153.60	72.0
154.90	114.0
157.00	128.0
158.80	185.0
160.90	265.0
161.80	112.0
163.00	282.0
163.70	64.0
164.70	301.0
165.10	206.0
166.00	68.0
171.00	86.0
172.10	487.0
173.90	46728.0
175.00	4386.0
176.00	51232.0
176.90	4279.0
177.90	331.0
178.80	497.0
180.00	75.0
189.20	225.0
190.10	185.0
190.90	1907.0
192.00	533.0
192.90	2670.0
194.00	597.0
194.80	350.0
202.90	360.0
205.10	633.0
206.10	227.0
207.00	2205.0
207.90	337.0
209.10	164.0
219.00	51.0
221.10	169.0
235.00	237.0
235.90	94.0
237.30	95.0
247.20	80.0
249.00	1708.0
249.90	504.0
251.10	716.0
251.90	149.0
253.20	89.0
265.00	1266.0
265.90	564.0
267.10	640.0
268.00	67.0
275.90	52.0
277.60	59.0
279.10	348.0
279.80	707.0
281.00	22360.0
282.10	7334.0
283.10	3678.0
284.10	1018.0
284.90	310.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

m/z	Abundance
37.00	60.0
39.00	55.0
40.00	256.0
42.10	78.0
43.90	288.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

m/z	Abundance
36.00	1176.0
37.00	5136.0
38.00	5238.0
39.10	2552.0
40.00	246.0
41.80	53.0
43.10	367.0
44.00	1289.0
45.00	1184.0
46.10	192.0
47.00	1389.0
47.70	559.0
48.00	508.0
49.00	4748.0
50.00	21360.0
51.00	6983.0
52.10	456.0
53.10	52.0
55.10	473.0
56.00	1837.0
57.10	2900.0
58.00	205.0
58.80	197.0
60.00	1287.0
61.00	6009.0
62.00	5917.0
63.00	4484.0
64.00	423.0
64.90	352.0
67.10	369.0
68.00	12256.0
69.00	11588.0
70.10	980.0
71.90	538.0
73.00	6712.0
74.00	20808.0
75.00	58568.0
76.00	5359.0
77.10	564.0
78.10	661.0
79.00	3926.0
80.00	1446.0
80.90	4090.0
81.90	961.0
83.20	92.0
85.90	89.0
87.00	4510.0
88.00	3844.0
90.80	500.0
92.00	3465.0
93.00	5547.0
94.00	13349.0
95.00	103856.0
96.00	7453.0
96.90	188.0
101.90	98.0
103.10	324.0
103.80	623.0
105.00	331.0
105.90	557.0
107.10	121.0
107.90	82.0
109.90	170.0
110.60	168.0
111.00	200.0
112.00	170.0
112.80	166.0
114.80	216.0
115.80	335.0
117.00	841.0
118.00	756.0
119.00	1036.0
119.80	60.0
120.90	70.0
122.00	58.0
123.90	103.0
125.00	614.0
125.60	195.0
126.10	115.0
128.00	468.0
129.00	299.0
129.80	393.0
130.90	216.0
131.80	91.0
133.00	1900.0
134.00	289.0
134.90	318.0
136.90	185.0
140.00	142.0
140.90	1089.0
142.10	182.0
142.90	1324.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

144.00	116.0
144.80	102.0
146.00	130.0
146.80	345.0
147.80	406.0
148.80	147.0
149.80	206.0
153.70	92.0
154.80	145.0
156.90	116.0
159.00	164.0
160.90	334.0
162.80	220.0
163.70	56.0
164.90	188.0
170.00	74.0
171.00	151.0
172.20	423.0
173.90	79952.0
175.00	6155.0
175.90	76944.0
177.00	5043.0
178.10	323.0
178.90	486.0
181.30	114.0
188.90	130.0
190.90	1270.0
192.00	278.0
193.00	2316.0
193.90	413.0
194.70	118.0
195.00	115.0
203.00	258.0
204.70	160.0
205.20	386.0
206.00	70.0
206.90	1144.0
207.90	333.0
209.00	67.0
218.80	133.0
221.00	63.0
235.10	271.0
237.20	71.0
249.00	1338.0
249.90	308.0
250.80	413.0
251.20	420.0
252.10	172.0
252.70	77.0
264.90	1101.0
266.00	707.0
267.10	379.0
278.60	128.0
280.00	683.0
281.00	19080.0
282.10	5193.0
283.10	3850.0
284.20	994.0
284.90	340.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

m/z	Abundance
36.10	1236.0
37.00	4880.0
38.00	4505.0
39.00	2075.0
40.10	340.0
41.50	77.0
43.10	132.0
44.00	1059.0
45.00	1114.0
45.90	62.0
46.90	760.0
48.00	768.0
49.00	3972.0
50.00	18952.0
51.00	5971.0
52.10	258.0
53.10	118.0
55.10	416.0
56.00	1547.0
57.00	3181.0
58.00	166.0
59.00	220.0
59.90	833.0
61.00	6396.0
62.00	4696.0
63.00	4763.0
63.90	639.0
64.90	154.0
66.90	306.0
68.00	10926.0
69.00	11238.0
70.00	841.0
70.80	65.0
71.90	596.0
73.00	5781.0
74.00	19712.0
75.00	54136.0
76.10	4883.0
77.20	538.0
77.80	522.0
78.90	4605.0
80.00	1321.0
80.90	3920.0
81.90	823.0
86.90	3895.0
88.00	3976.0
91.00	791.0
92.00	3562.0
93.00	3984.0
94.00	12179.0
95.00	101840.0
96.00	6831.0
97.30	57.0
103.00	189.0
103.90	551.0
104.90	234.0
106.00	609.0
107.00	126.0
109.90	196.0
110.80	207.0
111.90	141.0
112.80	149.0
115.00	88.0
115.90	495.0
116.90	740.0
118.00	559.0
118.90	773.0
119.70	55.0
122.00	65.0
124.10	59.0
124.70	213.0
125.70	59.0
126.00	58.0
127.90	493.0
128.70	115.0
129.90	323.0
131.10	187.0
131.90	90.0
132.90	842.0
133.80	289.0
134.90	351.0
136.90	445.0
140.90	1110.0
142.00	137.0
143.00	1367.0
143.90	181.0
144.80	231.0
146.00	215.0
147.00	224.0
147.80	352.0
149.00	98.0
149.80	255.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

153.10	84.0
154.90	403.0
156.90	236.0
158.80	58.0
160.70	77.0
161.10	70.0
162.90	152.0
164.90	150.0
168.80	50.0
170.10	99.0
170.80	71.0
172.00	495.0
173.90	77536.0
175.00	6615.0
175.90	77360.0
177.00	4630.0
178.00	136.0
179.00	302.0
191.00	625.0
192.00	282.0
193.10	1241.0
194.10	157.0
194.90	137.0
203.00	183.0
204.80	90.0
206.20	103.0
207.00	637.0
208.00	173.0
234.80	153.0
235.30	189.0
249.00	1045.0
250.20	82.0
251.10	447.0
265.00	1069.0
265.70	95.0
266.10	157.0
266.90	260.0
278.80	237.0
279.60	194.0
281.00	12591.0
282.10	3247.0
283.10	1865.0
284.10	516.0
284.90	148.0
285.20	163.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30