

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022427.D
 Acq On : 07 Apr 2022 13:19
 Operator : SY/VA
 Sample : N2262-09RE
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 08 06:31:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	347591	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	324945	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	143531	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	156063	20.310	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.240%
7) Chloroethane-d5	2.891	69	91137	18.924	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.680%
11) 1,1-Dichloroethene-d2	4.019	63	143347	14.383	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.520%
21) 2-Butanone-d5	7.074	46	71465	53.270	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.540%
24) Chloroform-d	7.647	84	250878	23.092	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.360%
26) 1,2-Dichloroethane-d4	8.451	65	49	0.008	ug/L	0.15
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.274	84	464679	23.406	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.640%
36) 1,2-Dichloropropane-d6	9.274	67	145258	25.283	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.120%
41) Toluene-d8	10.323	98	435815	22.414	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.640%
43) trans-1,3-Dichloroprop...	10.579	79	63468	23.408	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.640%
47) 2-Hexanone-d5	10.920	63	56810	53.148	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.300%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	118982	24.356	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	128749	25.325	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.280%
Target Compounds					Qvalue	
13) Acetone	4.123	43	5136	5.623	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022427.D
Acq On : 07 Apr 2022 13:19
Operator : SY/VA
Sample : N2262-09RE
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 08 06:31:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

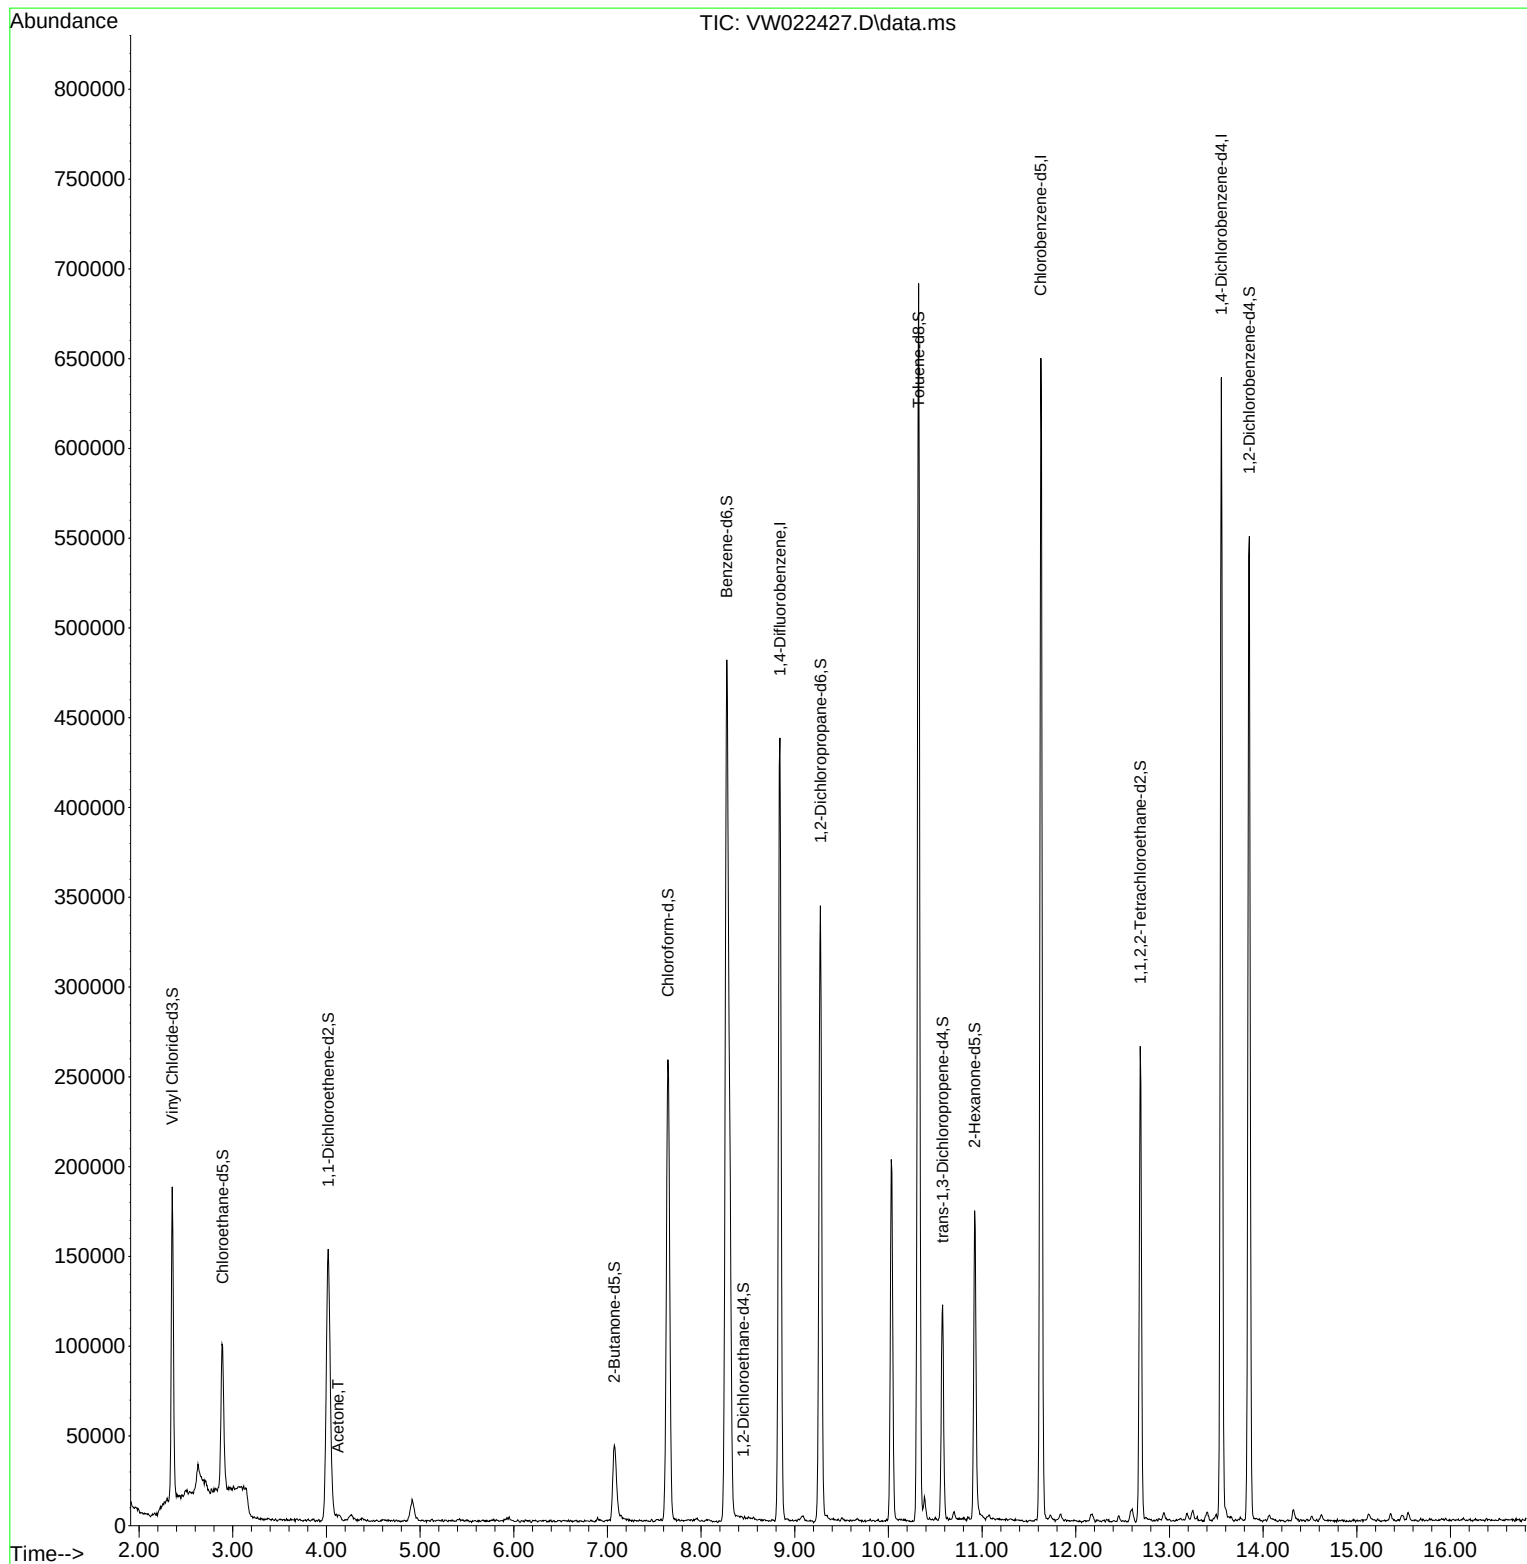

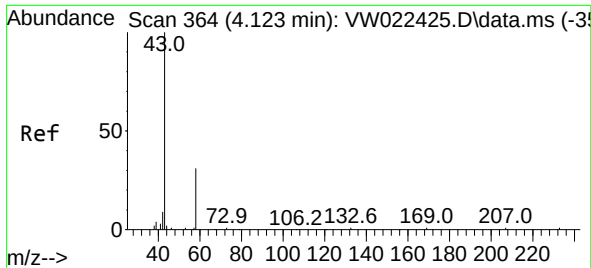

#13

Acetone

Concen: 5.623 ug/L

RT: 4.123 min Scan# 3

Delta R.T. -0.000 min


Lab File: VW022427.D

Acq: 07 Apr 2022 13:19

Instrument :

MSVOA_W

ClientSampleId :

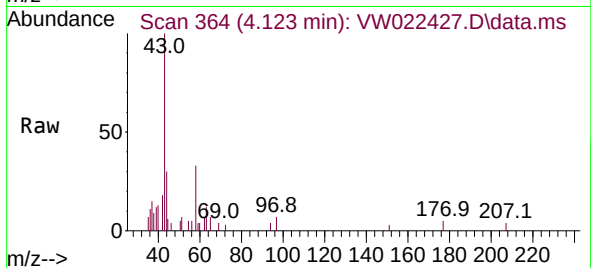

Tgt Ion: 43 Resp: 5136

Ion Ratio Lower Upper

43 100

58 34.7 0.0 57.0

