


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022427.D
Acq On : 07 Apr 2022 13:19
Operator : SY/VA
Sample : N2262-09
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

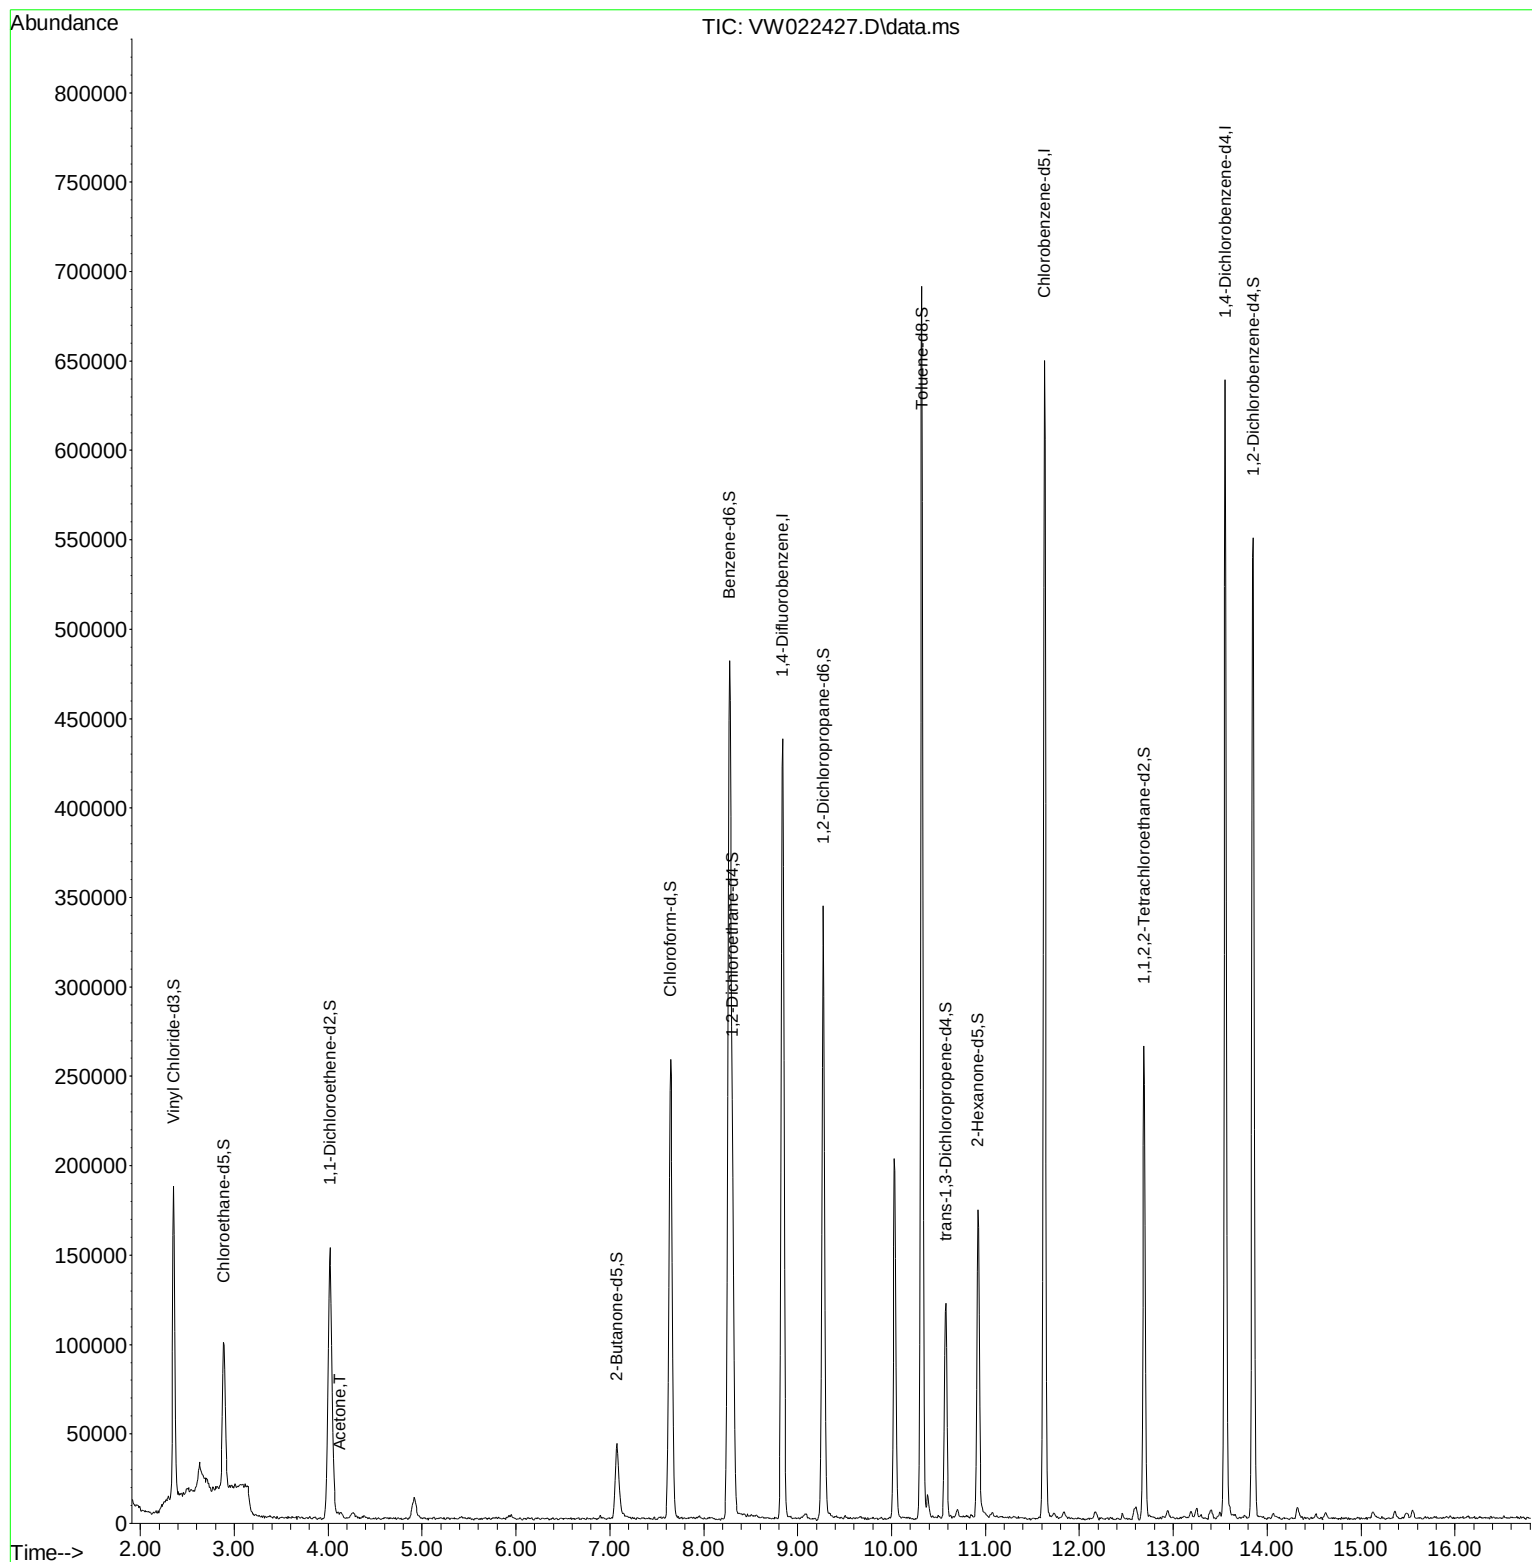




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022427.D
 Acq On : 07 Apr 2022 13:19
 Operator : SY/VA
 Sample : N2262-09
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual IntegrationsAPPROVED

Quant Time: Apr 17 03:52:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

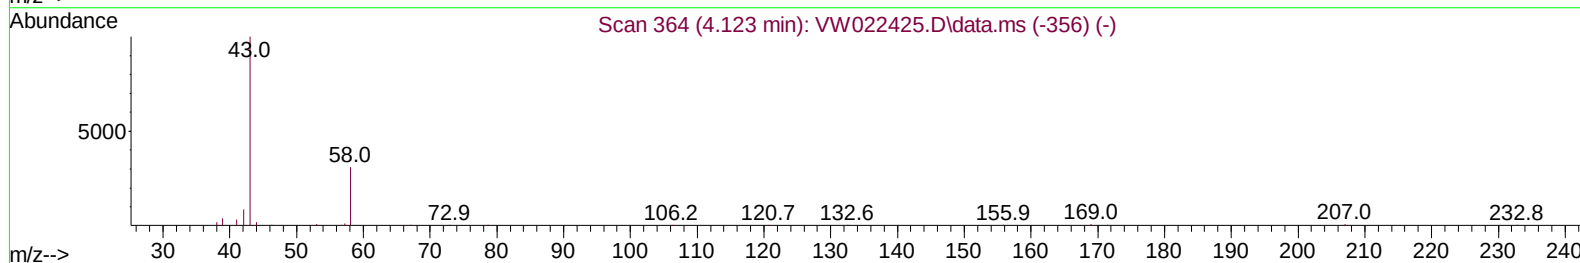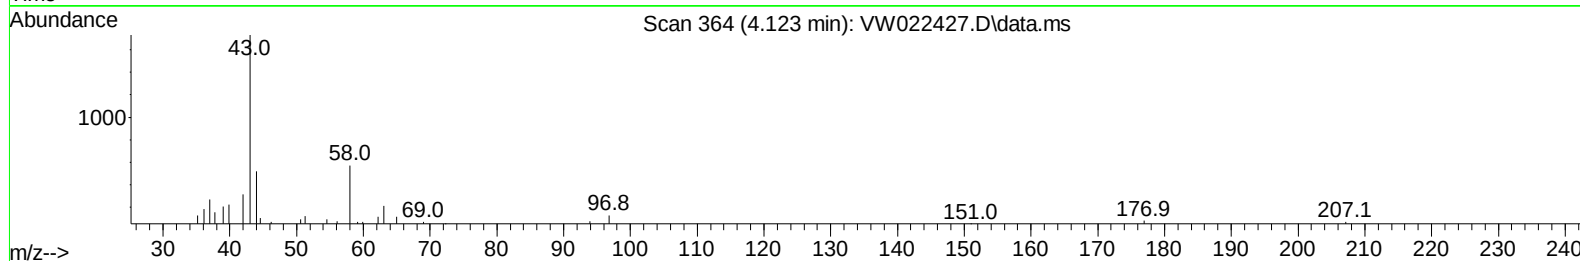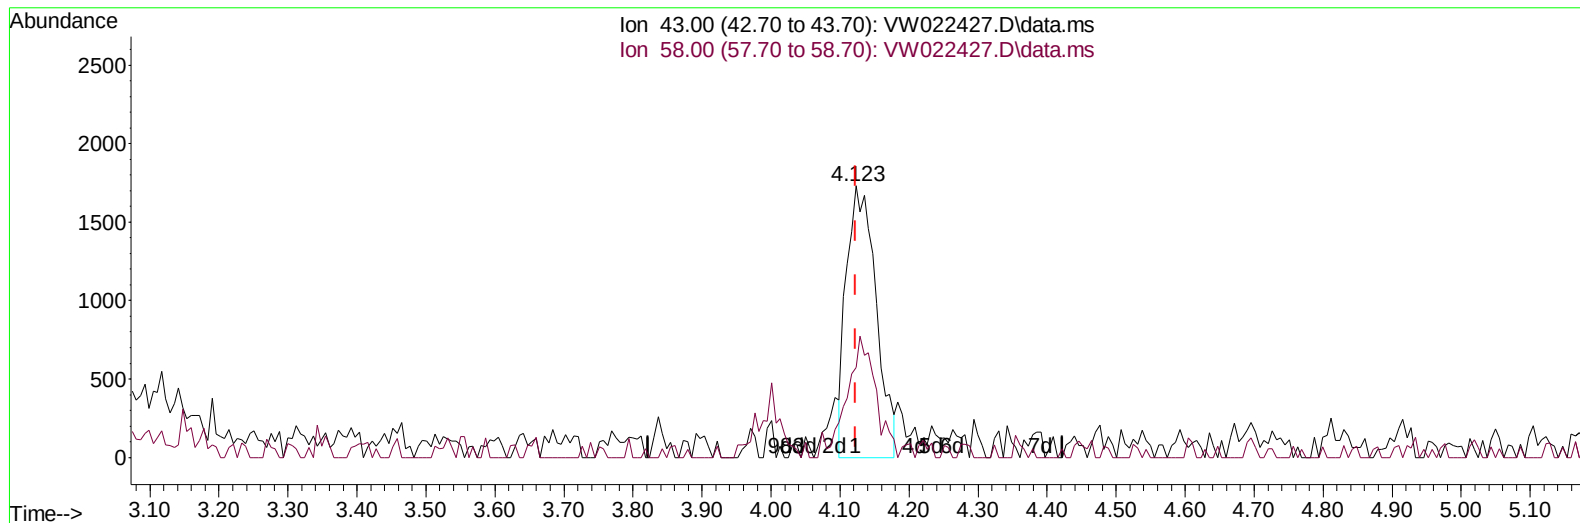

TIC: VW022427.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 5.62 ug/L

response 5136

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	34.70
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022427.D
 Acq On : 07 Apr 2022 13:19
 Operator : SY/VA
 Sample : N2262-09
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:31:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

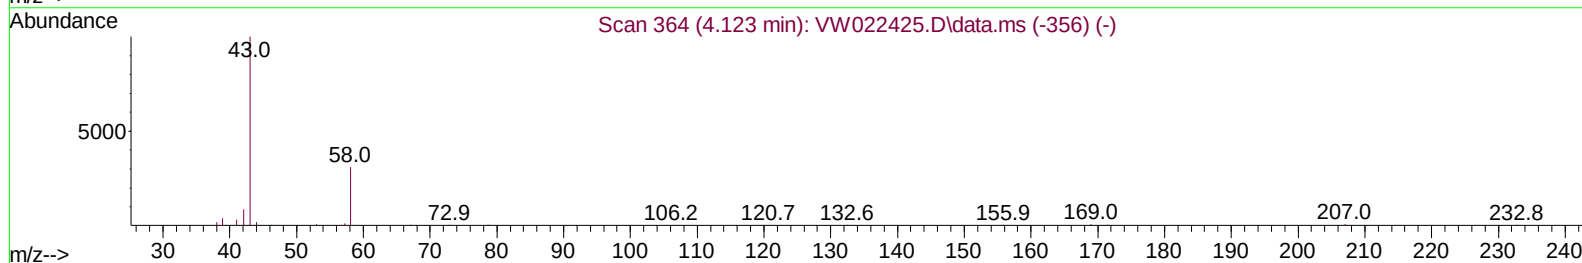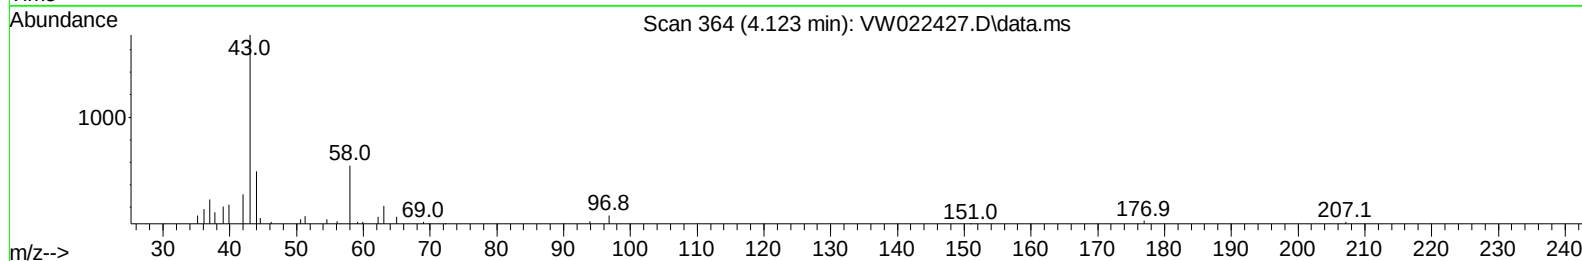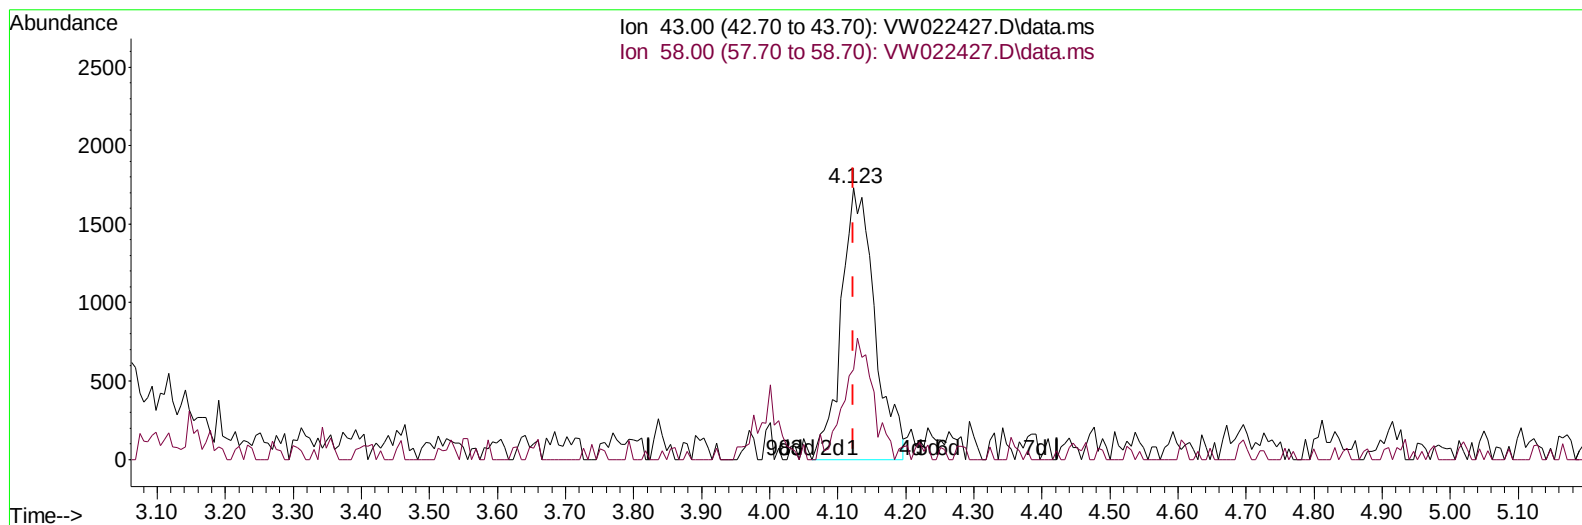

TIC: VW022427.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 6.49 ug/L m

response 5932

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	30.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022427.D
 Acq On : 07 Apr 2022 13:19
 Operator : SY/VA
 Sample : N2262-09
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual IntegrationsAPPROVED

Quant Time: Apr 17 03:52:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

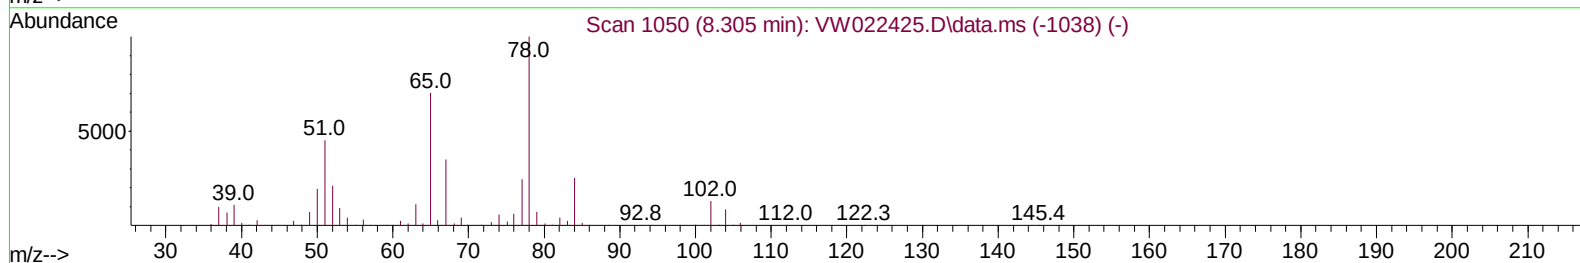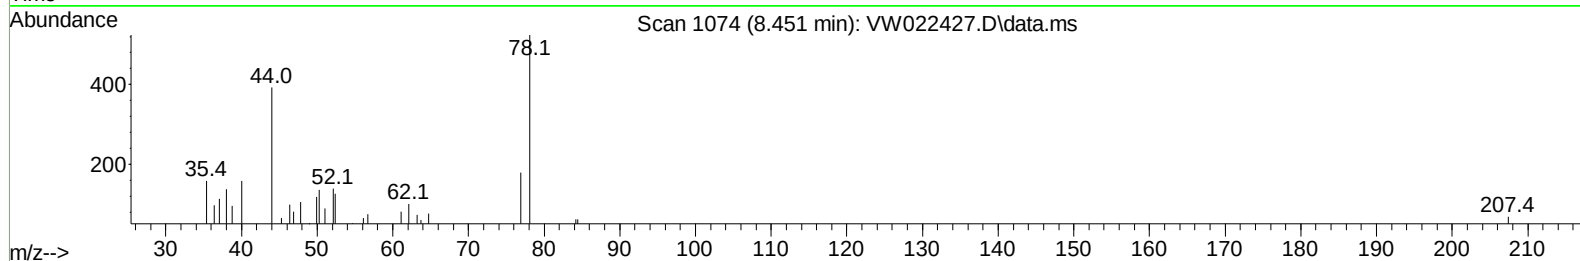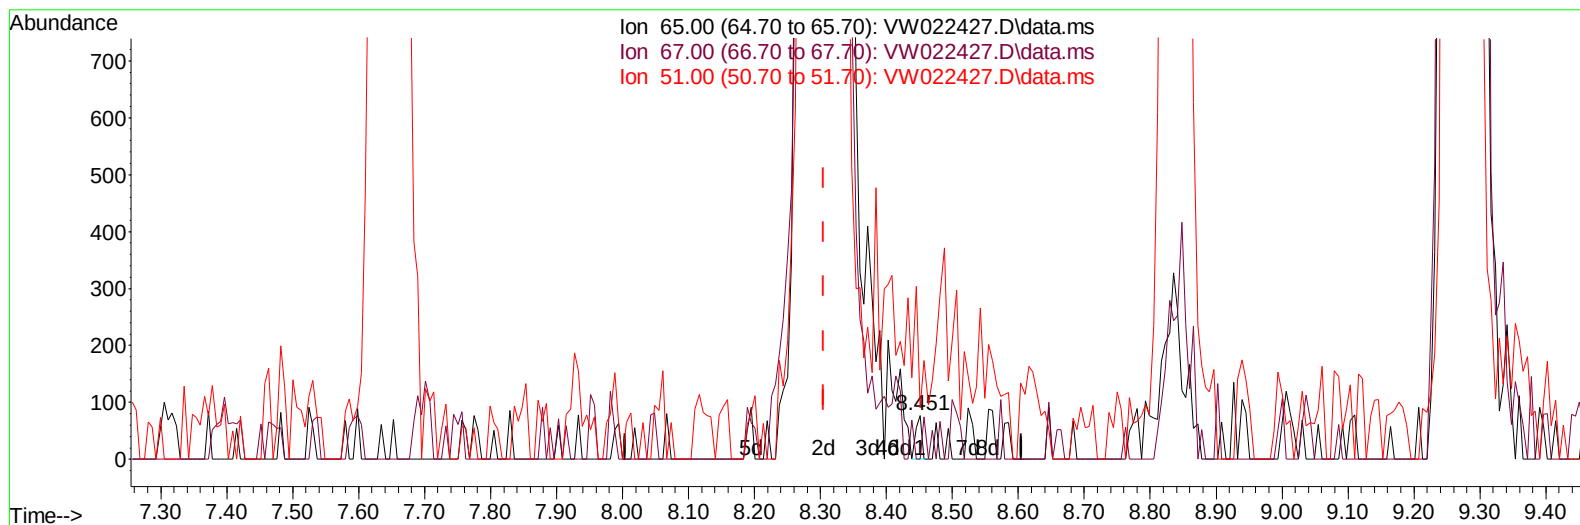

TIC: VW022427.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.451min (+ 0.147) 0.01 ug/L

response 49

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	55.10
51.00	99.30	73.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022427.D
 Acq On : 07 Apr 2022 13:19
 Operator : SY/VA
 Sample : N2262-09
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

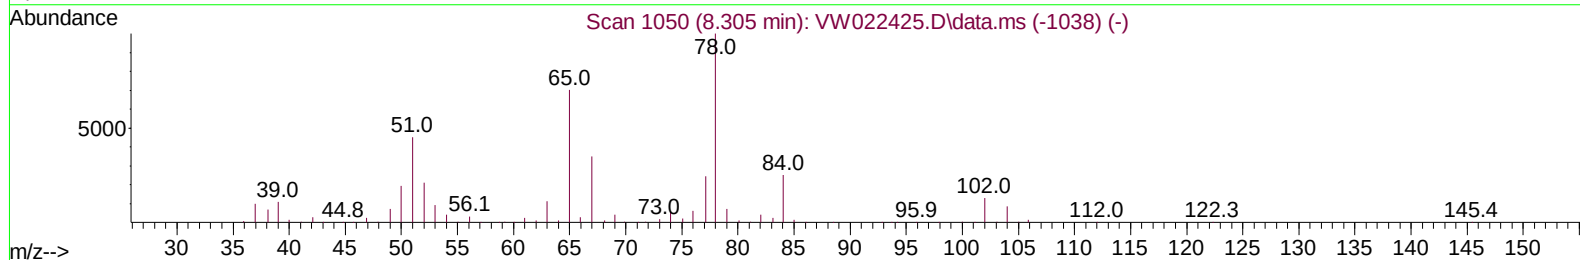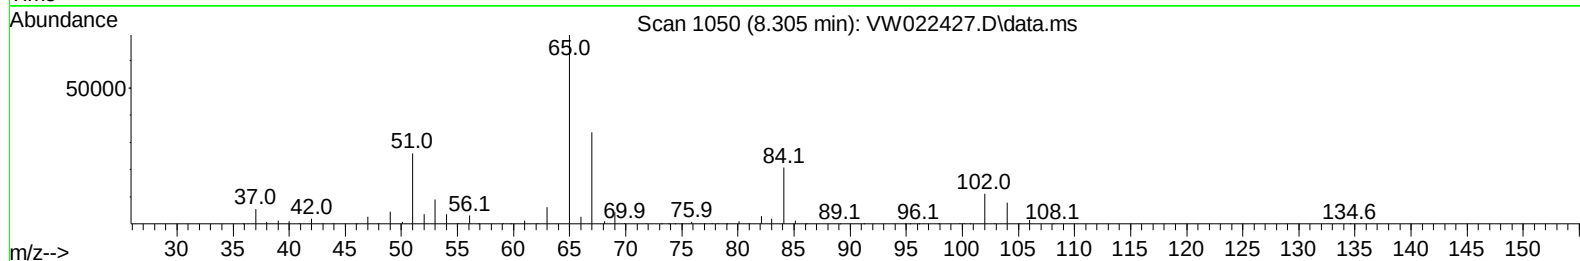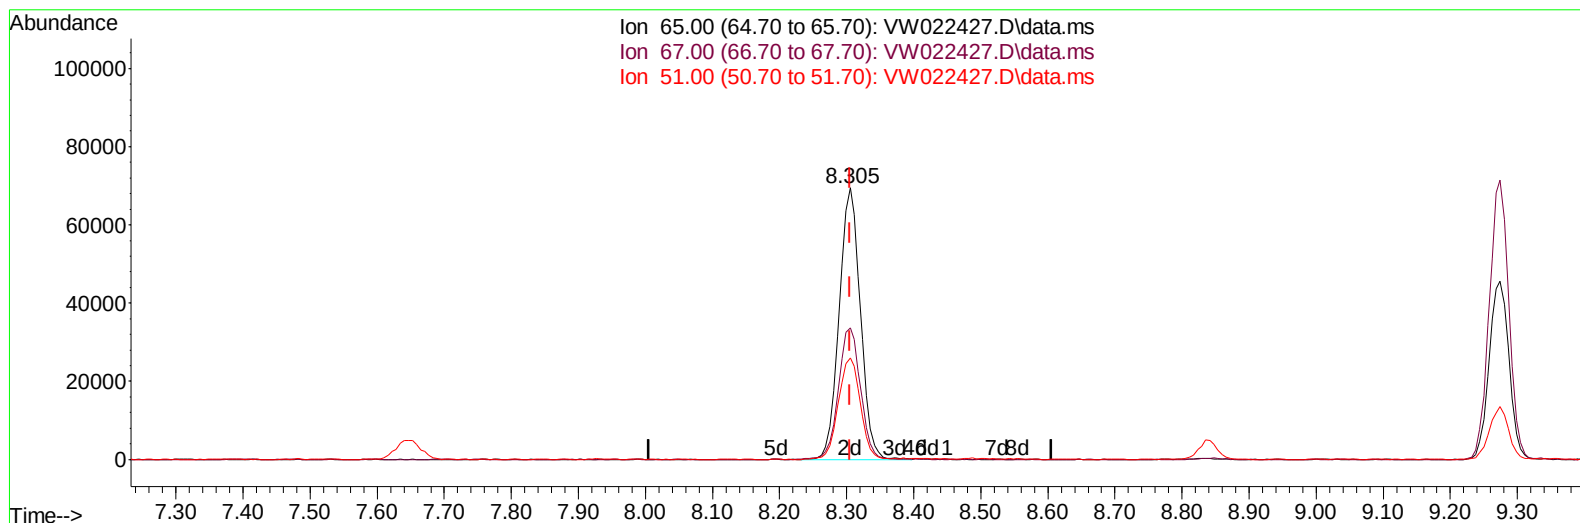

TIC: VW022427.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 24.62 ug/L m

response 152814

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.02#
51.00	99.30	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022427.D
 Acq On : 07 Apr 2022 13:19
 Operator : SY/VA
 Sample : N2262-09
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:31:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		347591	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		324945	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		143531	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		156063	20.310	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	81.240%	
7) Chloroethane-d5	2.891	69		91137	18.924	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	75.680%	
11) 1,1-Dichloroethene-d2	4.019	63		143347	14.383	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	57.520%	
21) 2-Butanone-d5	7.074	46		71465	53.270	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	106.540%	
24) Chloroform-d	7.647	84		250878	23.092	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	92.360%	
26) 1,2-Dichloroethane-d4	8.305	65		152814m	24.617	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	98.480%	
32) Benzene-d6	8.274	84		464679	23.406	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	93.640%	
36) 1,2-Dichloropropane-d6	9.274	67		145258	25.283	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	101.120%	
41) Toluene-d8	10.323	98		435815	22.414	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	89.640%	
43) trans-1,3-Dichloroprop...	10.579	79		63468	23.408	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	93.640%	
47) 2-Hexanone-d5	10.920	63		56810	53.148	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	106.300%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		118982	24.356	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	97.440%	
66) 1,2-Dichlorobenzene-d4	13.853	152		128749	25.325	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	101.280%	
Target Compounds							
13) Acetone	4.123	43		5932m	6.494	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed