




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022428.D
Acq On : 07 Apr 2022 13:43
Operator : SY/VA
Sample : N2262-14
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L4

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:31:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

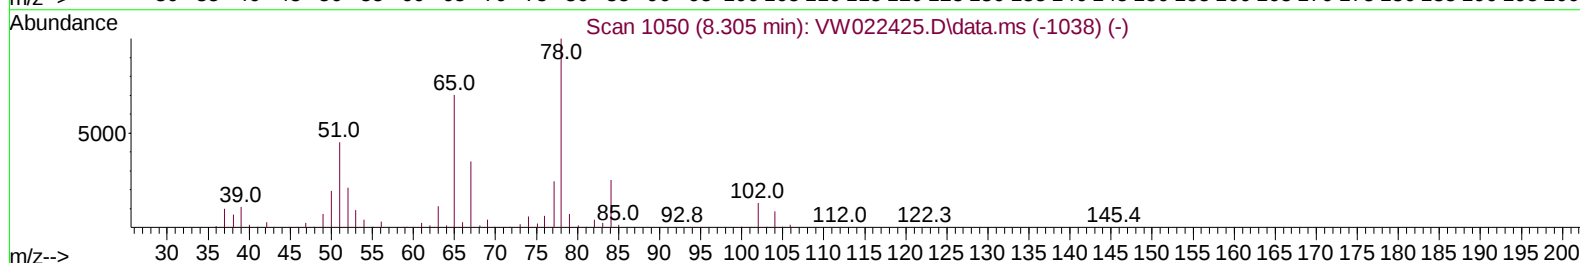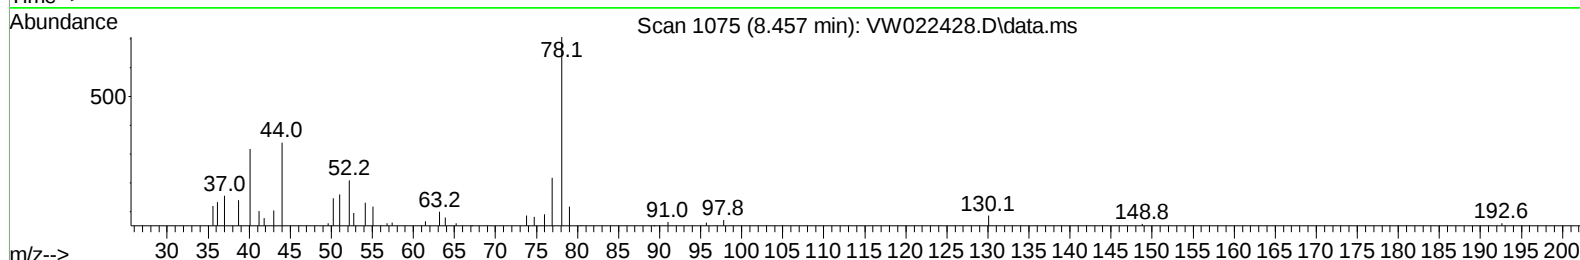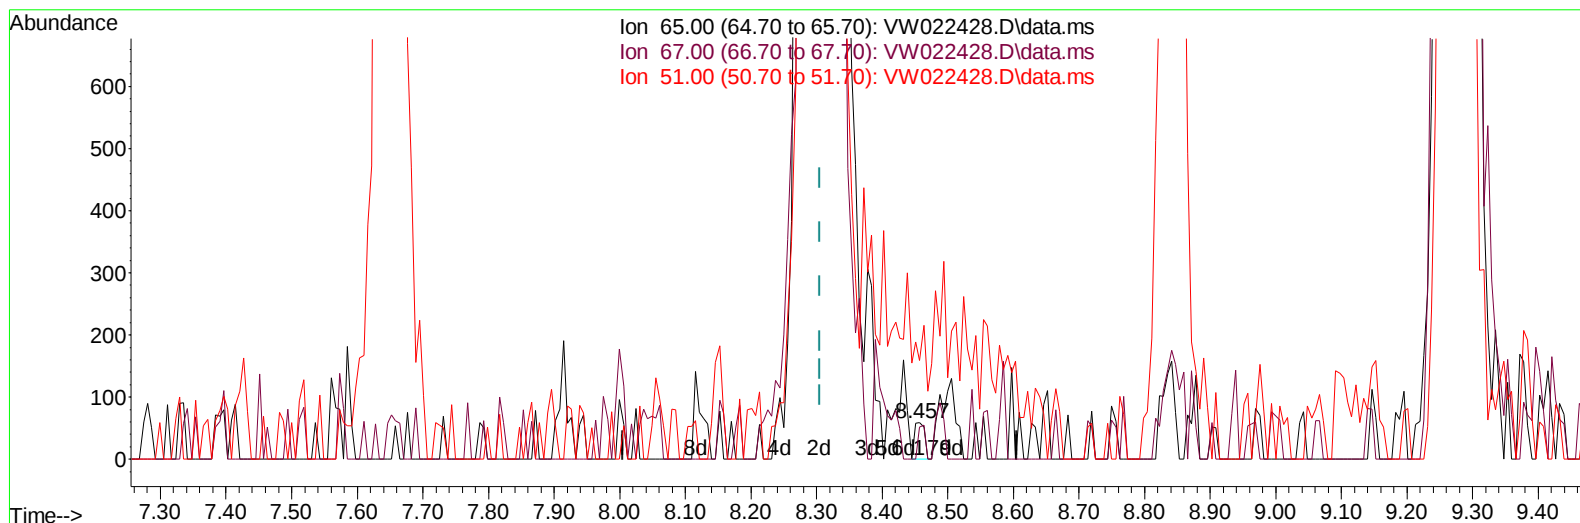

TIC: VW022428.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.457min (+ 0.152) 0.02 ug/L

response 62

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	62.90
51.00	99.30	91.94
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022428.D
 Acq On : 07 Apr 2022 13:43
 Operator : SY/VA
 Sample : N2262-14
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

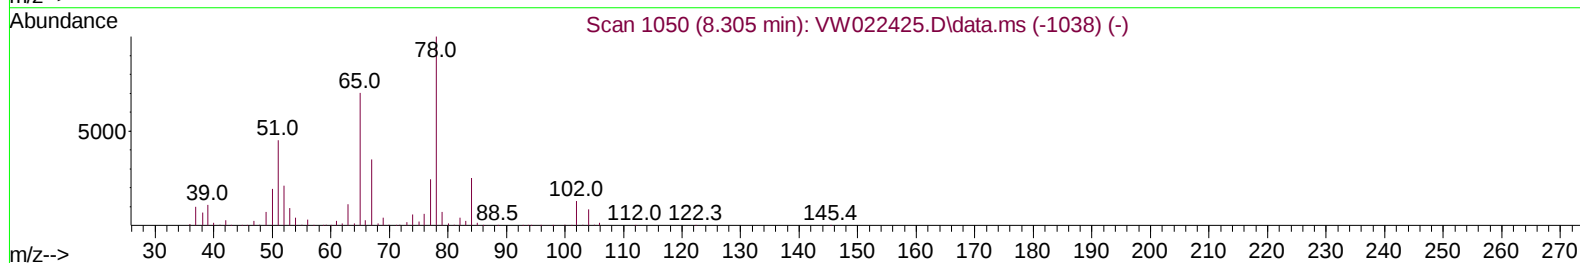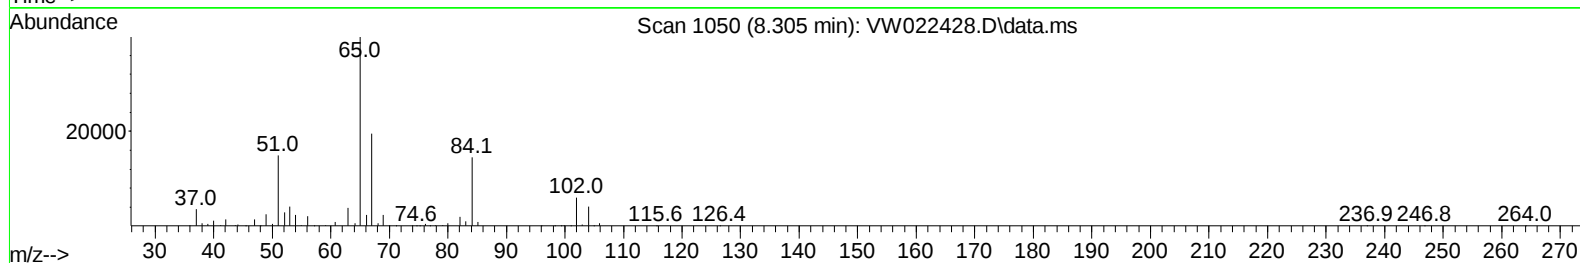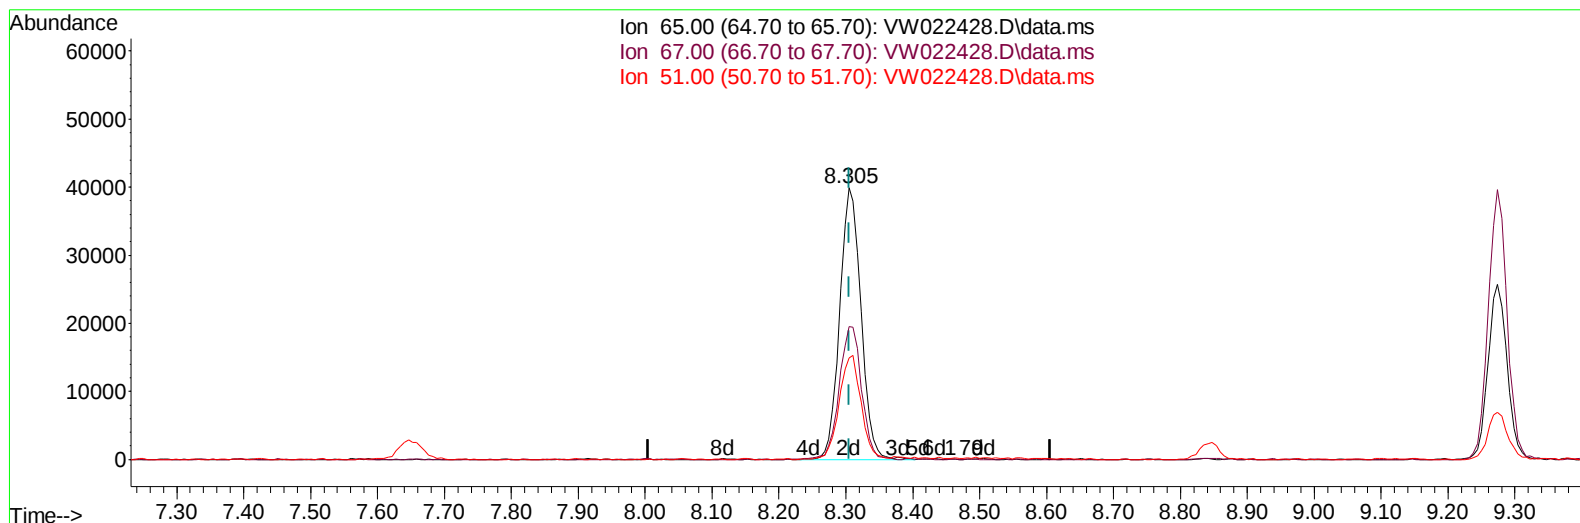

TIC: VW022428.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 26.37 ug/L m

response 88260

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.04#
51.00	99.30	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022428.D
 Acq On : 07 Apr 2022 13:43
 Operator : SY/VA
 Sample : N2262-14
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	187398	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	158688	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	59452	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	87666	21.161	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.640%	
7) Chloroethane-d5	2.891	69	63887	24.606	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	98.440%	
11) 1,1-Dichloroethene-d2	4.019	63	83564	15.552	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.200%	
21) 2-Butanone-d5	7.079	46	49606	68.585	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.160%#	
24) Chloroform-d	7.652	84	132943	22.696	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	90.800%	
26) 1,2-Dichloroethane-d4	8.305	65	88260m	26.372	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	105.480%	
32) Benzene-d6	8.274	84	237811	24.529	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	98.120%	
36) 1,2-Dichloropropane-d6	9.274	67	77666	27.682	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	110.720%	
41) Toluene-d8	10.323	98	212490	22.378	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.520%	
43) trans-1,3-Dichloroprop...	10.579	79	33310	25.156	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	100.640%	
47) 2-Hexanone-d5	10.920	63	38059	72.909	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	145.820%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	72772	30.504	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	122.000%#	
66) 1,2-Dichlorobenzene-d4	13.852	152	48727	23.139	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.560%	
Target Compounds					Qvalue	
46) Tetrachloroethene	10.865	164	2482	1.170	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022428.D
Acq On : 07 Apr 2022 13:43
Operator : SY/VA
Sample : N2262-14
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

