




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022429.D
Acq On : 07 Apr 2022 14:07
Operator : SY/VA
Sample : N2262-15
Misc : 4.79g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L5

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:31:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

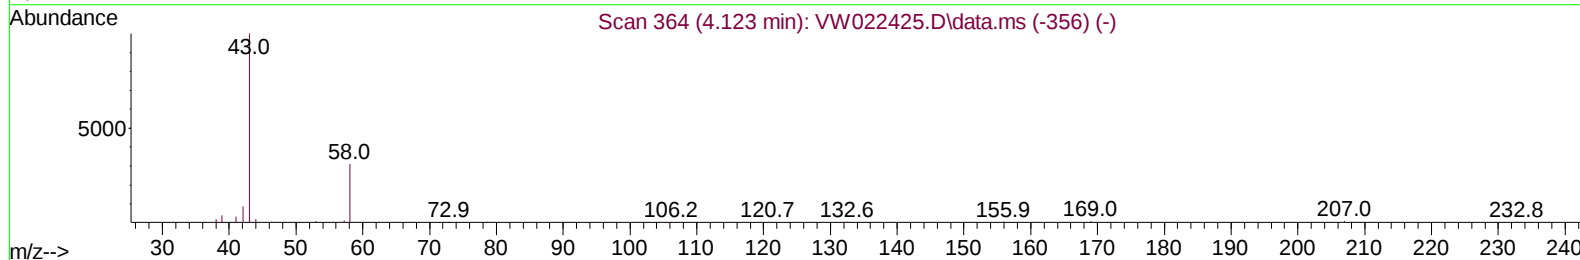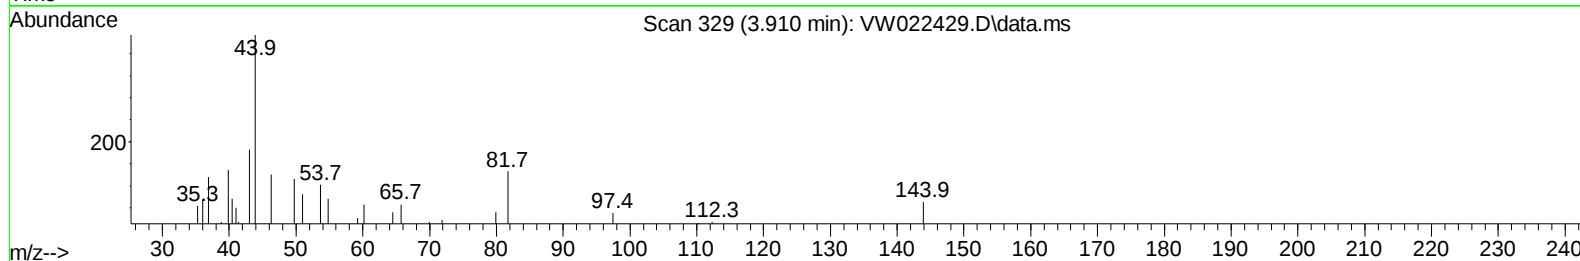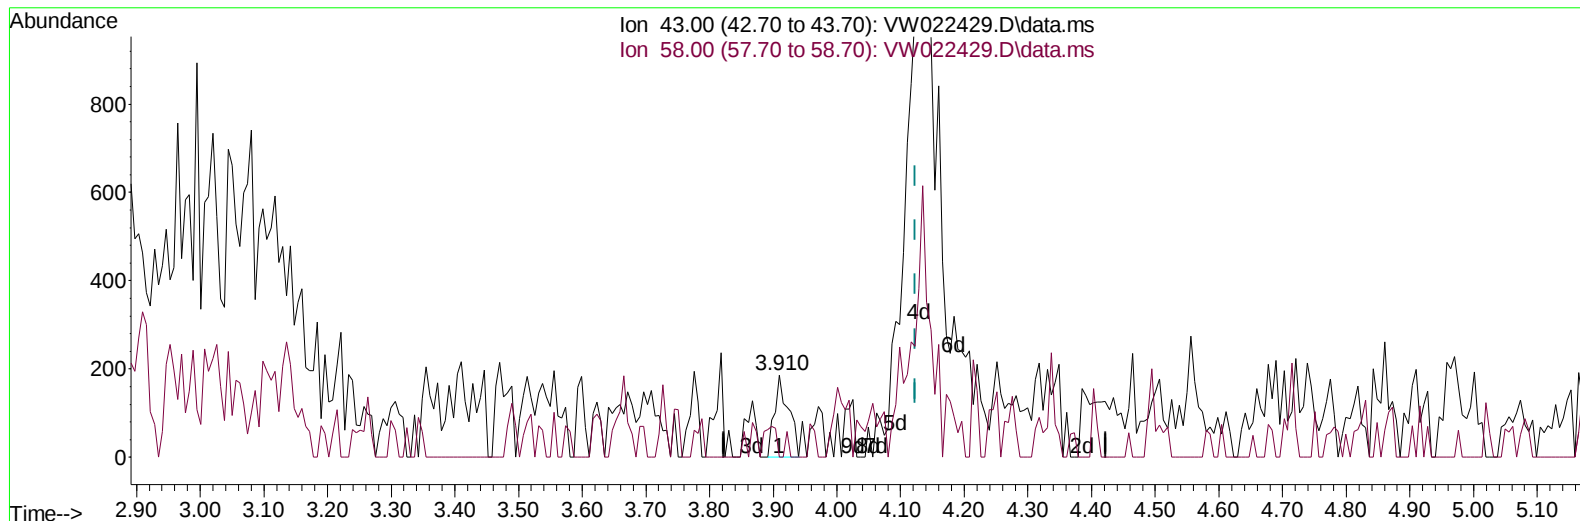

TIC: VW022429.D\data.ms

(13) Acetone (T)

3.910min (-0.213) 0.35 ug/L

response 289

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	32.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022429.D
 Acq On : 07 Apr 2022 14:07
 Operator : SY/VA
 Sample : N2262-15
 Misc : 4.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L5

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:31:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

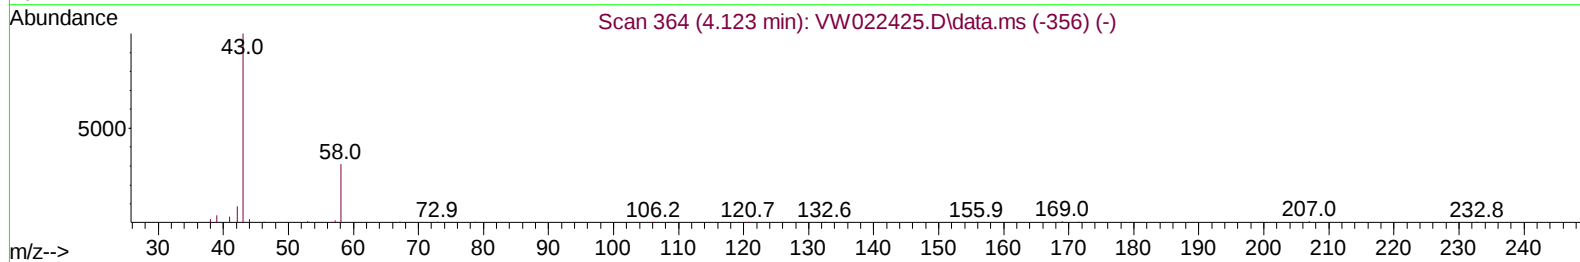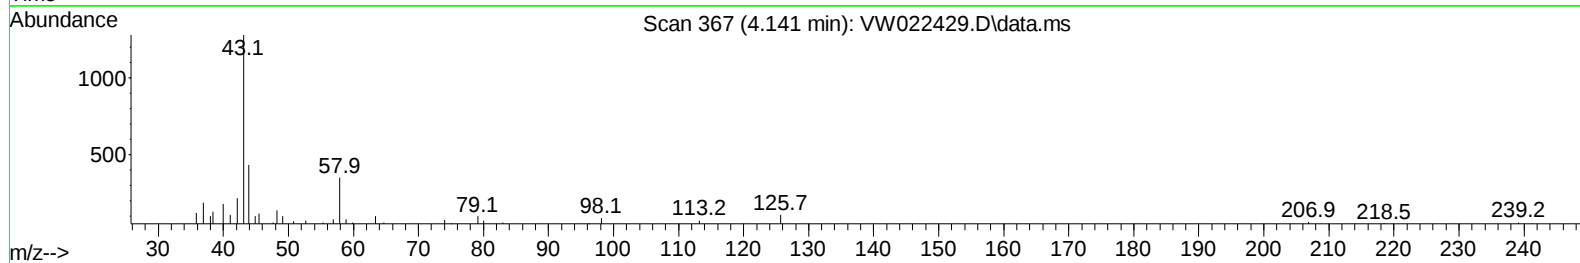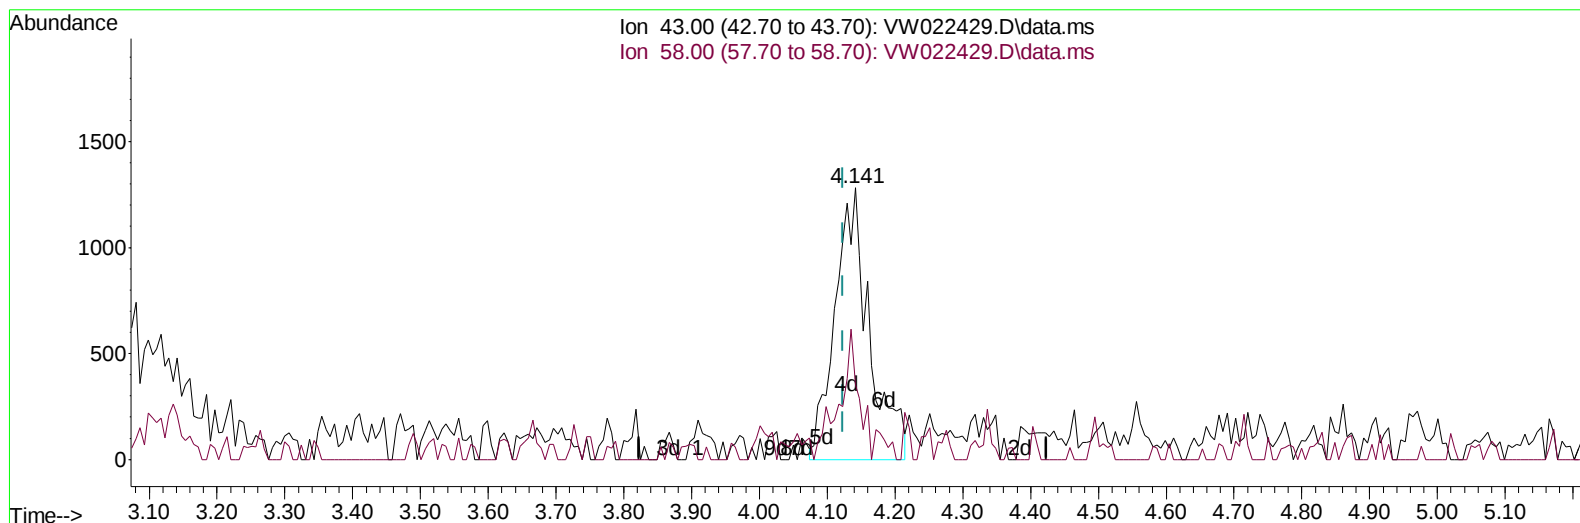

TIC: VW022429.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 5.48 ug/L m

response 4477

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	2.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022429.D
 Acq On : 07 Apr 2022 14:07
 Operator : SY/VA
 Sample : N2262-15
 Misc : 4.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L5

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:31:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		311094	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		313713	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		159659	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		144595	21.025	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	84.080%		
7) Chloroethane-d5	2.891	69		93235	21.631	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	86.520%		
11) 1,1-Dichloroethene-d2	4.019	63		125247	14.041	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	56.160%		
21) 2-Butanone-d5	7.074	46		87536	72.905	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	145.800%#		
24) Chloroform-d	7.647	84		229278	23.579	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	94.320%		
26) 1,2-Dichloroethane-d4	8.305	65		149986	26.996	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	108.000%		
32) Benzene-d6	8.275	84		426041	22.228	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	88.920%		
36) 1,2-Dichloropropane-d6	9.274	67		134639	24.274	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	97.080%		
41) Toluene-d8	10.323	98		398463	21.227	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	84.920%		
43) trans-1,3-Dichloroprop...	10.579	79		62861	24.014	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	96.040%		
47) 2-Hexanone-d5	10.920	63		70593	68.407	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	136.820%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		135525	28.736	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	114.960%		
66) 1,2-Dichlorobenzene-d4	13.853	152		140522	24.849	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	99.400%		
Target Compounds							
13) Acetone	4.141	43		4477m	5.476	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022429.D
Acq On : 07 Apr 2022 14:07
Operator : SY/VA
Sample : N2262-15
Misc : 4.79g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

