




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022431.D
 Acq On : 07 Apr 2022 14:55
 Operator : SY/VA
 Sample : N2262-17
 Misc : 4.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

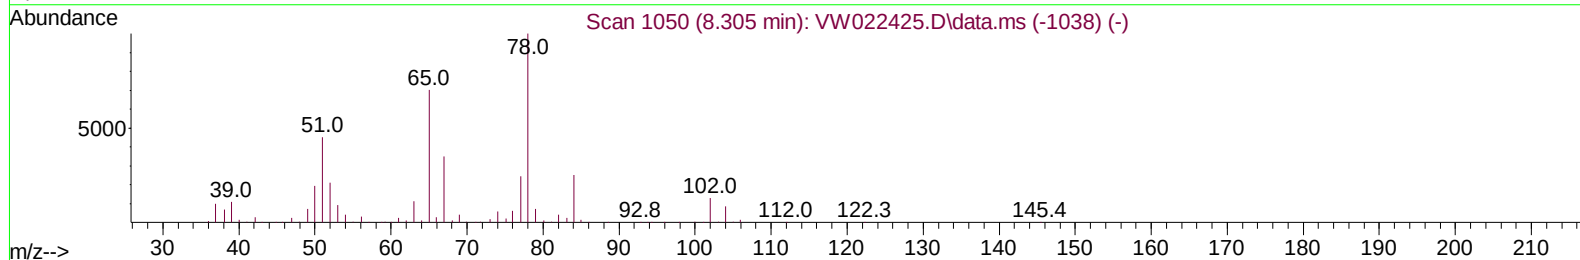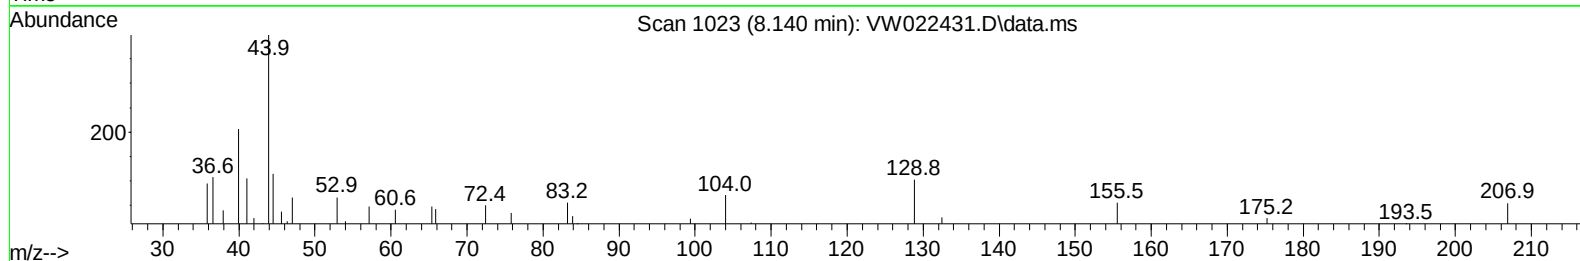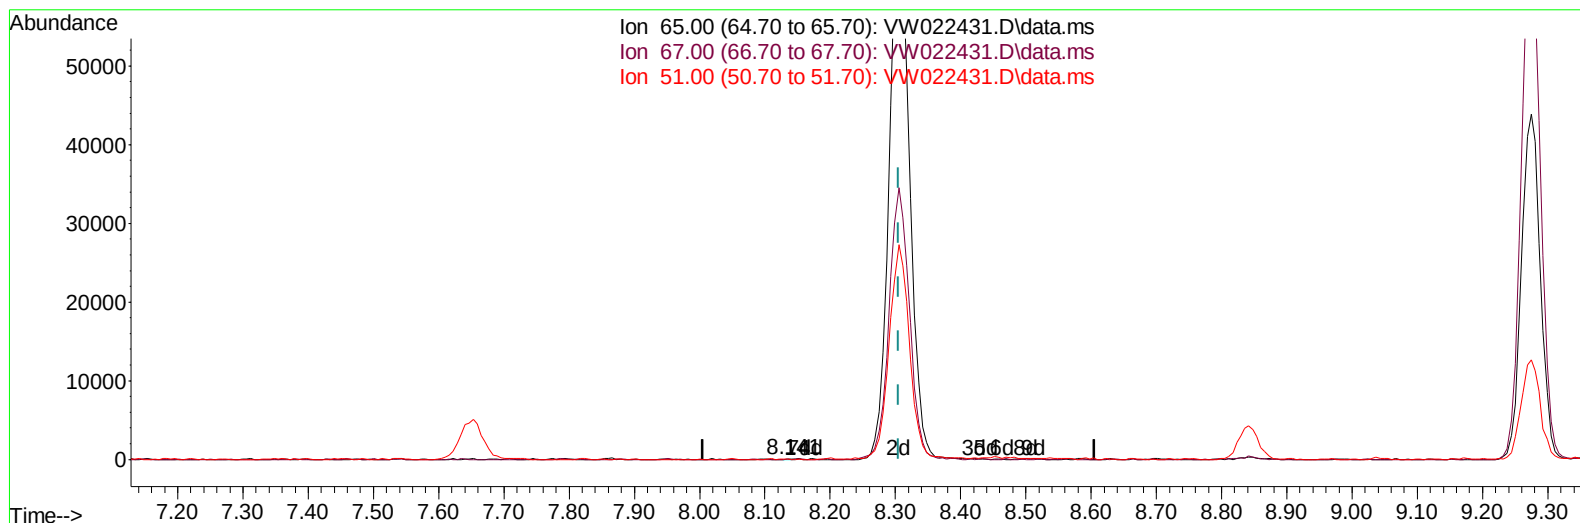

TIC: VW022431.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.140min (-0.165) 0.01 ug/L

response 72

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	43.06
51.00	99.30	102.78
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022431.D
 Acq On : 07 Apr 2022 14:55
 Operator : SY/VA
 Sample : N2262-17
 Misc : 4.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

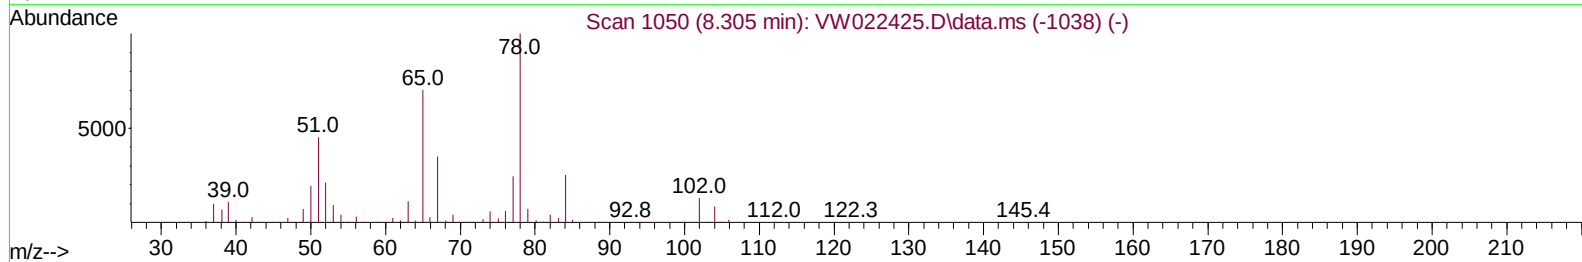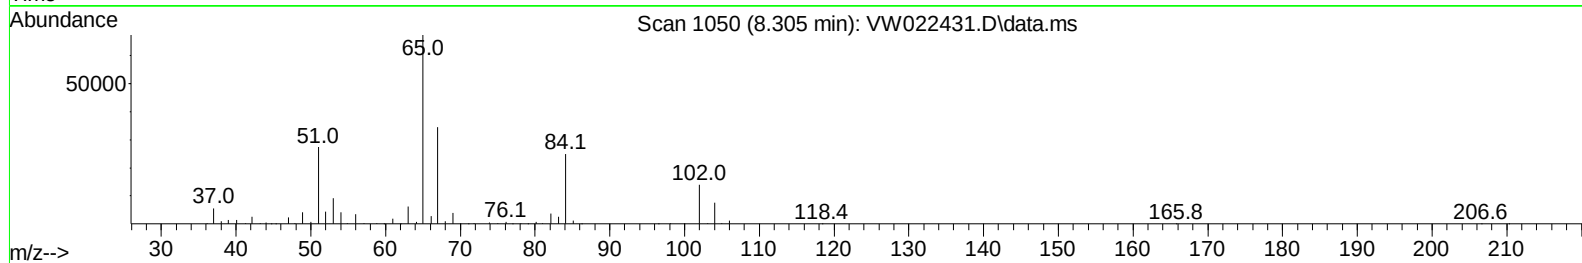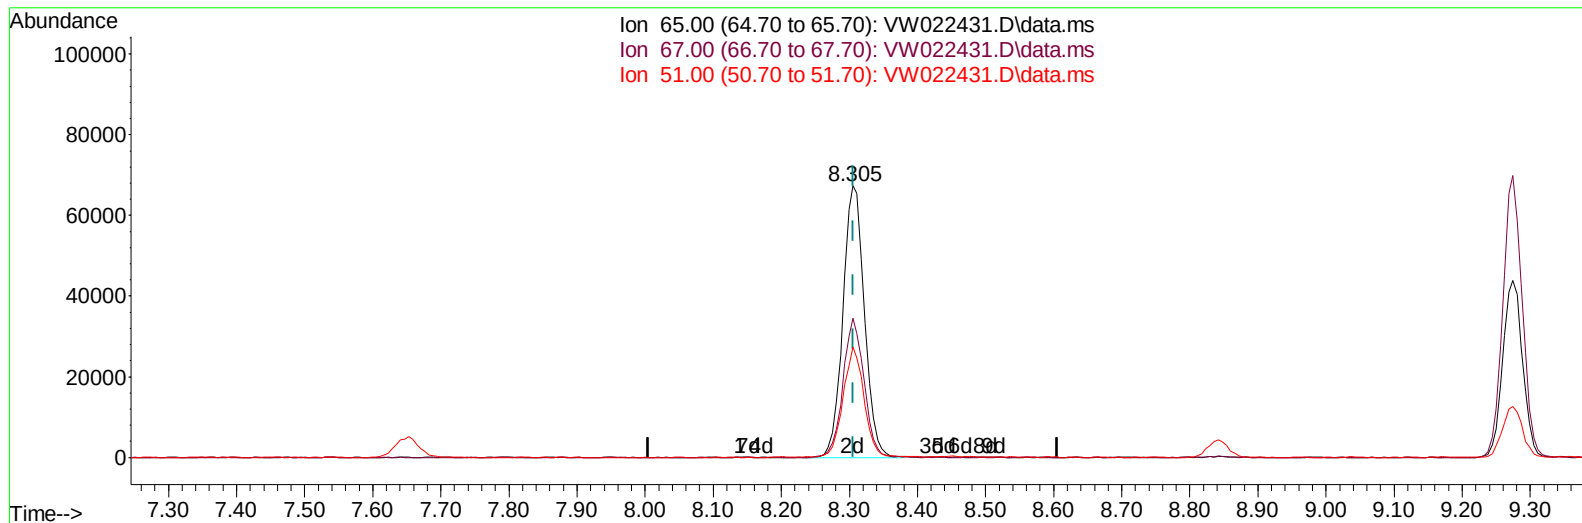

TIC: VW022431.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 24.97 ug/L m

response 148770

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.02#
51.00	99.30	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022431.D
 Acq On : 07 Apr 2022 14:55
 Operator : SY/VA
 Sample : N2262-17
 Misc : 4.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		333584	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		321268	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		159995	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		150066	20.349	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	81.400%	
7) Chloroethane-d5	2.891	69		98069	21.219	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	84.880%	
11) 1,1-Dichloroethene-d2	4.019	63		132748	13.879	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	55.520%	
21) 2-Butanone-d5	7.074	46		77871	60.483	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	120.960%	
24) Chloroform-d	7.653	84		234344	22.475	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	89.920%	
26) 1,2-Dichloroethane-d4	8.305	65		148770m	24.972	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	99.880%	
32) Benzene-d6	8.275	84		430624	21.939	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	87.760%	
36) 1,2-Dichloropropane-d6	9.274	67		137256	24.164	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	96.640%	
41) Toluene-d8	10.323	98		415063	21.591	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	86.360%	
43) trans-1,3-Dichloroprop...	10.579	79		60550	22.587	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	90.360%	
47) 2-Hexanone-d5	10.921	63		62698	59.327	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	118.660%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		128774	26.663	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	106.640%	
66) 1,2-Dichlorobenzene-d4	13.847	152		135253	23.867	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	95.480%	
Target Compounds							
13) Acetone	4.129	43		4881	5.568	ug/L	82
46) Tetrachloroethene	10.866	164		37076	8.636	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022431.D
Acq On : 07 Apr 2022 14:55
Operator : SY/VA
Sample : N2262-17
Misc : 4.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

