




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW040722\  
Data File : VW022432.D  
Acq On : 07 Apr 2022 15:20  
Operator : SY/VA  
Sample : N2262-18  
Misc : 4.36g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
EW6L8

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:32:00 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM040722SMA.M  
Quant Title : SFAM01.0  
QLast Update : Fri Apr 08 06:30:01 2022  
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022  
Supervised By :Mahesh Dadoda 04/11/2022

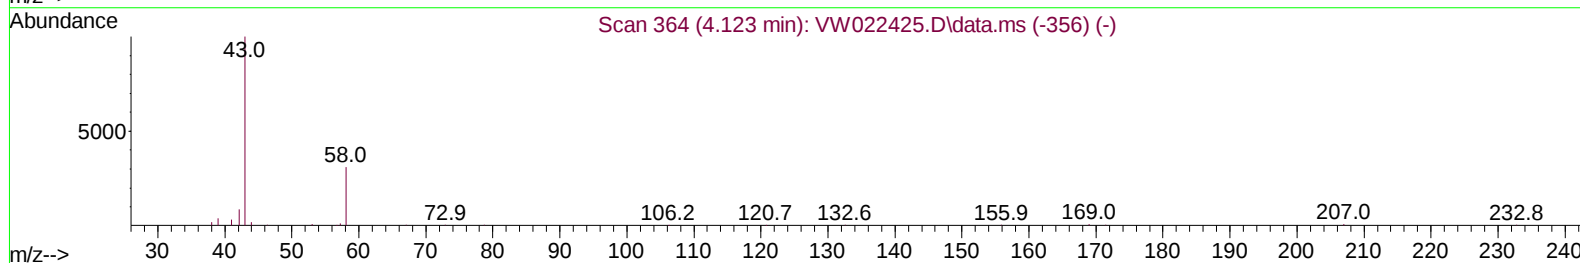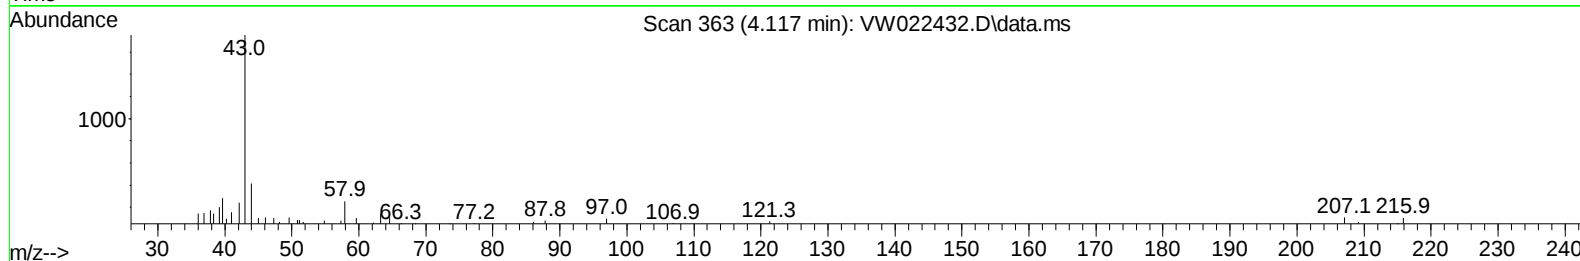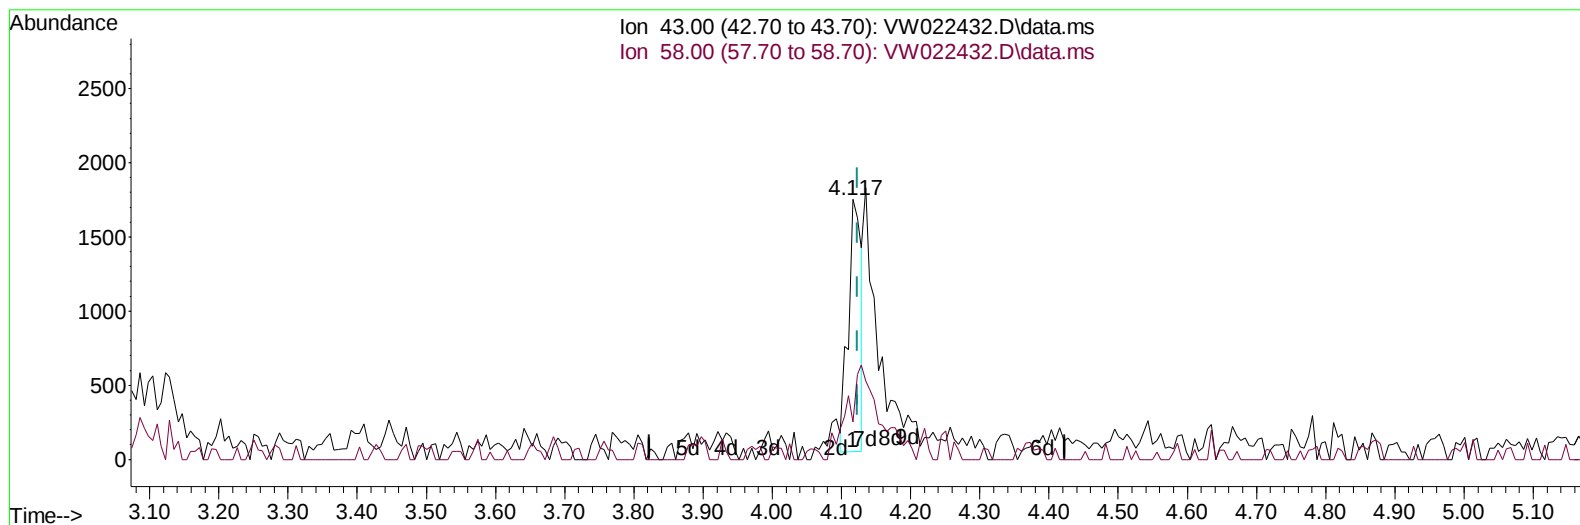

TIC: VW022432.D\data.ms

(13) Acetone (T)

4.117min (-0.006) 2.42 ug/L

response 2215

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 28.50  | 19.55  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW040722\  
 Data File : VW022432.D  
 Acq On : 07 Apr 2022 15:20  
 Operator : SY/VA  
 Sample : N2262-18  
 Misc : 4.36g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 EW6L8

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:32:00 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM040722SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Fri Apr 08 06:30:01 2022  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022  
 Supervised By :Mahesh Dadoda 04/11/2022

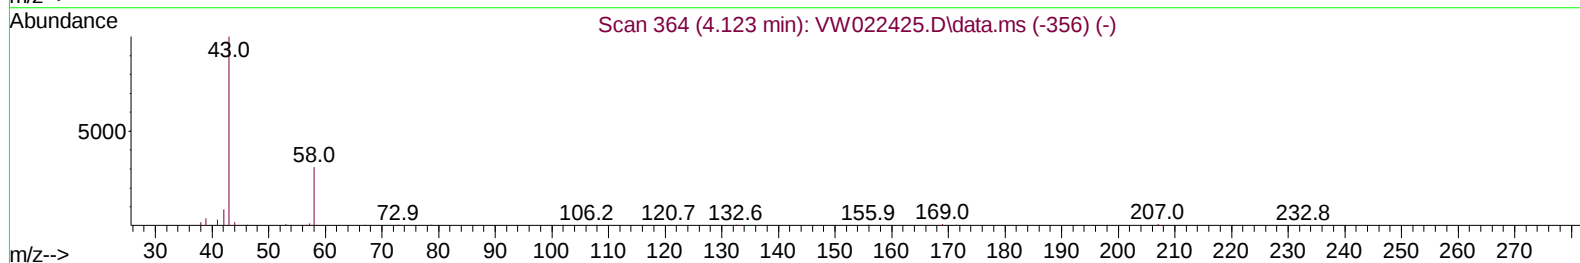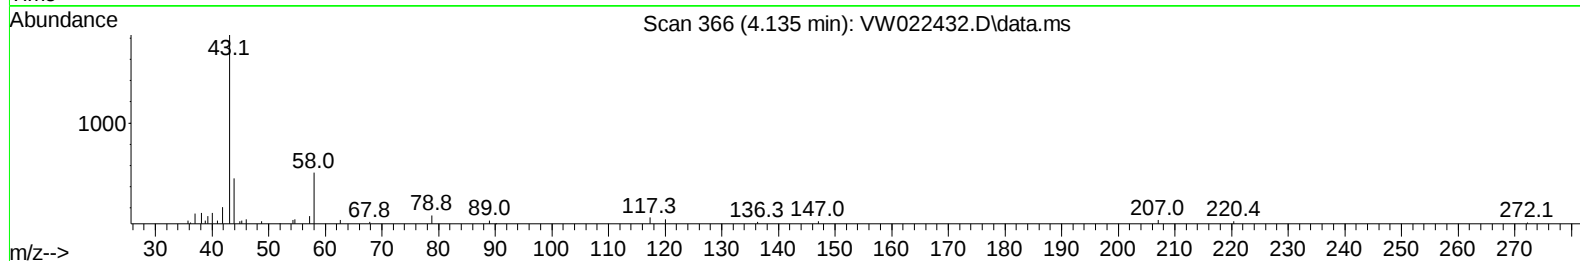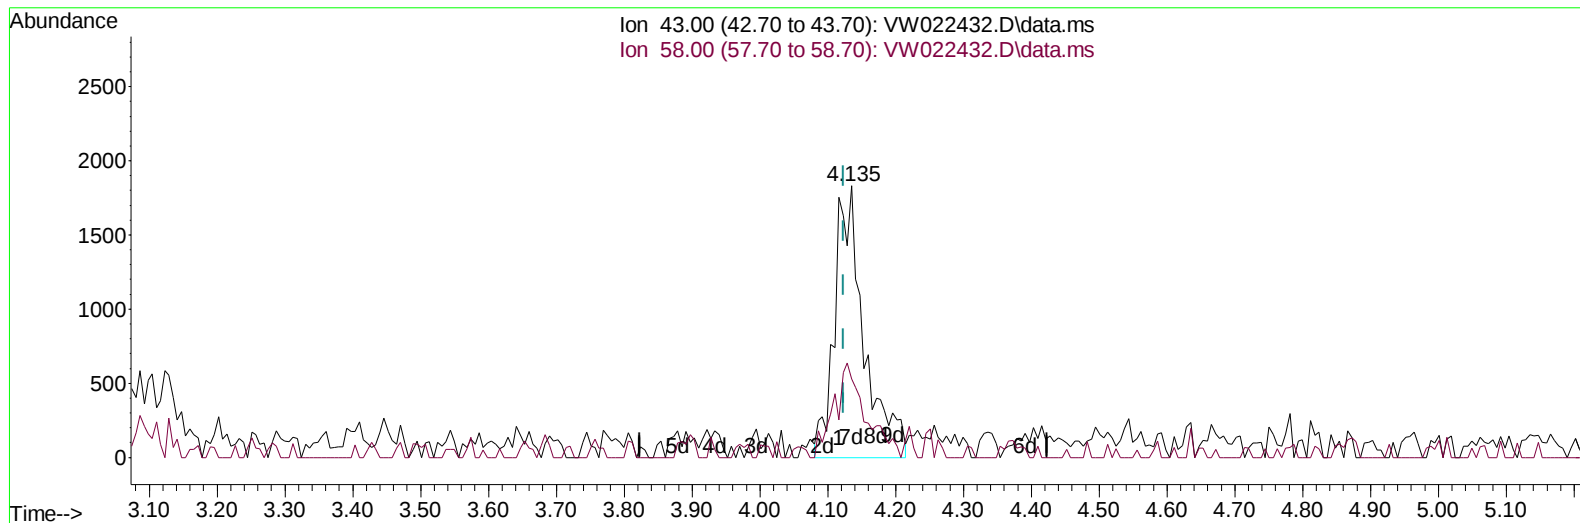

TIC: VW022432.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 5.98 ug/L m

response 5475

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 28.50  | 7.91   |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW040722\  
 Data File : VW022432.D  
 Acq On : 07 Apr 2022 15:20  
 Operator : SY/VA  
 Sample : N2262-18  
 Misc : 4.36g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 EW6L8

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:32:00 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM040722SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Fri Apr 08 06:30:01 2022  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022  
 Supervised By :Mahesh Dadoda 04/11/2022

| Compound                      | R.T.     | Q     | Ion | Response   | Conc     | Units | Dev(Min) |
|-------------------------------|----------|-------|-----|------------|----------|-------|----------|
| -----                         |          |       |     |            |          |       |          |
| Internal Standards            |          |       |     |            |          |       |          |
| 1) 1,4-Difluorobenzene        | 8.841    | 114   |     | 348206     | 25.000   | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 11.627   | 117   |     | 339256     | 25.000   | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 13.560   | 152   |     | 161876     | 25.000   | ug/L  | 0.00     |
| System Monitoring Compounds   |          |       |     |            |          |       |          |
| 4) Vinyl Chloride-d3          | 2.355    | 65    |     | 141424     | 18.372   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 30 | - 150 |     | Recovery = | 73.480%  |       |          |
| 7) Chloroethane-d5            | 2.885    | 69    |     | 93395      | 19.359   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 30 | - 150 |     | Recovery = | 77.440%  |       |          |
| 11) 1,1-Dichloroethene-d2     | 4.019    | 63    |     | 124425     | 12.462   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 45 | - 110 |     | Recovery = | 49.840%  |       |          |
| 21) 2-Butanone-d5             | 7.079    | 46    |     | 69883      | 51.999   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 20 | - 135 |     | Recovery = | 104.000% |       |          |
| 24) Chloroform-d              | 7.646    | 84    |     | 217150     | 19.952   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 40 | - 150 |     | Recovery = | 79.800%  |       |          |
| 26) 1,2-Dichloroethane-d4     | 8.305    | 65    |     | 139246     | 22.392   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 70 | - 130 |     | Recovery = | 89.560%  |       |          |
| 32) Benzene-d6                | 8.274    | 84    |     | 408906     | 19.728   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 20 | - 135 |     | Recovery = | 78.920%  |       |          |
| 36) 1,2-Dichloropropane-d6    | 9.274    | 67    |     | 126925     | 21.160   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 70 | - 120 |     | Recovery = | 84.640%  |       |          |
| 41) Toluene-d8                | 10.323   | 98    |     | 375025     | 18.474   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 30 | - 130 |     | Recovery = | 73.880%  |       |          |
| 43) trans-1,3-Dichloroprop... | 10.579   | 79    |     | 56218      | 19.859   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 30 | - 135 |     | Recovery = | 79.440%  |       |          |
| 47) 2-Hexanone-d5             | 10.920   | 63    |     | 56326      | 50.472   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 20 | - 135 |     | Recovery = | 100.940% |       |          |
| 56) 1,1,2,2-Tetrachloroeth... | 12.688   | 84    |     | 116434     | 22.829   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 45 | - 120 |     | Recovery = | 91.320%  |       |          |
| 66) 1,2-Dichlorobenzene-d4    | 13.853   | 152   |     | 128527     | 22.416   | ug/L  | 0.00     |
| Spiked Amount 25.000          | Range 75 | - 120 |     | Recovery = | 89.680%  |       |          |
| Target Compounds              |          |       |     |            |          |       |          |
| 13) Acetone                   | 4.135    | 43    |     | 5475m      | 5.983    | ug/L  |          |
| 46) Tetrachloroethene         | 10.859   | 164   |     | 21976      | 4.848    | ug/L  | 90       |
| -----                         |          |       |     |            |          |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW040722\  
Data File : VW022432.D  
Acq On : 07 Apr 2022 15:20  
Operator : SY/VA  
Sample : N2262-18  
Misc : 4.36g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
EW6L8

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022  
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:32:00 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM040722SMA.M  
Quant Title : SFAM01.0  
QLast Update : Fri Apr 08 06:30:01 2022  
Response via : Initial Calibration

