




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022434.D
 Acq On : 07 Apr 2022 16:08
 Operator : SY/VA
 Sample : N2262-20
 Misc : 6.46g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6M0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:32:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

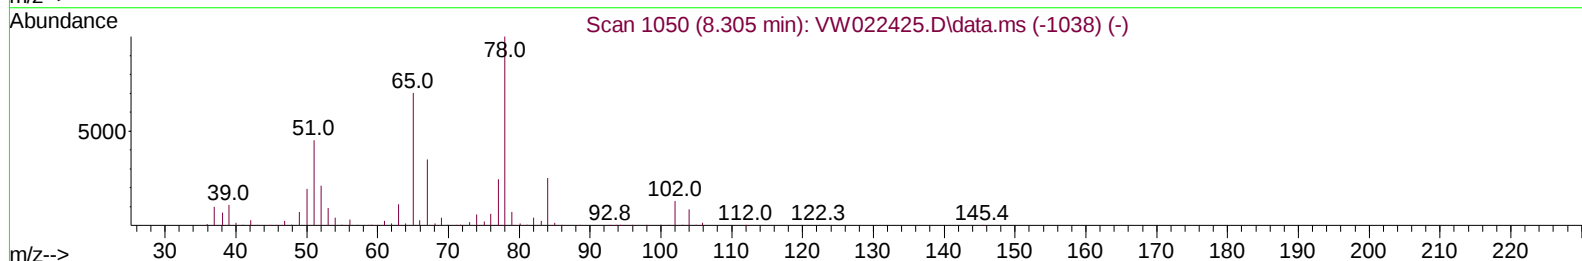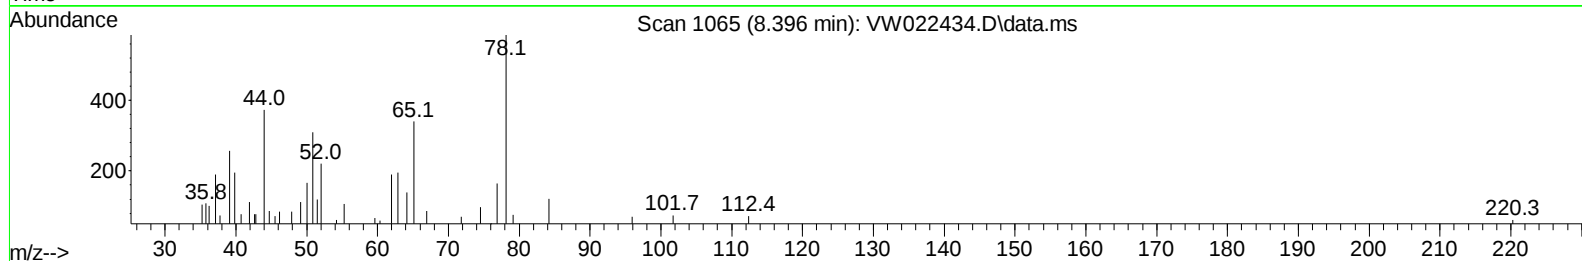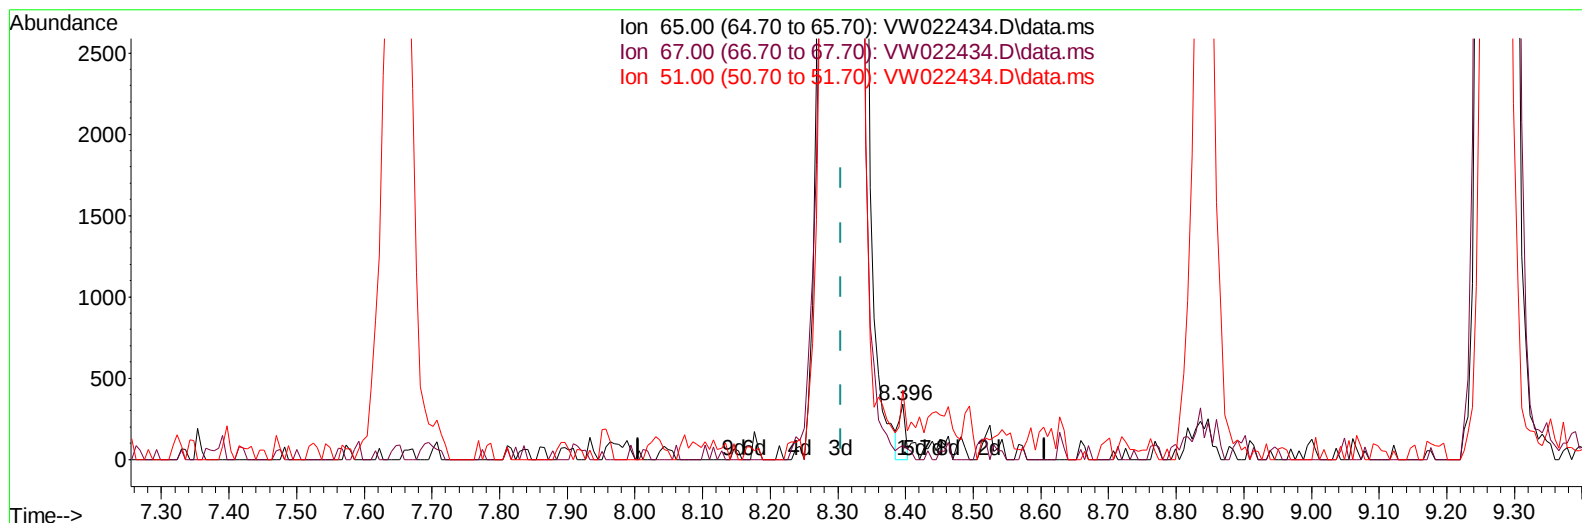

TIC: VW022434.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.396min (+ 0.091) 0.04 ug/L

response 233

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	43.35
51.00	99.30	112.88
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022434.D
 Acq On : 07 Apr 2022 16:08
 Operator : SY/VA
 Sample : N2262-20
 Misc : 6.46g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6M0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:32:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

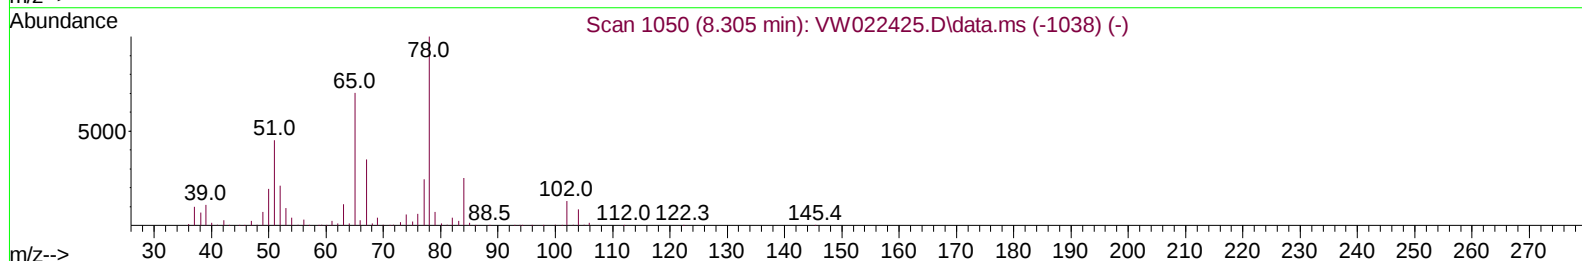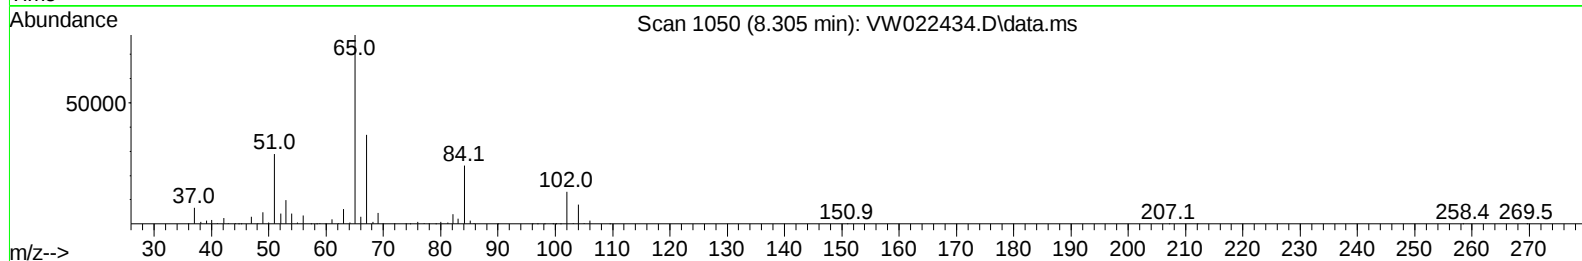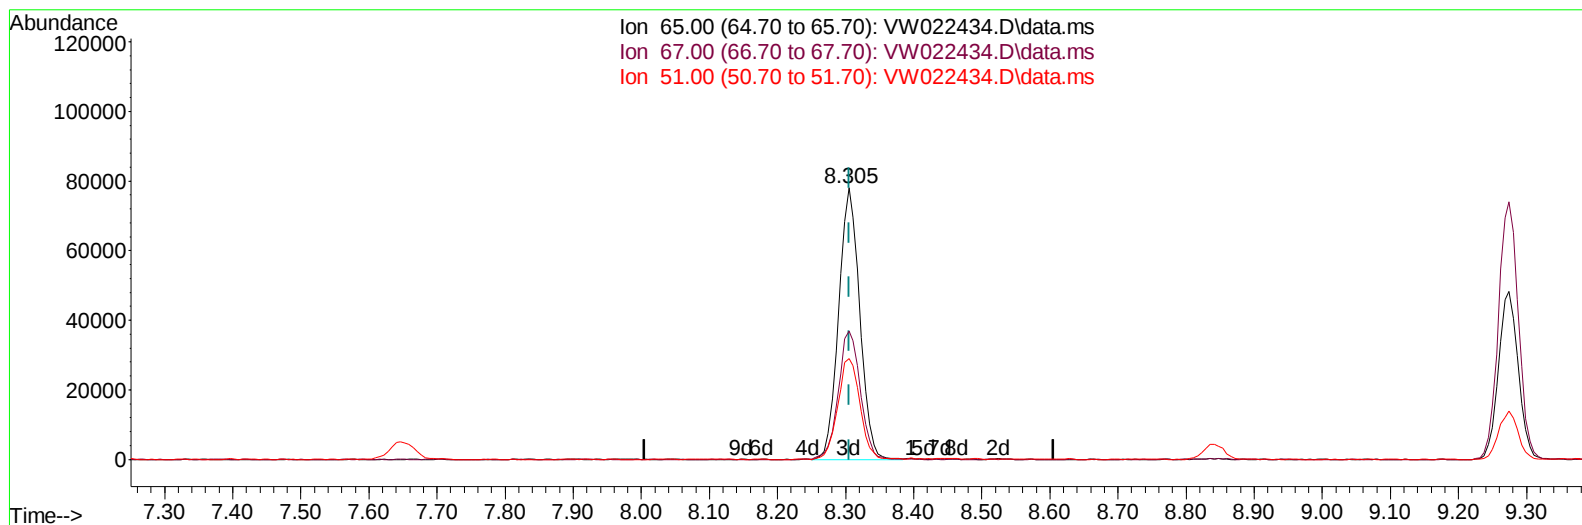

TIC: VW022434.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 27.21 ug/L m

response 167175

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.06#
51.00	99.30	0.16#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022434.D
 Acq On : 07 Apr 2022 16:08
 Operator : SY/VA
 Sample : N2262-20
 Misc : 6.46g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6M0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:32:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	344006	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	333849	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	158563	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	164385	21.616	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	86.480%	
7) Chloroethane-d5	2.885	69	111676	23.431	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	93.720%	
11) 1,1-Dichloroethene-d2	4.013	63	142309	14.427	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	57.720%	
21) 2-Butanone-d5	7.080	46	93993	70.793	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	141.580%#	
24) Chloroform-d	7.647	84	256105	23.818	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.280%	
26) 1,2-Dichloroethane-d4	8.305	65	167175m	27.211	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	108.840%	
32) Benzene-d6	8.275	84	477934	23.432	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	93.720%	
36) 1,2-Dichloropropane-d6	9.274	67	150443	25.487	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	101.960%	
41) Toluene-d8	10.323	98	446116	22.332	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.320%	
43) trans-1,3-Dichloroprop...	10.579	79	67529	24.241	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	96.960%	
47) 2-Hexanone-d5	10.920	63	77890	70.925	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	141.860%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	142999	28.492	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	113.960%	
66) 1,2-Dichlorobenzene-d4	13.853	152	138551	24.669	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	98.680%	
Target Compounds						
13) Acetone	4.129	43	7018	7.763	ug/L	Qvalue 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022434.D
Acq On : 07 Apr 2022 16:08
Operator : SY/VA
Sample : N2262-20
Misc : 6.46g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6M0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:32:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

