




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022439.D
Acq On : 07 Apr 2022 18:08
Operator : SY/VA
Sample : N2293-04
Misc : 6.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNN4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:33:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

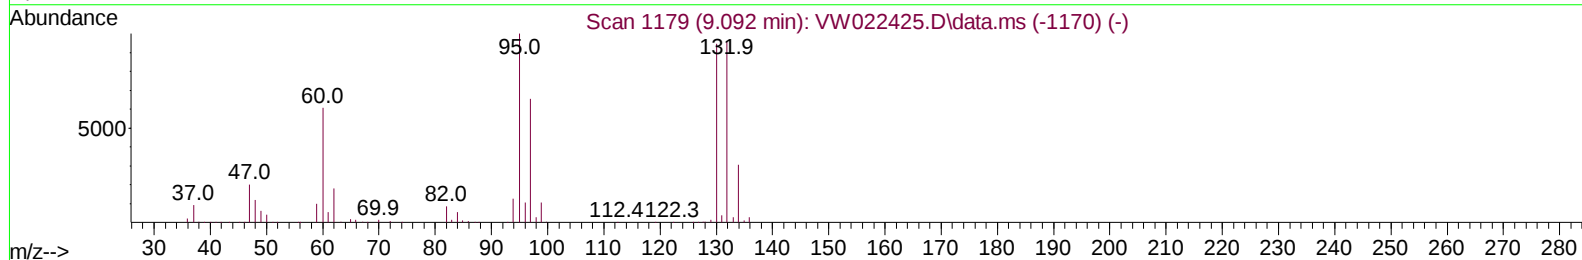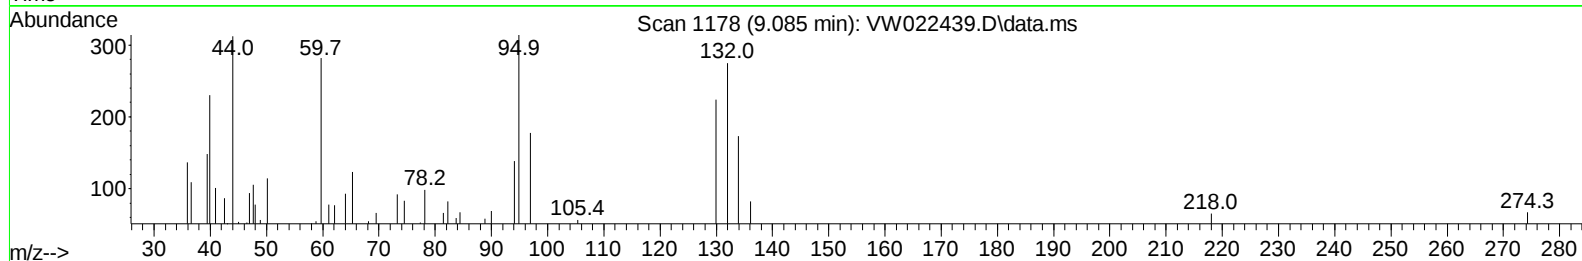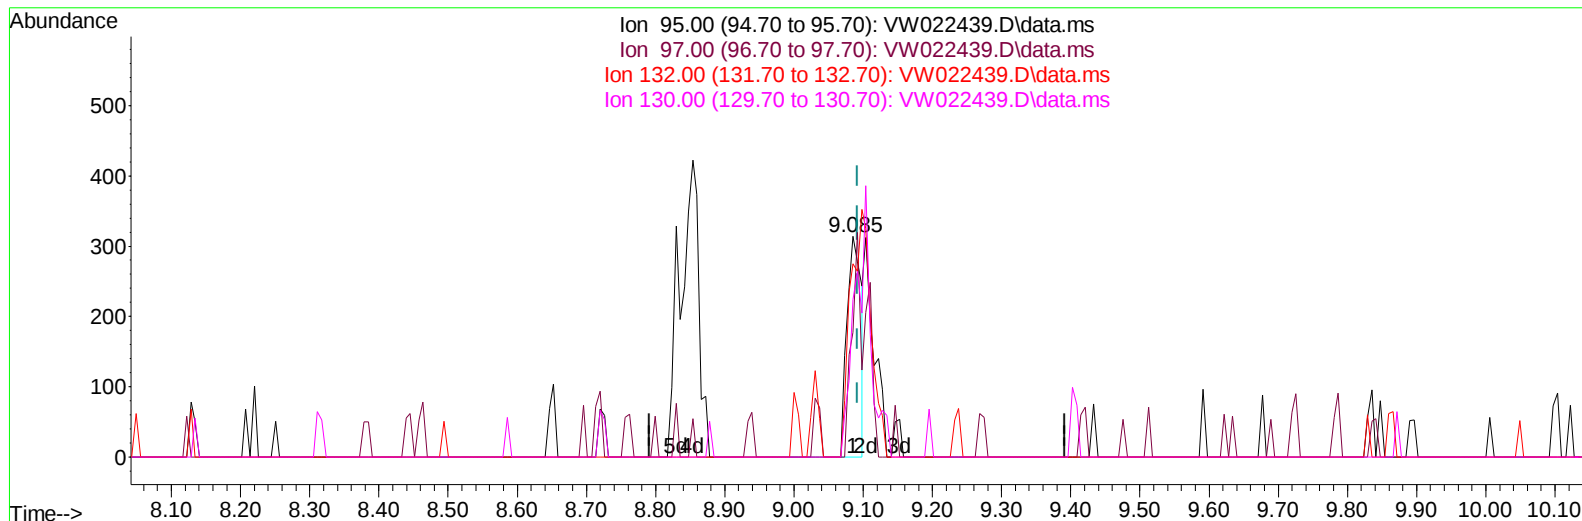

TIC: VW022439.D\data.ms

(34) Trichloroethene (T)

9.085min (-0.006) 2.34 ug/L

response 447

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	66.30	56.69
132.00	96.30	87.58
130.00	97.70	71.34




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022439.D
 Acq On : 07 Apr 2022 18:08
 Operator : SY/VA
 Sample : N2293-04
 Misc : 6.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

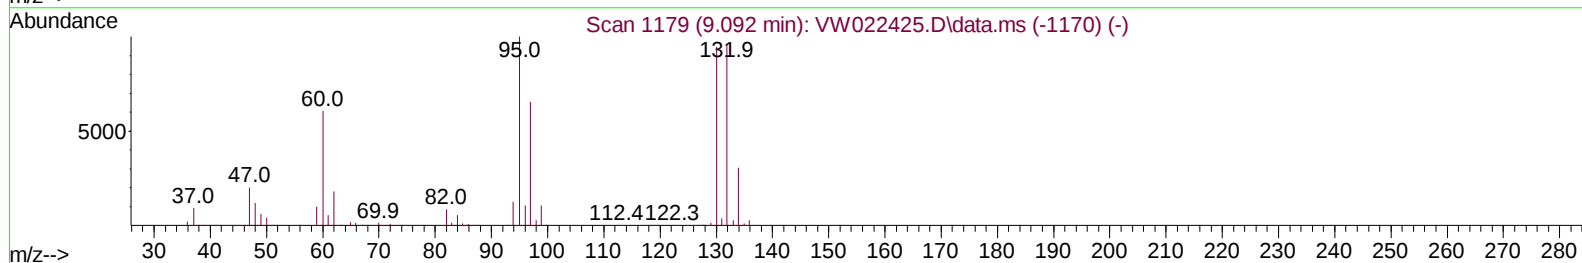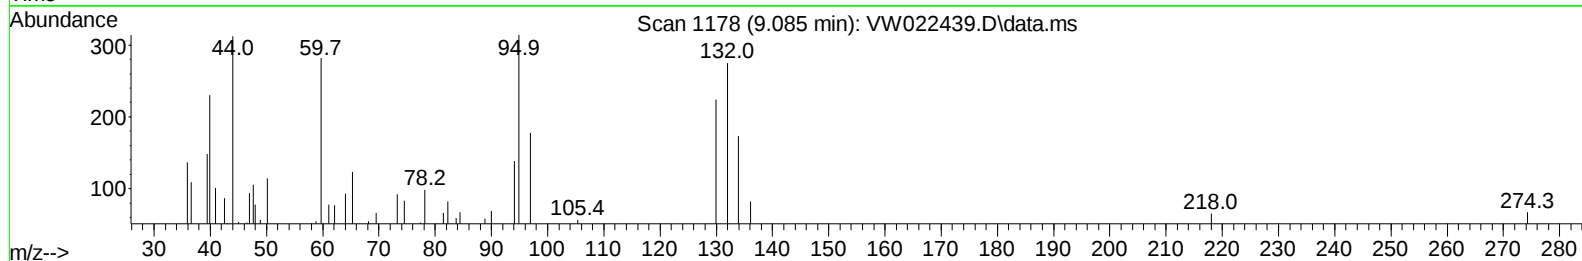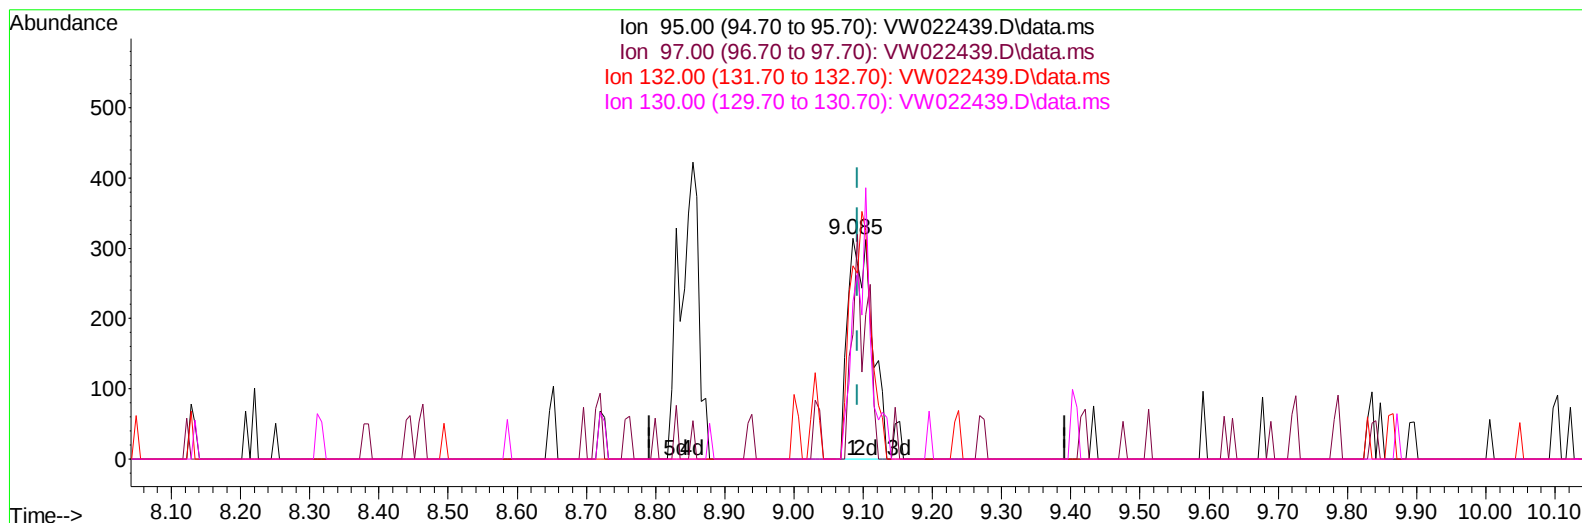

TIC: VW022439.D\data.ms

(34) Trichloroethene (T)

9.085min (-0.006) 4.01 ug/L m

response 766

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	66.30	56.69
132.00	96.30	87.58
130.00	97.70	71.34




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022439.D
Acq On : 07 Apr 2022 18:08
Operator : SY/VA
Sample : N2293-04
Misc : 6.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNN4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:33:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

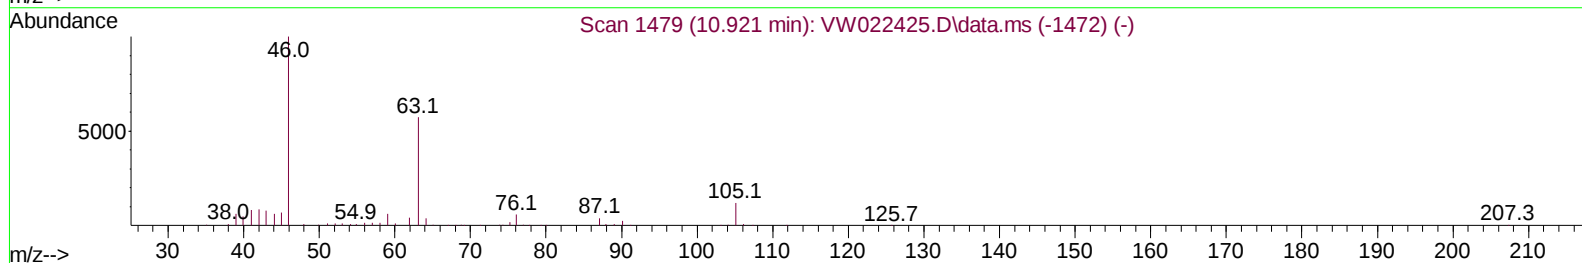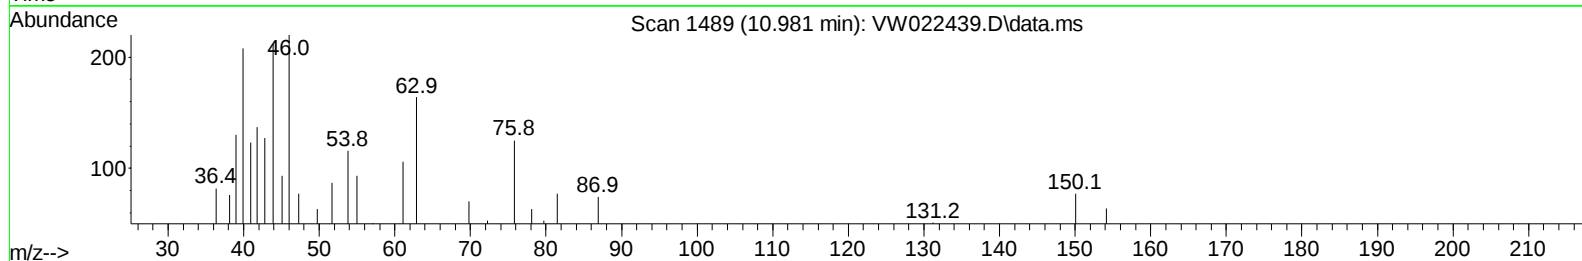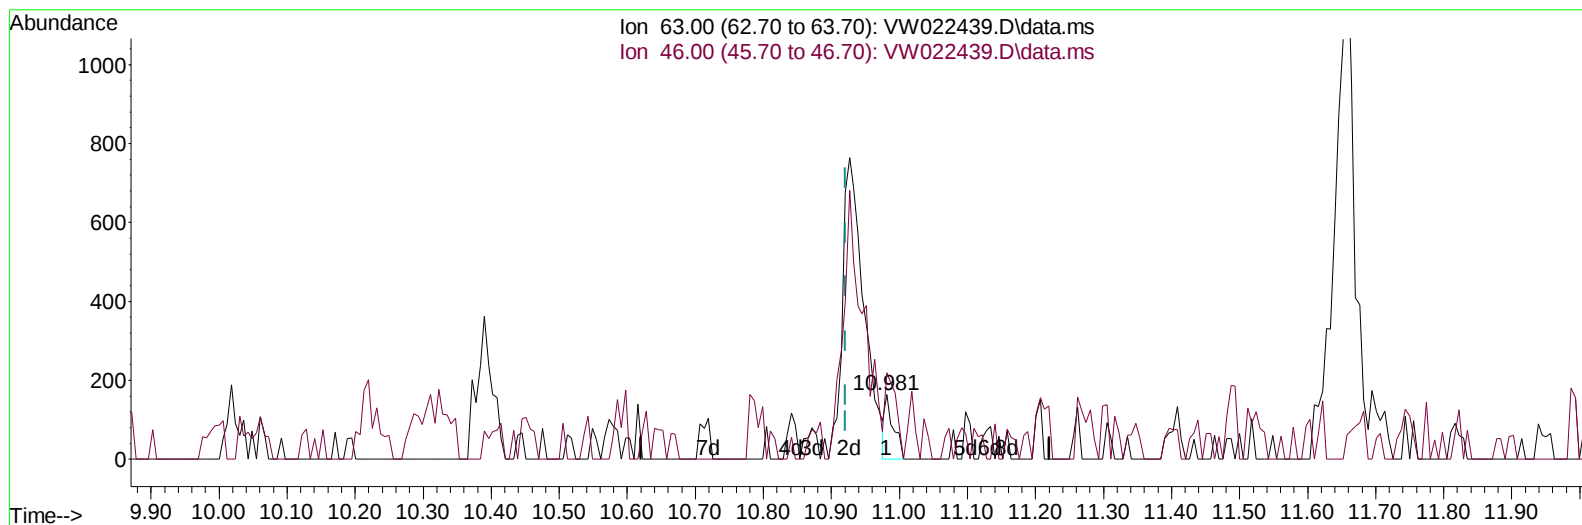

TIC: VW022439.D\data.ms

(47) 2-Hexanone-d5 (S)

10.981min (+ 0.061) 4.14 ug/L

response 143

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	177.60	171.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022439.D
 Acq On : 07 Apr 2022 18:08
 Operator : SY/VA
 Sample : N2293-04
 Misc : 6.93g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN4

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

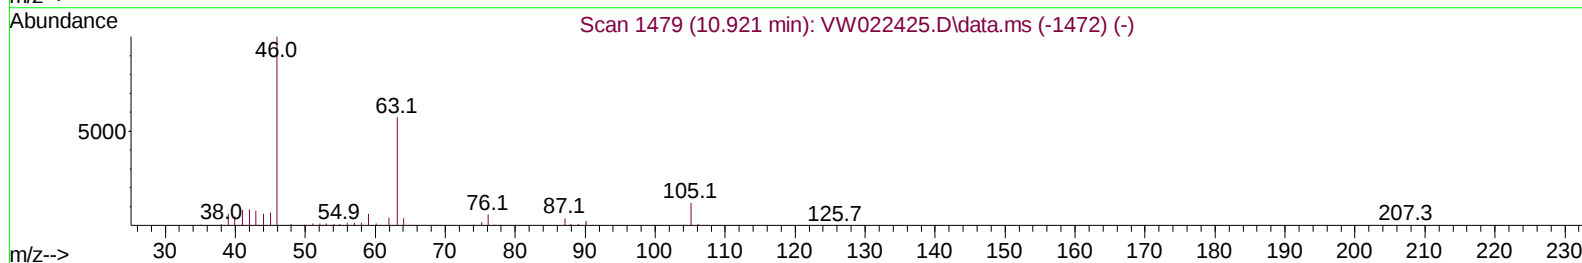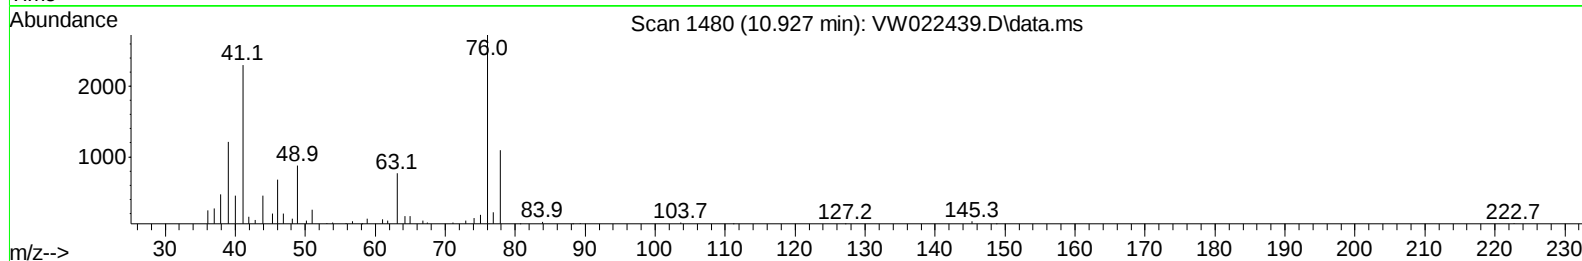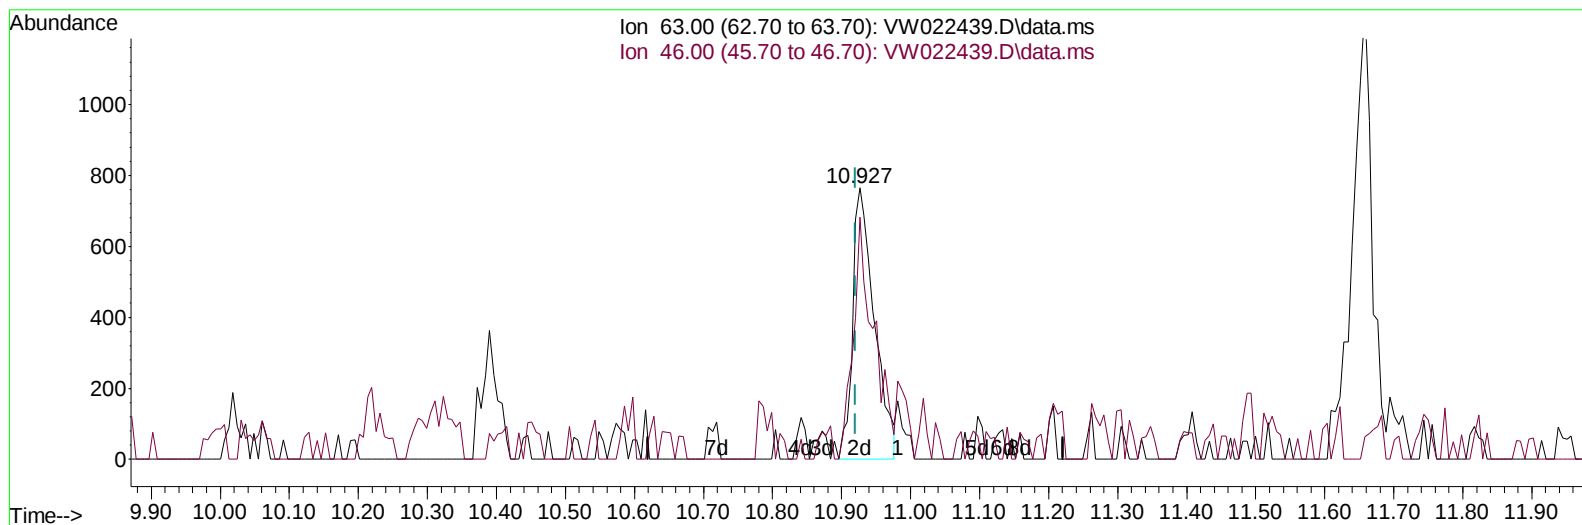

TIC: VW022439.D\data.ms

(47) 2-Hexanone-d5 (S)

10.927min (+ 0.006) 48.22 ug/L m

response 1666

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	177.60	14.71#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022439.D
Acq On : 07 Apr 2022 18:08
Operator : SY/VA
Sample : N2293-04
Misc : 6.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNN4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:33:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

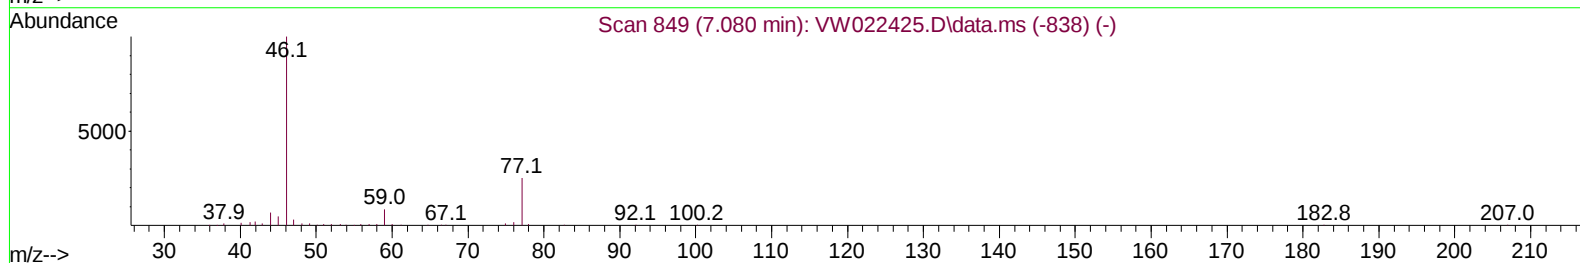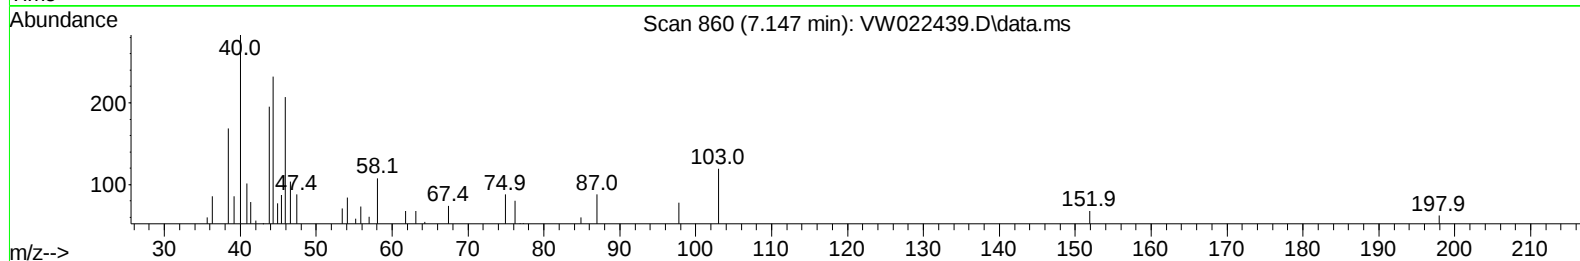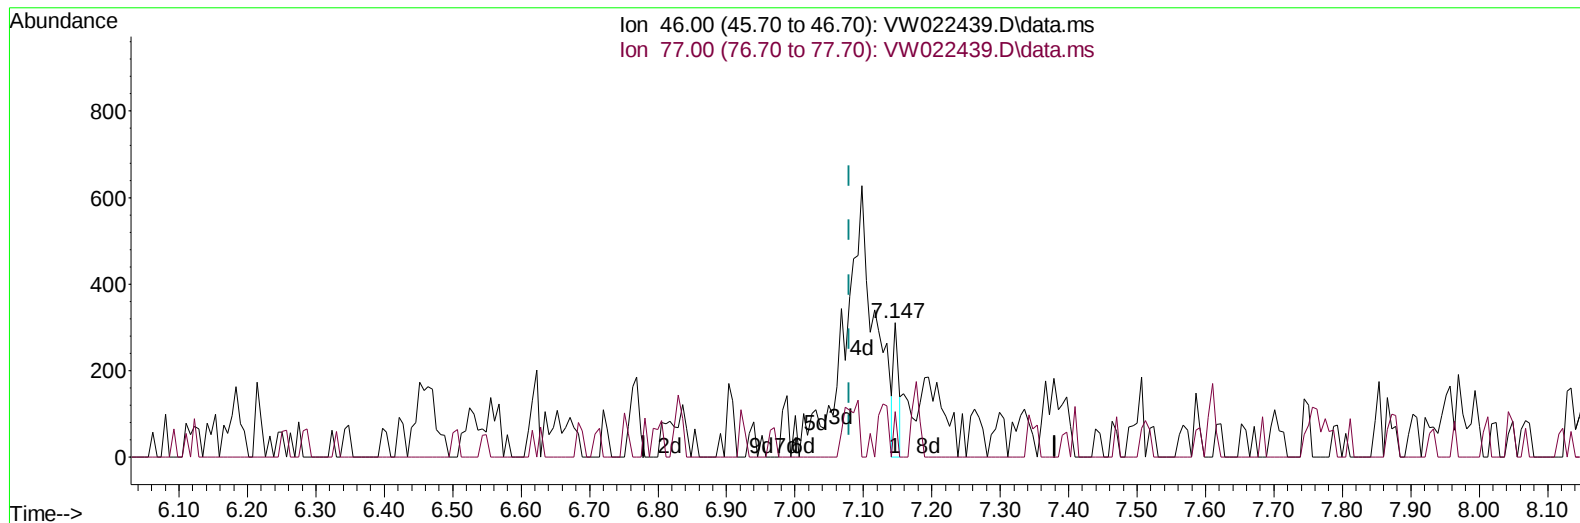

TIC: VW022439.D\data.ms

(21) 2-Butanone-d5 (S)

7.147min (+ 0.067) 3.33 ug/L

response 164

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	23.78
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022439.D
 Acq On : 07 Apr 2022 18:08
 Operator : SY/VA
 Sample : N2293-04
 Misc : 6.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN4

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

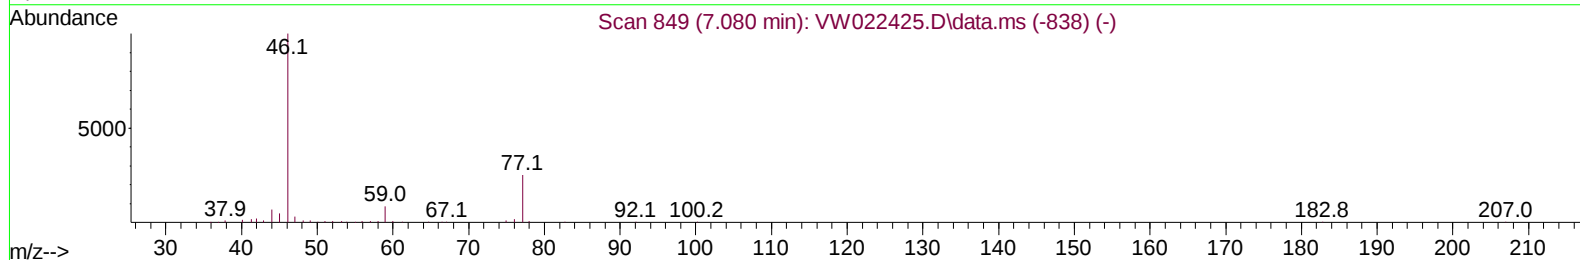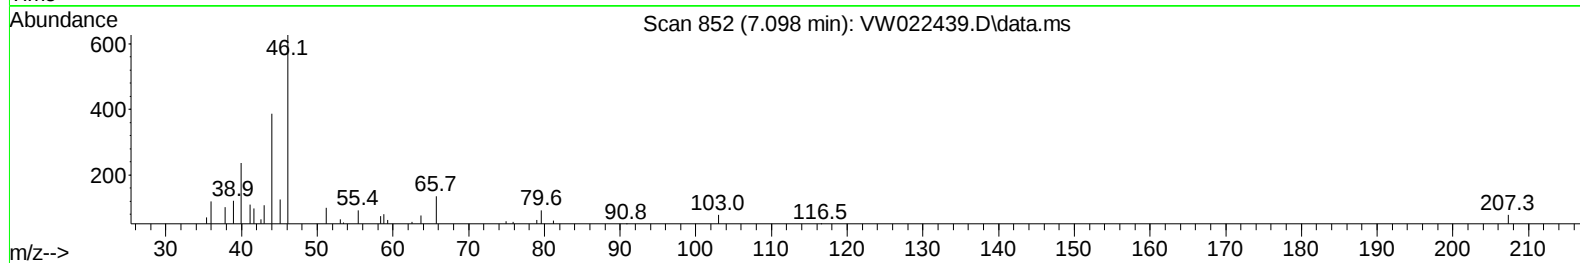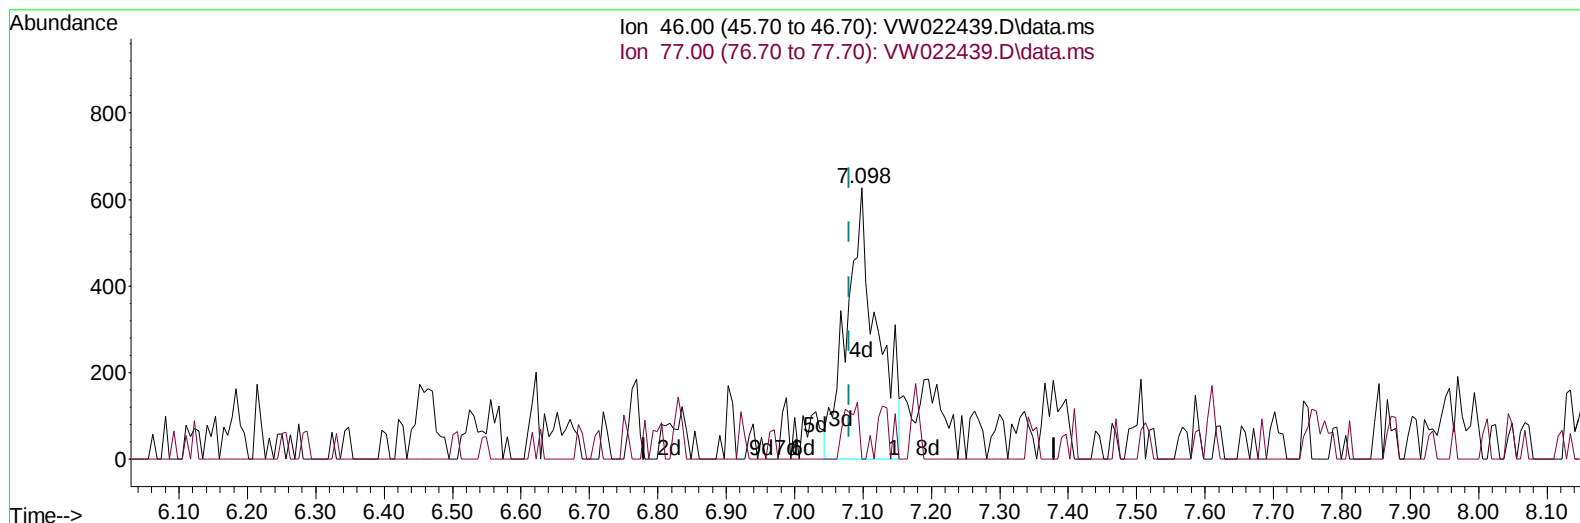

TIC: VW022439.D\data.ms

(21) 2-Butanone-d5 (S)

7.098min (+ 0.018) 39.42 ug/L m

response 1939

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	2.01#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022439.D
 Acq On : 07 Apr 2022 18:08
 Operator : SY/VA
 Sample : N2293-04
 Misc : 6.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:33:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	12745	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	10504	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	2542	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	7165	25.430	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	101.720%	
7) Chloroethane-d5	2.904	69	3675	20.812	ug/L	0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	83.240%	
11) 1,1-Dichloroethene-d2	4.031	63	6704	18.345	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	73.360%	
21) 2-Butanone-d5	7.098	46	1939m	39.418	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	78.840%	
24) Chloroform-d	7.659	84	9002	22.597	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	90.400%	
26) 1,2-Dichloroethane-d4	8.311	65	5500	24.164	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	96.640%	
32) Benzene-d6	8.281	84	16177	25.208	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	100.840%	
36) 1,2-Dichloropropane-d6	9.281	67	4960	26.707	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	106.840%	
41) Toluene-d8	10.317	98	13571	21.592	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	86.360%	
43) trans-1,3-Dichloroprop...	10.585	79	1704	19.442	ug/L	0.01
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.760%	
47) 2-Hexanone-d5	10.927	63	1666m	48.216	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.440%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	2523	15.977	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	63.920%	
66) 1,2-Dichlorobenzene-d4	13.859	152	2079	23.090	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.360%	
Target Compounds						
33) Benzene	8.329	78	16680	23.389	ug/L	Qvalue 100
34) Trichloroethene	9.085	95	766m	4.012	ug/L	
42) Toluene	10.390	91	2650	3.243	ug/L #	65
51) Chlorobenzene	11.658	112	77925	156.044	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022439.D
Acq On : 07 Apr 2022 18:08
Operator : SY/VA
Sample : N2293-04
Misc : 6.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNN4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:33:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

