




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022444.D
 Acq On : 07 Apr 2022 20:08
 Operator : SY/VA
 Sample : N2293-09
 Misc : 6.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:34:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

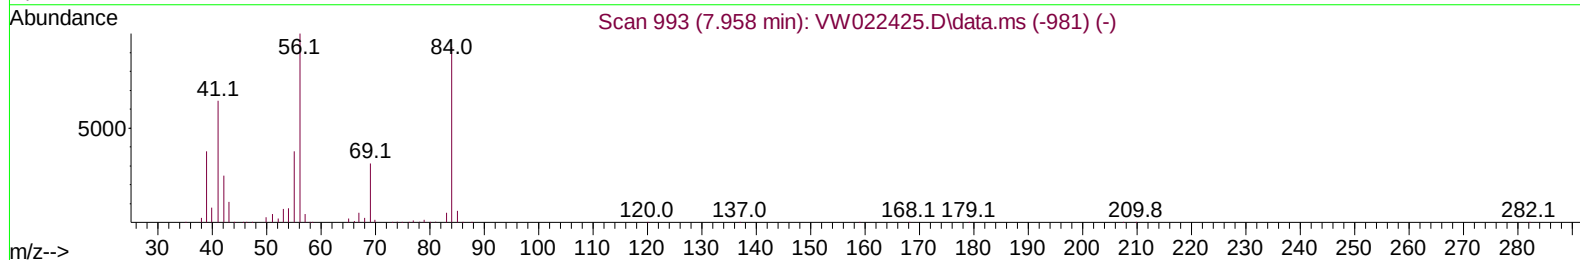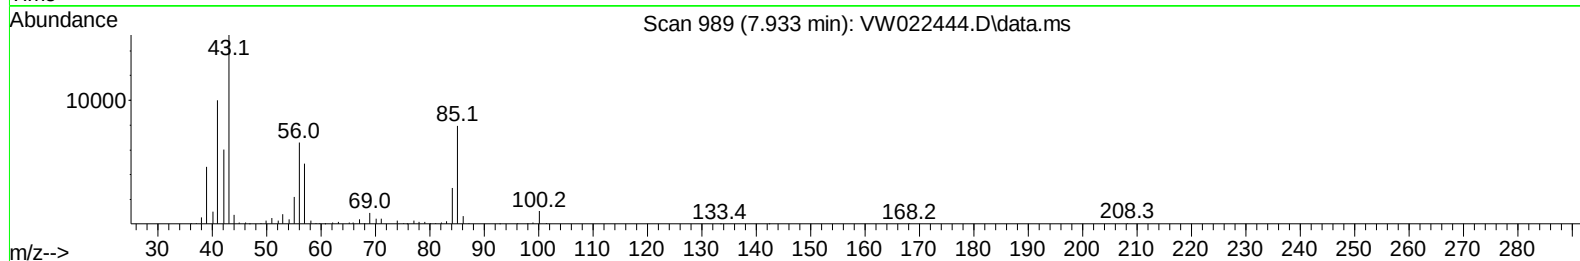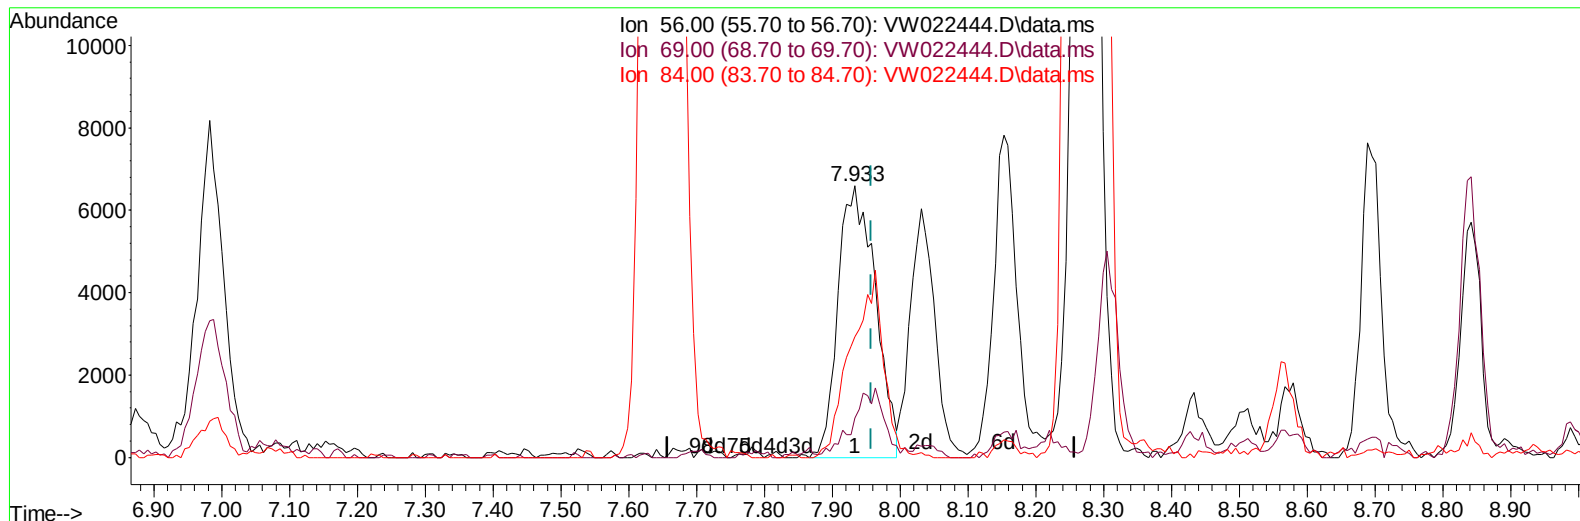

TIC: VW022444.D\data.ms

(29) Cyclohexane (T)

7.933min (-0.024) 2.11 ug/L

response 25144

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	30.50	7.92#
84.00	90.70	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022444.D
 Acq On : 07 Apr 2022 20:08
 Operator : SY/VA
 Sample : N2293-09
 Misc : 6.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:34:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

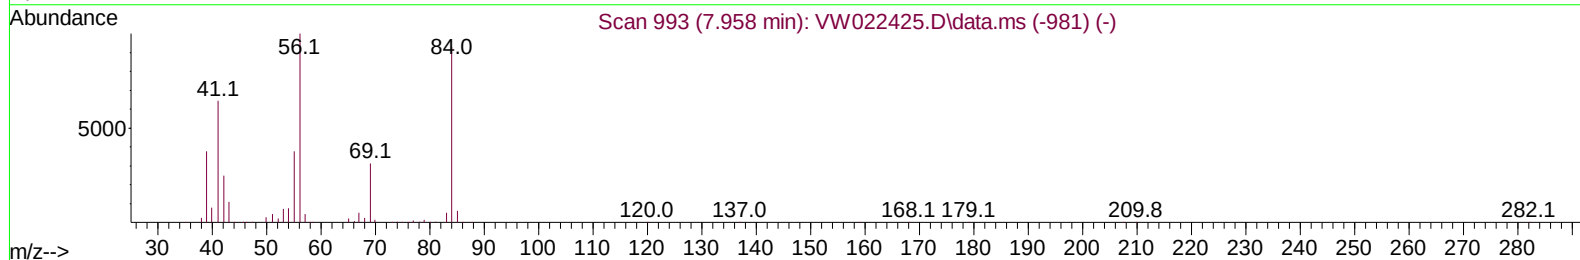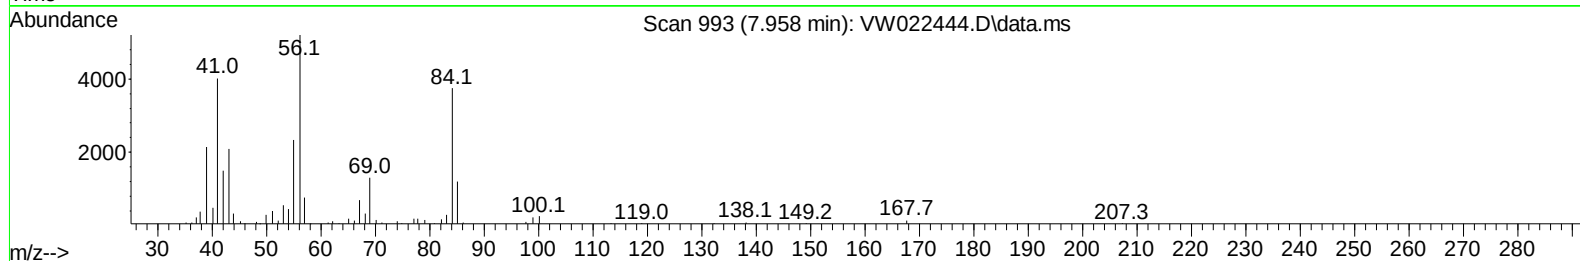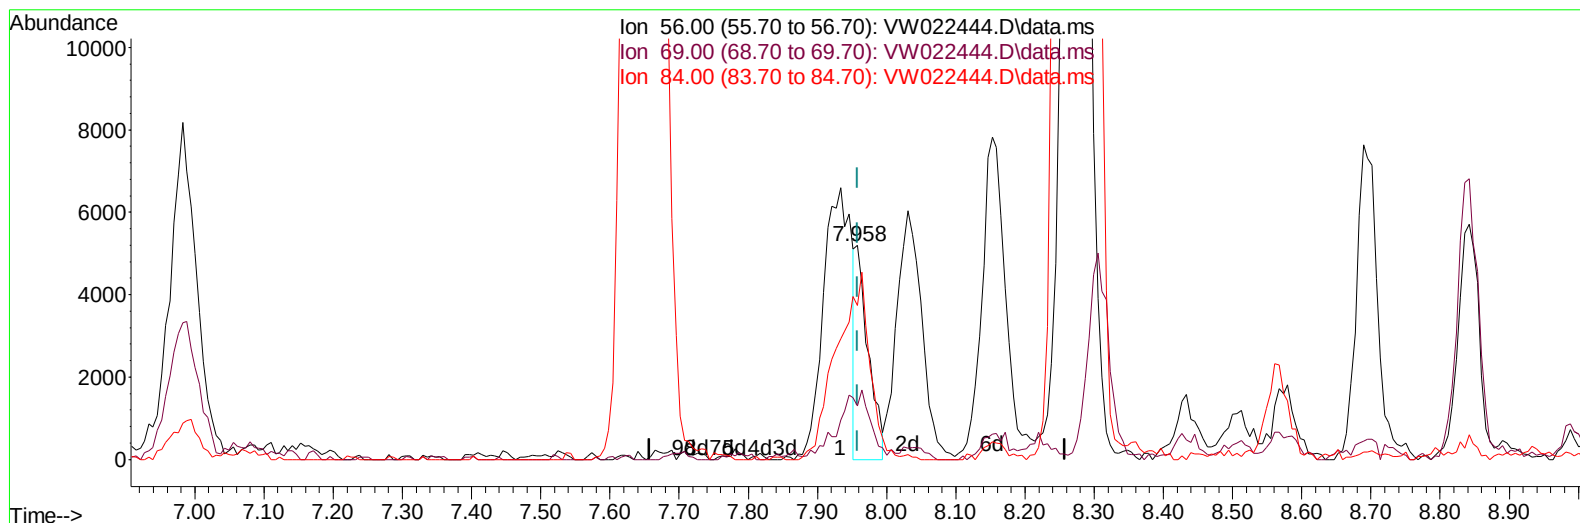

TIC: VW022444.D\data.ms

(29) Cyclohexane (T)

7.958min (-0.000) 0.56 ug/L m

response 6625

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	30.50	30.05
84.00	90.70	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022444.D
 Acq On : 07 Apr 2022 20:08
 Operator : SY/VA
 Sample : N2293-09
 Misc : 6.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN9

Manual IntegrationsAPPROVED

Quant Time: Apr 08 06:34:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	391807	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	415977	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	188380	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	167300	19.315	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.240%	
7) Chloroethane-d5	2.885	69	102374	18.859	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.440%	
11) 1,1-Dichloroethene-d2	4.013	63	150492	13.396	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	53.600%	
21) 2-Butanone-d5	7.080	46	92091	60.898	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	121.800%	
24) Chloroform-d	7.647	84	281058	22.950	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.800%	
26) 1,2-Dichloroethane-d4	8.305	65	178063	25.448	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	101.800%	
32) Benzene-d6	8.275	84	525918	20.694	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.760%	
36) 1,2-Dichloropropane-d6	9.274	67	170674	23.206	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	92.840%	
41) Toluene-d8	10.323	98	489379	19.661	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	78.640%	
43) trans-1,3-Dichloroprop...	10.579	79	73153	21.076	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.320%	
47) 2-Hexanone-d5	10.921	63	99277	72.552	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	145.100%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	163469	26.140	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	104.560%	
66) 1,2-Dichlorobenzene-d4	13.847	152	172676	25.879	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	103.520%	
Target Compounds						
						Qvalue
13) Acetone	4.123	43	196725	191.068	ug/L	98
14) Carbon disulfide	4.385	76	50567	2.914	ug/L	96
22) 2-Butanone	7.177	43	35997	23.149	ug/L	99
27) 1,2-Dichloroethane	8.403	62	96125	11.516	ug/L	98
29) Cyclohexane	7.958	56	6625m	0.556	ug/L	
33) Benzene	8.323	78	2786624	98.669	ug/L	100
35) Methylcyclohexane	9.335	83	13138	0.968	ug/L	91
37) 1,2-Dichloropropane	9.366	63	2952	0.436	ug/L #	87
40) 4-Methyl-2-pentanone	10.201	43	11335	2.745	ug/L	98
42) Toluene	10.384	91	400058	12.362	ug/L	95
48) 2-Hexanone	10.969	43	14857	5.100	ug/L	94
51) Chlorobenzene	11.658	112	10036384	507.495	ug/L	96
53) m,p-Xylene	11.829	106	12908	0.936	ug/L	89
54) o-Xylene	12.164	106	9903	0.751	ug/L	84
62) 1,3,5-Trimethylbenzene	12.932	105	5540	0.322	ug/L	93
63) 1,2,4-Trimethylbenzene	13.243	105	13391	0.512	ug/L	97
65) 1,4-Dichlorobenzene	13.572	146	18508	1.461	ug/L	97
67) 1,2-Dichlorobenzene	13.865	146	168448	14.831	ug/L	95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022444.D
 Acq On : 07 Apr 2022 20:08
 Operator : SY/VA
 Sample : N2293-09
 Misc : 6.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:34:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022444.D
Acq On : 07 Apr 2022 20:08
Operator : SY/VA
Sample : N2293-09
Misc : 6.00g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNN9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:34:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

