

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022427.D
 Acq On : 07 Apr 2022 13:19
 Operator : SY/VA
 Sample : N2262-09
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	347591	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	324945	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	143531	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	156063	20.310	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.240%		
7) Chloroethane-d5	2.891	69	91137	18.924	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.680%		
11) 1,1-Dichloroethene-d2	4.019	63	143347	14.383	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.520%		
21) 2-Butanone-d5	7.074	46	71465	53.270	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.540%		
24) Chloroform-d	7.647	84	250878	23.092	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.360%		
26) 1,2-Dichloroethane-d4	8.305	65	152814m	24.617	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	98.480%		
32) Benzene-d6	8.274	84	464679	23.406	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	93.640%		
36) 1,2-Dichloropropane-d6	9.274	67	145258	25.283	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.120%		
41) Toluene-d8	10.323	98	435815	22.414	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	89.640%		
43) trans-1,3-Dichloroprop...	10.579	79	63468	23.408	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	93.640%		
47) 2-Hexanone-d5	10.920	63	56810	53.148	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.300%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	118982	24.356	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	97.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152	128749	25.325	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	101.280%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	5932m	6.494	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022427.D
Acq On : 07 Apr 2022 13:19
Operator : SY/VA
Sample : N2262-09
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW6L3

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022


Quant Time: Apr 08 06:31:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

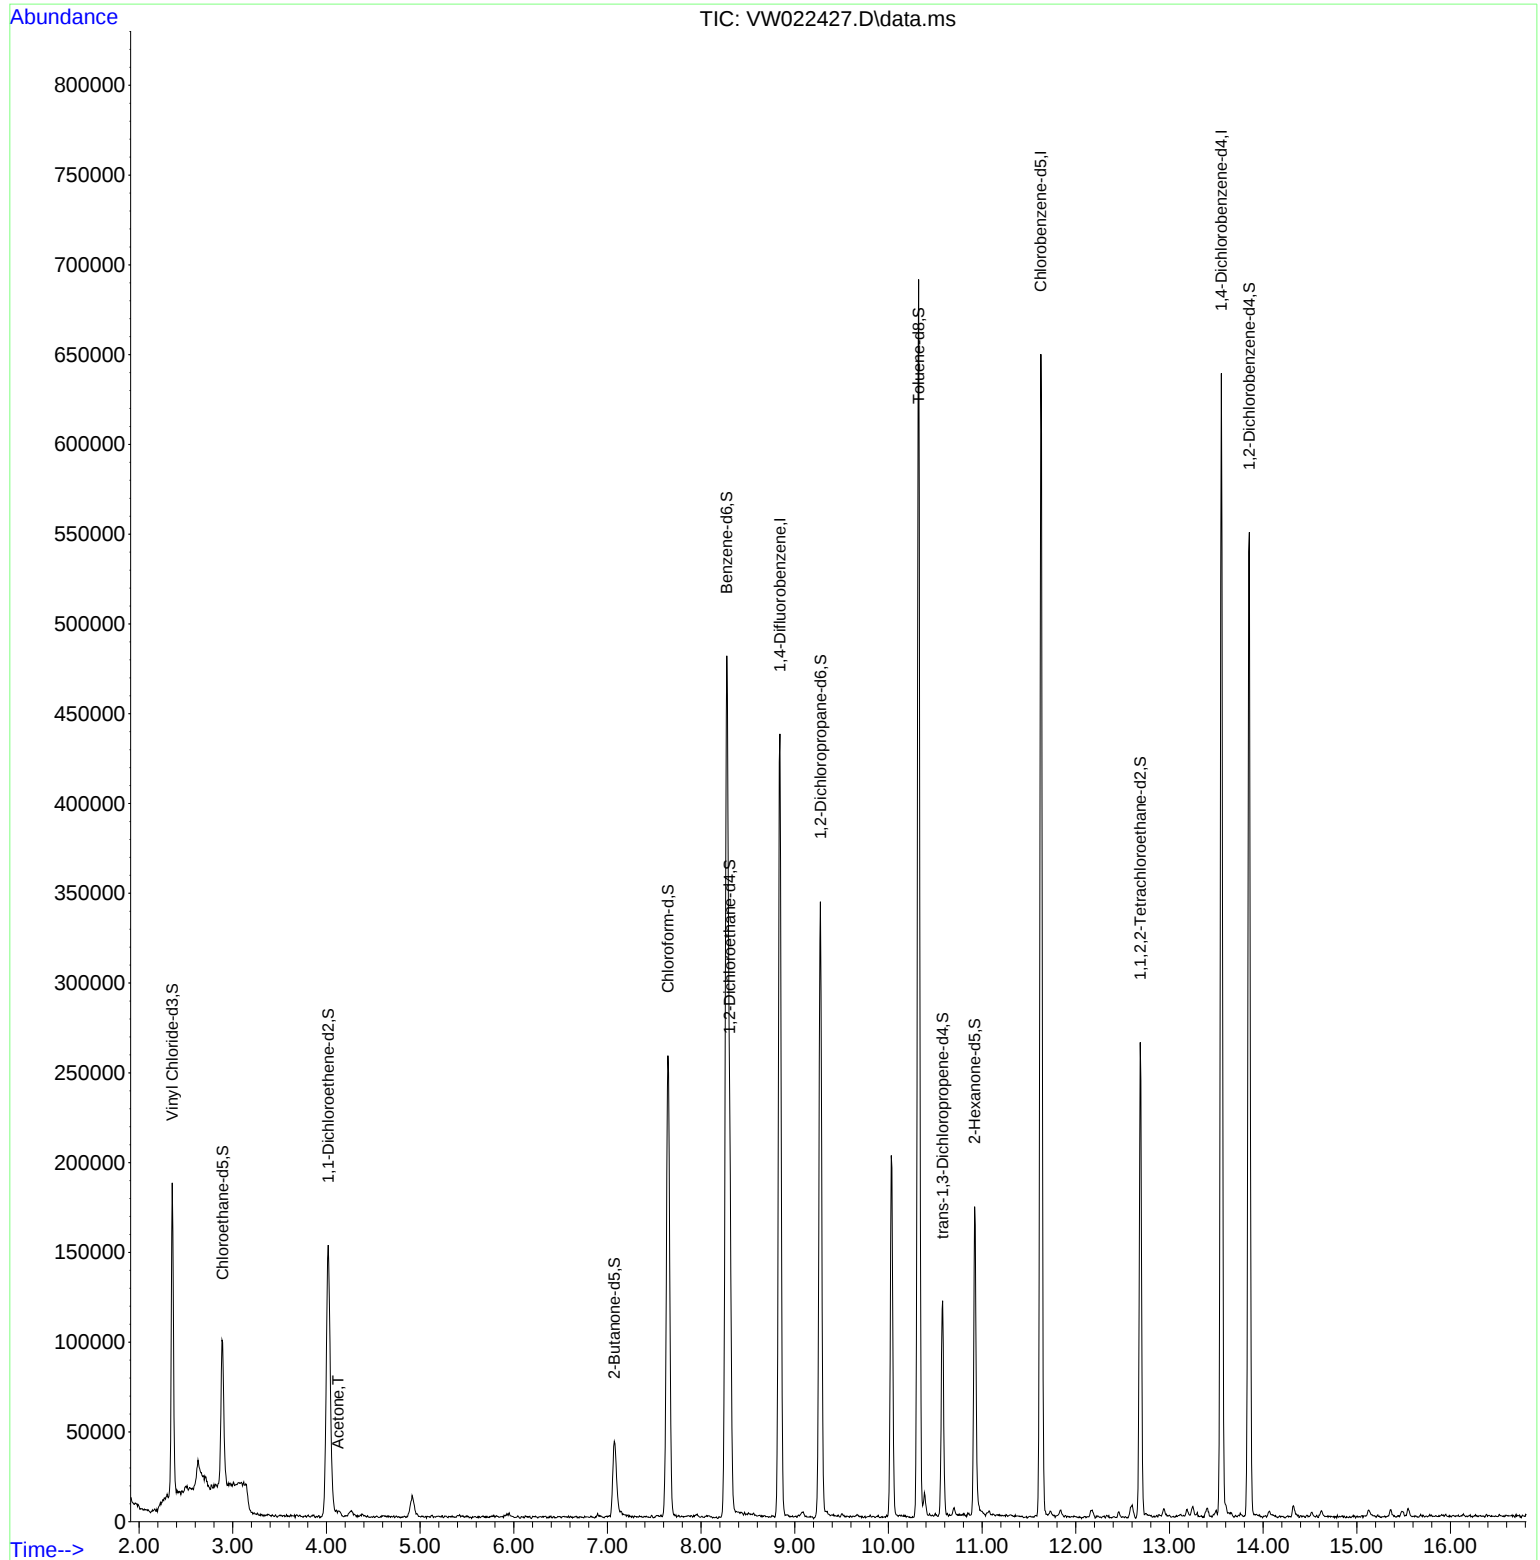

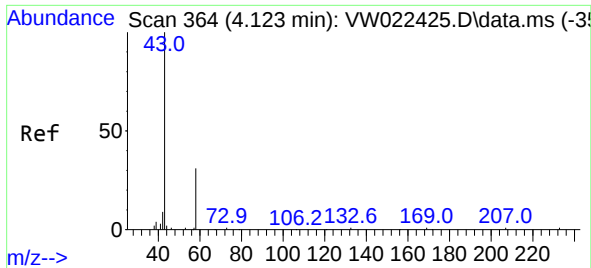

#13
Acetone
Concen: 6.494 ug/L m
RT: 4.123 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW022427.D
Acq: 07 Apr 2022 13:19

Instrument :
MSVOA_W
ClientSampleId :
EW6L3

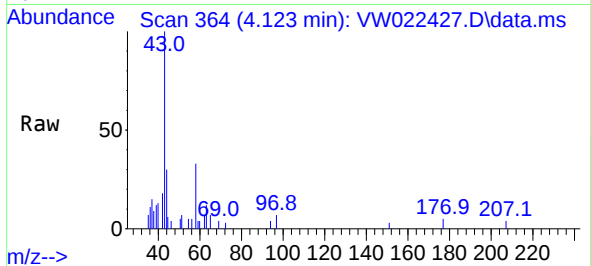

Tgt Ion: 43 Resp: 593
Ion Ratio Lower Upper
43 100
58 30.0 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

