

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022429.D
 Acq On : 07 Apr 2022 14:07
 Operator : SY/VA
 Sample : N2262-15
 Misc : 4.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:31:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	311094	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	313713	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	159659	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	144595	21.025	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.080%
7) Chloroethane-d5	2.891	69	93235	21.631	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.520%
11) 1,1-Dichloroethene-d2	4.019	63	125247	14.041	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.160%
21) 2-Butanone-d5	7.074	46	87536	72.905	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	145.800%#
24) Chloroform-d	7.647	84	229278	23.579	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.320%
26) 1,2-Dichloroethane-d4	8.305	65	149986	26.996	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.000%
32) Benzene-d6	8.275	84	426041	22.228	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.920%
36) 1,2-Dichloropropane-d6	9.274	67	134639	24.274	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.080%
41) Toluene-d8	10.323	98	398463	21.227	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.920%
43) trans-1,3-Dichloroprop...	10.579	79	62861	24.014	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.040%
47) 2-Hexanone-d5	10.920	63	70593	68.407	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	136.820%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	135525	28.736	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	140522	24.849	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.400%
Target Compounds					Qvalue	
13) Acetone	4.141	43	4477m	5.476	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022429.D
Acq On : 07 Apr 2022 14:07
Operator : SY/VA
Sample : N2262-15
Misc : 4.79g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW6L5

Quant Time: Apr 08 06:31:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 04/09/2022
Supervised By : Mahesh Dadoda 04/11/2022

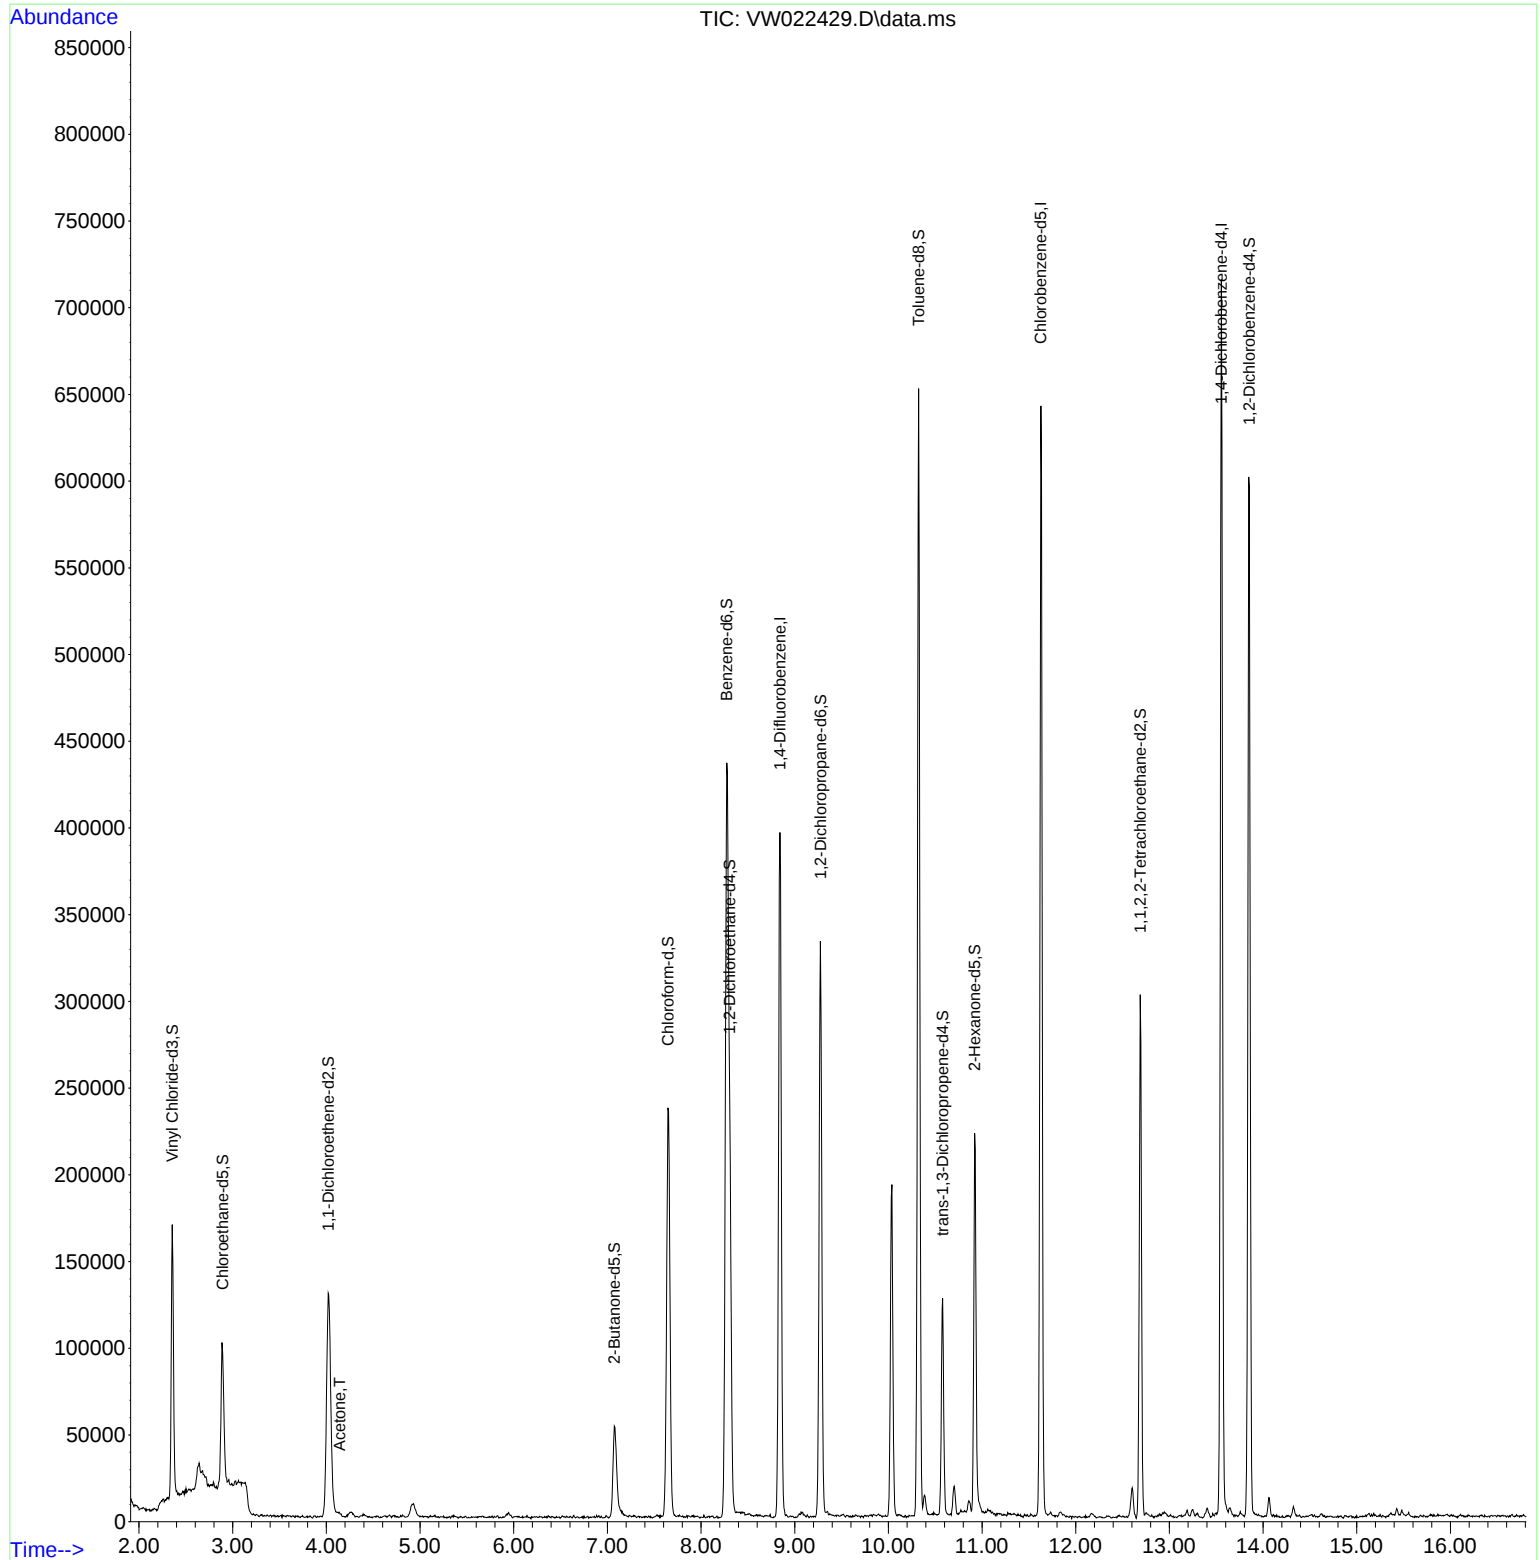

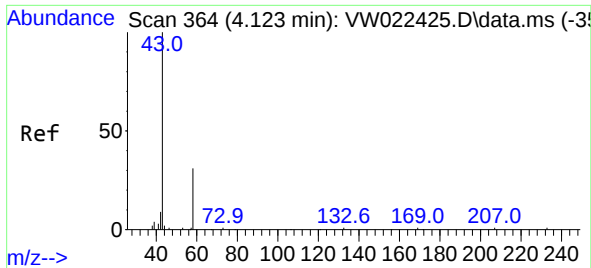

#13
Acetone
Concen: 5.476 ug/L m
RT: 4.141 min Scan# 30
Delta R.T. 0.018 min
Lab File: VW022429.D
Acq: 07 Apr 2022 14:07

Instrument :
MSVOA_W
ClientSampleId :
EW6L5

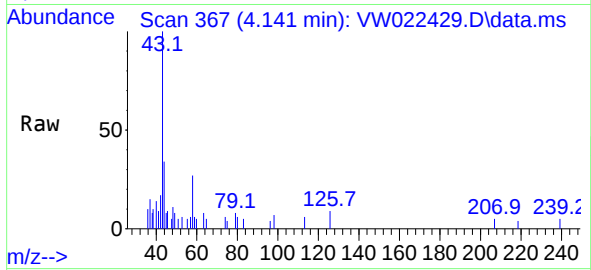

Tgt Ion: 43 Resp: 447
Ion Ratio Lower Upper
43 100
58 2.1 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

