

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022434.D
 Acq On : 07 Apr 2022 16:08
 Operator : SY/VA
 Sample : N2262-20
 Misc : 6.46g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6M0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:32:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	344006	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	333849	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	158563	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	164385	21.616	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.480%
7) Chloroethane-d5	2.885	69	111676	23.431	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.720%
11) 1,1-Dichloroethene-d2	4.013	63	142309	14.427	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.720%
21) 2-Butanone-d5	7.080	46	93993	70.793	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	141.580%#
24) Chloroform-d	7.647	84	256105	23.818	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.280%
26) 1,2-Dichloroethane-d4	8.305	65	167175m	27.211	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.840%
32) Benzene-d6	8.275	84	477934	23.432	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.720%
36) 1,2-Dichloropropane-d6	9.274	67	150443	25.487	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.960%
41) Toluene-d8	10.323	98	446116	22.332	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.320%
43) trans-1,3-Dichloroprop...	10.579	79	67529	24.241	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.960%
47) 2-Hexanone-d5	10.920	63	77890	70.925	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	141.860%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	142999	28.492	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	138551	24.669	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.680%
Target Compounds					Qvalue	
13) Acetone	4.129	43	7018	7.763	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
Data File : VW022434.D
Acq On : 07 Apr 2022 16:08
Operator : SY/VA
Sample : N2262-20
Misc : 6.46g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW6M0

Quant Time: Apr 08 06:32:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 04/09/2022
Supervised By : Mahesh Dadoda 04/11/2022

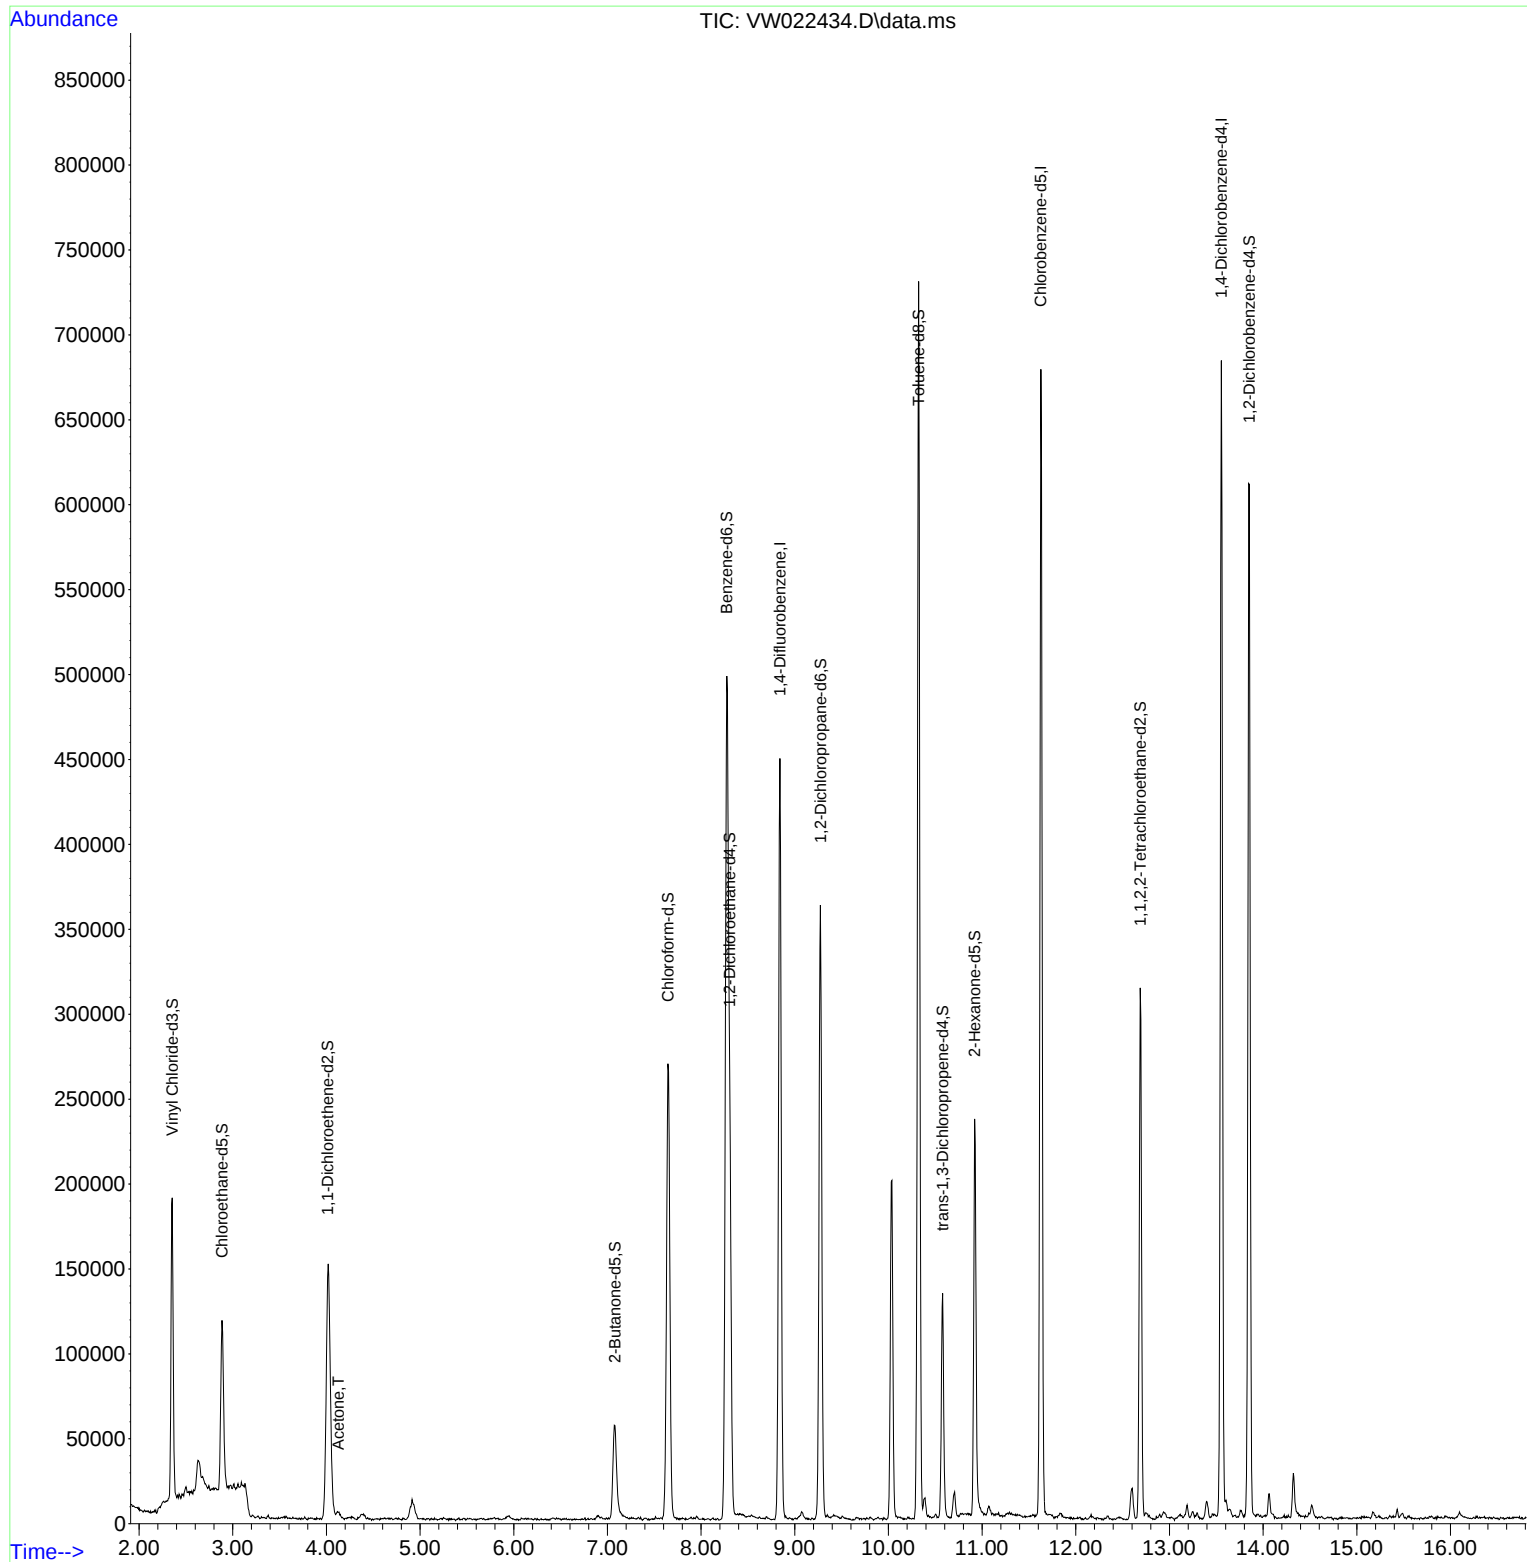

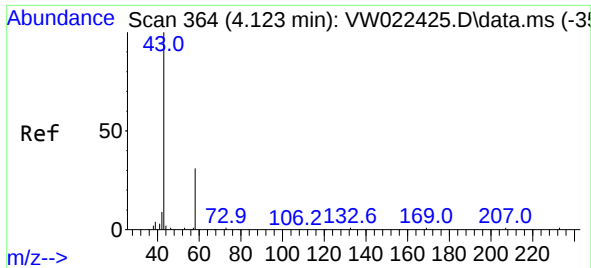

#13
Acetone
Concen: 7.763 ug/L
RT: 4.129 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW022434.D
Acq: 07 Apr 2022 16:08

Instrument :
MSVOA_W
ClientSampleId :
EW6M0

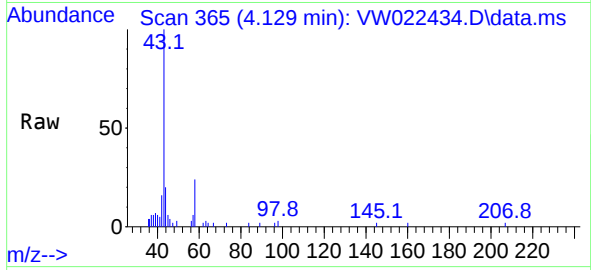

Tgt Ion: 43 Resp: 7018
Ion Ratio Lower Upper
43 100
58 20.6 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

