

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040722\
 Data File : VW022440.D
 Acq On : 07 Apr 2022 18:32
 Operator : SY/VA
 Sample : N2293-05
 Misc : 6.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNN5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 06:33:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 06:30:01 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	353097	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	353393	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	174994	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	144332	18.490	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.960%		
7) Chloroethane-d5	2.891	69	95580	19.538	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.160%		
11) 1,1-Dichloroethene-d2	4.019	63	117319	11.588	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	46.360%		
21) 2-Butanone-d5	7.080	46	74621	54.755	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	109.520%		
24) Chloroform-d	7.647	84	222168	20.130	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.520%		
26) 1,2-Dichloroethane-d4	8.305	65	145668m	23.100	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.400%		
32) Benzene-d6	8.275	84	415179	19.229	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.920%		
36) 1,2-Dichloropropane-d6	9.274	67	132925	21.274	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	85.080%		
41) Toluene-d8	10.323	98	390126	18.449	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	73.800%		
43) trans-1,3-Dichloroprop...	10.579	79	57679	19.560	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	78.240%		
47) 2-Hexanone-d5	10.920	63	61857	53.211	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.420%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	119735	22.537	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	90.160%		
66) 1,2-Dichlorobenzene-d4	13.847	152	138426	22.333	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.320%		
Target Compounds						Qvalue
13) Acetone	4.129	43	22228	23.956	ug/L	89
14) Carbon disulfide	4.385	76	74981	4.794	ug/L	96
20) cis-1,2-Dichloroethene	7.171	96	5188	0.882	ug/L #	85
25) Chloroform	7.671	83	6794	0.635	ug/L	88
27) 1,2-Dichloroethane	8.409	62	4194	0.558	ug/L #	77
33) Benzene	8.323	78	742104	30.930	ug/L	100
42) Toluene	10.384	91	132433	4.817	ug/L	98
51) Chlorobenzene	11.658	112	1908584	113.600	ug/L	97
52) Ethylbenzene	11.731	91	18055	0.586	ug/L #	84
53) m,p-Xylene	11.835	106	17382	1.483	ug/L	97
54) o-Xylene	12.164	106	11266	1.006	ug/L	95
62) 1,3,5-Trimethylbenzene	12.938	105	12043	0.753	ug/L	96
63) 1,2,4-Trimethylbenzene	13.249	105	25904	1.066	ug/L	100
67) 1,2-Dichlorobenzene	13.865	146	26070	2.471	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations APPROVED


Quant Time: Apr 08 06:33:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 06:30:01 2022
Response via : Initial Calibration





#13
Acetone
Concen: 23.956 ug/L
RT: 4.129 min Scan# 364
Delta R.T. 0.006 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32




Instrument :
MSVOA_W
ClientSampleId :
ETNN5

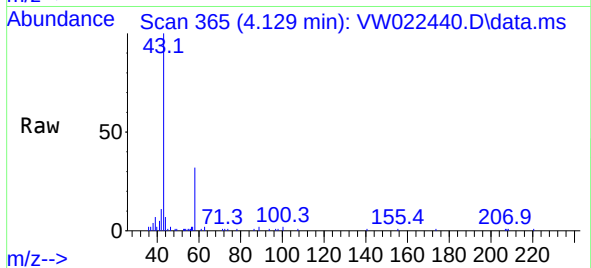


Tgt Ion: 43 Resp: 22228
Ion Ratio Lower Upper
43 100
58 34.3 0.0 57.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

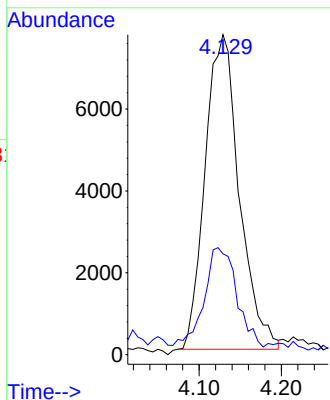


#14
Carbon disulfide
Concen: 4.794 ug/L
RT: 4.385 min Scan# 407
Delta R.T. -0.006 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32




Tgt Ion: 76 Resp: 74981
Ion Ratio Lower Upper
76 100
78 10.9 7.6 11.4

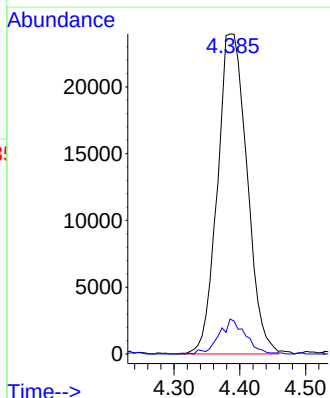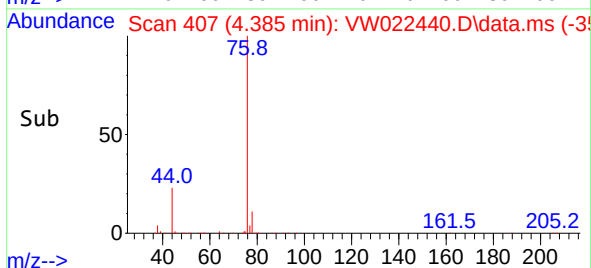



#20
cis-1,2-Dichloroethene
Concen: 0.882 ug/L
RT: 7.171 min Scan# 864
Delta R.T. -0.000 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32




Instrument :
MSVOA_W
ClientSampleId :
ETNN5



Tgt Ion: 96 Resp: 518
Ion Ratio Lower Upper
96 100
61 119.4 96.4 179.0
68 0.0 0.1 0.3




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

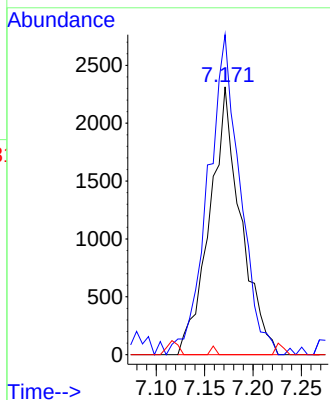

#25
Chloroform
Concen: 0.635 ug/L
RT: 7.671 min Scan# 946
Delta R.T. -0.006 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32

Tgt Ion: 83 Resp: 6794
Ion Ratio Lower Upper
83 100
85 75.1 45.8 85.0

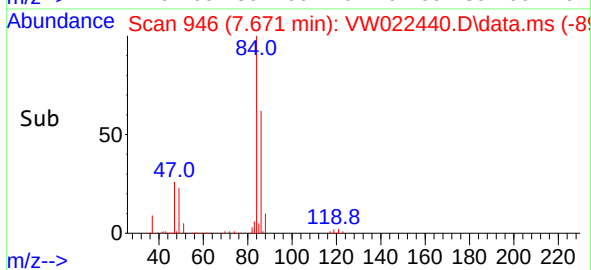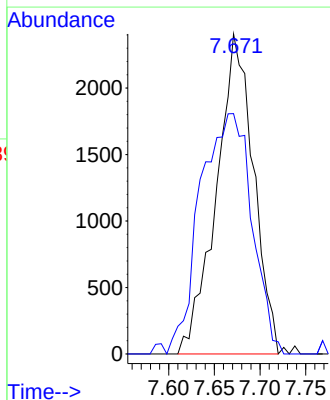

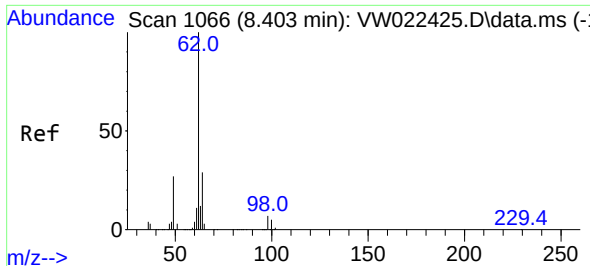

#27

1,2-Dichloroethane

Concen: 0.558 ug/L

RT: 8.409 min Scan# 1066

Delta R.T. 0.006 min

Lab File: VW022440.D

Acq: 07 Apr 2022 18:32

Instrument :

MSVOA_W

ClientSampleId :

ETNN5

Tgt Ion: 62 Resp: 4194

Ion Ratio Lower Upper

62 100





98 15.6 6.2 9.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022

Supervised By :Mahesh Dadoda 04/11/2022

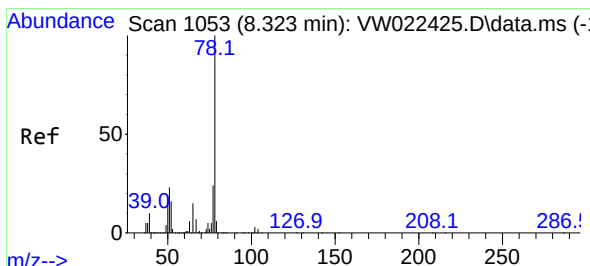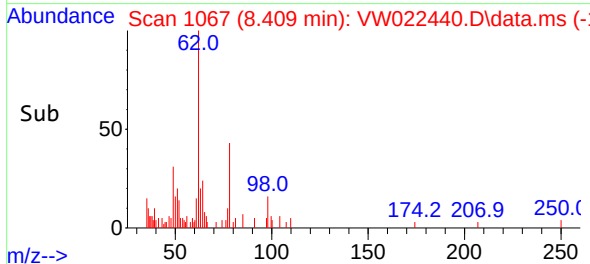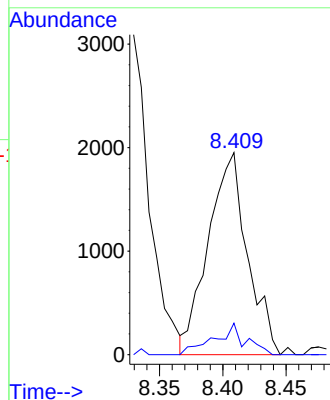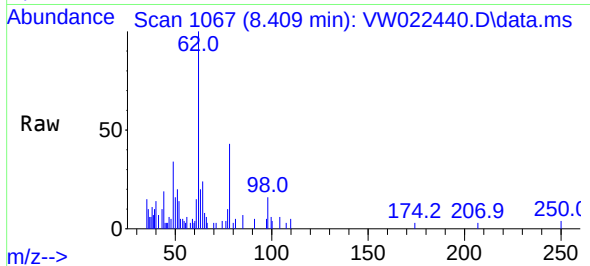

#33

Benzene

Concen: 30.930 ug/L




RT: 8.323 min Scan# 1053


Delta R.T. -0.000 min

Lab File: VW022440.D

Acq: 07 Apr 2022 18:32


Tgt Ion: 78 Resp: 742104

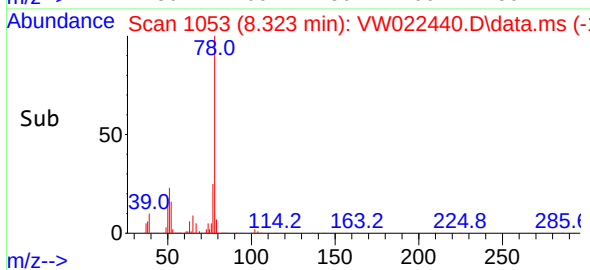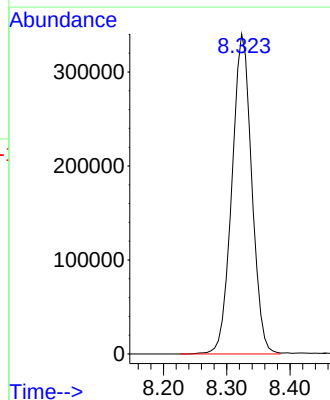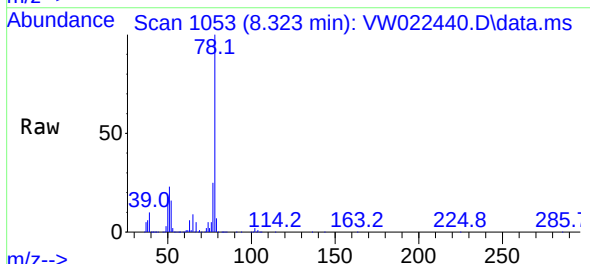



#42
Toluene
Concen: 4.817 ug/L
RT: 10.384 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32




Instrument :
MSVOA_W
ClientSampleId :
ETNN5




Tgt Ion: 91 Resp: 13243
Ion Ratio Lower Upper
91 100
92 55.7 38.0 70.6

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

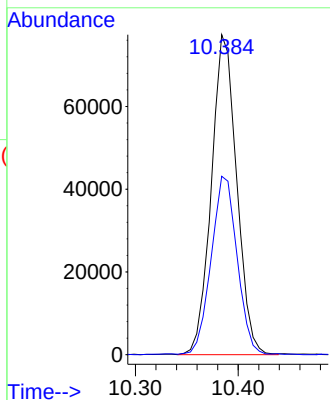


#51
Chlorobenzene
Concen: 113.600 ug/L
RT: 11.658 min Scan# 1600
Delta R.T. 0.006 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32




Tgt Ion:112 Resp: 1908584
Ion Ratio Lower Upper
112 100
114 32.4 20.5 38.1
77 58.8 48.1 72.1

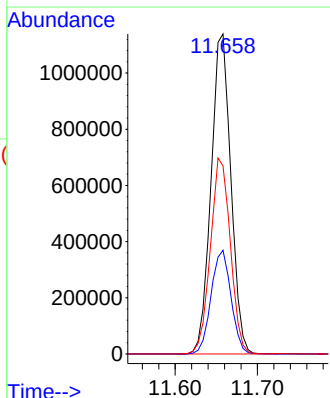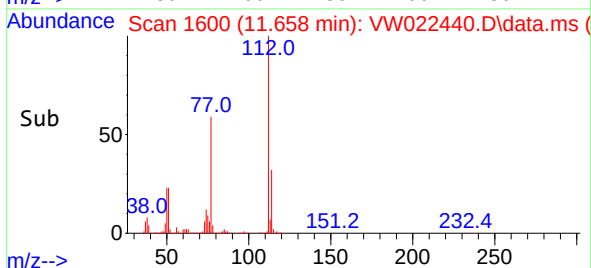



#52
Ethylbenzene
Concen: 0.586 ug/L
RT: 11.731 min Scan# 1611
Delta R.T. 0.006 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32




Instrument :
MSVOA_W
ClientSampleId :
ETNN5




Tgt Ion: 91 Resp: 1805
Ion Ratio Lower Upper
91 100
106 38.1 20.5 38.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

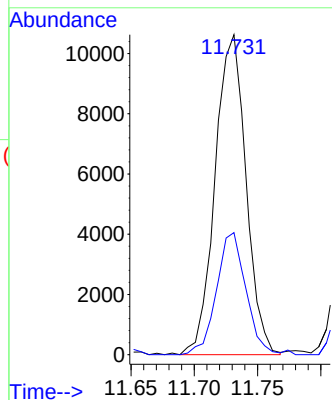


#53
m,p-Xylene
Concen: 1.483 ug/L
RT: 11.835 min Scan# 1629
Delta R.T. -0.000 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32




Tgt Ion:106 Resp: 17382
Ion Ratio Lower Upper
106 100
91 209.4 149.9 278.5

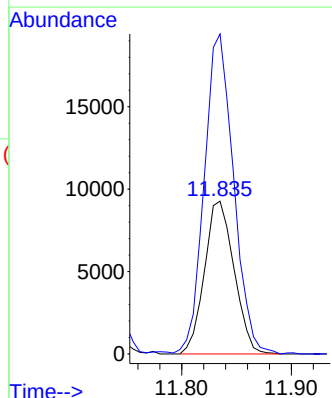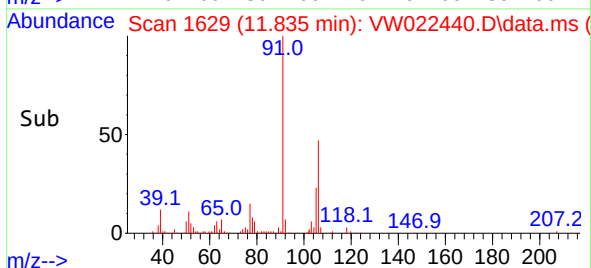



#54
o-Xylene
Concen: 1.006 ug/L
RT: 12.164 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32




Instrument :
MSVOA_W
ClientSampleId :
ETNN5




Tgt Ion:106 Resp: 1126
Ion Ratio Lower Upper
106 100
91 213.1 155.3 288.3

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

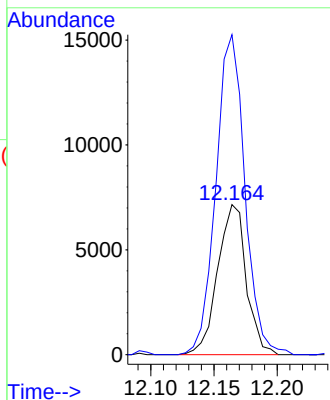


#62
1,3,5-Trimethylbenzene
Concen: 0.753 ug/L
RT: 12.938 min Scan# 1810
Delta R.T. -0.000 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32



Tgt Ion:105 Resp: 12043
Ion Ratio Lower Upper
105 100
120 44.5 37.5 56.3

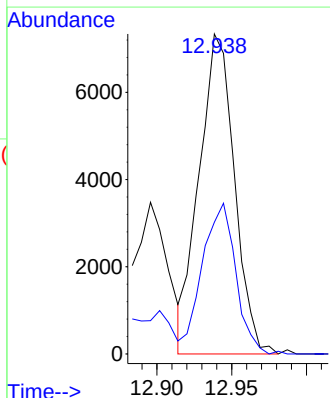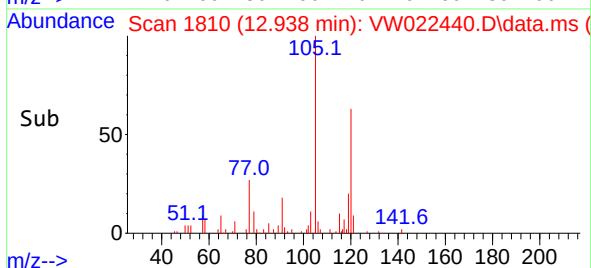







#63
1,2,4-Trimethylbenzene
Concen: 1.066 ug/L
RT: 13.249 min Scan# 1861
Delta R.T. -0.000 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32

Instrument :
MSVOA_W
ClientSampleId :
ETNN5

Tgt Ion:105 Resp: 25904
Ion Ratio Lower Upper
105 100
120 42.9 34.2 51.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

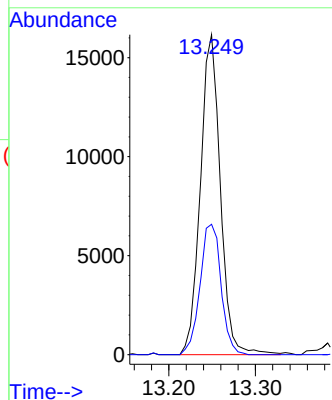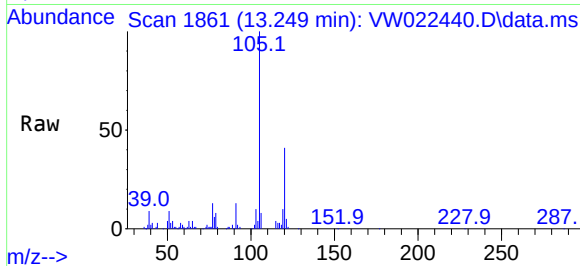

#67
1,2-Dichlorobenzene
Concen: 2.471 ug/L
RT: 13.865 min Scan# 1962
Delta R.T. -0.000 min
Lab File: VW022440.D
Acq: 07 Apr 2022 18:32

Tgt Ion:146 Resp: 26070
Ion Ratio Lower Upper
146 100
111 48.2 39.0 58.4
148 58.3 52.1 78.1

