

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009830.D
 Acq On : 09 Apr 2019 09:51
 Operator : SY/VA
 Sample : K2303-04
 Misc : 4.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF899

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:03:52 PM

Quant Time: Apr 10 02:46:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 00:56:07 2019
 Response via : Initial Calibration

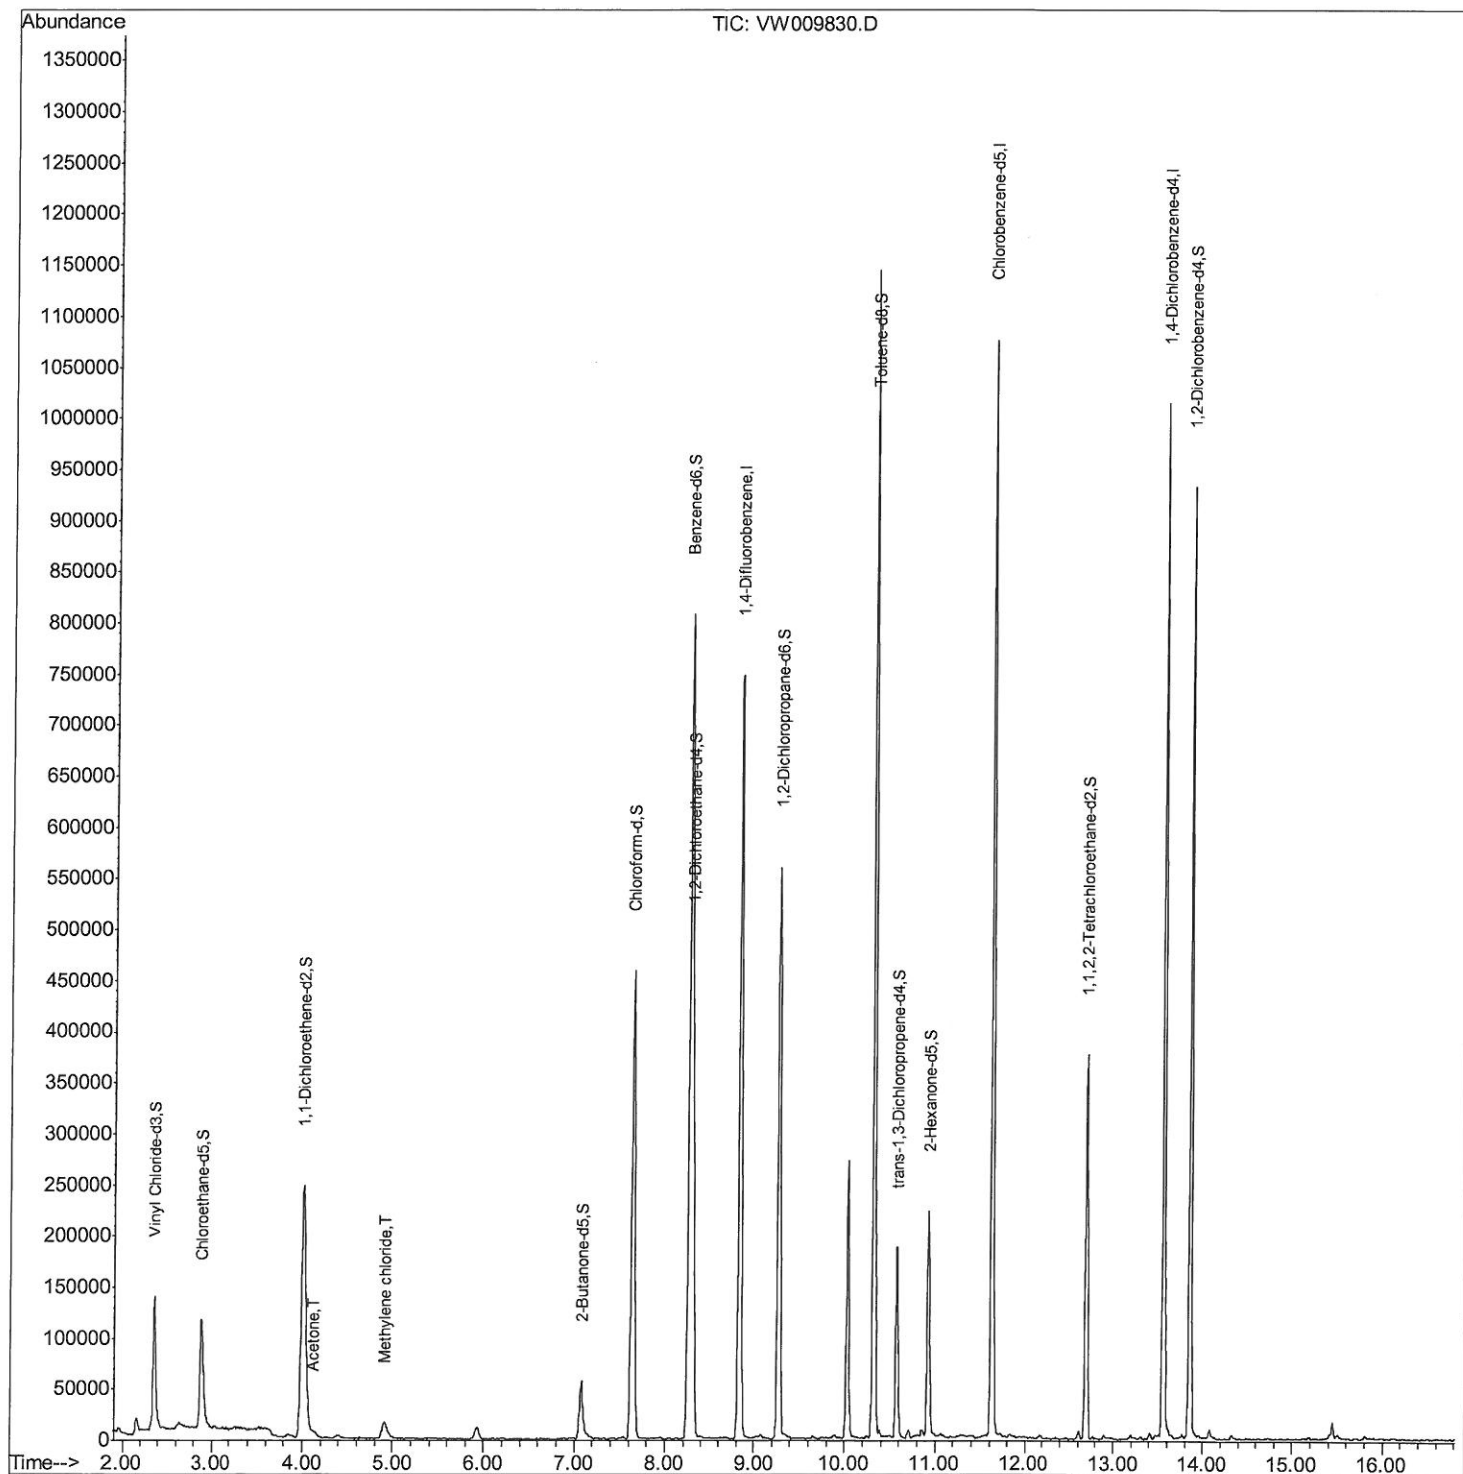

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009830.D
 Acq On : 09 Apr 2019 09:51
 Operator : SY/VA
 Sample : K2303-04
 Misc : 4.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF899

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:03:52 PM

Quant Time: Apr 10 01:00:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 00:56:07 2019
 Response via : Initial Calibration

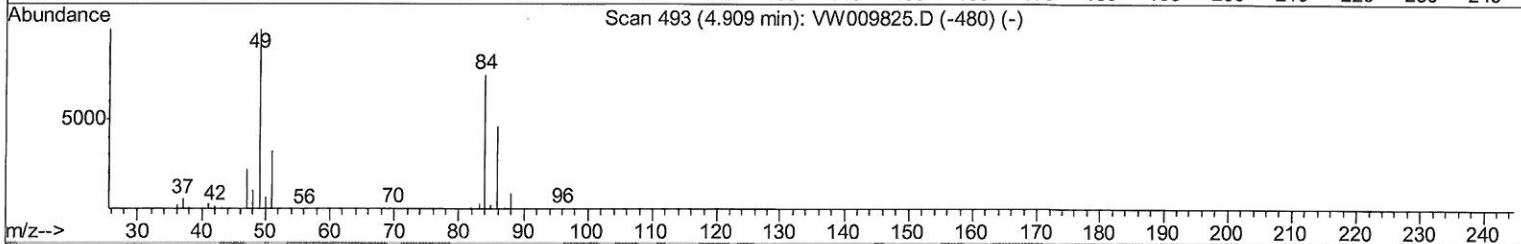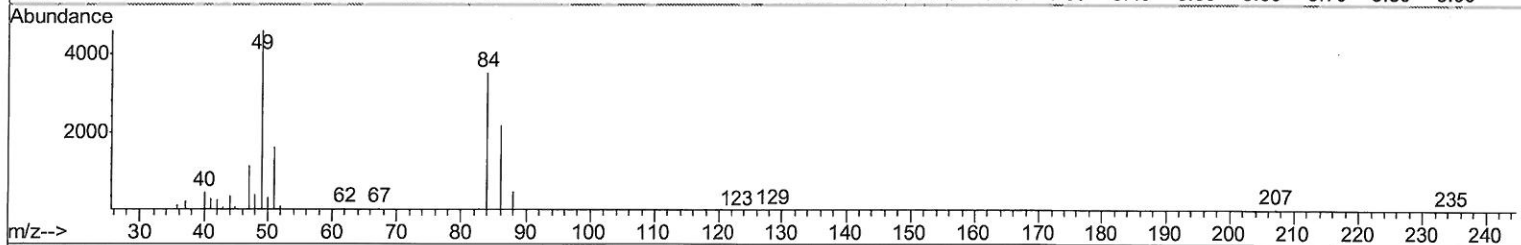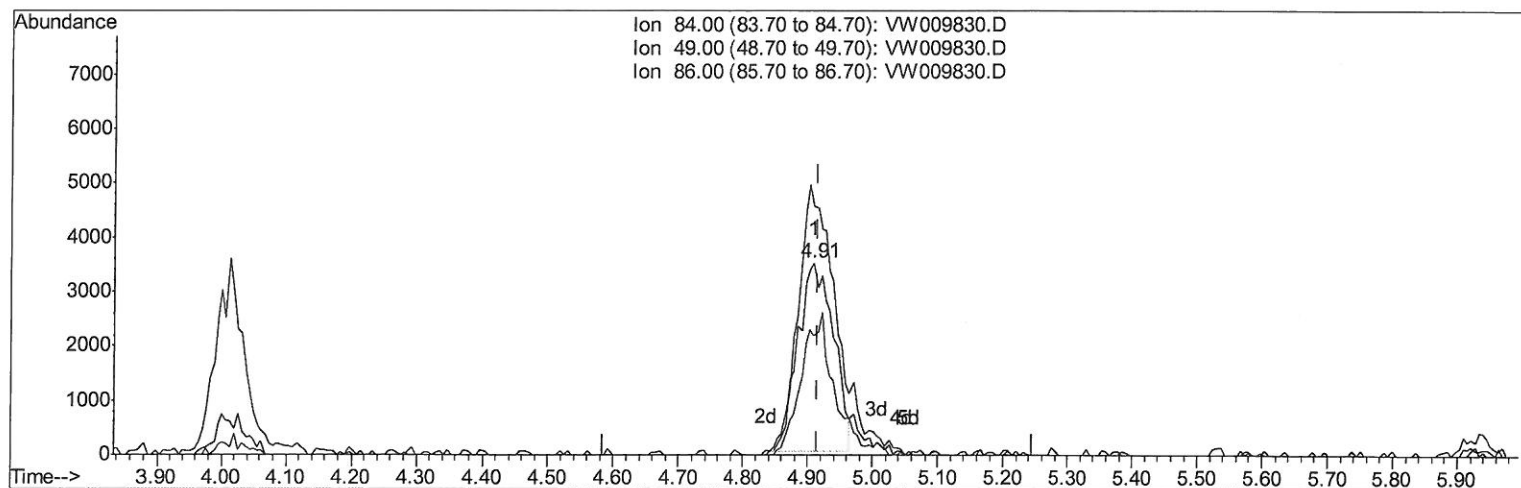

TIC: VW009830.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.29ug/L

response 13328

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	129.67
86.00	66.30	62.34
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009830.D
 Acq On : 09 Apr 2019 09:51
 Operator : SY/VA
 Sample : K2303-04
 Misc : 4.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF899

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:03:52 PM

Quant Time: Apr 10 01:00:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 00:56:07 2019
 Response via : Initial Calibration

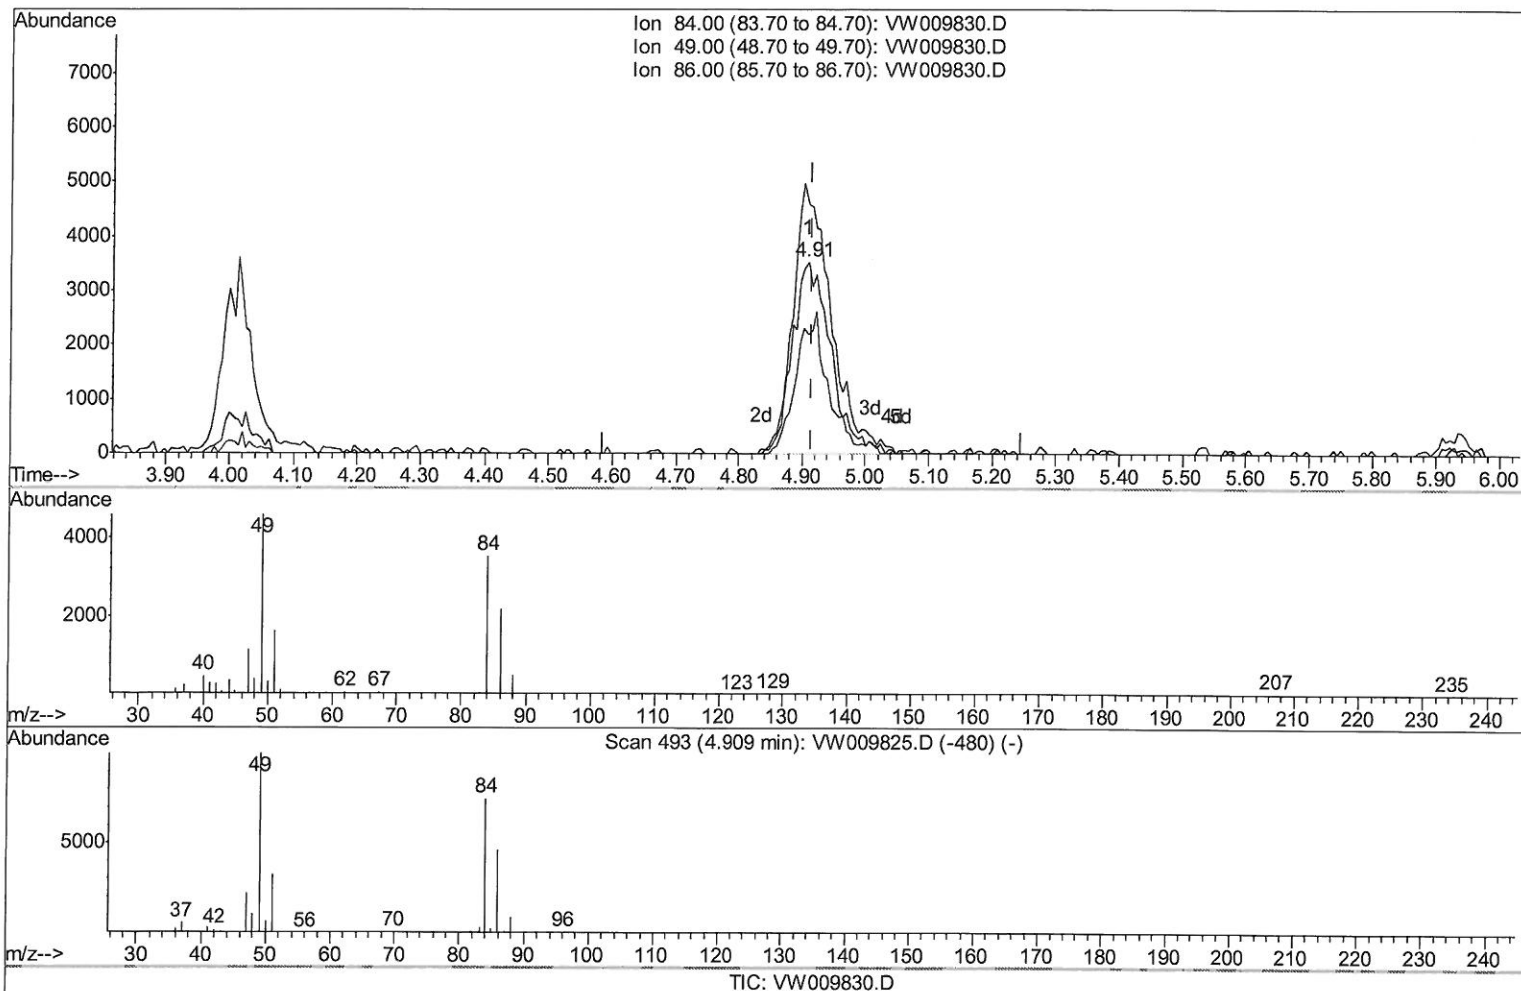

(16) Methylene chloride (T)

4.909min (-0.006) 1.45ug/L m

response 14916

7 MD
 4/11/19

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	129.67
86.00	66.30	62.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009830.D
 Acq On : 09 Apr 2019 09:51
 Operator : SY/VA
 Sample : K2303-04
 Misc : 4.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF899

Quant Time: Apr 10 01:00:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 00:56:07 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:03:52 PM

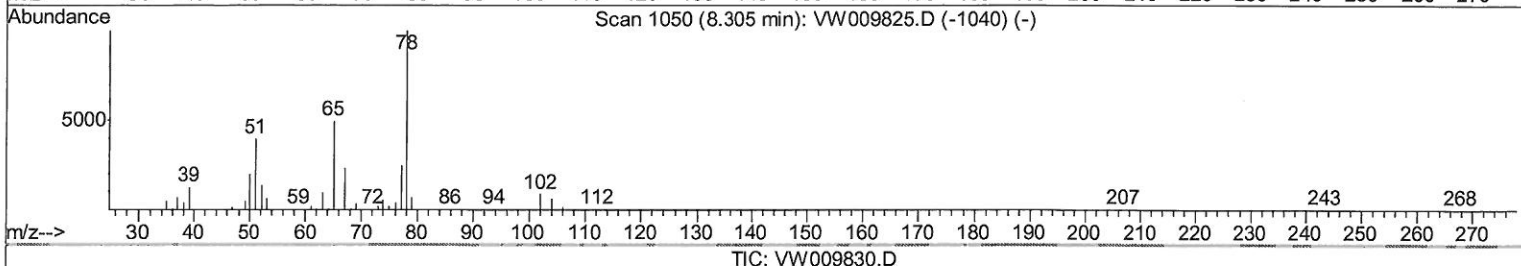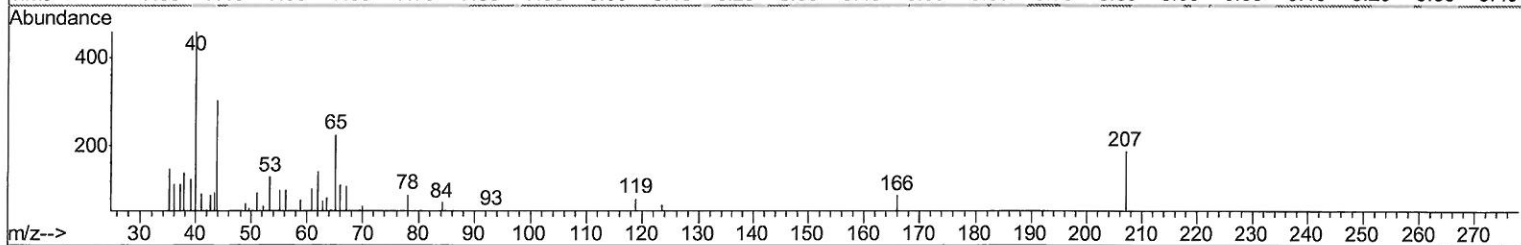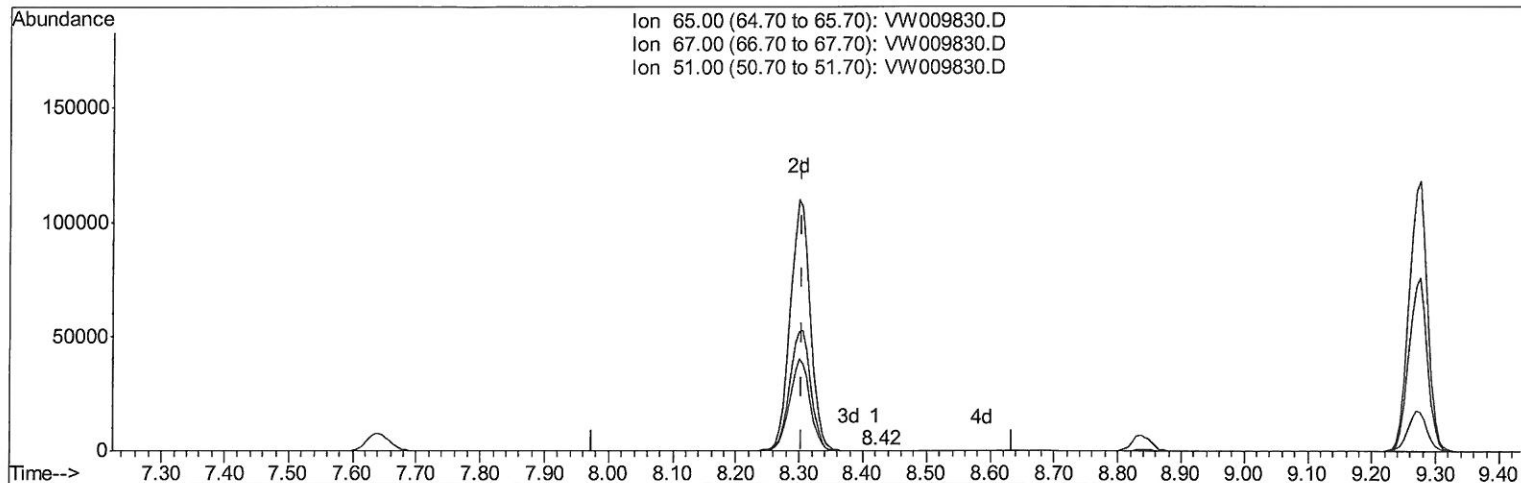

(26) 1,2-Dichloroethane-d4 (S)

8.421min (+0.116) 0.02ug/L

response 156

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	47.44
51.00	109.90	130.77
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009830.D
 Acq On : 09 Apr 2019 09:51
 Operator : SY/VA
 Sample : K2303-04
 Misc : 4.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF899

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:03:52 PM

Quant Time: Apr 10 01:00:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 00:56:07 2019
 Response via : Initial Calibration

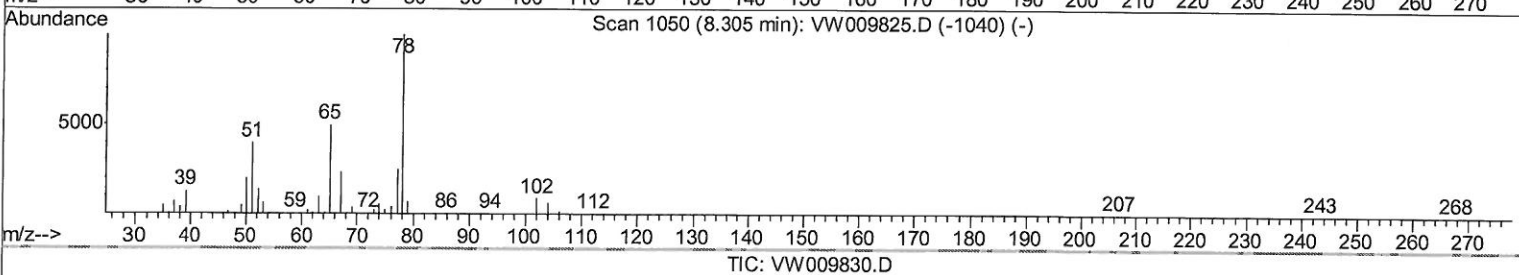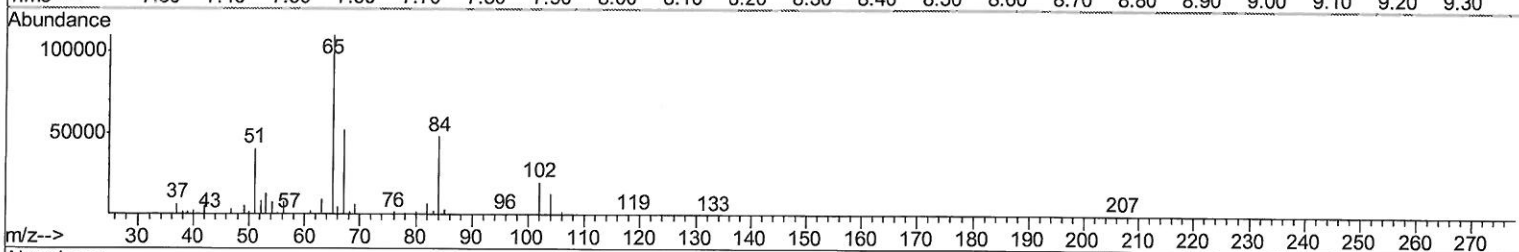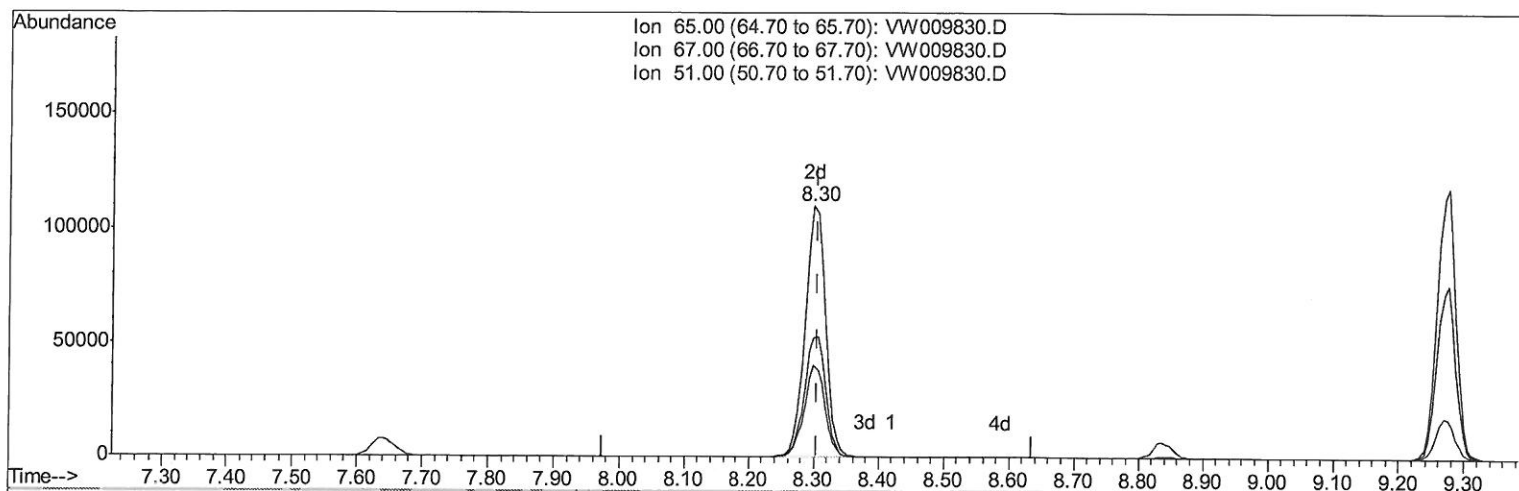

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 24.36ug/L m

response 238423

Handwritten: 7MD
 4/11/19

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	0.03#
51.00	109.90	0.09#
0.00	0.00	0.00

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009830.D
 Acq On : 09 Apr 2019 09:51
 Operator : SY/VA
 Sample : K2303-04
 Misc : 4.78G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF899

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:03:52 PM

Quant Time: Apr 10 02:46:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 00:56:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	584195	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	548037	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	233399	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	172012	22.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.00%
7) Chloroethane-d5	2.89	69	156168	22.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.20%
10) 1,1-Dichloroethene-d2	4.01	63	318994	19.40	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.60%
20) 2-Butanone-d5	7.08	46	94296	37.99	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.98%
24) Chloroform-d	7.64	84	415734	26.08	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.32%
26) 1,2-Dichloroethane-d4	8.30	65	238423m	24.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.44%
29) Benzene-d6	8.27	84	772370	26.85	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.40%
33) 1,2-Dichloropropane-d6	9.27	67	235178	26.47	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.88%
37) Toluene-d8	10.32	98	688222	25.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.48%
38) trans-1,3-Dichloropropene-	10.57	79	96505	22.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.08%
39) 2-Hexanone-d5	10.93	63	65325	39.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.00%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	169001	20.46	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.84%
61) 1,2-Dichlorobenzene-d4	13.86	152	227250	27.75	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.00%

Target Compounds

					Qvalue
13) Acetone	4.12	43	5529	2.079	ug/L 66
16) Methylene chloride	4.91	84	14916m	1.448	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed