

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009852.D
 Acq On : 09 Apr 2019 22:17
 Operator : SY/VA
 Sample : K2327-19
 Misc : 6.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF2N1

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:39 PM

Quant Time: Apr 10 04:46:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

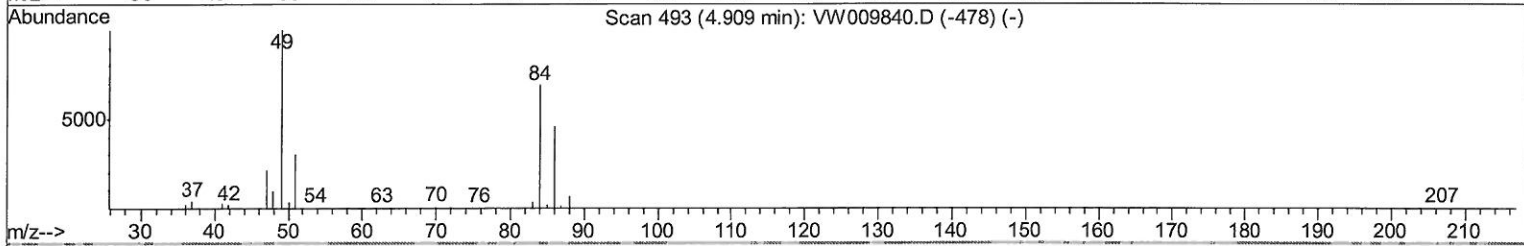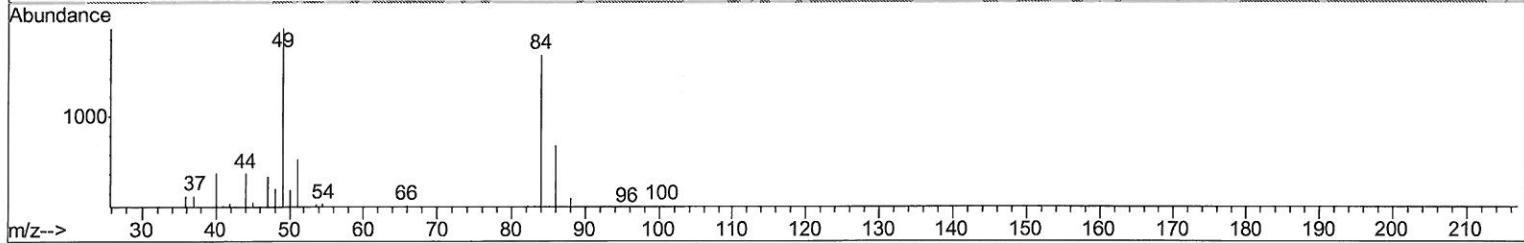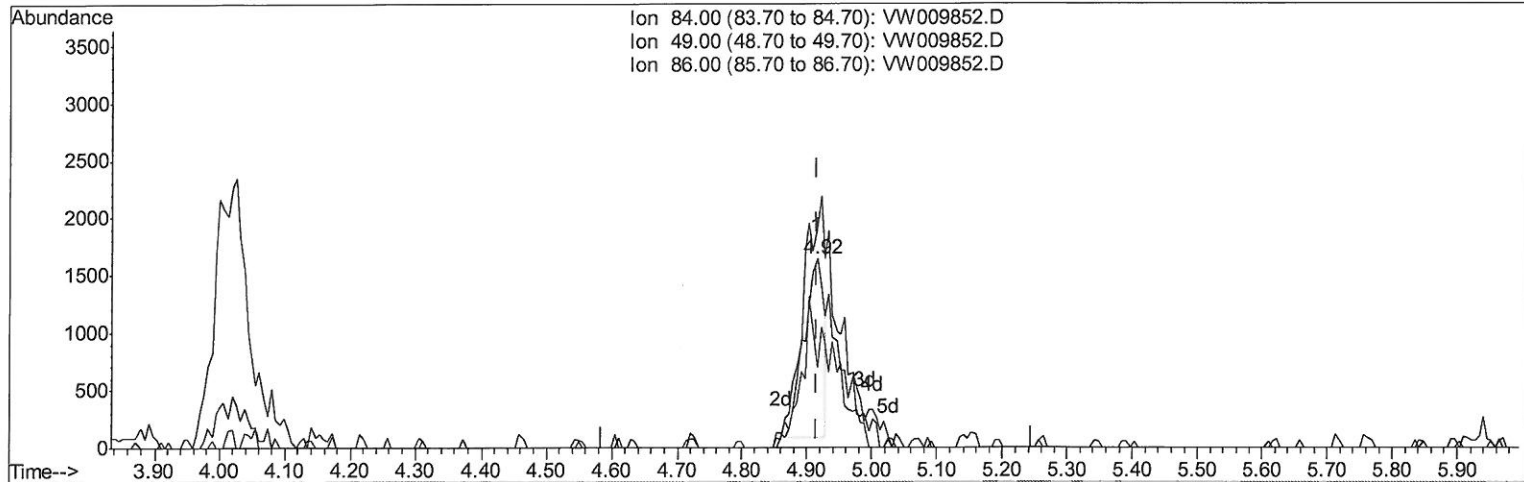

TIC: VW009852.D

(16) Methylene chloride (T)

4.915min (-0.000) 0.50ug/L

response 3267

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	117.09
86.00	66.30	42.12#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009852.D
 Acq On : 09 Apr 2019 22:17
 Operator : SY/VA
 Sample : K2327-19
 Misc : 6.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF2N1

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:39 PM

Quant Time: Apr 10 04:46:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

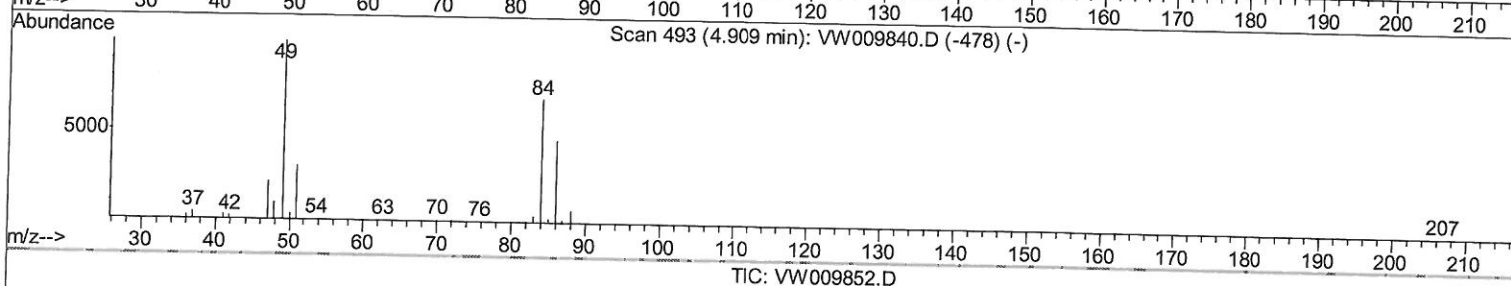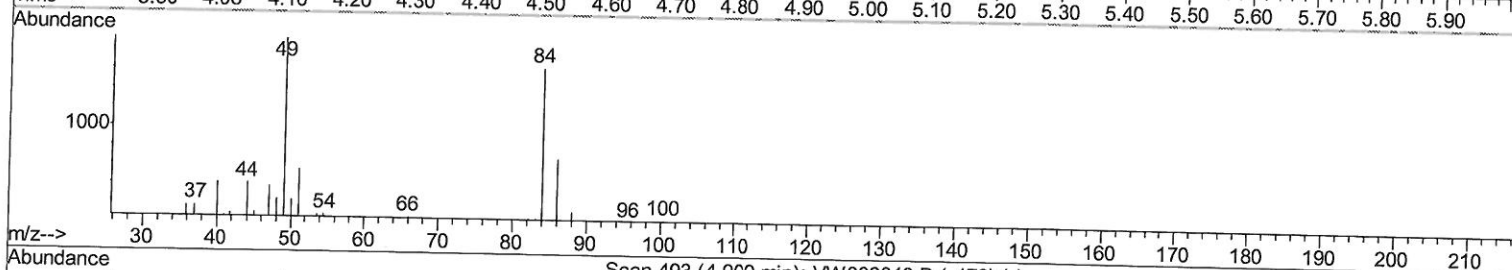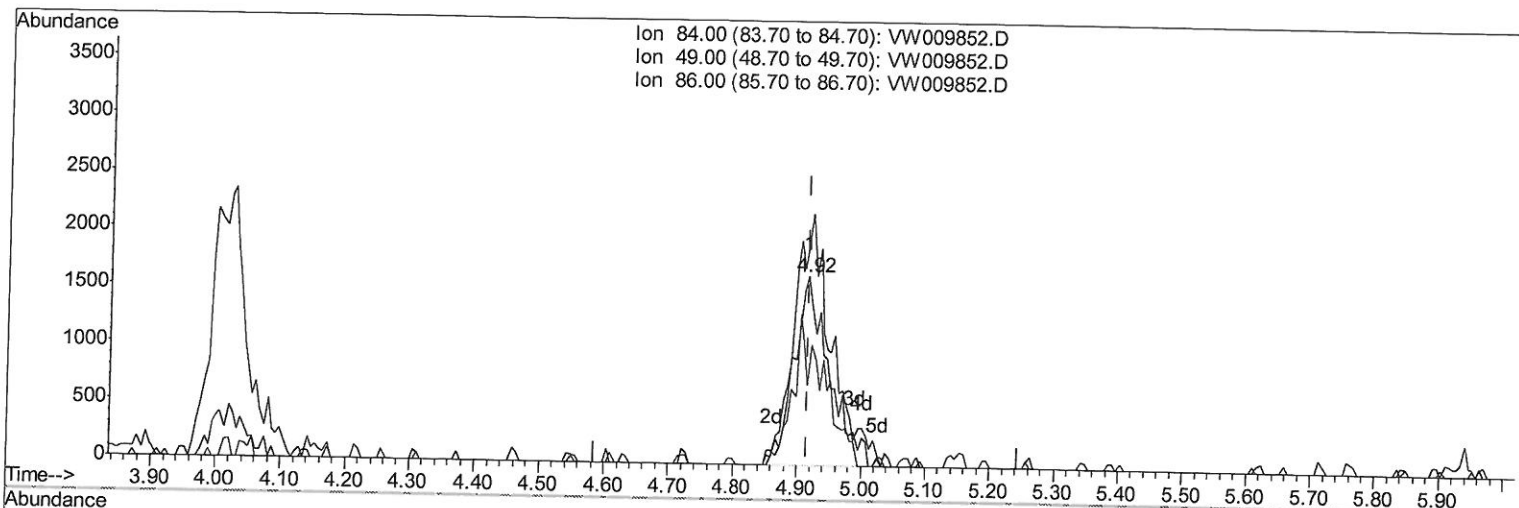

TIC: VW009852.D

(16) Methylene chloride (T)

4.915min (-0.000) 0.97ug/L m

response 6305

Handwritten: > MD
 411119

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	117.09
86.00	66.30	42.12#
0.00	0.00	0.00