

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009854.D
 Acq On : 09 Apr 2019 23:12
 Operator : SY/VA
 Sample : K2327-11
 Misc : 6.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF0N5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:46 PM

Quant Time: Apr 10 05:45:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

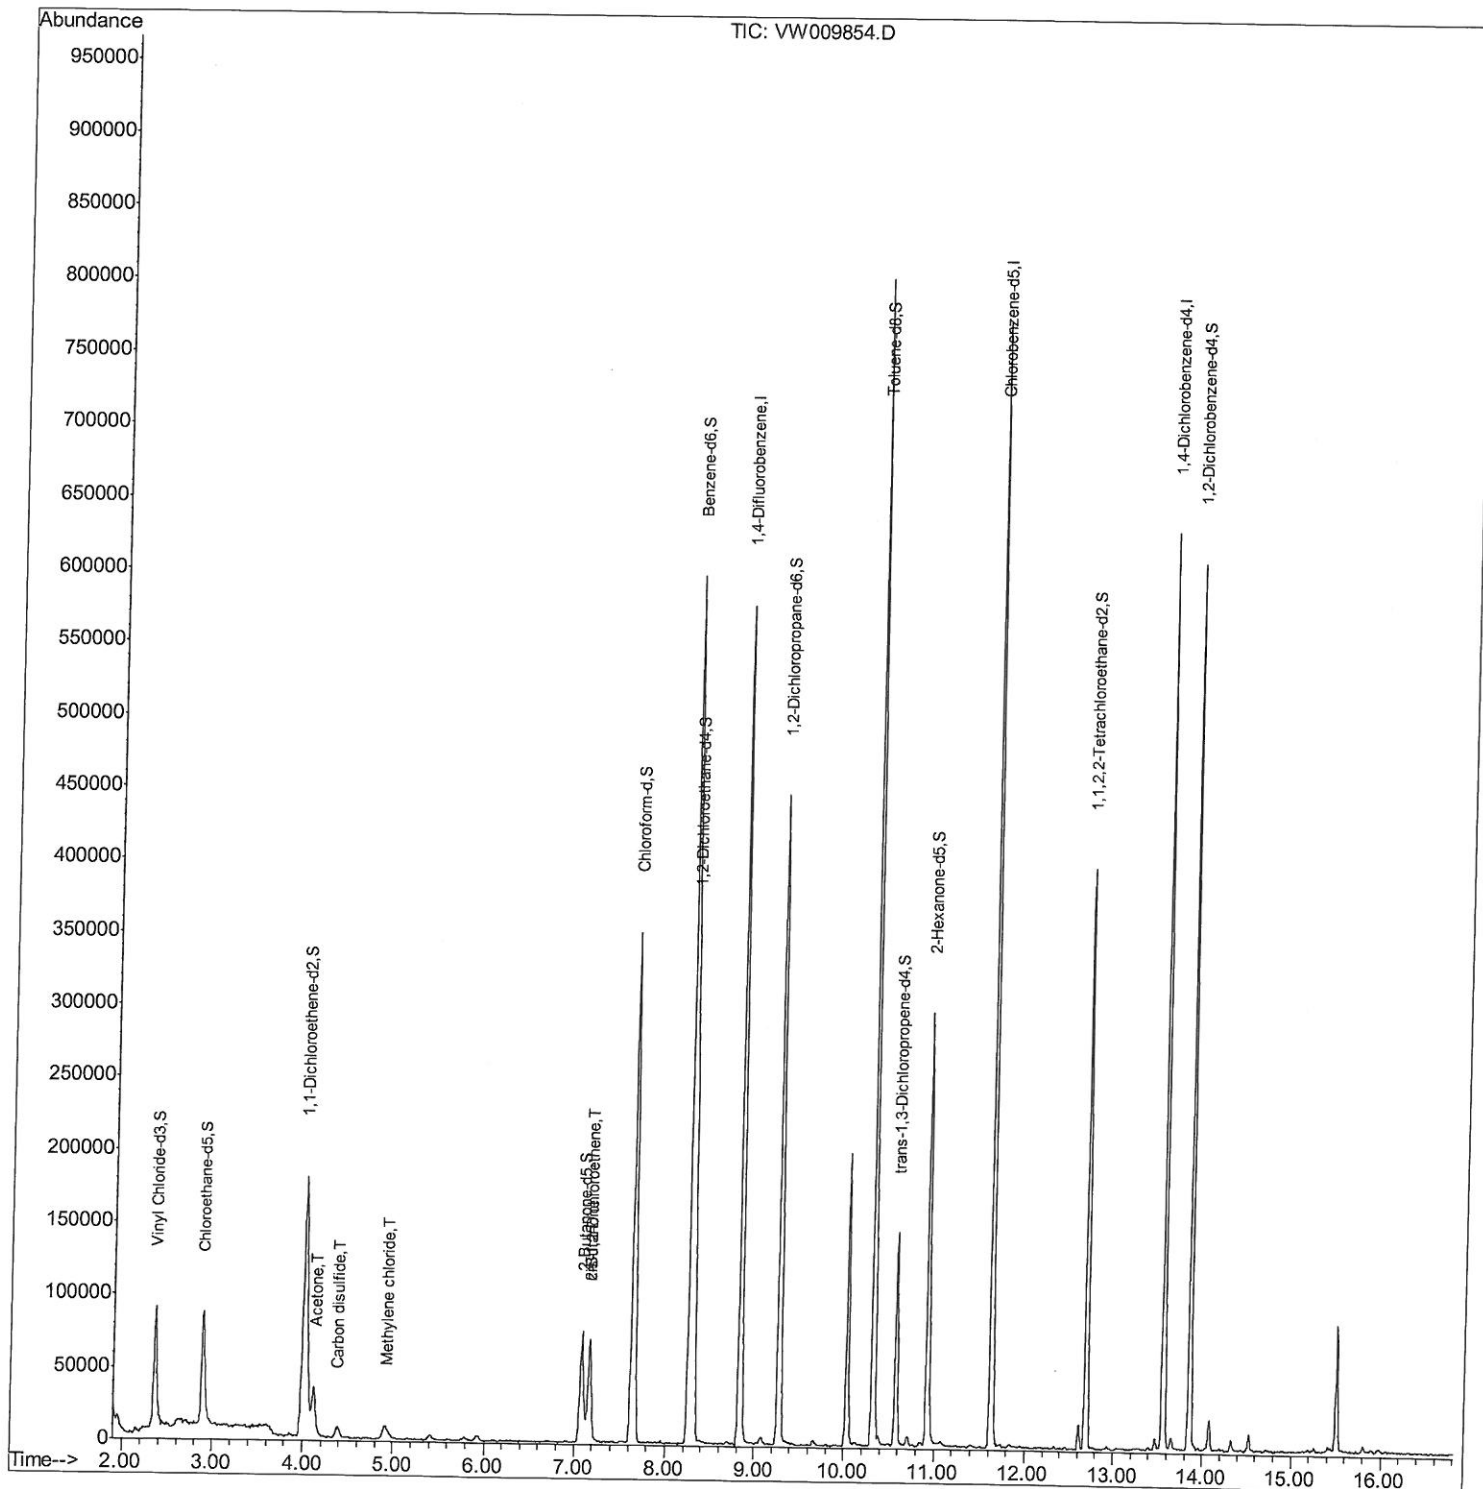

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009854.D
 Acq On : 09 Apr 2019 23:12
 Operator : SY/VA
 Sample : K2327-11
 Misc : 6.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF0N5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:46 PM

Quant Time: Apr 10 04:46:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

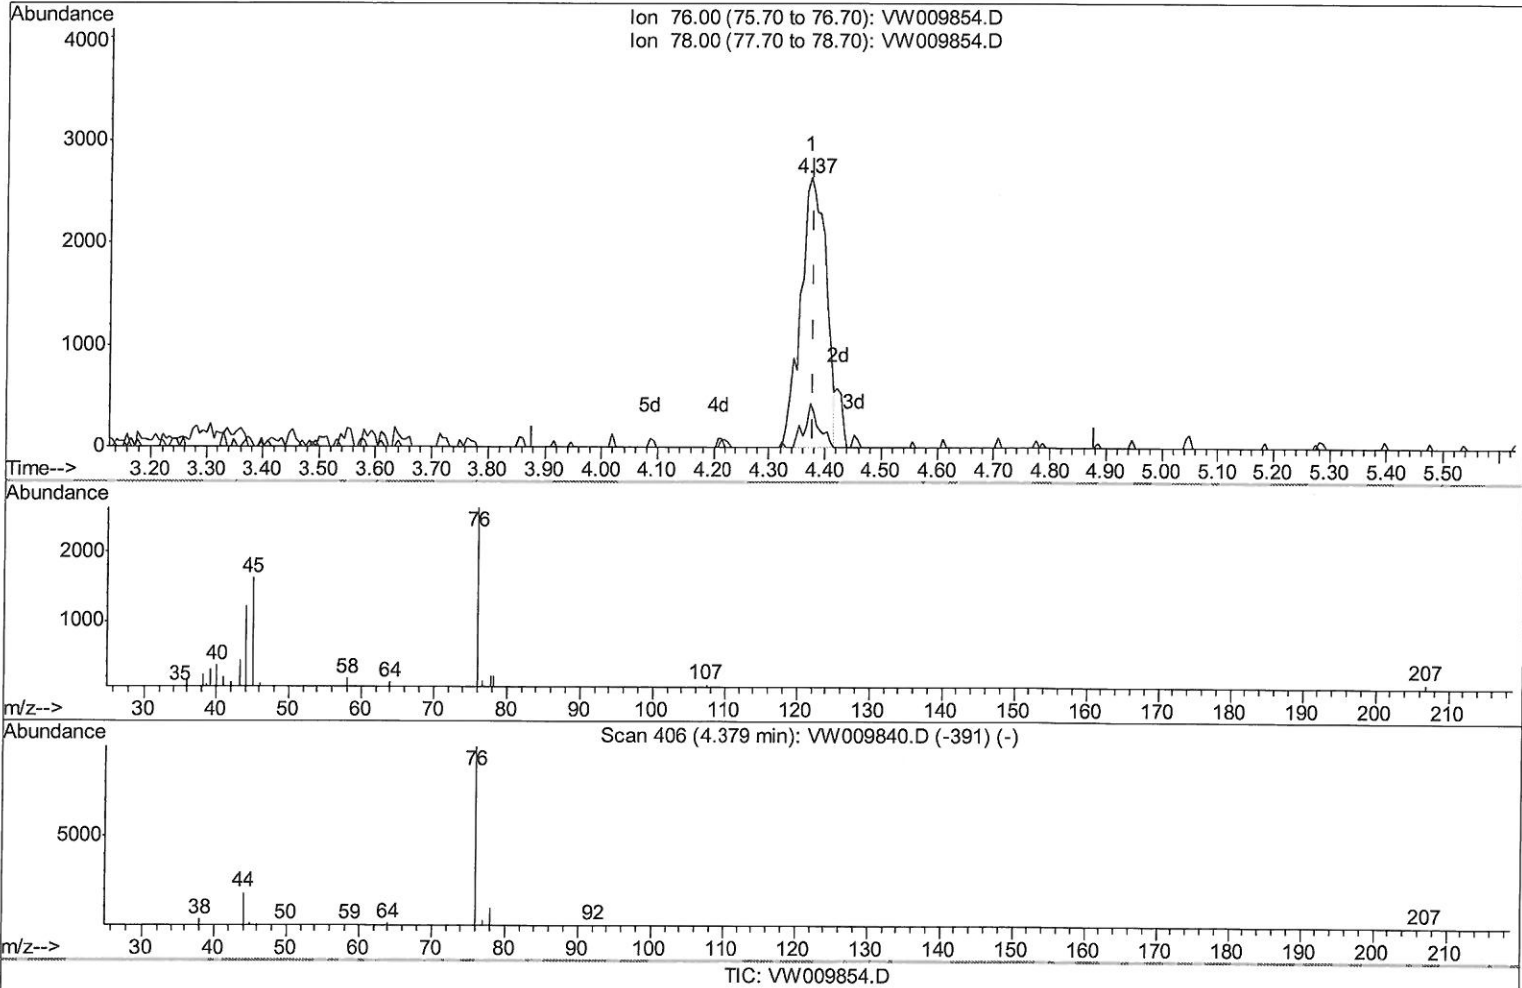

(14) Carbon disulfide (T)
 4.373min (-0.006) 0.47ug/L
 response 8307

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	15.43#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009854.D
 Acq On : 09 Apr 2019 23:12
 Operator : SY/VA
 Sample : K2327-11
 Misc : 6.03G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0N5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:46 PM

Quant Time: Apr 10 04:46:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

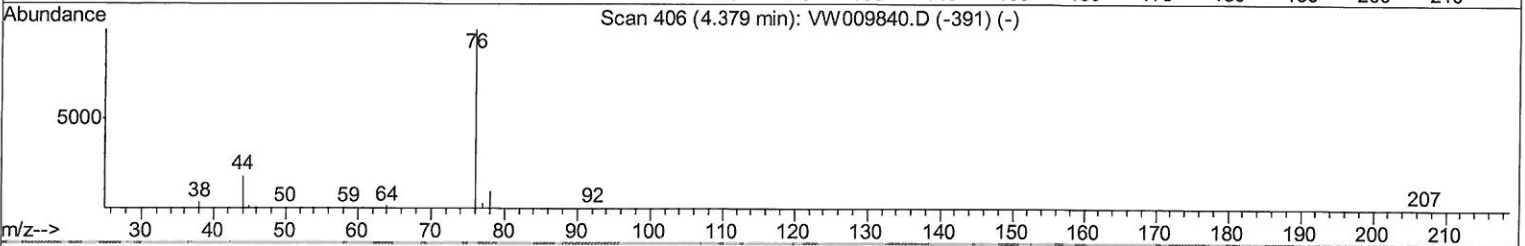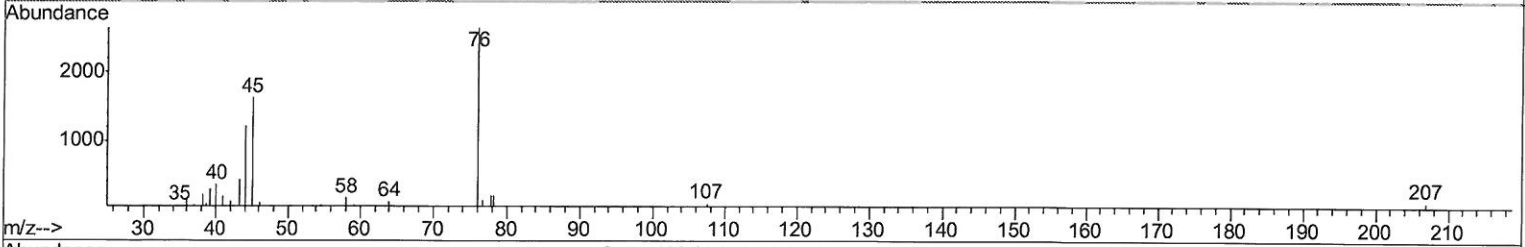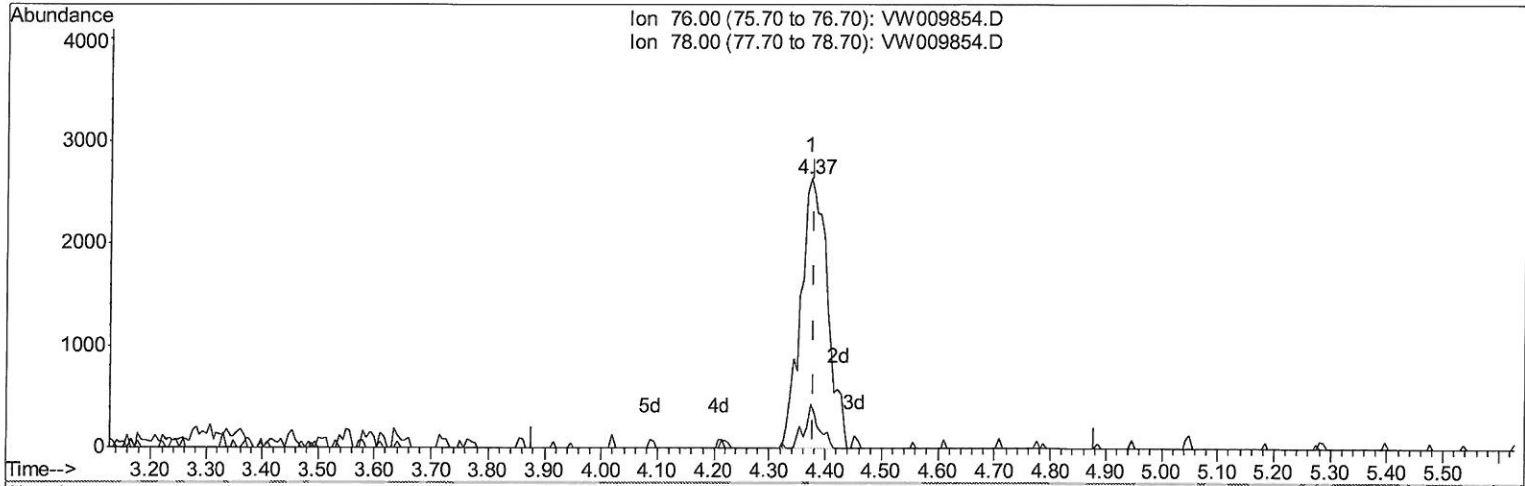

TIC: VW009854.D

(14) Carbon disulfide (T)

4.373min (-0.006) 0.50ug/L m

response 8843

→ MD
 411119

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	8.27
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009854.D
 Acq On : 09 Apr 2019 23:12
 Operator : SY/VA
 Sample : K2327-11
 Misc : 6.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0N5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:46 PM

Quant Time: Apr 10 04:46:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

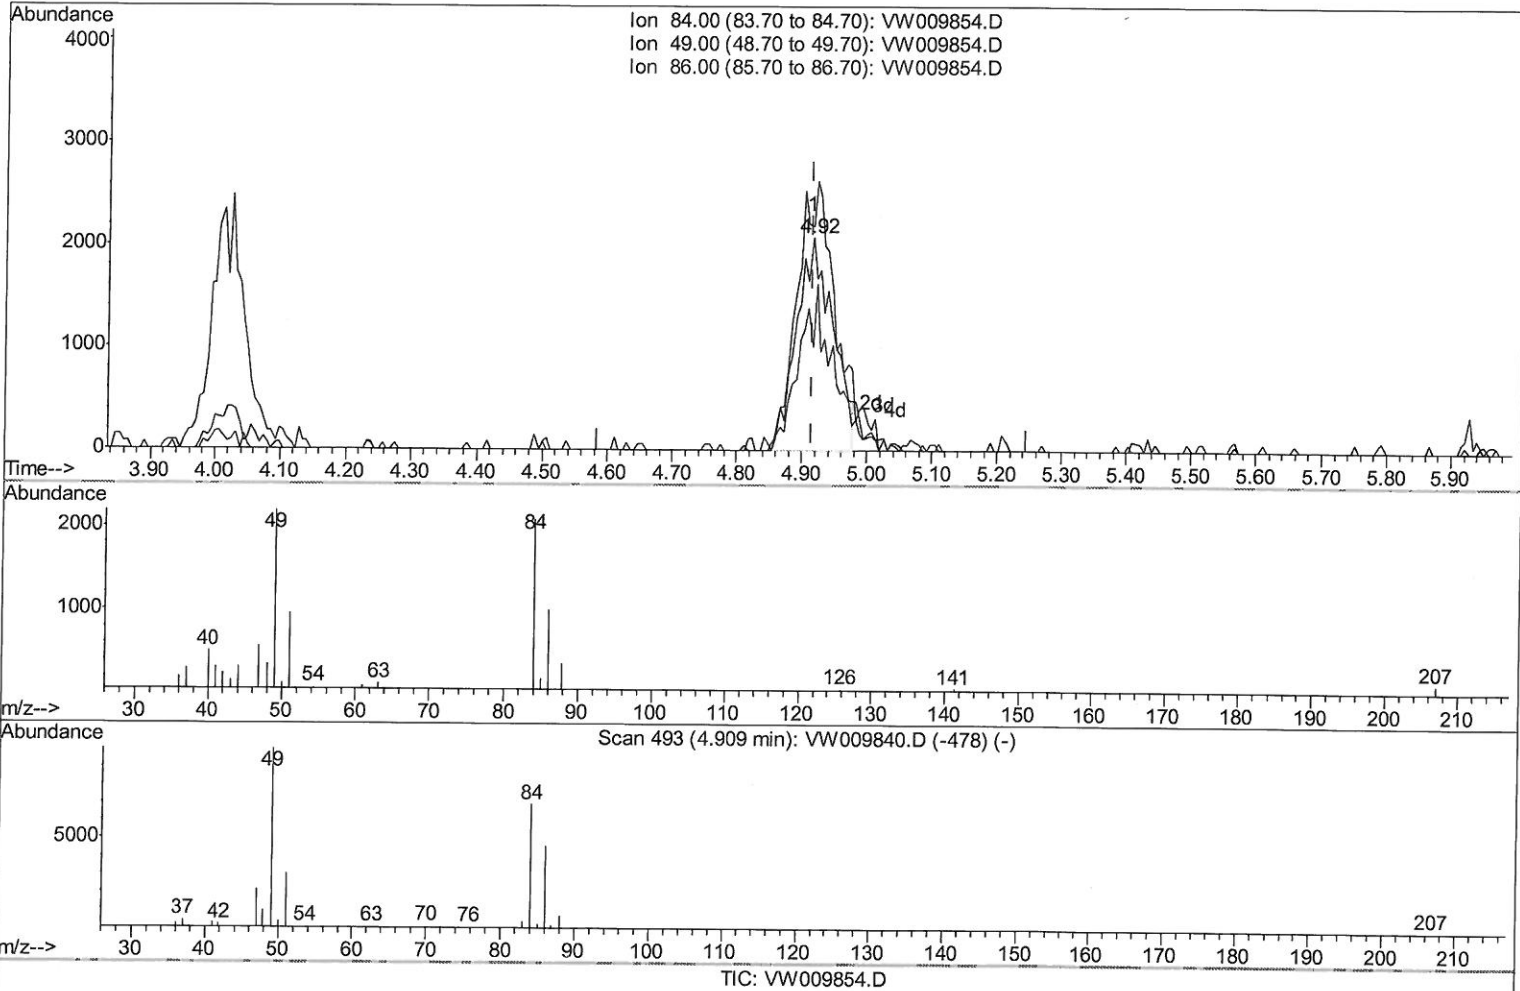

(16) Methylene chloride (T)

4.915min (+0.000) 1.06ug/L

response 8054

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	105.10
86.00	66.30	48.46
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009854.D
 Acq On : 09 Apr 2019 23:12
 Operator : SY/VA
 Sample : K2327-11
 Misc : 6.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF0N5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:46 PM

Quant Time: Apr 10 04:46:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

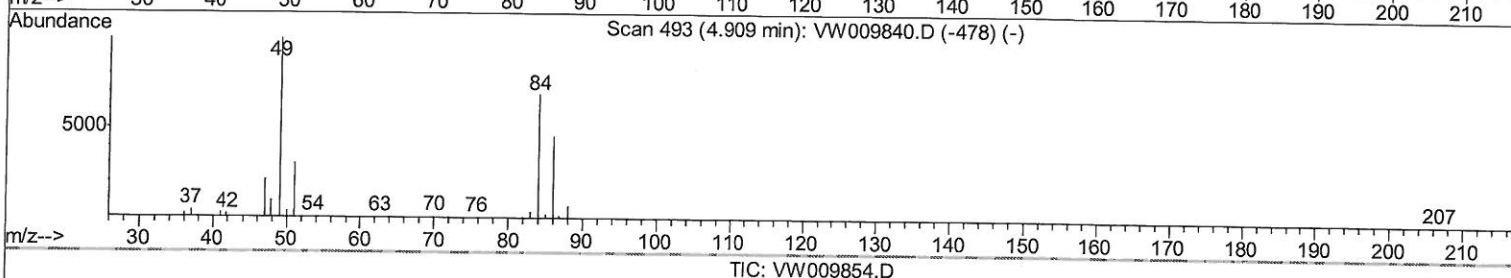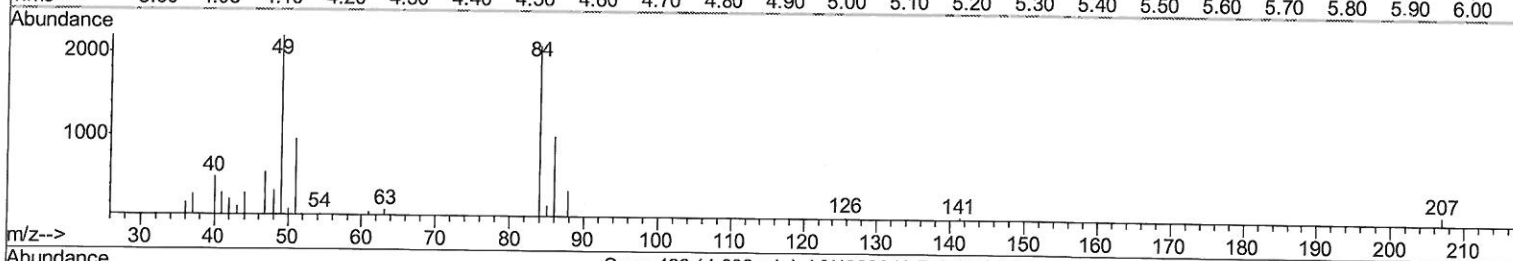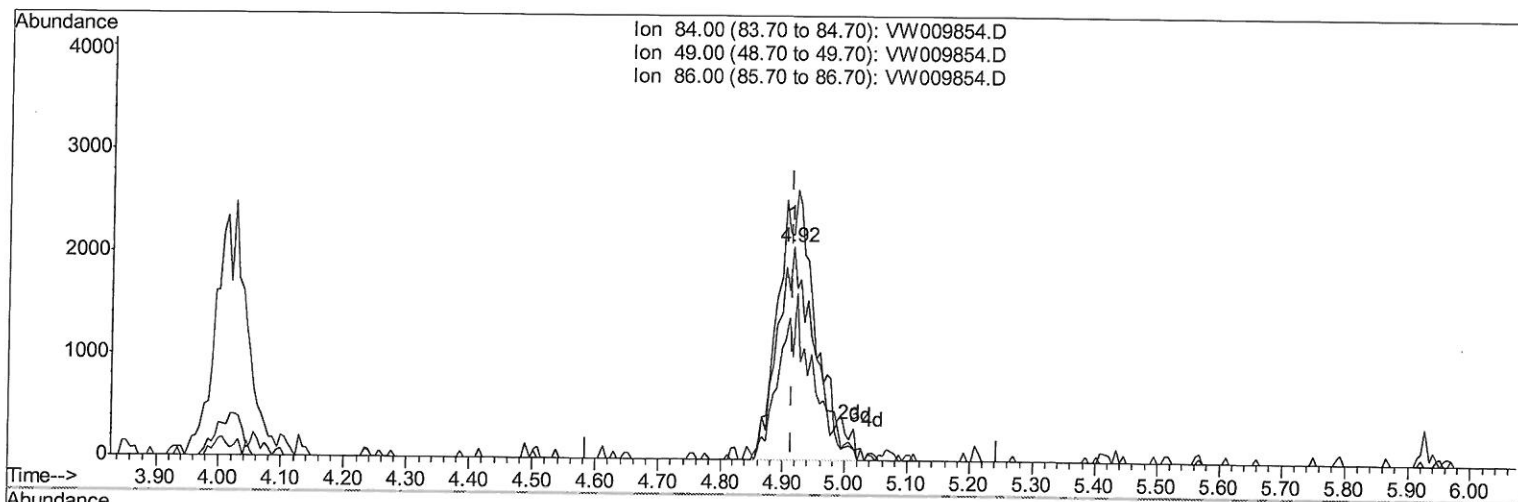

TIC: VW009854.D

(16) Methylene chloride (T)

4.915min (+0.000) 1.14ug/L m

response 8670

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	105.10
86.00	66.30	48.46
0.00	0.00	0.00

7 MO
 4 111119

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009854.D
 Acq On : 09 Apr 2019 23:12
 Operator : SY/VA
 Sample : K2327-11
 Misc : 6.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0N5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:46 PM

Quant Time: Apr 10 04:46:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

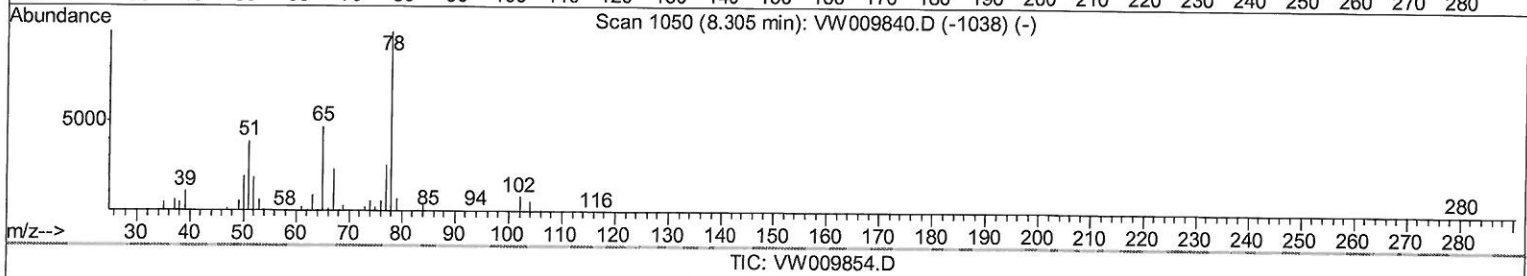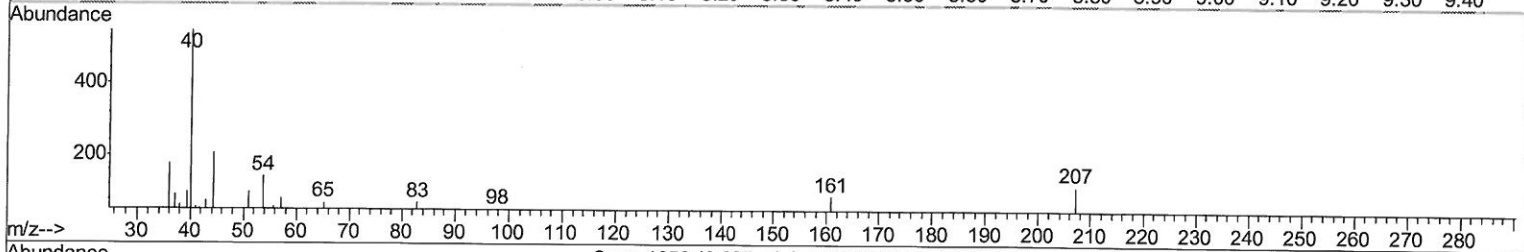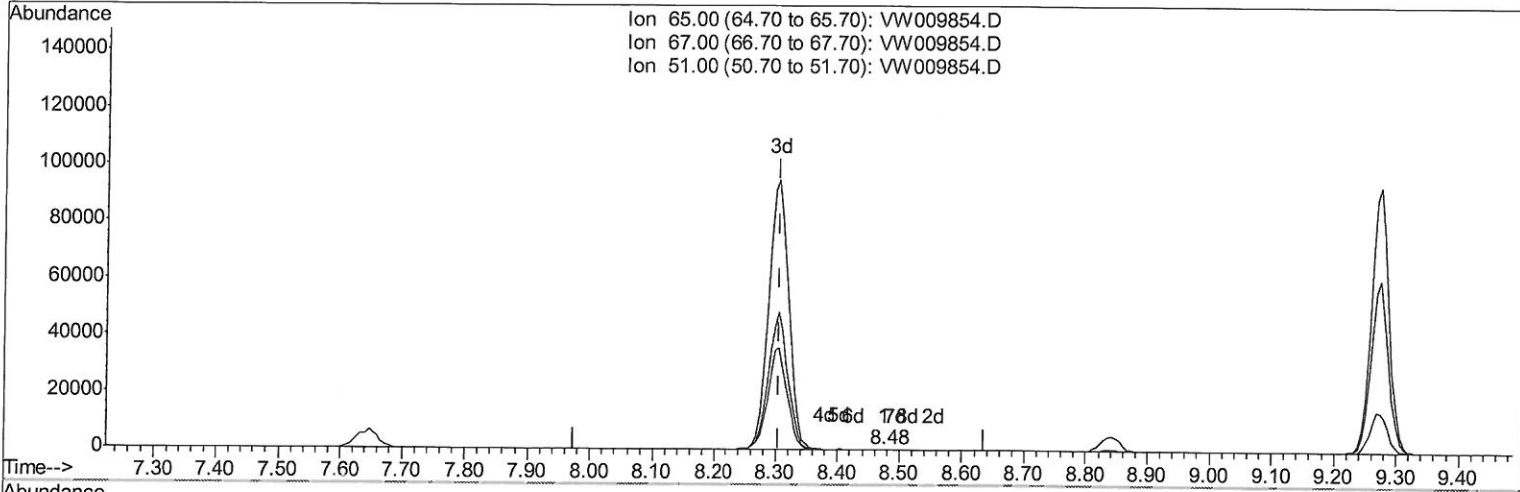

(26) 1,2-Dichloroethane-d4 (S)

8.476min (+0.171) 0.01ug/L

response 67

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	61.19
51.00	109.90	116.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009854.D
 Acq On : 09 Apr 2019 23:12
 Operator : SY/VA
 Sample : K2327-11
 Misc : 6.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0N5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:46 PM

Quant Time: Apr 10 04:46:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

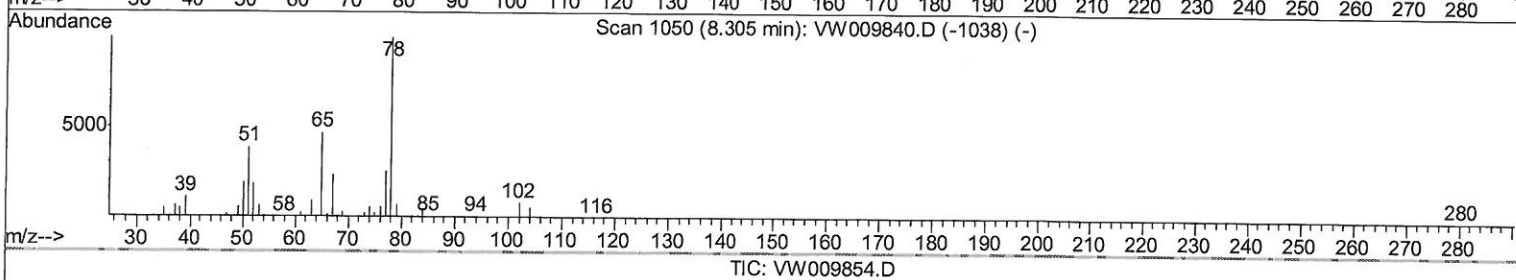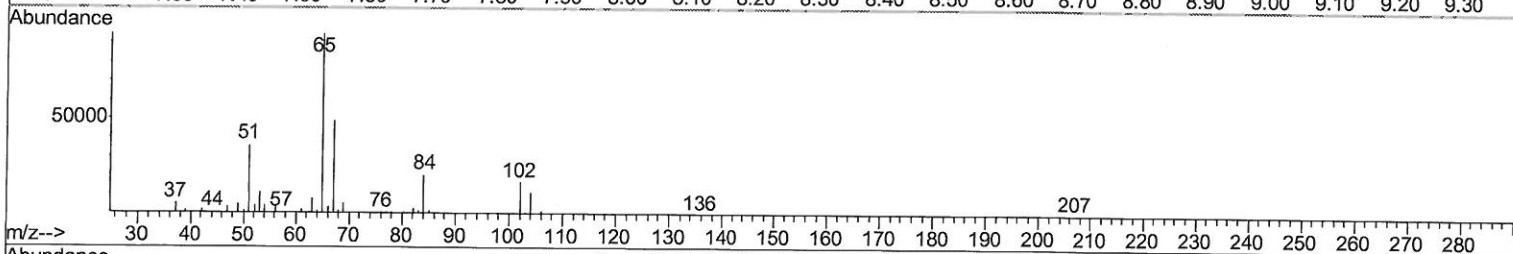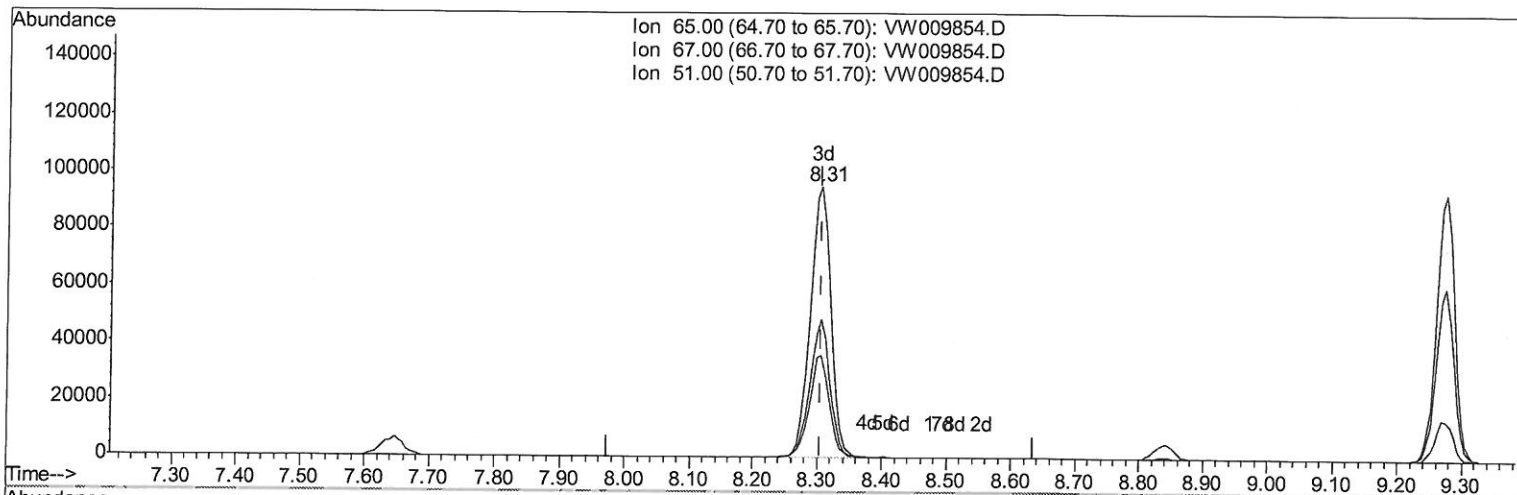

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.000) 29.04ug/L m

response 209093

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	0.02#
51.00	109.90	0.04#
0.00	0.00	0.00

7 mD
 4/11/19

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009854.D
 Acq On : 09 Apr 2019 23:12
 Operator : SY/VA
 Sample : K2327-11
 Misc : 6.03G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF0N5

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:05:46 PM

Quant Time: Apr 10 05:45:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	429844	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	397901	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	145198	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	119815	21.30	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.20%		
7) Chloroethane-d5	2.89	69	112759	21.88	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.52%		
10) 1,1-Dichloroethene-d2	4.01	63	222765	18.42	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	73.68%		
20) 2-Butanone-d5	7.08	46	128348	70.28	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	140.56%#		
24) Chloroform-d	7.65	84	316011	26.94	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	107.76%		
26) 1,2-Dichloroethane-d4	8.31	65	209093m	29.04	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	116.16%		
29) Benzene-d6	8.27	84	570359	27.31	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	109.24%		
33) 1,2-Dichloropropane-d6	9.27	67	182720	28.32	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	113.28%		
37) Toluene-d8	10.32	98	489958	25.37	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	101.48%		
38) trans-1,3-Dichloropropene-	10.58	79	73280	23.82	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	95.28%		
39) 2-Hexanone-d5	10.93	63	80230	65.98	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	131.96%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	180094	30.03	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	120.12%#		
61) 1,2-Dichlorobenzene-d4	13.86	152	150980	29.63	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	118.52%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.12	43	58351	29.820	ug/L	98
14) Carbon disulfide	4.37	76	8843m	0.498	ug/L	
16) Methylene chloride	4.92	84	8670m	1.144	ug/L	
21) 2-Butanone	7.17	43	13791	5.542	ug/L	93
22) cis-1,2-Dichloroethene	7.17	96	32341	5.093	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed