

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009864.D
 Acq On : 10 Apr 2019 06:01
 Operator : SY/VA
 Sample : K2278-02
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB6W9

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:06:44 PM

Quant Time: Apr 10 06:49:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 06:04:24 2019
 Response via : Initial Calibration

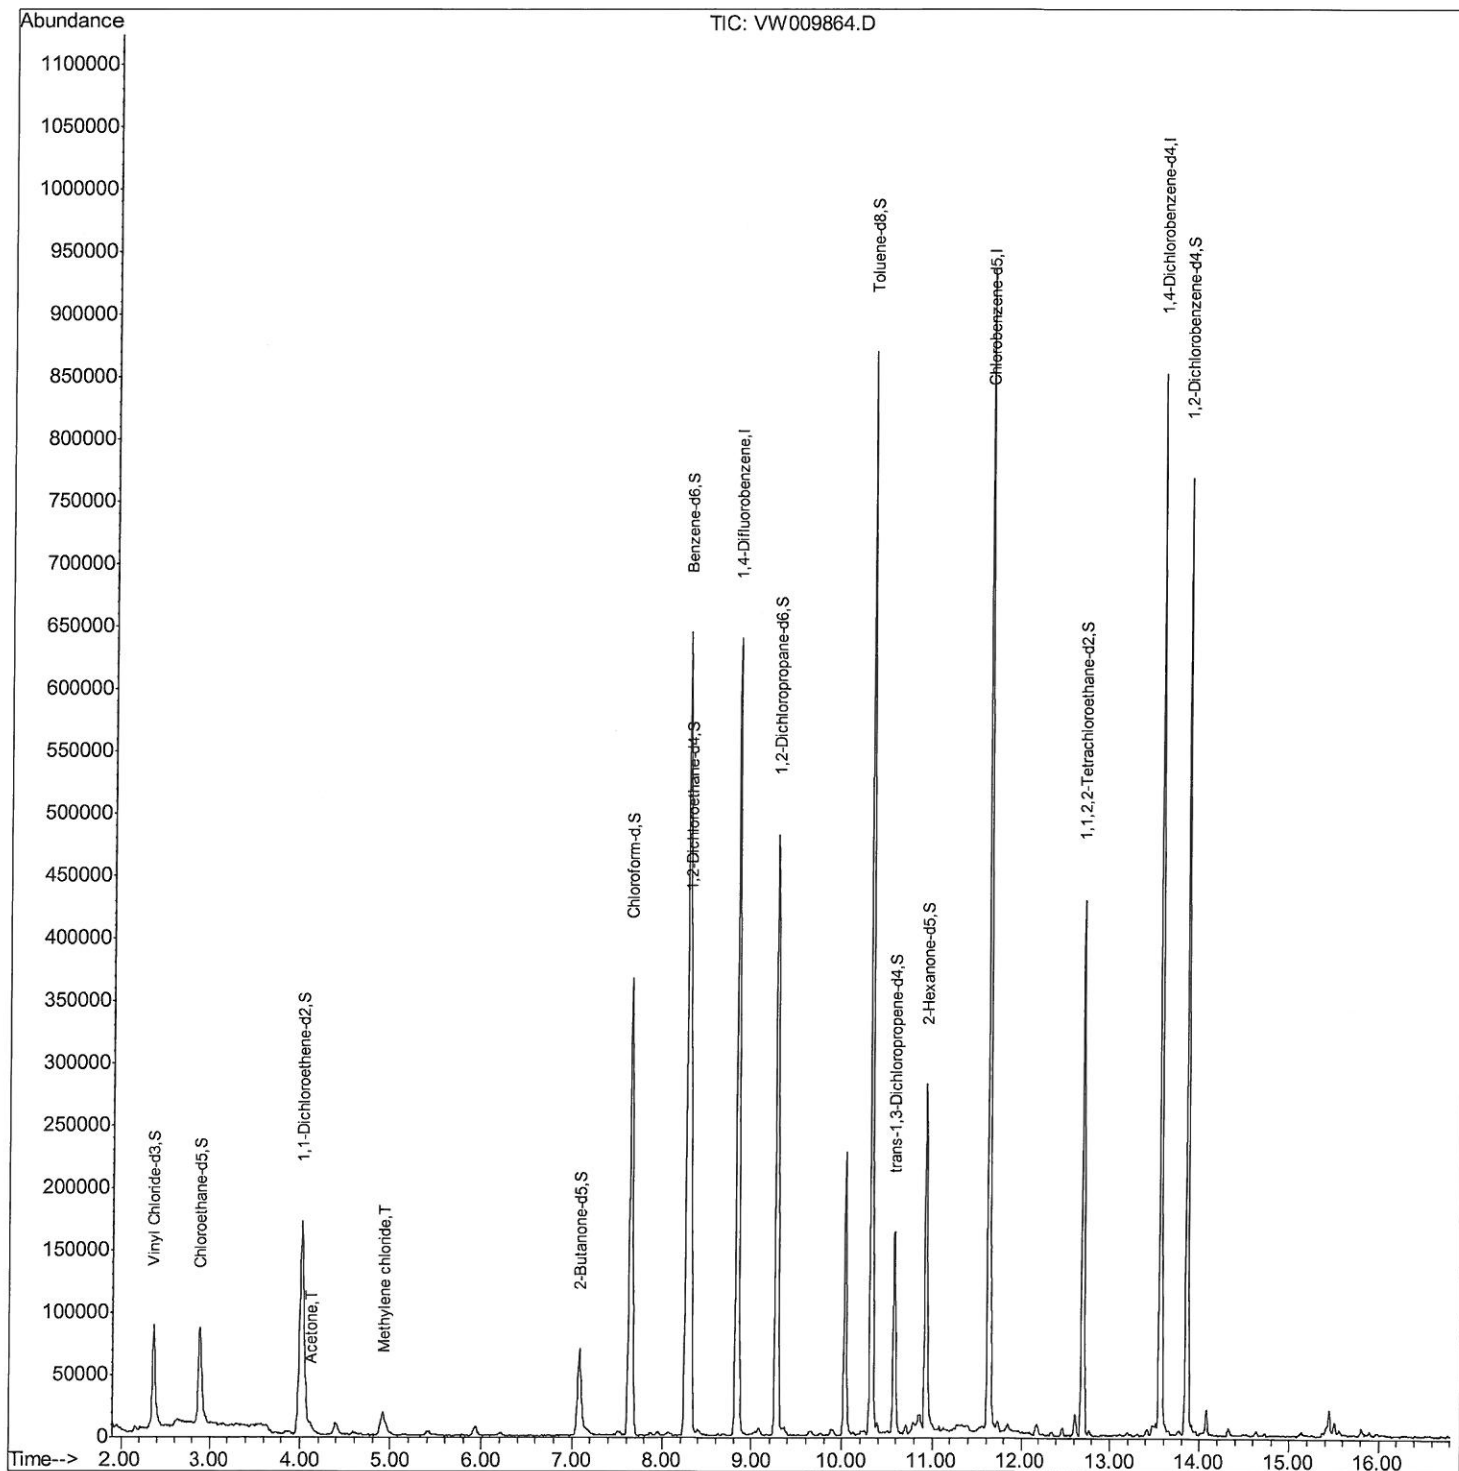

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009864.D
 Acq On : 10 Apr 2019 06:01
 Operator : SY/VA
 Sample : K2278-02
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB6W9

Quant Time: Apr 10 06:47:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 06:04:24 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:06:44 PM

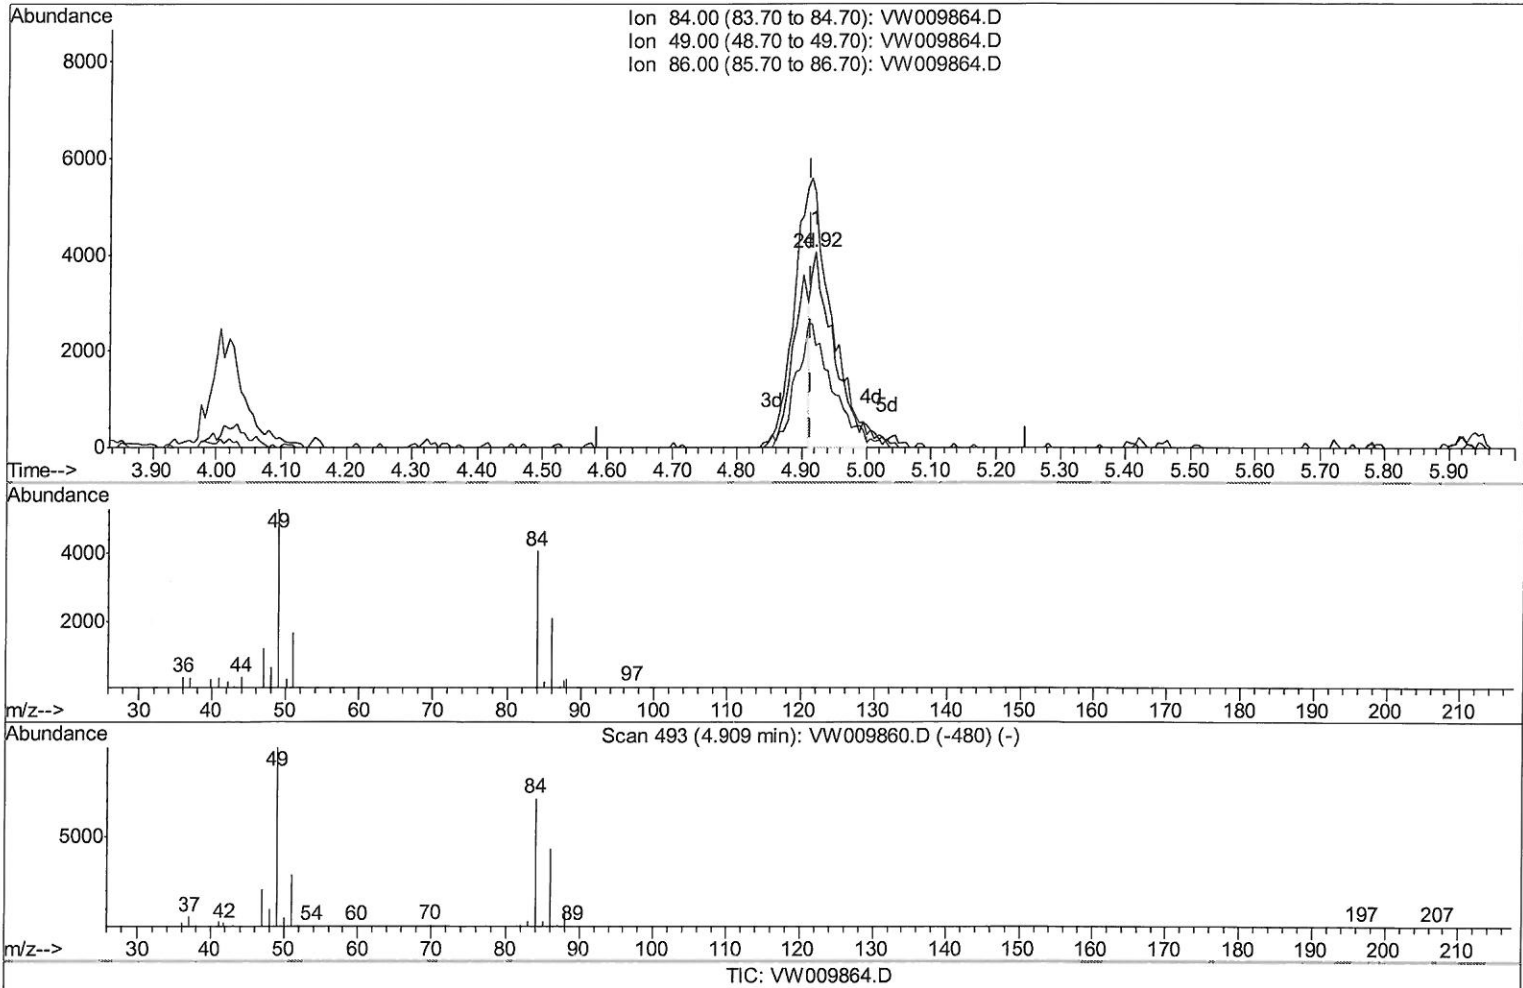

(16) Methylene chloride (T)

4.922min (+0.006) 1.15ug/L

response 9808

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	130.09
86.00	66.30	51.87
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009864.D
 Acq On : 10 Apr 2019 06:01
 Operator : SY/VA
 Sample : K2278-02
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 DB6W9

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:06:44 PM

Quant Time: Apr 10 06:47:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 06:04:24 2019
 Response via : Initial Calibration

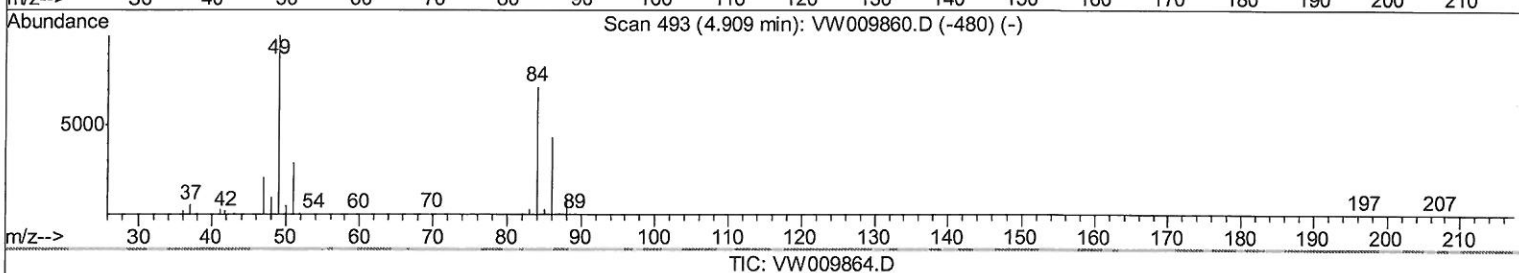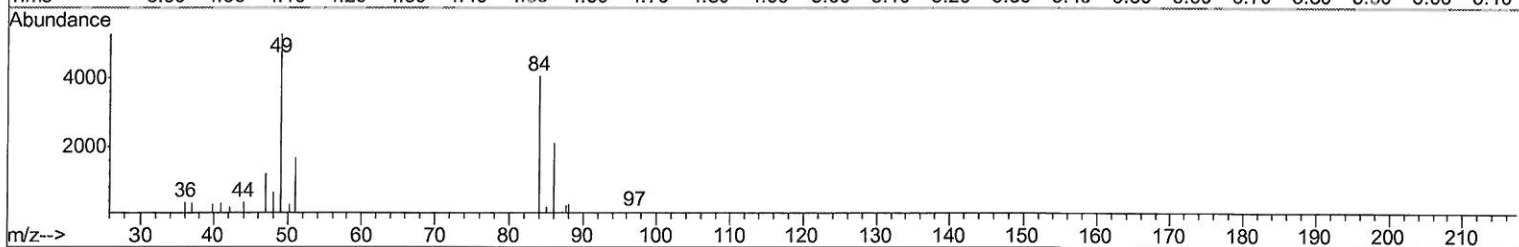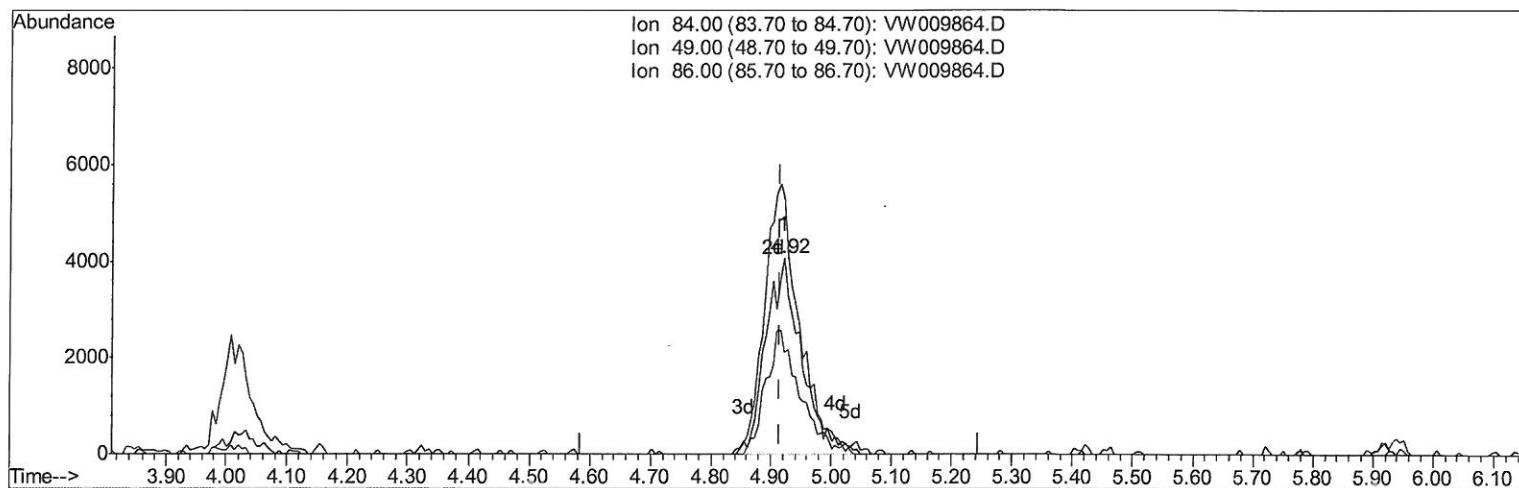

(16) Methylene chloride (T)

4.922min (+0.006) 1.94ug/L m

response 16561

Ion Exp% Act%

84.00 100 100

49.00 140.40 130.09

86.00 66.30 51.87

0.00 0.00 0.00

MMD
4/11/19

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040819\
 Data File : VW009864.D
 Acq On : 10 Apr 2019 06:01
 Operator : SY/VA
 Sample : K2278-02
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DB6W9

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 2:06:44 PM

Quant Time: Apr 10 06:49:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 06:04:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	483113	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	475065	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	198171	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	111917	17.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.80%
7) Chloroethane-d5	2.89	69	114209	19.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.88%
10) 1,1-Dichloroethene-d2	4.01	63	217509	16.00	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.00%
20) 2-Butanone-d5	7.08	46	119488	58.21	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.42%
24) Chloroform-d	7.65	84	342397	25.97	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.88%
26) 1,2-Dichloroethane-d4	8.31	65	228550	28.24	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	112.96%
29) Benzene-d6	8.27	84	609867	24.45	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.80%
33) 1,2-Dichloropropane-d6	9.27	67	199345	25.88	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.52%
37) Toluene-d8	10.32	98	528346	22.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.64%
38) trans-1,3-Dichloropropene-	10.58	79	80636	21.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.80%
39) 2-Hexanone-d5	10.93	63	75333	51.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.78%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	188357	26.30	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.20%
61) 1,2-Dichlorobenzene-d4	13.86	152	191557	27.55	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.20%

Target Compounds

				Qvalue
13) Acetone	4.12	43	8525	3.876 ug/L 75
16) Methylene chloride	4.92	84	16561m	1.944 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7MD
 4/11/19