

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040819\
 Data File : VW009846.D
 Acq On : 09 Apr 2019 19:34
 Operator : SY/VA
 Sample : K2218-11RE
 Misc : 5.33G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF612RE

Quant Time: Apr 10 05:10:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	460944	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	398338	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	129081	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	119147	19.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.00%
7) Chloroethane-d5	2.90	69	109664	19.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.36%
10) 1,1-Dichloroethene-d2	4.01	63	217115	16.74	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.96%
20) 2-Butanone-d5	7.08	46	77083	39.36	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.72%
24) Chloroform-d	7.65	84	305397	24.28	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.12%
26) 1,2-Dichloroethane-d4	8.31	65	188413	24.40	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.60%
29) Benzene-d6	8.27	84	544395	26.03	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.12%
33) 1,2-Dichloropropane-d6	9.27	67	174018	26.94	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.76%
37) Toluene-d8	10.32	98	452683	23.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.64%
38) trans-1,3-Dichloropropene-	10.58	79	61529	19.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.88%
39) 2-Hexanone-d5	10.93	63	46513	38.21	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.42%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	132079	22.00	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.00%
61) 1,2-Dichlorobenzene-d4	13.86	152	108067	23.86	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.44%


Target Compounds					Ovalue
13) Acetone	4.12	43	34923	16.643 ug/L	98
16) Methylene chloride	4.90	84	37715	4.639 ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW040819\
Data File : VW009846.D
Acq On : 09 Apr 2019 19:34
Operator : SY/VA
Sample : K2218-11RE
Misc : 5.33G/10ML/MSVOA W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF612RE

Quant Time: Apr 10 05:10:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:42:28 2019
Response via : Initial Calibration

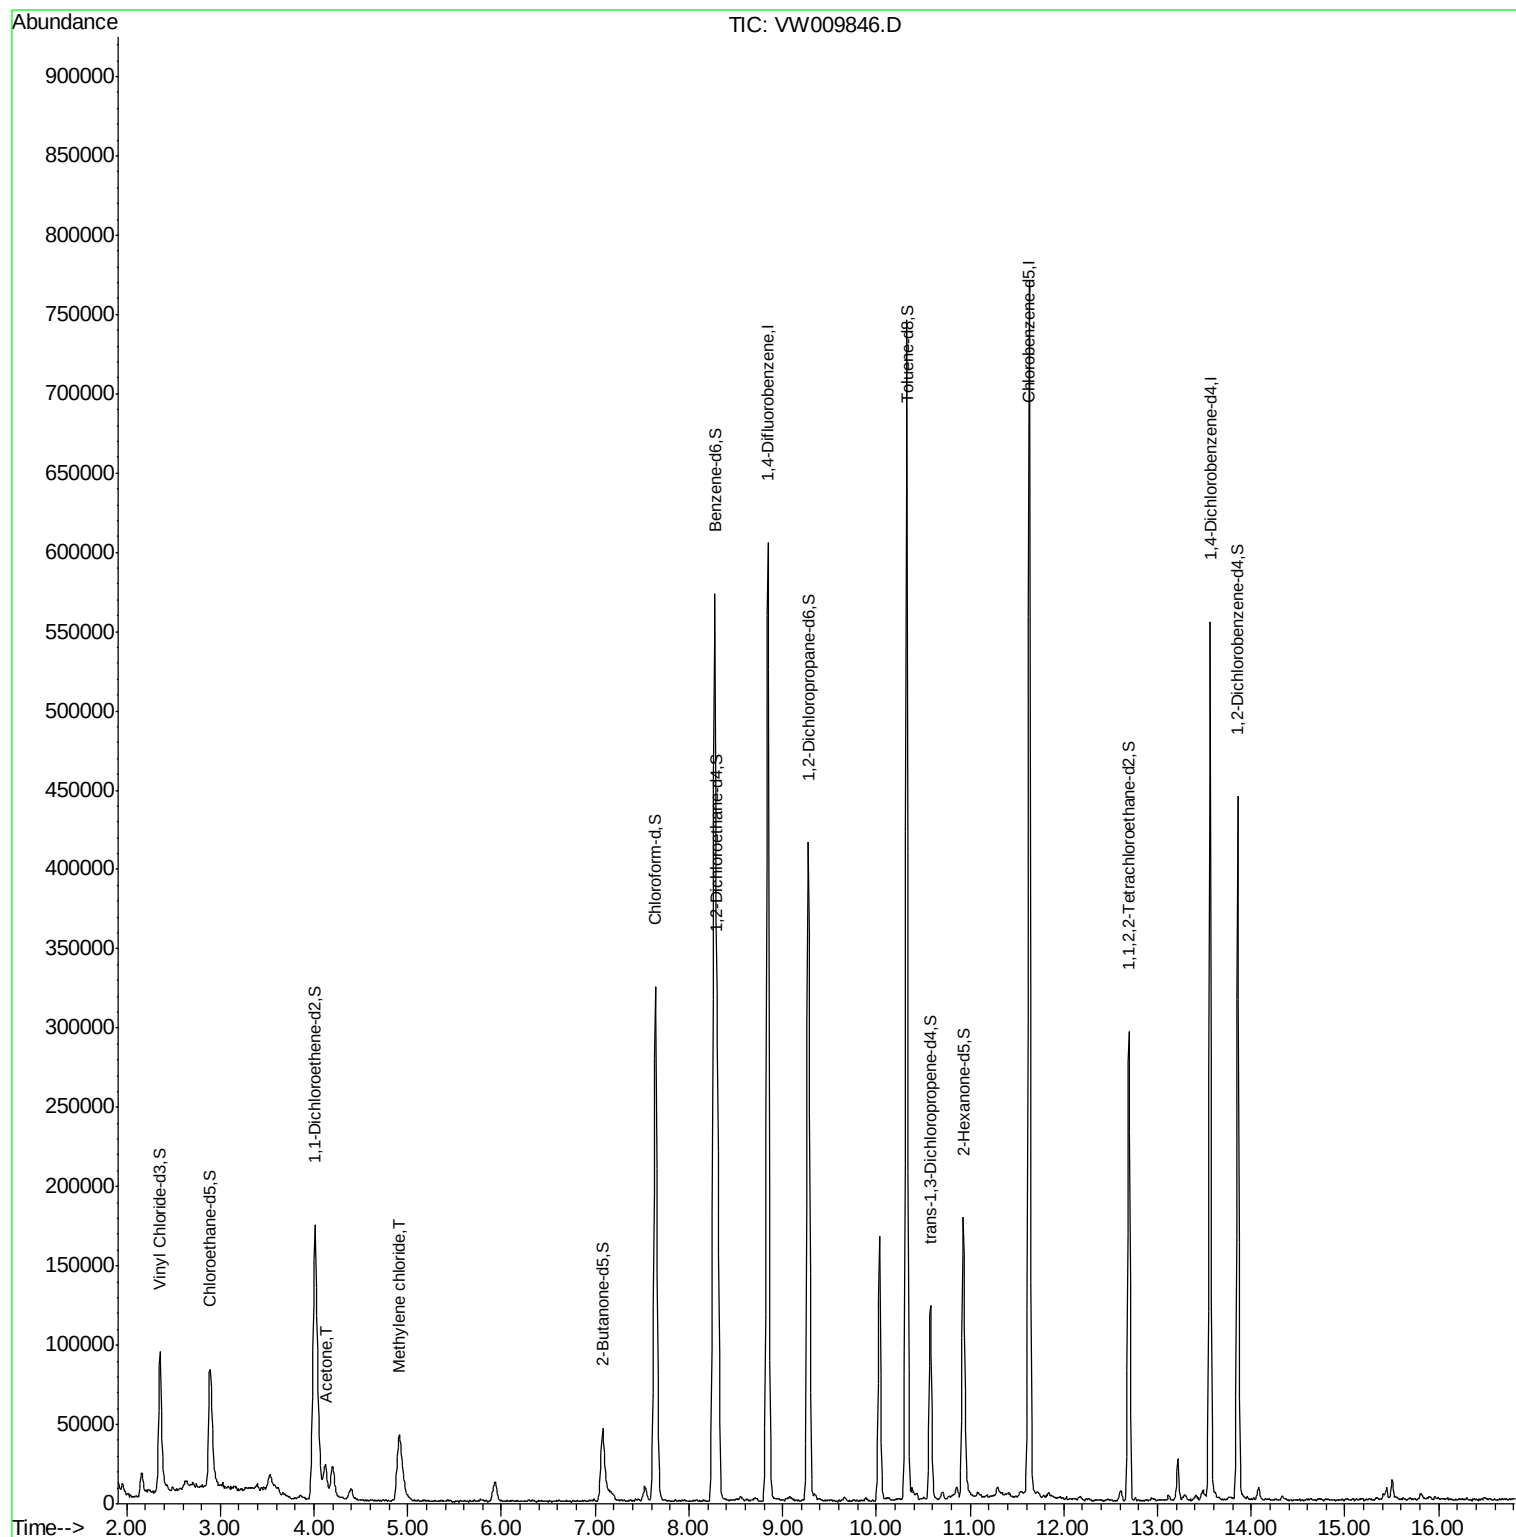

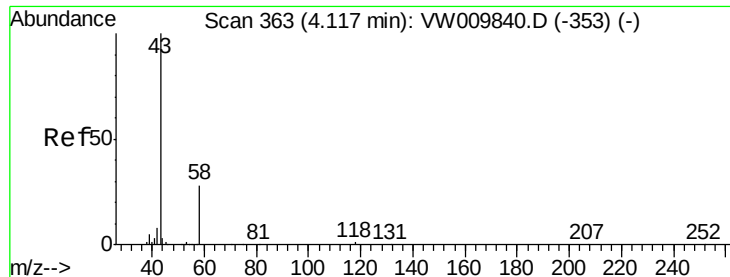

#13

Acetone

Concen: 16.643 ug/L

RT: 4.12 min Scan# 363

Delta R.T. -0.01 min

Lab File: VW009846.D

Acq: 09 Apr 2019 19:34

Instrument :

MSVOA_W

ClientSampled :


BF612RE

Tot Ion: 43 Resp: 34923

Ion Ratio Lower Upper

43 100

58 27.4 0.0 53.0

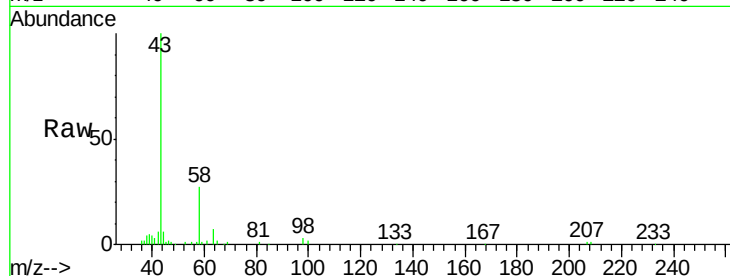

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

15000

10000



5000

0

Time-->

4.05 4.10 4.15 4.20

4.12

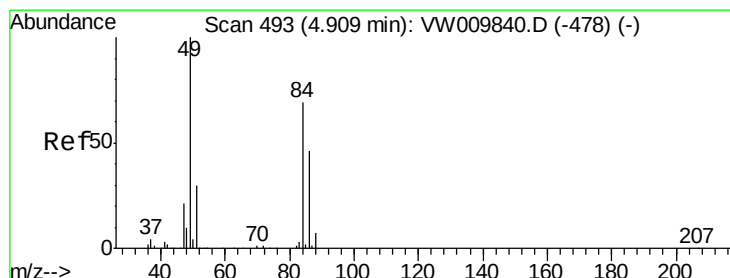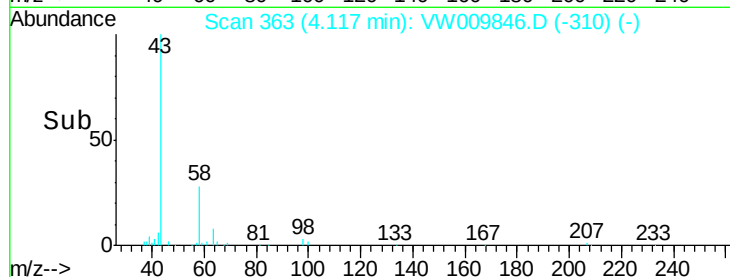

#16

Methylene chloride

Concen: 4.639 ug/L

RT: 4.90 min Scan# 492

Delta R.T. -0.01 min

Lab File: VW009846.D

Acq: 09 Apr 2019 19:34


Tgt Ion: 84 Resp: 37715

Ion Ratio Lower Upper

84 100

49 124.0 98.3 182.5

86 49.7 46.4 86.2

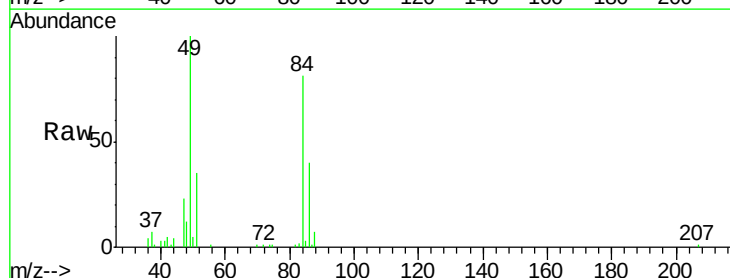

Abundance Ion 84.00 (83.70 to 84.70): VW

Ion 49.00 (48.70 to 49.70): VW

Ion 86.00 (85.70 to 86.70): VW

15000

10000

5000

0

Time-->

4.80 4.90 5.00

4.90

