

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW040819\
 Data File : VW009850.D
 Acq On : 09 Apr 2019 21:23
 Operator : SY/VA
 Sample : K2340-03
 Misc : 6.32G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF2N6

Quant Time: Apr 25 04:38:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 10 04:42:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	493371	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	481685	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	213941	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	142814	22.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.48%
7) Chloroethane-d5	2.89	69	135266	22.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.48%
10) 1,1-Dichloroethene-d2	4.02	63	266068	19.16	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.64%
20) 2-Butanone-d5	7.08	46	132222	63.08	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.16%
24) Chloroform-d	7.64	84	384637	28.57	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	114.28%
26) 1,2-Dichloroethane-d4	8.30	65	250934	30.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	121.44%
29) Benzene-d6	8.27	84	697489	27.58	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.32%
33) 1,2-Dichloropropane-d6	9.27	67	223870	28.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.64%
37) Toluene-d8	10.32	98	615402	26.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.28%
38) trans-1,3-Dichloropropene-	10.58	79	95304	25.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	102.36%
39) 2-Hexanone-d5	10.93	63	88134	59.87	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.74%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	216328	29.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	119.16%
61) 1,2-Dichlorobenzene-d4	13.86	152	232198	30.93	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	123.72%#


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	7.16	96	6922	0.950 ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW040819\
Data File : VW009850.D
Acq On : 09 Apr 2019 21:23
Operator : SY/VA
Sample : K2340-03
Misc : 6.32G/10ML/MSVOA W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF2N6

Quant Time: Apr 25 04:38:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 10 04:42:28 2019
Response via : Initial Calibration

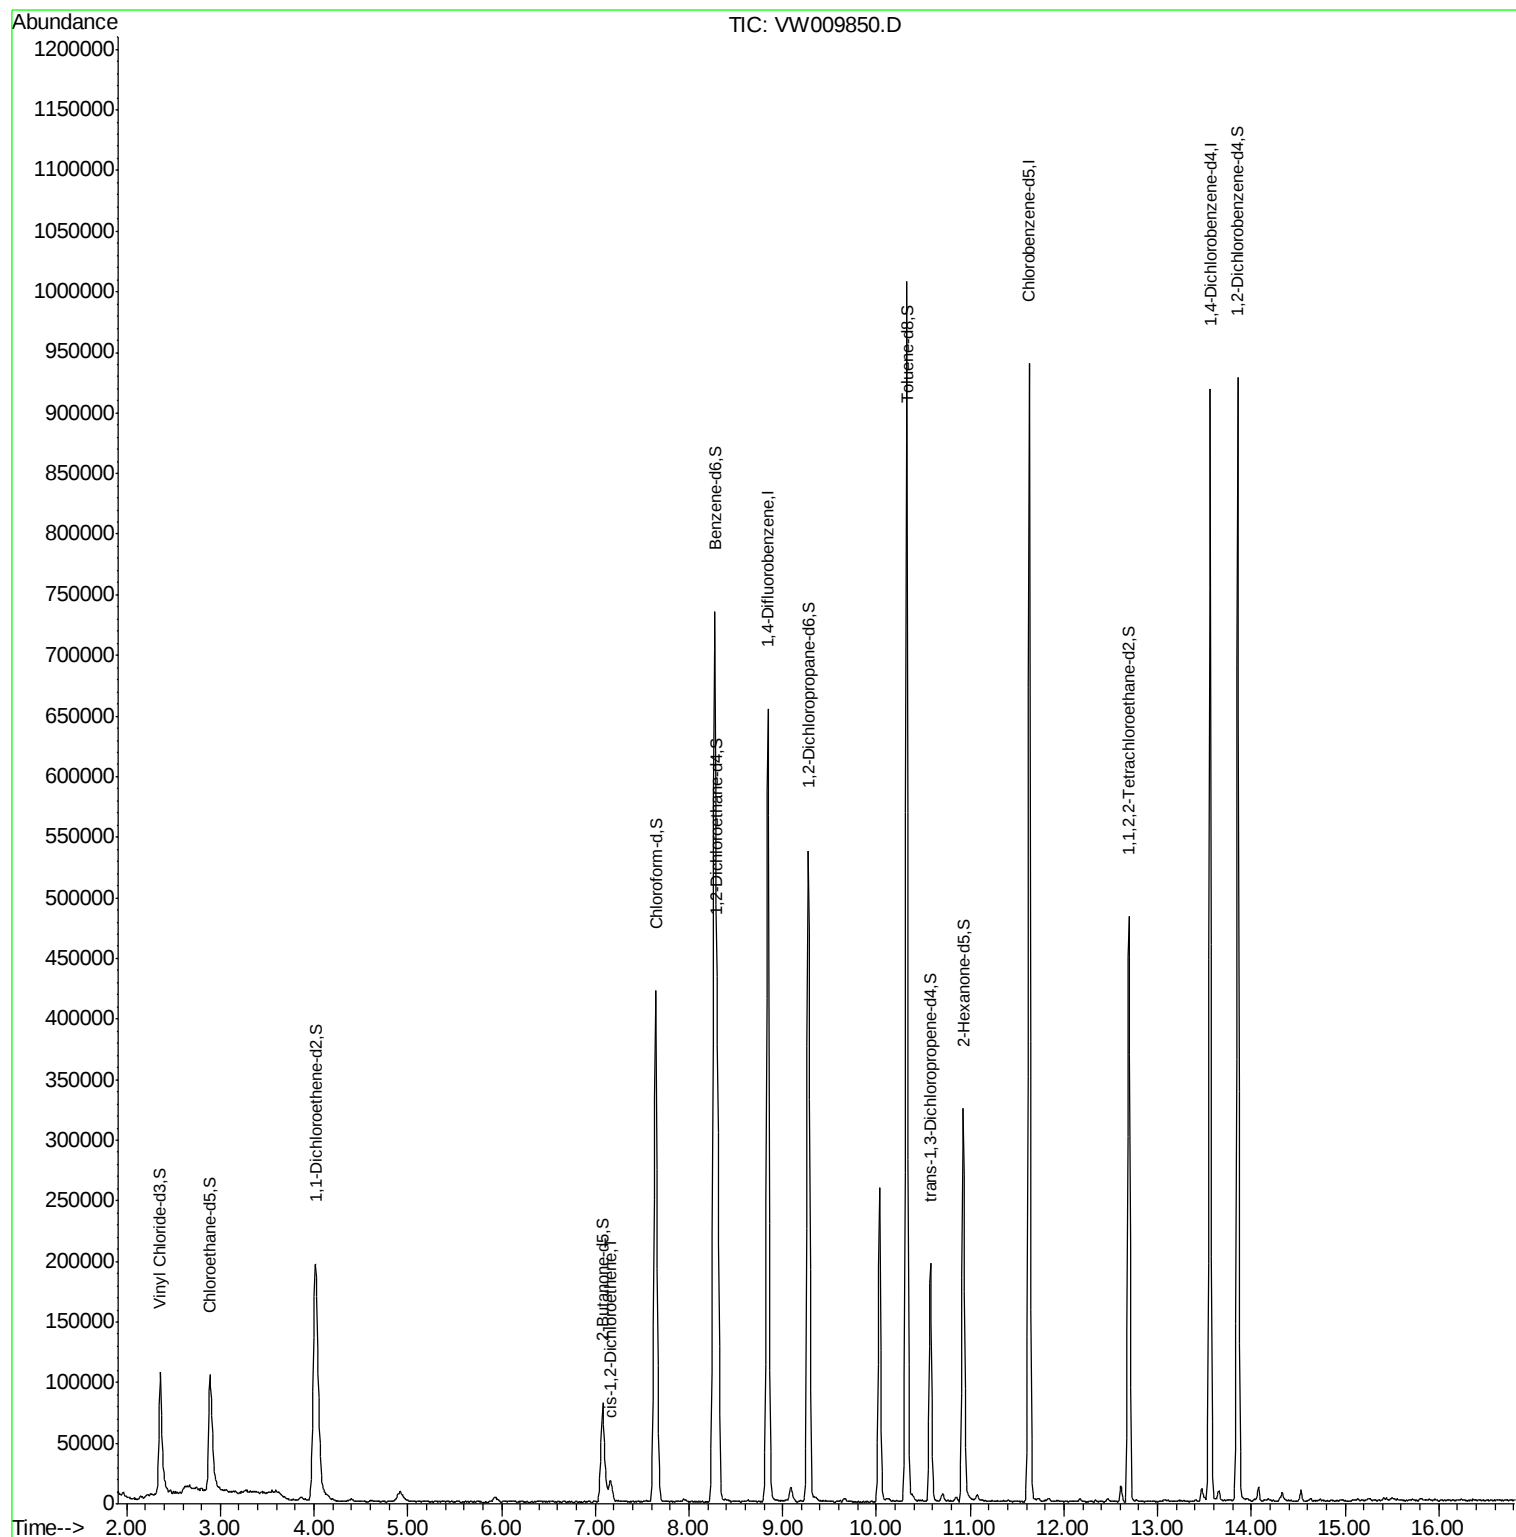

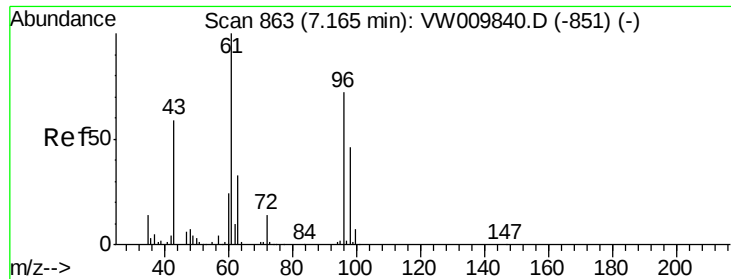

#22

cis-1,2-Dichloroethene
Concen: 0.950 ug/L
RT: 7.16 min Scan# 862
Delta R.T. -0.00 min
Lab File: VW009850.D
Acq: 09 Apr 2019 21:23

Instrument :
MSVOA_W
ClientSampleId :
BF2N6

Tot Ion	Ion	Ratio	Lower	Upper
96	100			
61	113.7	96.8	179.8	
98	51.4	43.5	80.9	

