

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040821\
 Data File : VW018608.D
 Acq On : 08 Apr 2021 17:31
 Operator : SY/VA
 Sample : M1968-15
 Misc : 5.47G/10ML/MSVOA_W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5B7

Manual Integrations
 APPROVED

MMDadoda
 4/9/2021 7:55:46 PM

Quant Time: Apr 09 03:14:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 09 03:11:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	626515	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	571516	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	276292	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	150033	17.21	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	68.84%		
7) Chloroethane-d5	2.891	69	129357	16.95	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	67.80%		
10) 1,1-Dichloroethene-d2	4.025	63	181372	12.05	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.20%		
20) 2-Butanone-d5	7.080	46	65415	33.70	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	67.40%		
24) Chloroform-d	7.646	84	276956	17.36	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	69.44%		
26) 1,2-Dichloroethane-d4	8.311	65	166348	17.86	ug/L	0.01
Spiked Amount 25.000	Range 70 - 130		Recovery =	71.44%		
29) Benzene-d6	8.274	84	532878	17.54	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	70.16%		
33) 1,2-Dichloropropane-d6	9.274	67	158303	18.06	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	72.24%		
37) Toluene-d8	10.323	98	522075	17.85	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	71.40%		
38) trans-1,3-Dichloroprop...	10.579	79	67821	15.01	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	60.04%		
39) 2-Hexanone-d5	10.926	63	54126	31.56	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	63.12%		
48) 1,1,2,2-Tetrachloroeth...	12.694	84	134443	17.15	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	68.60%		
61) 1,2-Dichlorobenzene-d4	13.853	152	171999	17.51	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	70.04%#		
Target Compounds					Qvalue	
13) Acetone	4.129	43	6241m	4.48	ug/L	
16) Methylene chloride	4.915	84	25716	2.50	ug/L	95
44) Toluene	10.390	91	9058	0.24	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040821\
Data File : VW018608.D
Acq On : 08 Apr 2021 17:31
Operator : SY/VA
Sample : M1968-15
Misc : 5.47G/10ML/MSVOA_W/SOIL
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BG5B7

Manual Integrations
APPROVED

MMDadoda
4/9/2021 7:55:46 PM

Quant Time: Apr 09 03:14:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 09 03:11:49 2021
Response via : Initial Calibration

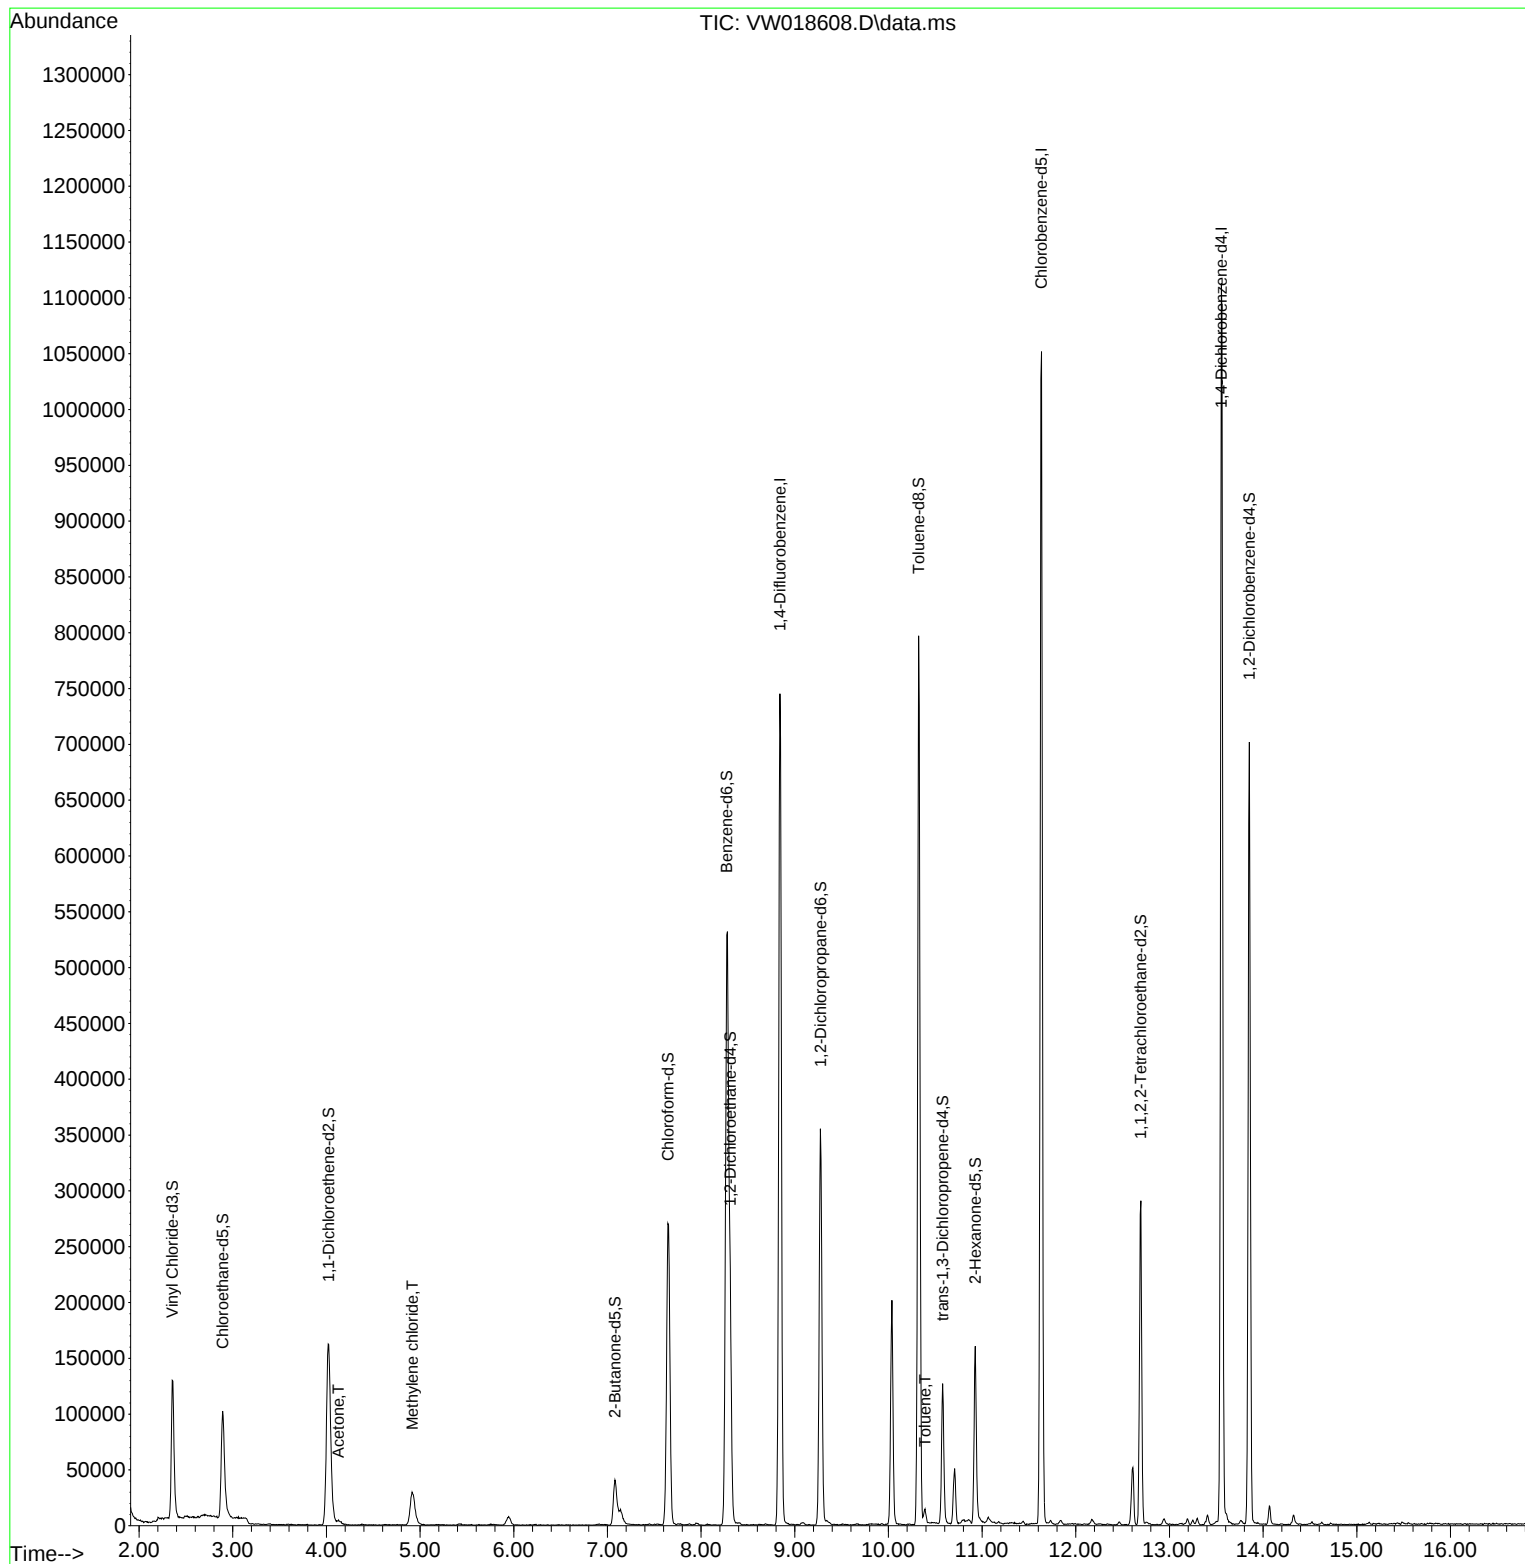

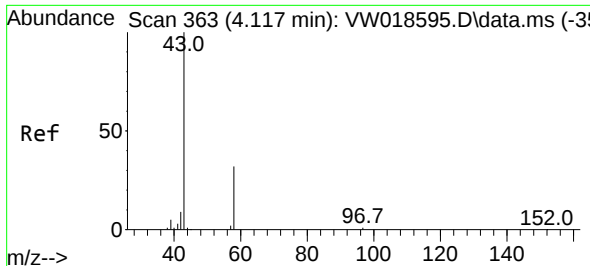





#13
Acetone
Concen: 4.48 ug/L m
RT: 4.129 min Scan# 365
Delta R.T. 0.012 min
Lab File: VW018608.D
Acq: 08 Apr 2021 17:31

Tgt Ion: 43 Resp: 6241
Ion Ratio Lower Upper
43 100
58 20.8 0.0 62.2

Instrument :
MSVOA_W
ClientSampled :
BG5B7




Manual Integrations
APPROVED


MMDadoda
4/9/2021 7:55:46 PM

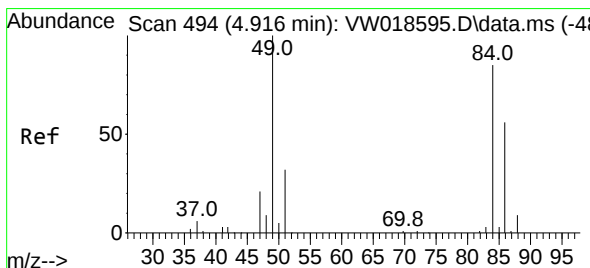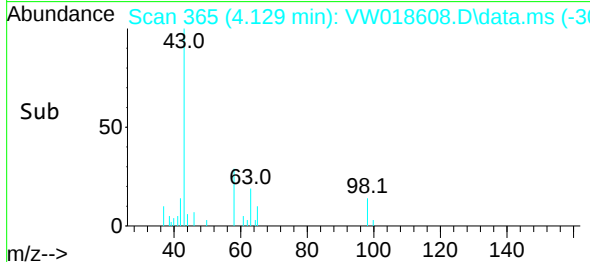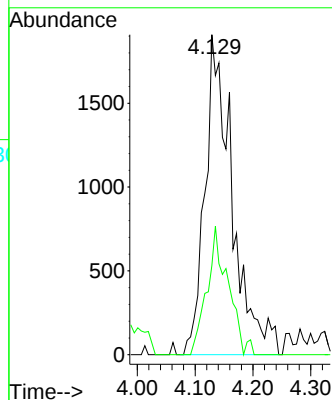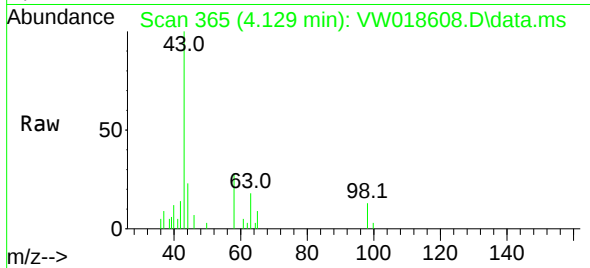

#16
Methylene chloride
Concen: 2.50 ug/L
RT: 4.915 min Scan# 494
Delta R.T. -0.000 min
Lab File: VW018608.D
Acq: 08 Apr 2021 17:31


Tgt Ion: 84 Resp: 25716
Ion Ratio Lower Upper
84 100
49 114.6 74.4 138.2
86 65.4 46.1 85.7

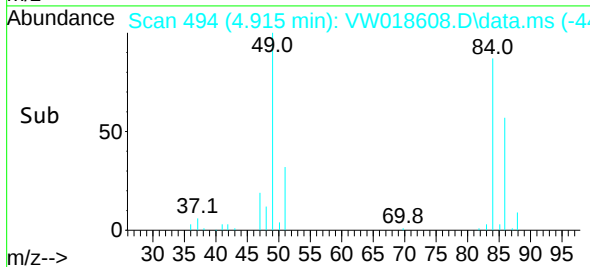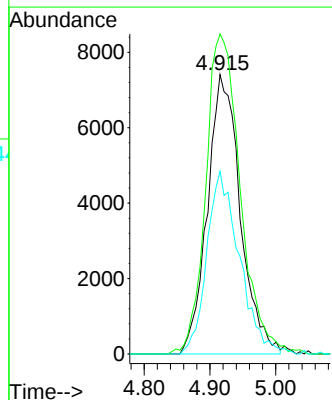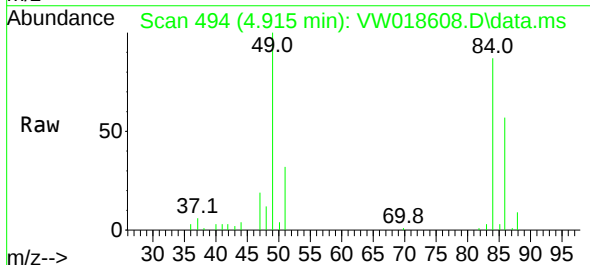

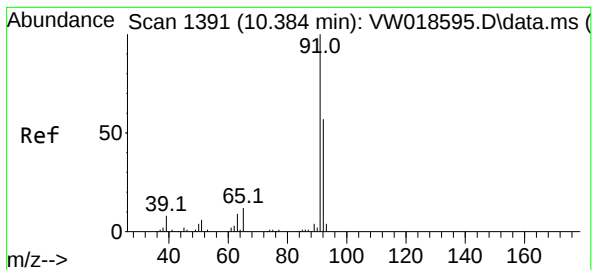

#44
Toluene
Concen: 0.24 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.006 min
Lab File: VW018608.D
Acq: 08 Apr 2021 17:31

Instrument :
MSVOA_W
ClientSampleId :
BG5B7

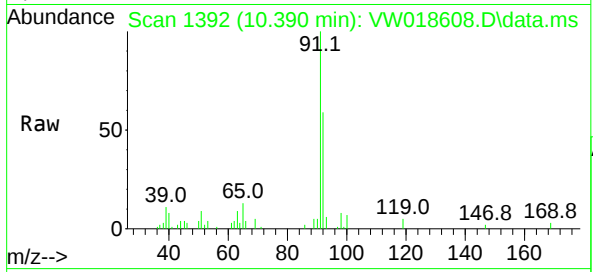

Tgt Ion: 91 Resp: 9058
Ion Ratio Lower Upper
91 100
92 59.3 42.3 78.5

Manual Integrations
APPROVED

MMDadoda
4/9/2021 7:55:46 PM

