
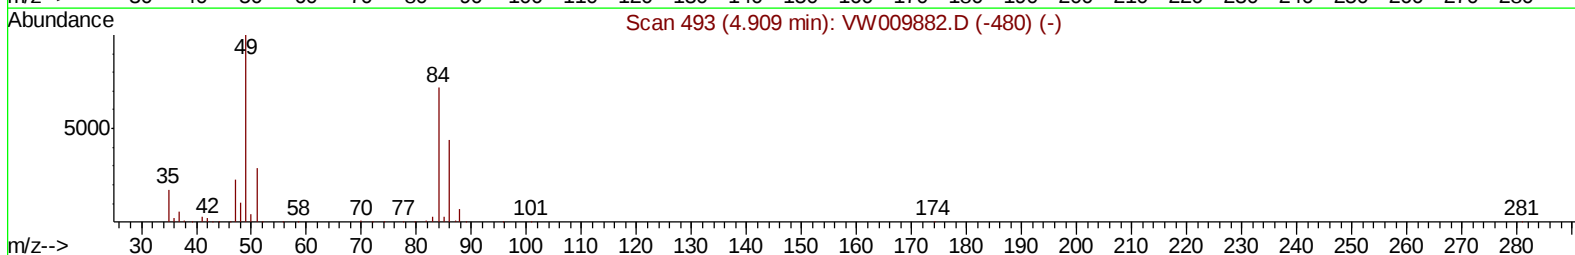
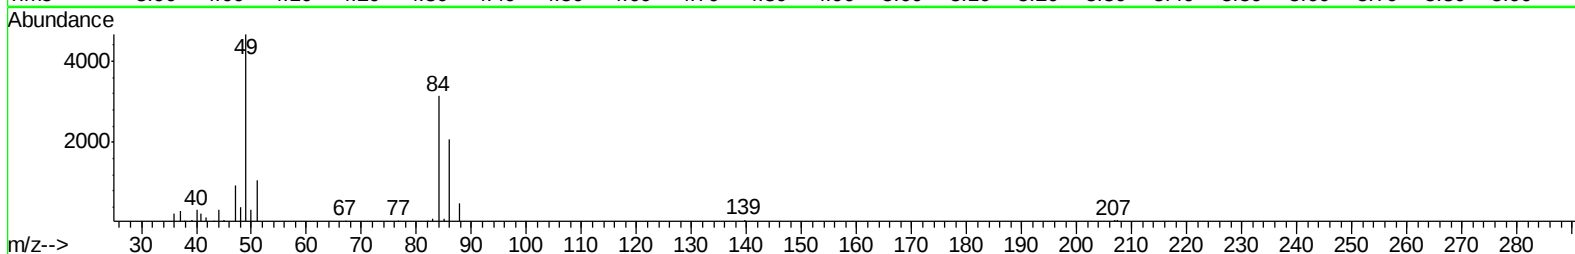


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
Data File : VW009884.D
Acq On : 10 Apr 2019 17:27
Operator : SY/VA
Sample : K2354-01
Misc : 5.72G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 11 04:01:19 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 03:44:42 2019
Response via : Initial Calibration

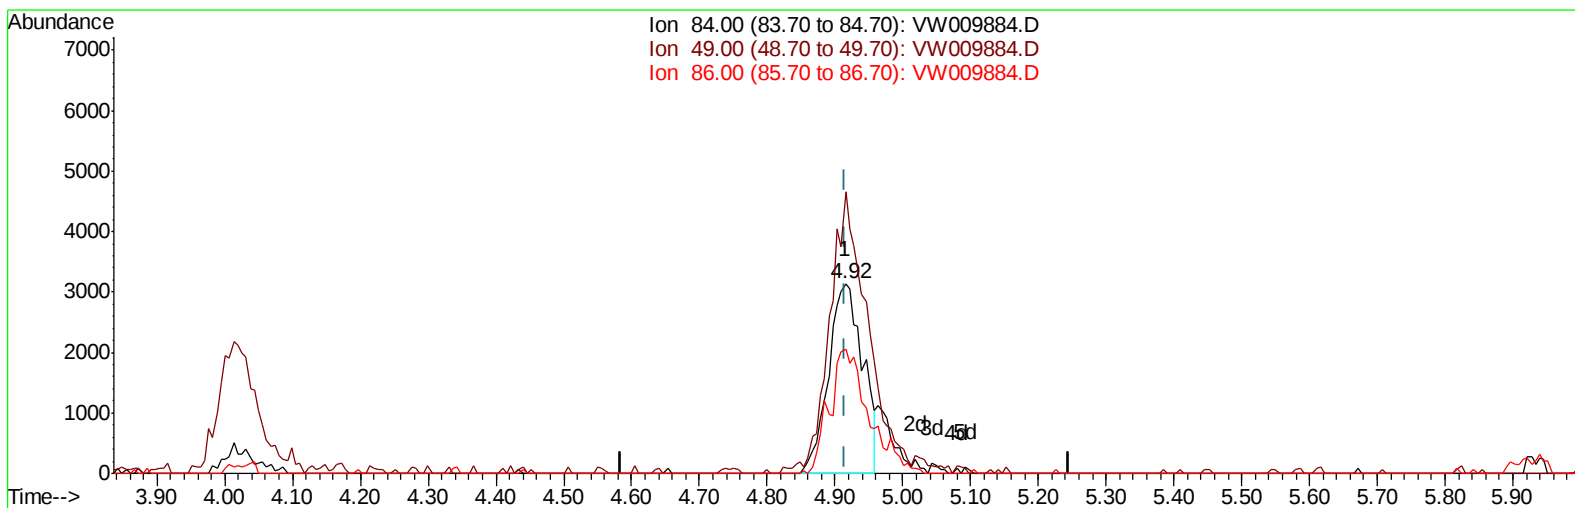

TIC: VW009884.D

(16) Methylene chloride (T)




4.915min (+0.000) 1.55ug/L

response 11069

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	148.47
86.00	66.30	65.65
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
Data File : VW009884.D
Acq On : 10 Apr 2019 17:27
Operator : SY/VA
Sample : K2354-01
Misc : 5.72G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 11 04:01:19 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 03:44:42 2019
Response via : Initial Calibration

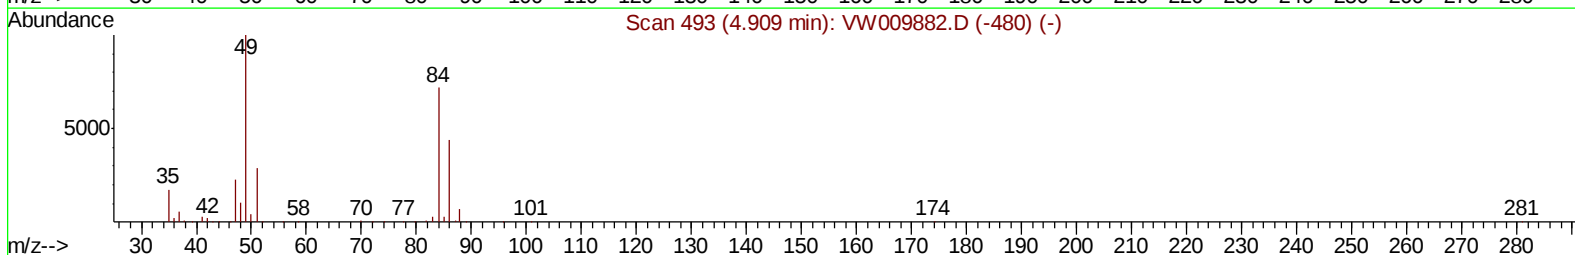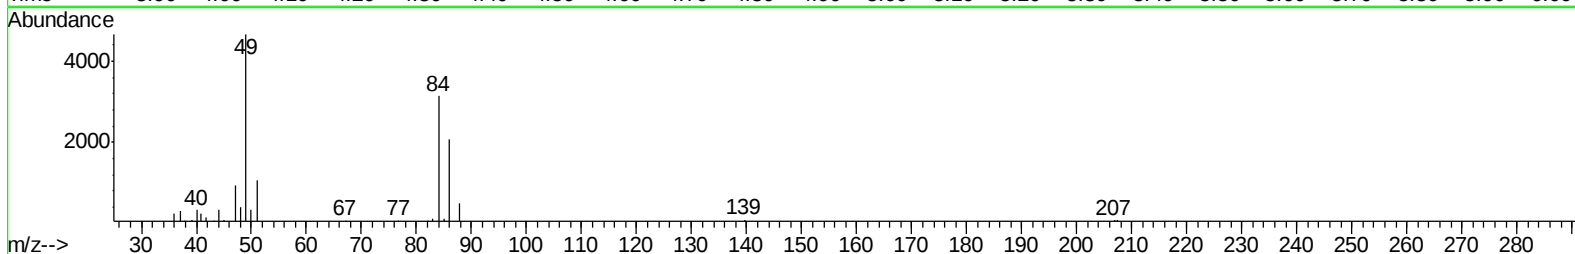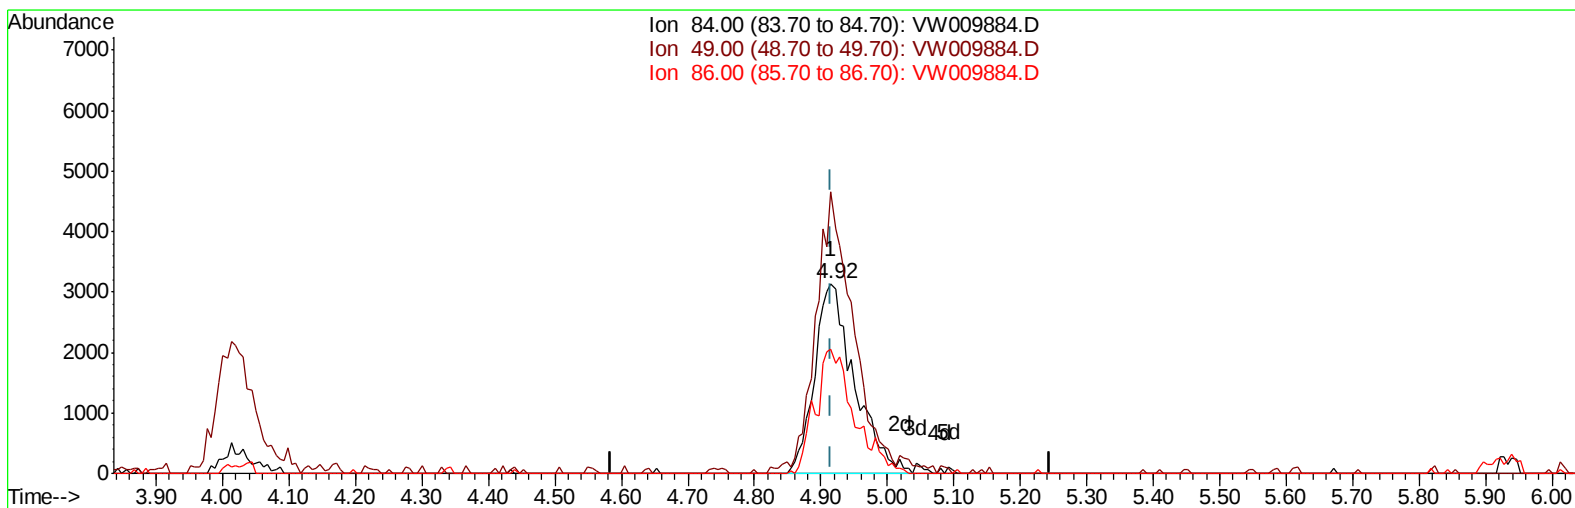

TIC: VW009884.D

(16) Methylene chloride (T)

4.915min (+0.000) 1.82ug/L m

response 13035

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	148.47
86.00	66.30	65.65
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
 Data File : VW009884.D
 Acq On : 10 Apr 2019 17:27
 Operator : SY/VA
 Sample : K2354-01
 Misc : 5.72G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 11 04:02:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 03:44:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	405274	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	392620	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	178059	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	107463	20.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.04%
7) Chloroethane-d5	2.89	69	97836	20.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.56%
10) 1,1-Dichloroethene-d2	4.02	63	211554	18.55	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.20%
20) 2-Butanone-d5	7.07	46	128087	74.39	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	148.78%#
24) Chloroform-d	7.65	84	296226	26.79	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	107.16%
26) 1,2-Dichloroethane-d4	8.31	65	197524	29.09	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	116.36%
29) Benzene-d6	8.27	84	531665	25.80	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.20%
33) 1,2-Dichloropropane-d6	9.27	67	172547	27.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.40%
37) Toluene-d8	10.32	98	455334	23.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.56%
38) trans-1,3-Dichloropropene-	10.58	79	77222	25.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.72%
39) 2-Hexanone-d5	10.93	63	94605	78.84	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	157.68%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	179065	30.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.04%#
61) 1,2-Dichlorobenzene-d4	13.86	152	180317	28.86	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	115.44%

Target Compounds					Qvalue
12) 1,1-Dichloroethene	4.04	96	18261	3.392 ug/L #	1
13) Acetone	4.12	43	8846	4.795 ug/L	78
47) Tetrachloroethene	10.86	164	1703273	349.829 ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
Data File : VW009884.D
Acq On : 10 Apr 2019 17:27
Operator : SY/VA
Sample : K2354-01
Misc : 5.72G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 11 04:02:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 03:44:42 2019
Response via : Initial Calibration

