


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
Data File : VW009890.D
Acq On : 10 Apr 2019 20:11
Operator : SY/VA
Sample : K2340-13
Misc : 5.17G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF2N7

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:33:15 AM

Quant Time: Apr 11 05:41:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 03:44:42 2019
Response via : Initial Calibration

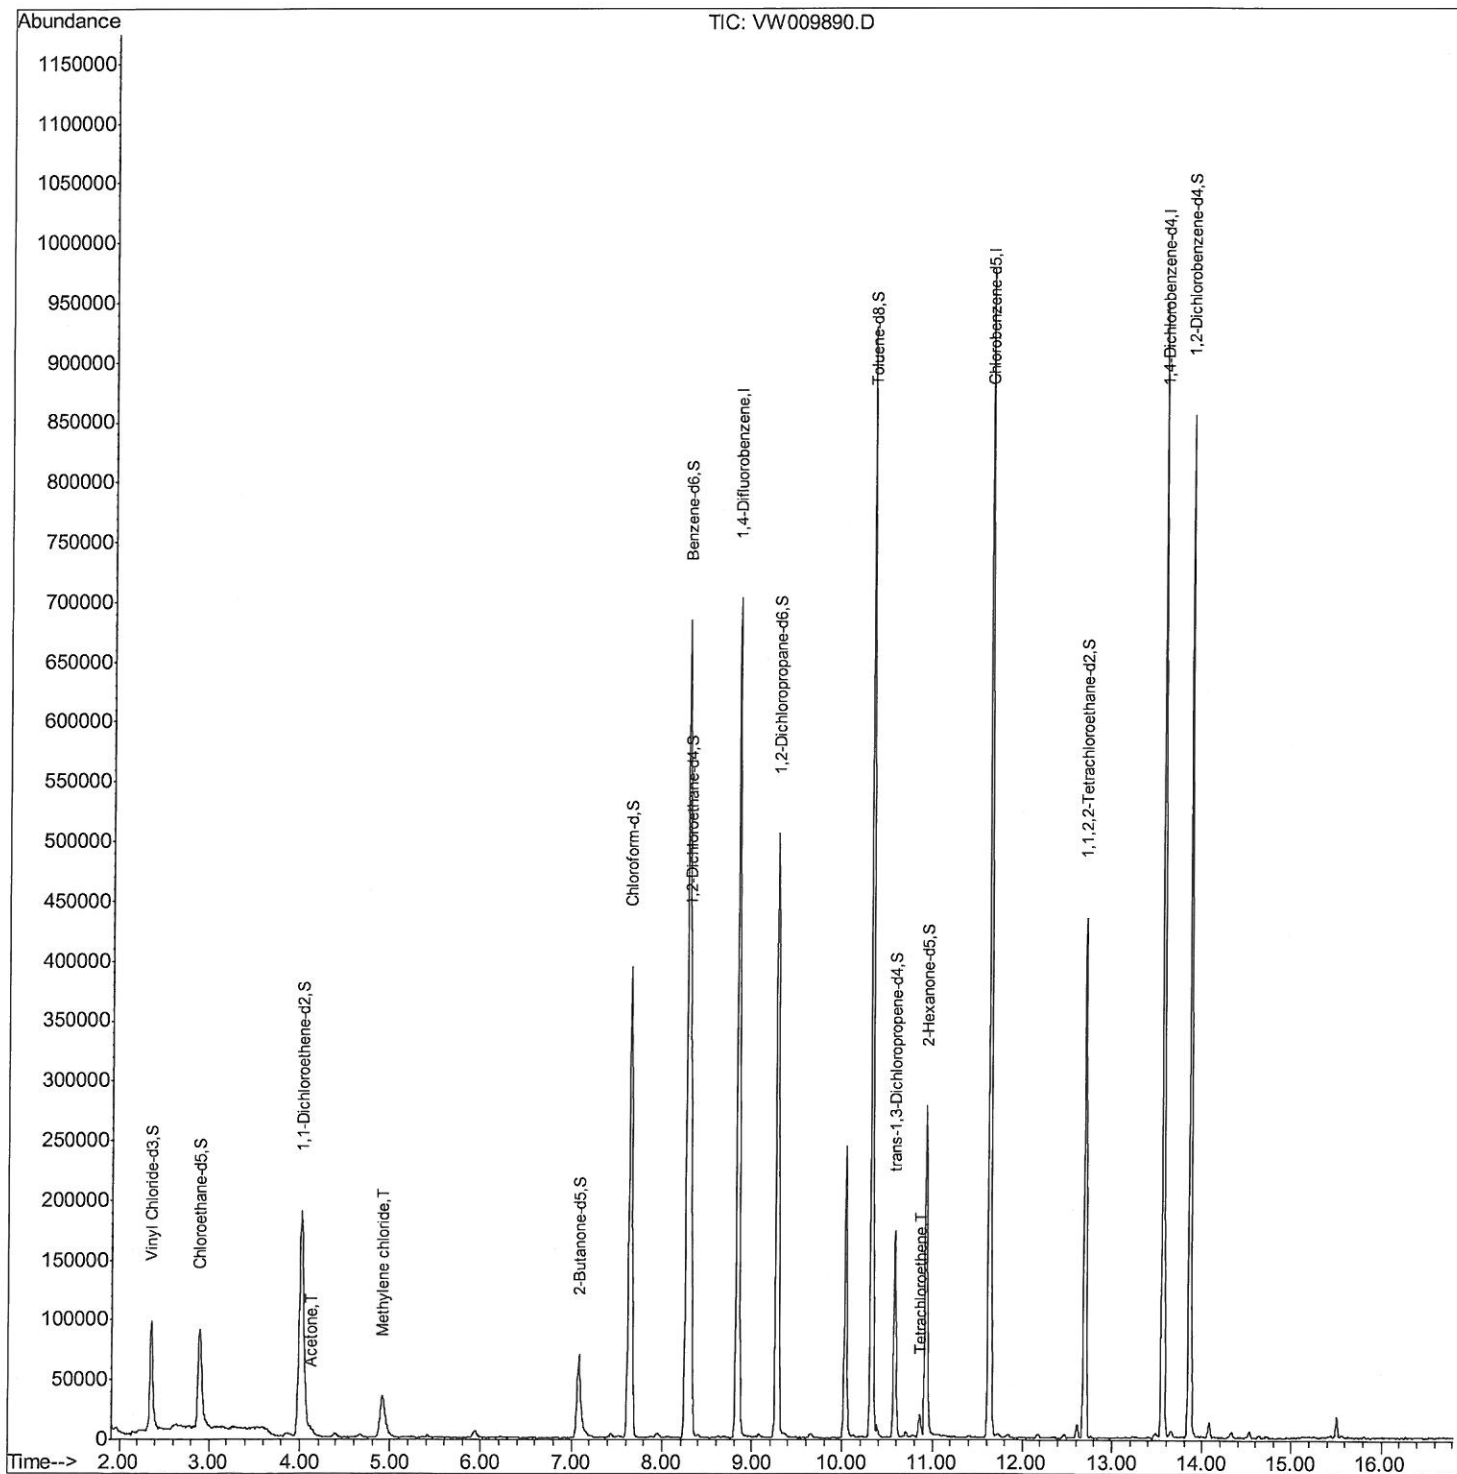

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
 Data File : VW009890.D
 Acq On : 10 Apr 2019 20:11
 Operator : SY/VA
 Sample : K2340-13
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF2N7

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:33:15 AM

Quant Time: Apr 11 03:48:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 03:44:42 2019
 Response via : Initial Calibration

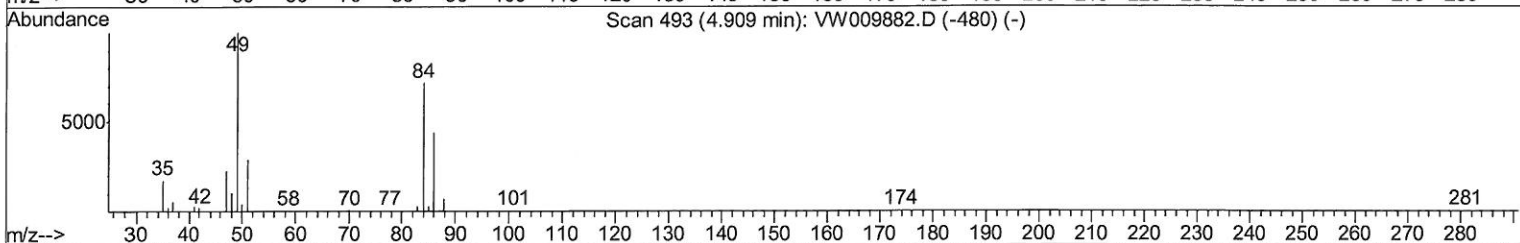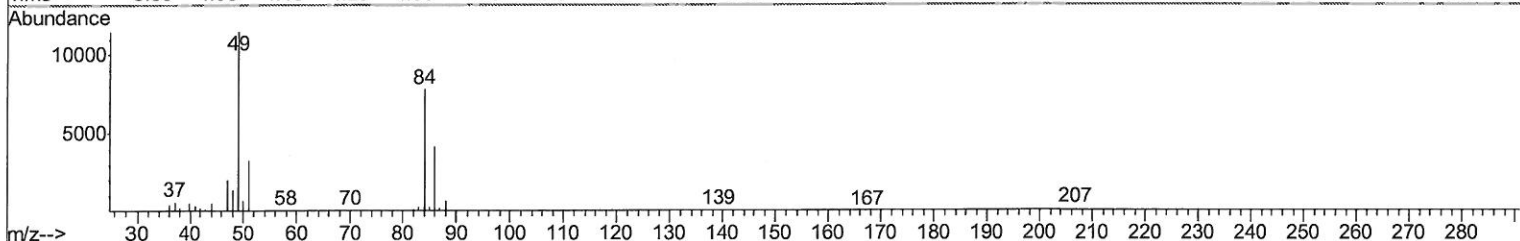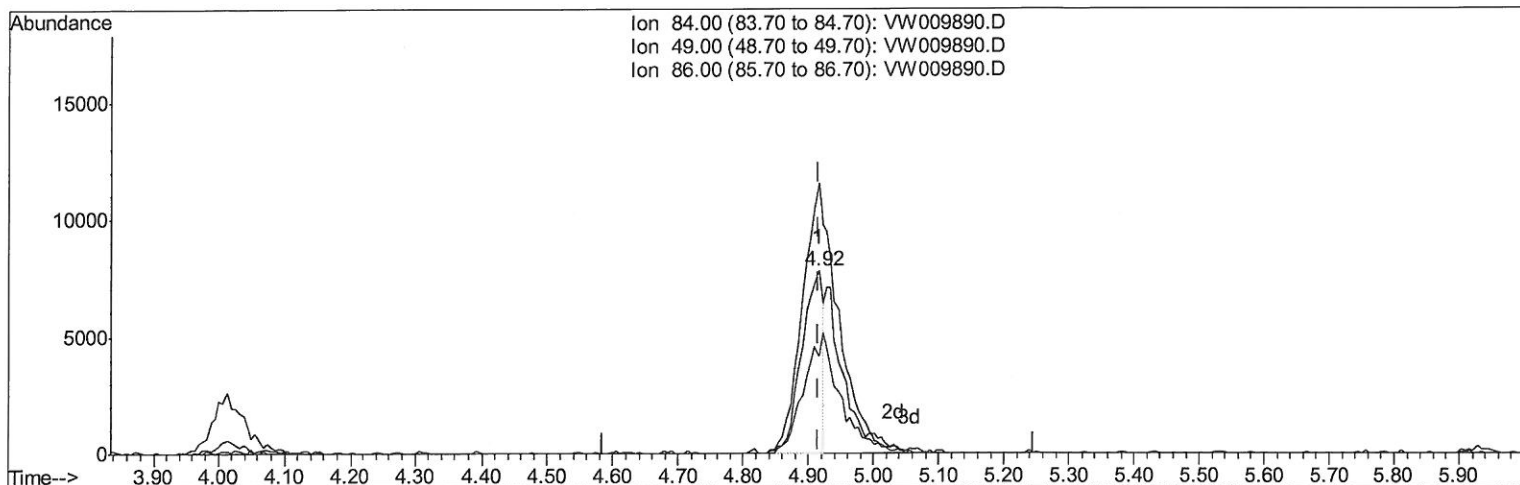

TIC: VW009890.D

(16) Methylene chloride (T)

4.915min (+0.000) 1.86ug/L

response 17395

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	147.69
86.00	66.30	53.22
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
 Data File : VW009890.D
 Acq On : 10 Apr 2019 20:11
 Operator : SY/VA
 Sample : K2340-13
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF2N7

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:33:15 AM

Quant Time: Apr 11 03:48:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 03:44:42 2019
 Response via : Initial Calibration

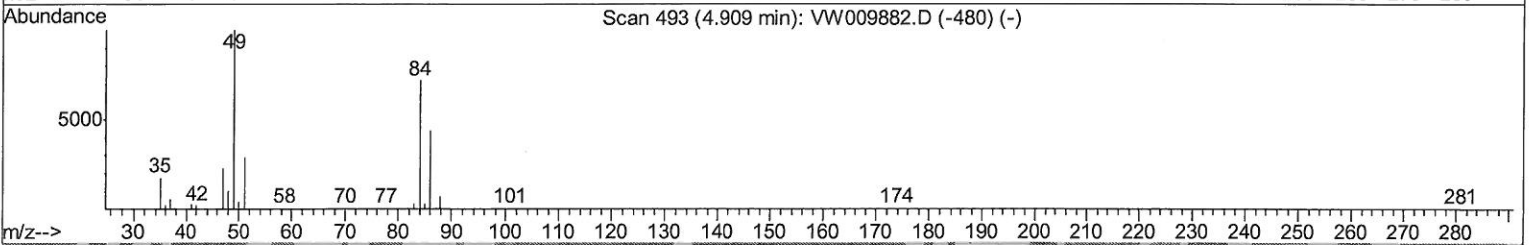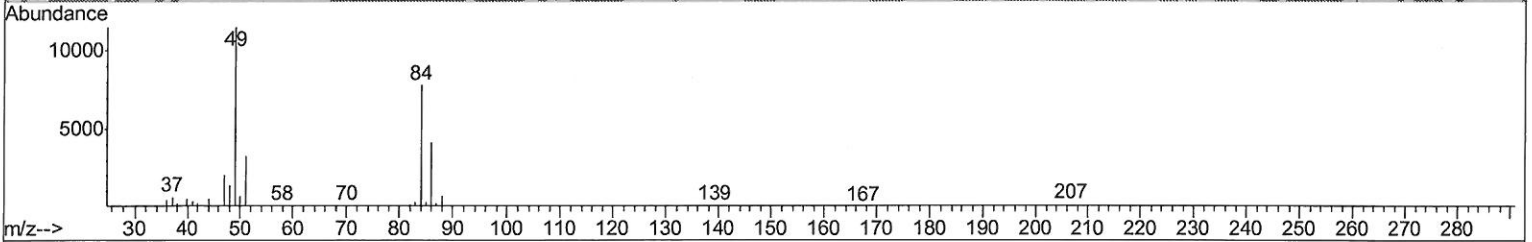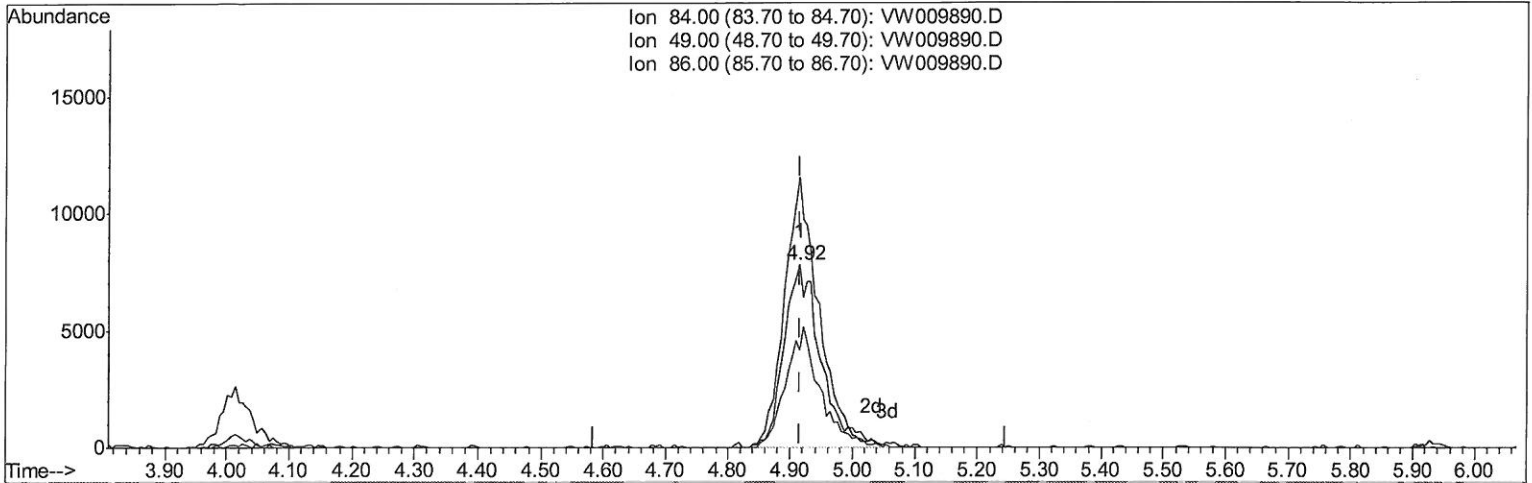

TIC: VW009890.D

(16) Methylene chloride (T)

4.915min (+0.000) 3.41ug/L m

response 31860

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	147.69
86.00	66.30	53.22
0.00	0.00	0.00

MMD
4/13/19

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
 Data File : VW009890.D
 Acq On : 10 Apr 2019 20:11
 Operator : SY/VA
 Sample : K2340-13
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BF2N7

Manual Integrations
APPROVED

MMDadoda
 4/15/2019 12:33:15 AM

Quant Time: Apr 11 03:48:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 03:44:42 2019
 Response via : Initial Calibration

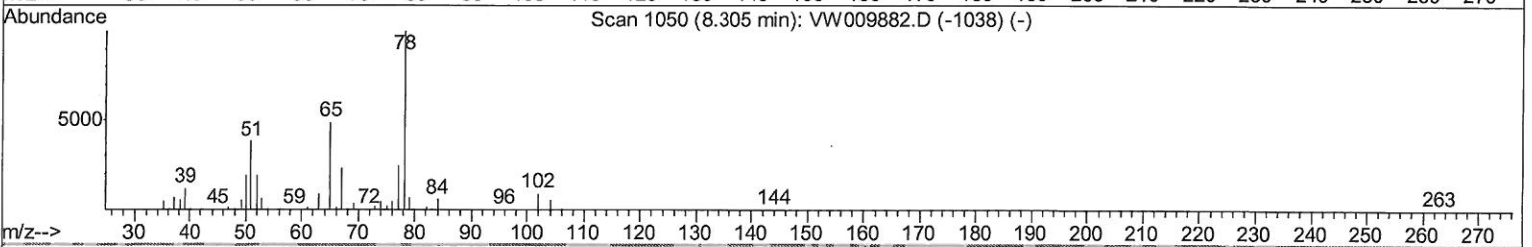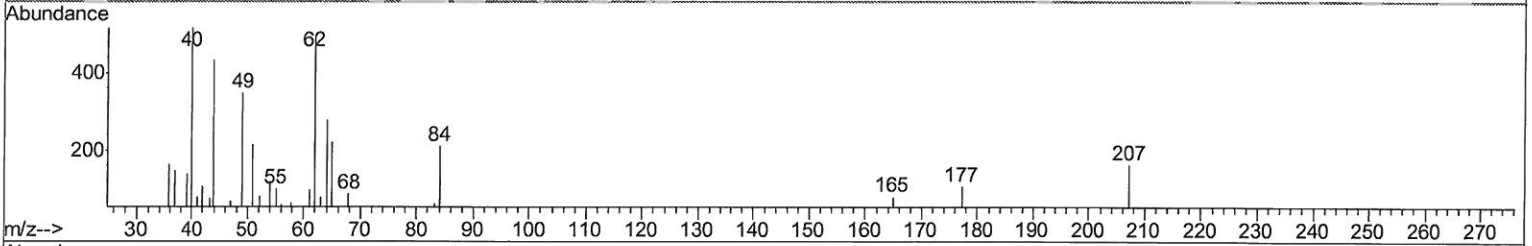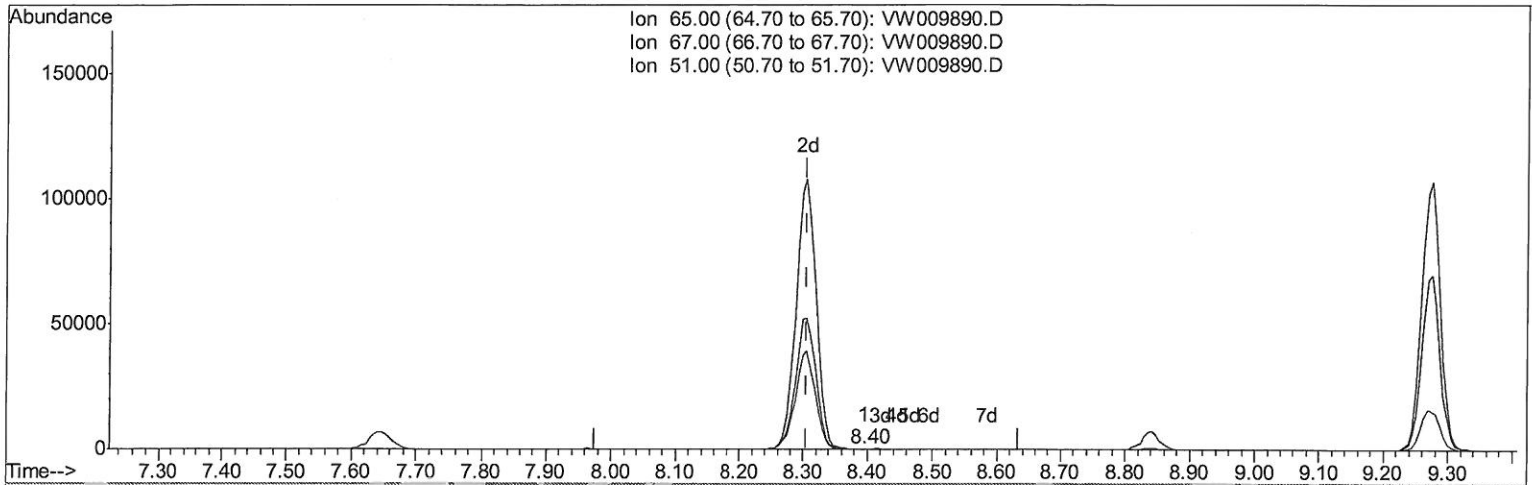

TIC: VW009890.D

(26) 1,2-Dichloroethane-d4 (S)

8.397min (+0.092) 0.02ug/L

response 204

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	46.08
51.00	109.90	139.71
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
 Data File : VW009890.D
 Acq On : 10 Apr 2019 20:11
 Operator : SY/VA
 Sample : K2340-13
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF2N7

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:33:15 AM

Quant Time: Apr 11 03:48:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 03:44:42 2019
 Response via : Initial Calibration

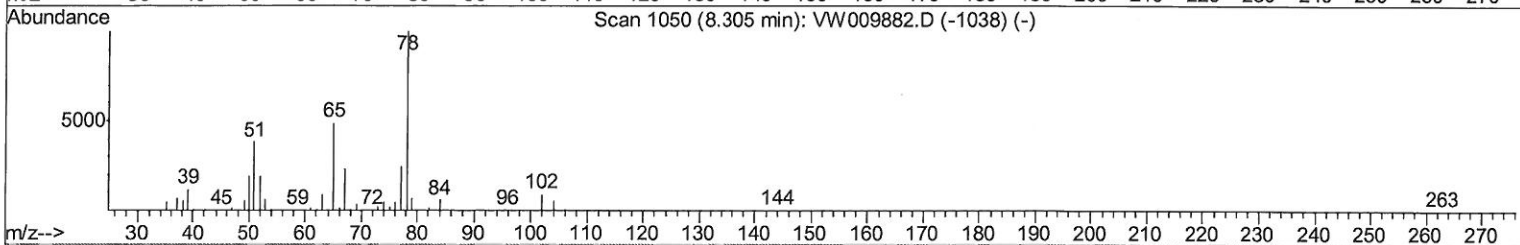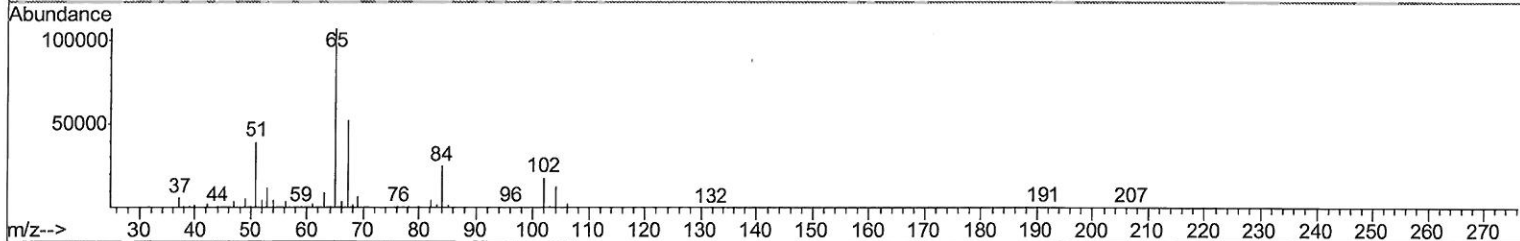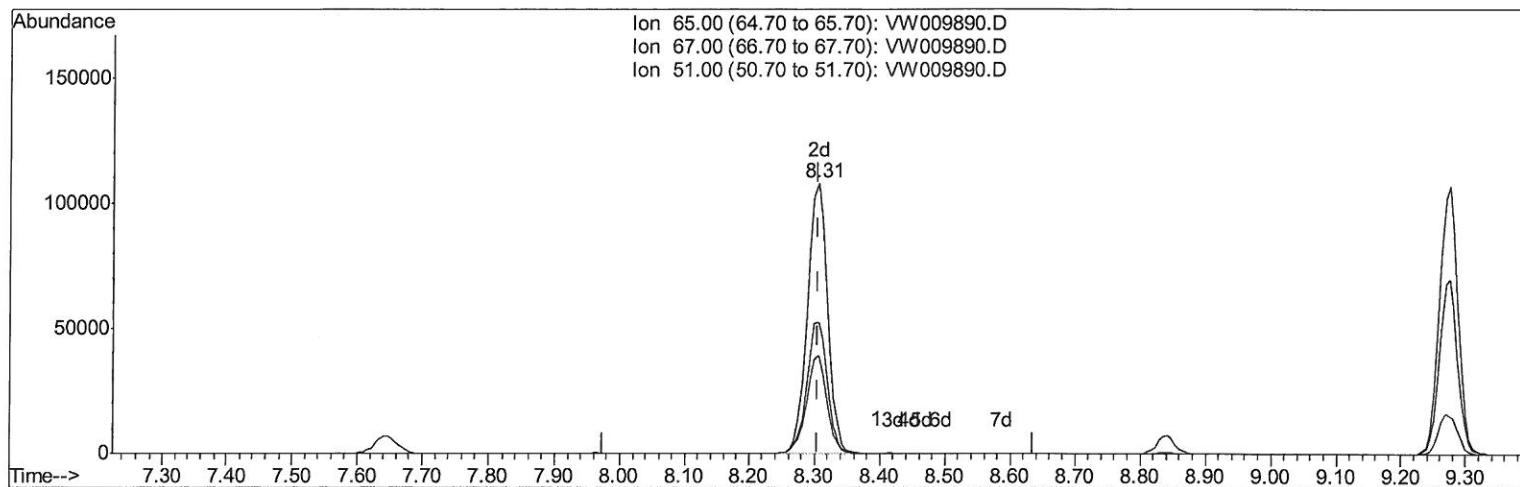

TIC: VW009890.D

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.000) 26.14ug/L m

response 232246

7 MD
 4/13/19

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	0.04#
51.00	109.90	0.12#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041019\
 Data File : VW009890.D
 Acq On : 10 Apr 2019 20:11
 Operator : SY/VA
 Sample : K2340-13
 Misc : 5.17G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF2N7

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:33:15 AM

Quant Time: Apr 11 05:41:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 03:44:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	530327	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	511741	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	218750	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	126345	18.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.84%
7) Chloroethane-d5	2.89	69	121842	19.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.64%
10) 1,1-Dichloroethene-d2	4.01	63	243537	16.32	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.28%
20) 2-Butanone-d5	7.07	46	117934	52.34	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.68%
24) Chloroform-d	7.65	84	368245	25.45	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.80%
26) 1,2-Dichloroethane-d4	8.31	65	232246m	26.14	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.56%
29) Benzene-d6	8.27	84	657865	24.49	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.96%
33) 1,2-Dichloropropane-d6	9.27	67	212870	25.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.60%
37) Toluene-d8	10.32	98	573252	23.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.32%
38) trans-1,3-Dichloropropene-	10.58	79	85964	21.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.88%
39) 2-Hexanone-d5	10.93	63	75461	48.25	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.50%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	193366	25.07	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.28%
61) 1,2-Dichlorobenzene-d4	13.86	152	211518	27.56	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.24%

MD
 4/13/19

Target Compounds

Target Compounds					Qvalue
13) Acetone	4.12	43	8762	3.629 ug/L	98
16) Methylene chloride	4.92	84	31860m	3.406 ug/L	
47) Tetrachloroethene	10.86	164	3638	0.573 ug/L	90

MD
 4/13/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed