

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041020\
Data File : VW015179.D
Acq On : 10 Apr 2020 14:24
Operator : SY/VA
Sample : VW0410SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VBLK19

Manual Integrations
APPROVED

MMDadoda
4/14/2020 4:02:43 PM

Quant Time: Apr 11 06:28:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041020S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 10 13:10:27 2020
Response via : Initial Calibration

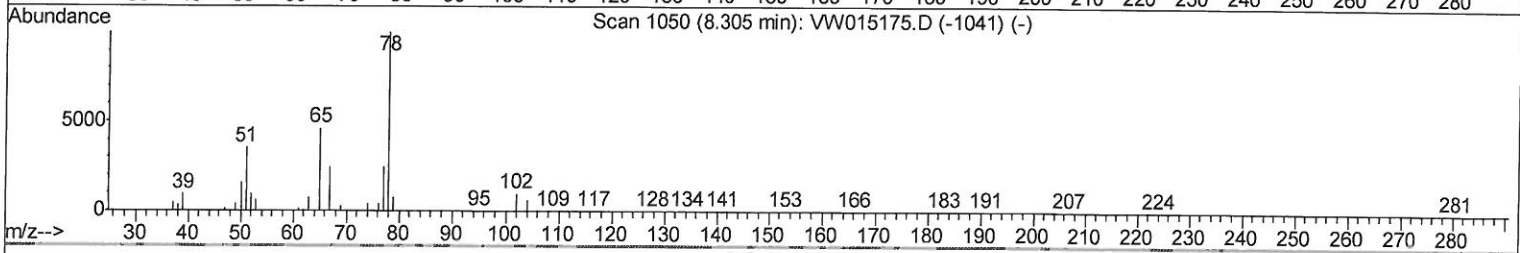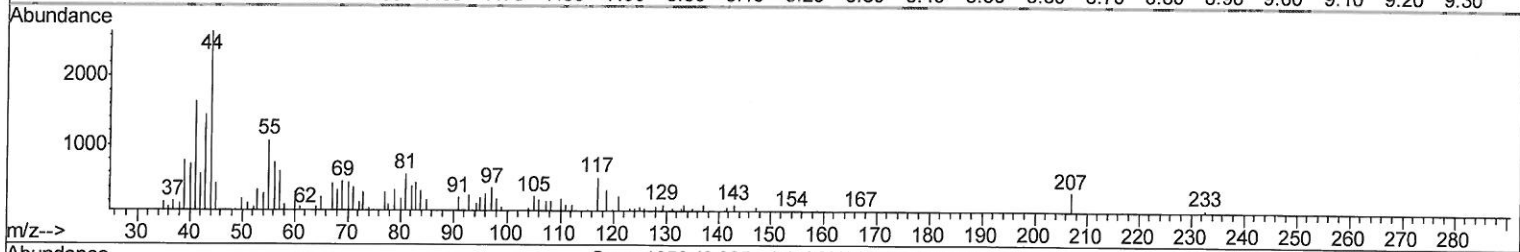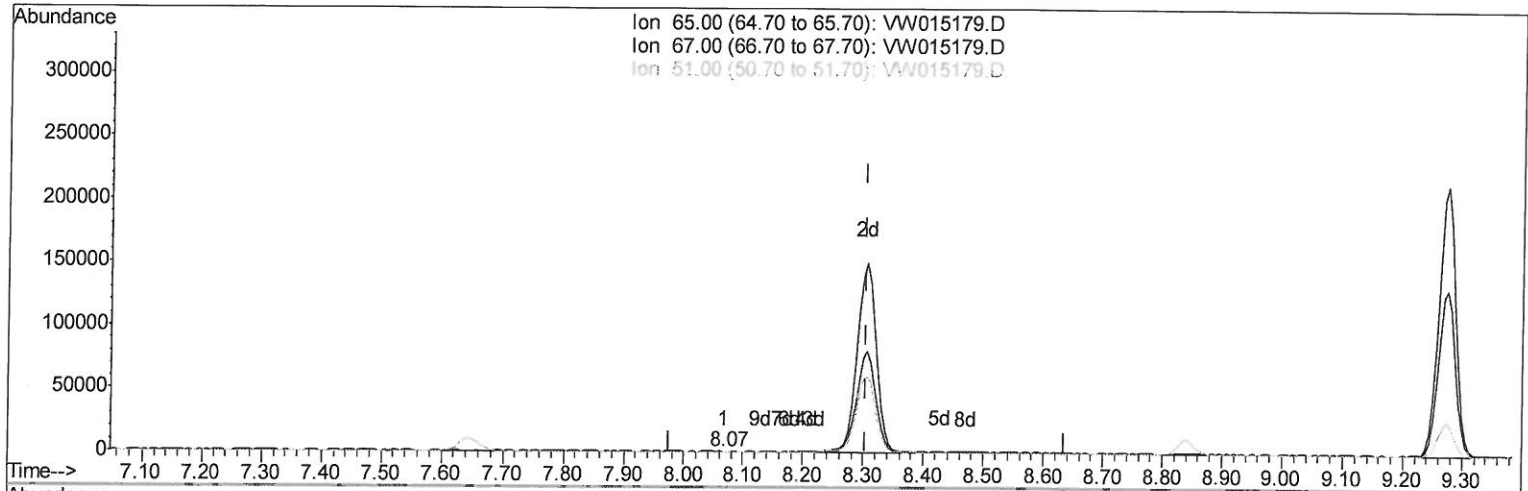

TIC: VW015179.D

(26) 1,2-Dichloroethane-d4 (S)

8.067min (-0.238) 0.01ug/L

response 164

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	58.54
51.00	117.30	142.07
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041020\
 Data File : VW015179.D
 Acq On : 10 Apr 2020 14:24
 Operator : SY/VA
 Sample : VW0410SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK19

Manual Integrations
 APPROVED

MMDadoda
 4/14/2020 4:02:43 PM

Quant Time: Apr 11 06:28:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041020S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 10 13:10:27 2020
 Response via : Initial Calibration

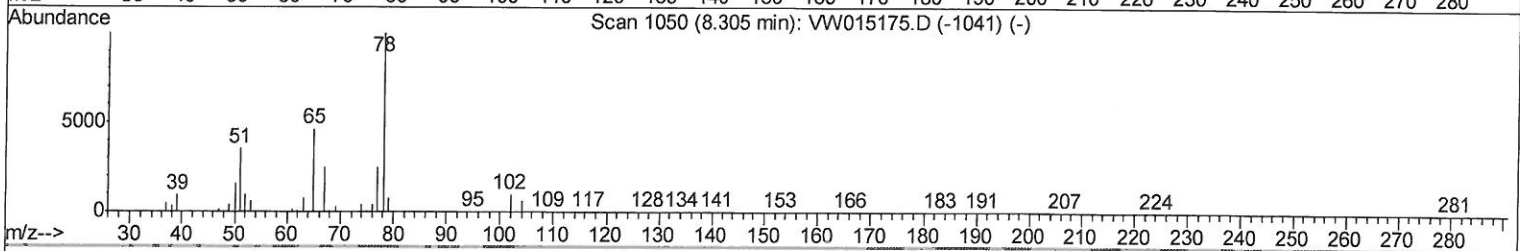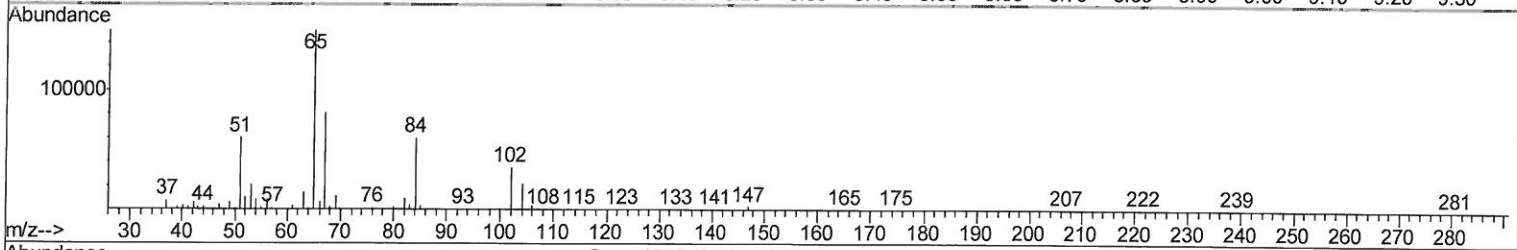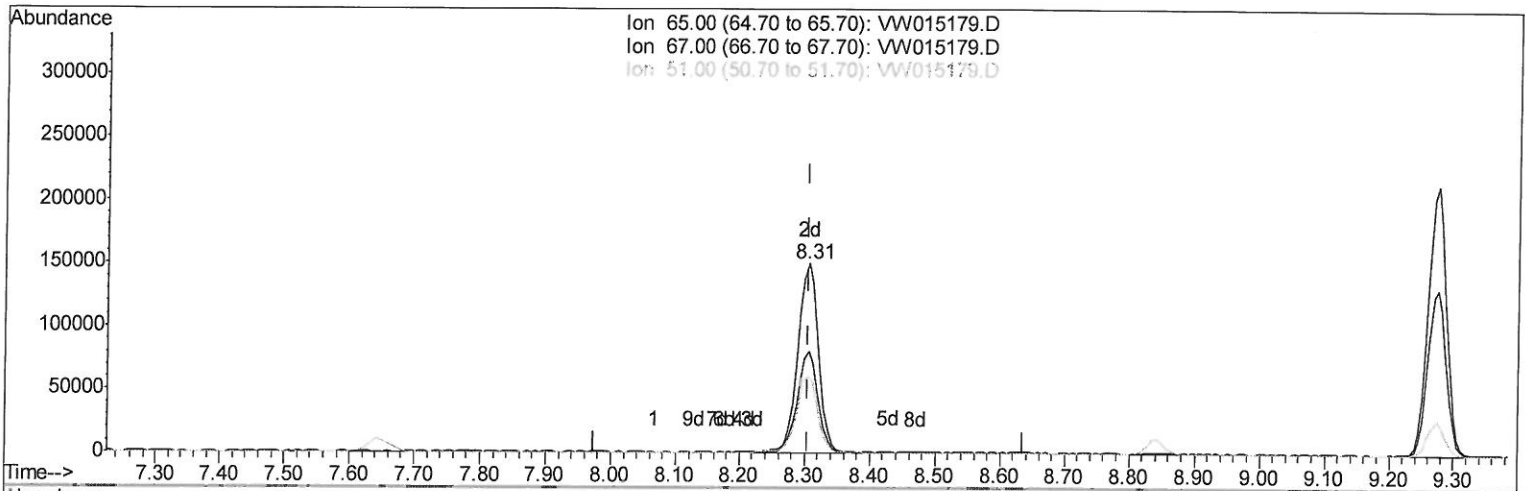

TIC: VW015179.D

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 24.12ug/L m

response 328614

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	0.03#
51.00	117.30	0.07#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041020\
 Data File : VW015179.D
 Acq On : 10 Apr 2020 14:24
 Operator : SY/VA
 Sample : VW0410SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK19

Manual Integrations
 APPROVED

MMDadoda
 4/14/2020 4:02:43 PM

Quant Time: Apr 11 06:39:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041020S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 10 13:10:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	1166618	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1025750	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	443279	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	262660	23.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.24%
7) Chloroethane-d5	2.89	69	187162	23.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.56%
10) 1,1-Dichloroethene-d2	4.02	63	471236	16.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.52%
20) 2-Butanone-d5	7.07	46	179803	47.64	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.28%
24) Chloroform-d	7.65	84	617890	22.46	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.84%
26) 1,2-Dichloroethane-d4	8.31	65	328614m	24.12	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.48%
29) Benzene-d6	8.27	84	1370156	24.14	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.56%
33) 1,2-Dichloropropane-d6	9.27	67	419808	23.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.68%
37) Toluene-d8	10.32	98	1264737	23.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.12%
38) trans-1,3-Dichloropropene-	10.57	79	184179	23.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.00%
39) 2-Hexanone-d5	10.92	63	151121	48.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	303785	23.68	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.72%
61) 1,2-Dichlorobenzene-d4	13.85	152	386692	24.34	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.36%

04/14/2020

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041020\
Data File : VW015179.D
Acq On : 10 Apr 2020 14:24
Operator : SY/VA
Sample : VW0410SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK19

Manual Integrations
APPROVED

MMDadoda
4/14/2020 4:02:43 PM

Quant Time: Apr 11 06:39:48 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM041020S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 10 13:10:27 2020
Response via : Initial Calibration

