
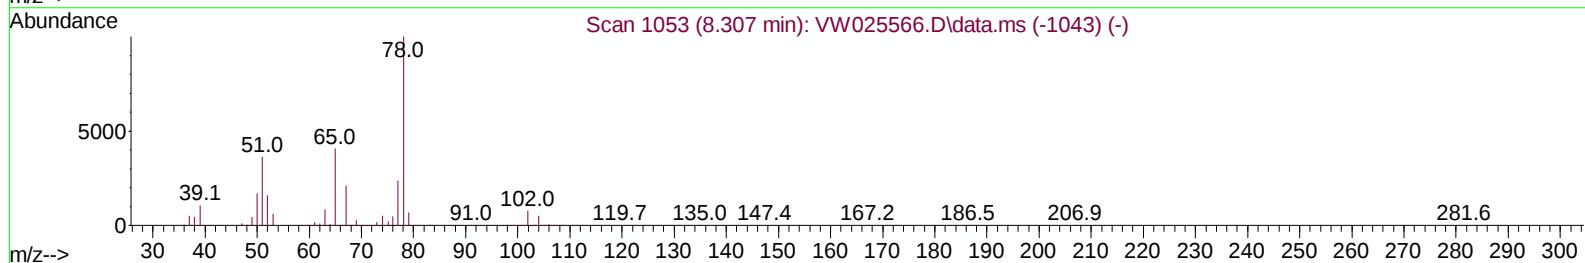
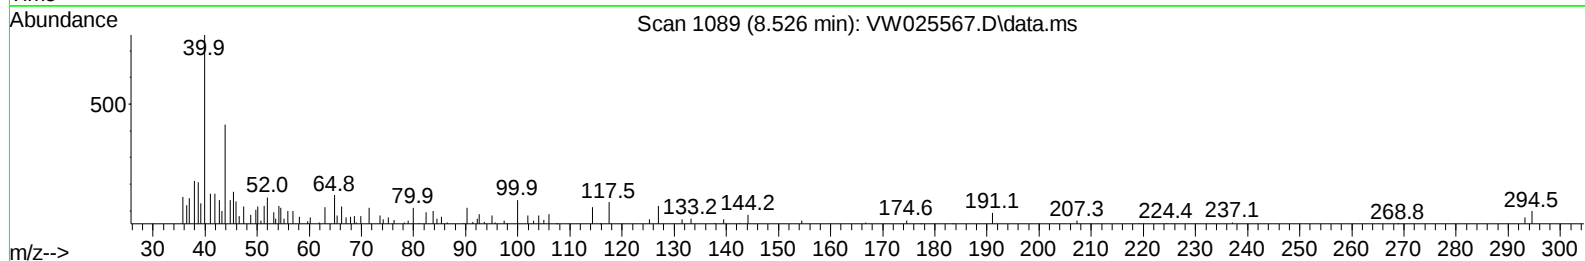


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041023\
 Data File : VW025567.D
 Acq On : 10 Apr 2023 10:37
 Operator : SY/MD
 Sample : VW0410SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 01:57:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 11 01:56:03 2023
 Response via : Initial Calibration

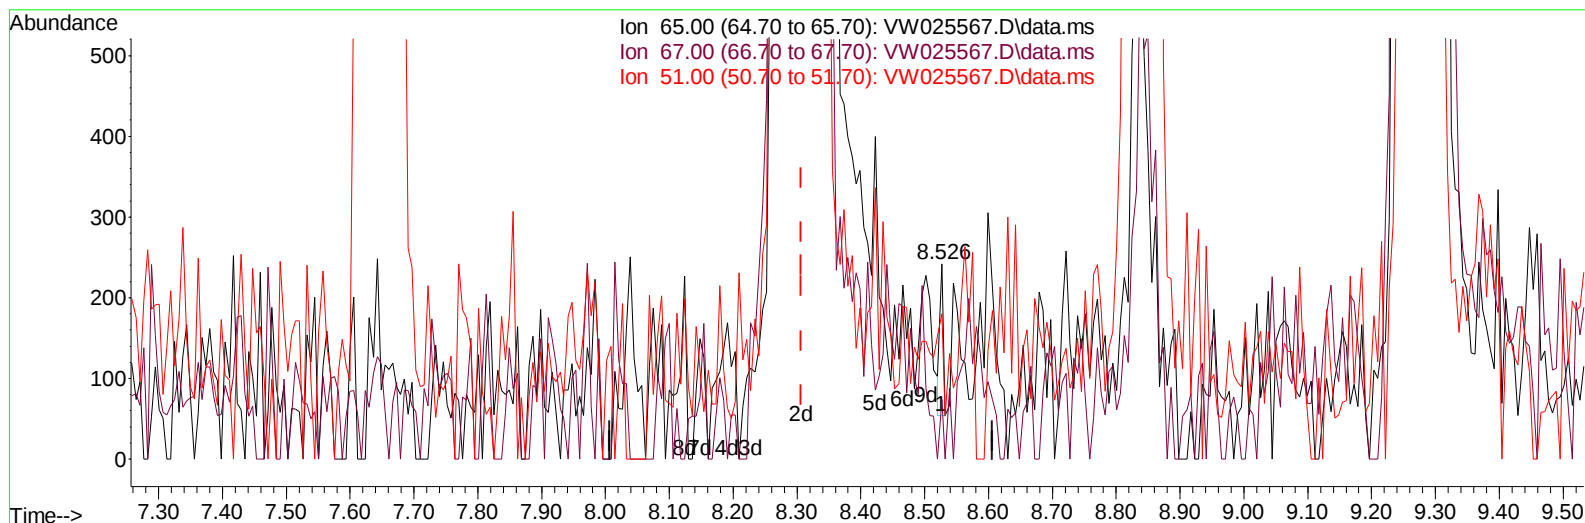

TIC: VW025567.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.526min (+ 0.220) 0.01 ug/L

response 69

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.50	39.13
51.00	124.00	120.29
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041023\
 Data File : VW025567.D
 Acq On : 10 Apr 2023 10:37
 Operator : SY/MD
 Sample : VW0410SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 01:57:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 11 01:56:03 2023
 Response via : Initial Calibration

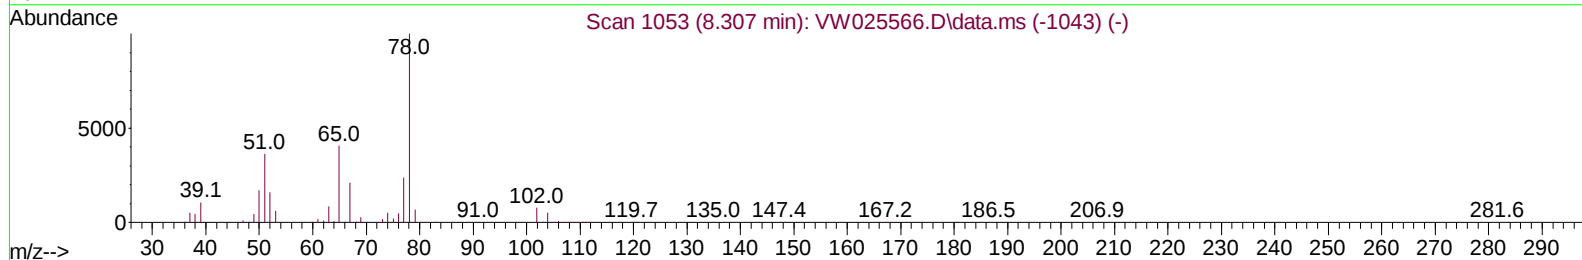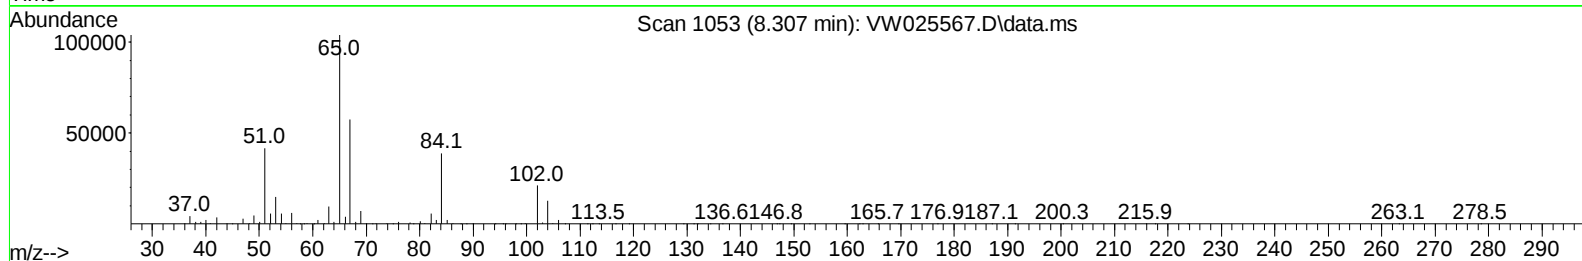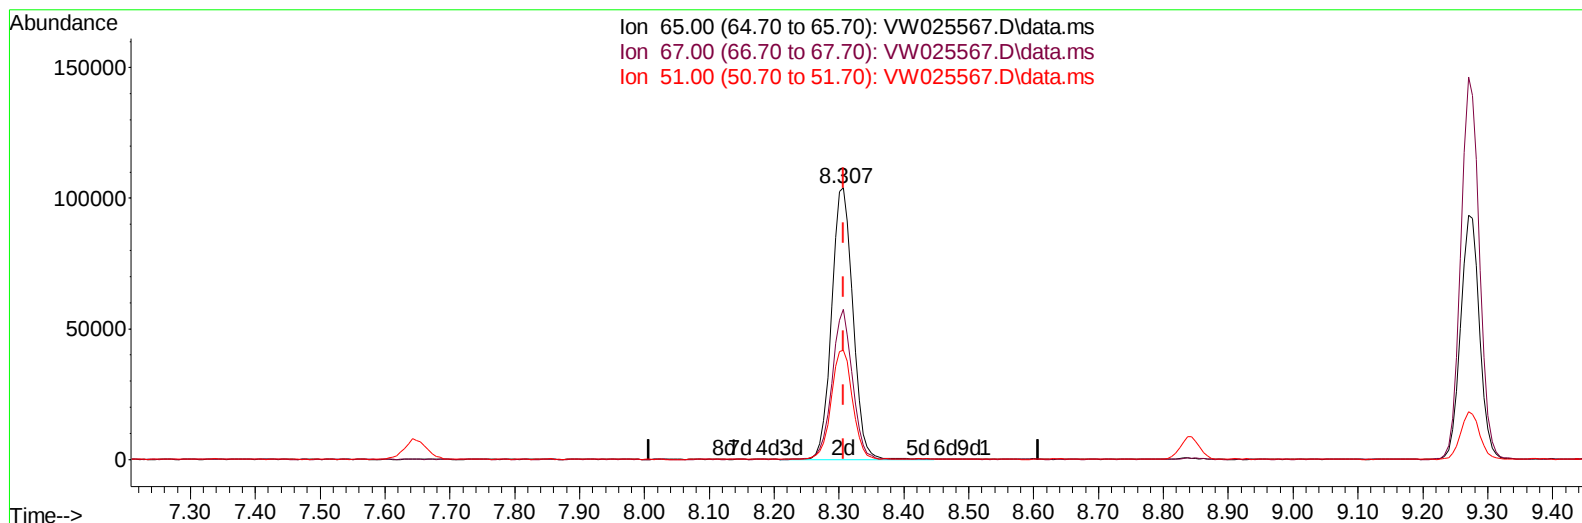

TIC: VW025567.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.307min (+ 0.000) 20.82 ug/L m****response 237488**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.50	0.01#
51.00	124.00	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041023\
 Data File : VW025567.D
 Acq On : 10 Apr 2023 10:37
 Operator : SY/MD
 Sample : VW0410SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 01:57:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 11 01:56:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	780969	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	679438	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	310082	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	241863	19.032	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	76.120%	
7) Chloroethane-d5	2.893	69	179218	19.807	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	79.240%	
11) 1,1-Dichloroethene-d2	4.021	63	387304	15.070	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	60.280%	
21) 2-Butanone-d5	7.075	46	110087	38.830	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	77.660%	
24) Chloroform-d	7.648	84	452988	20.658	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.640%	
26) 1,2-Dichloroethane-d4	8.307	65	237488m	20.818	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	83.280%	
32) Benzene-d6	8.270	84	951734	21.633	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	86.520%	
36) 1,2-Dichloropropane-d6	9.270	67	292303	21.309	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	85.240%	
41) Toluene-d8	10.325	98	829527	21.585	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	86.360%	
43) trans-1,3-Dichloroprop...	10.575	79	102392	19.909	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.640%	
47) 2-Hexanone-d5	10.922	63	70169	37.423	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	74.840%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	182350	19.695	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	78.760%	
66) 1,2-Dichlorobenzene-d4	13.849	152	237831	22.326	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.320%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041023\
Data File : VW025567.D
Acq On : 10 Apr 2023 10:37
Operator : SY/MD
Sample : VW0410SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 01:57:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040323SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 11 01:56:03 2023
Response via : Initial Calibration

