


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028378.D
 Acq On : 10 Apr 2024 10:48
 Operator : SY/MD
 Sample : P2007-11
 Misc : 5.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 11 05:55:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

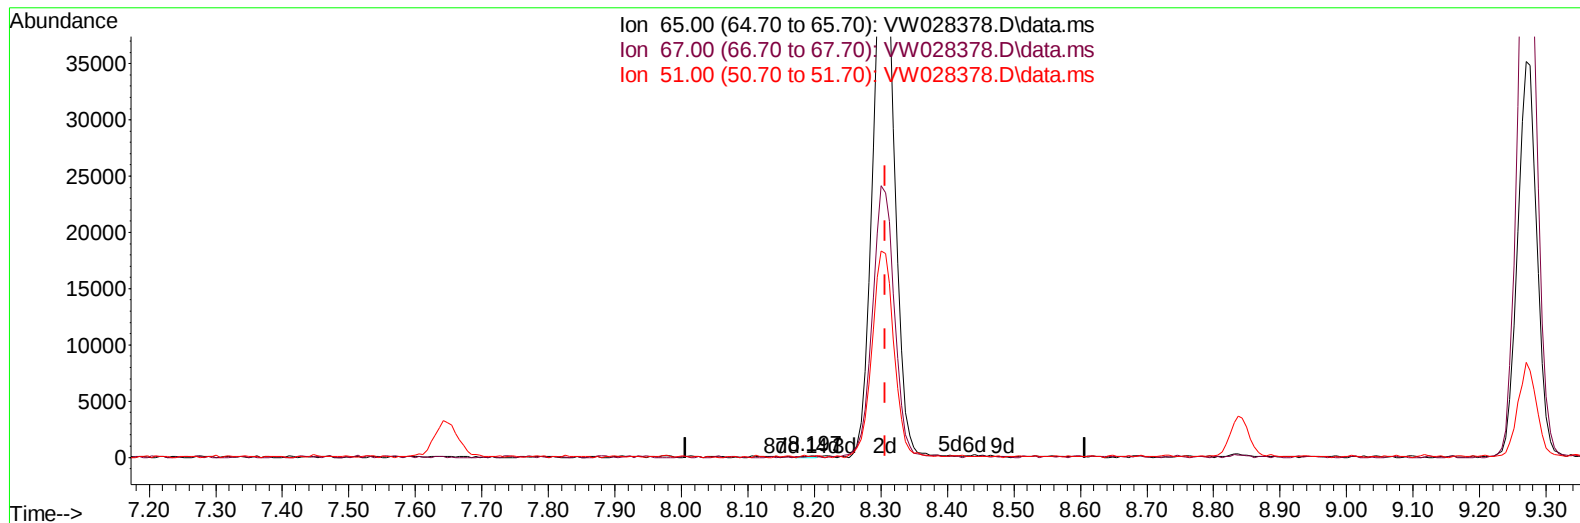




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
Data File : VW028378.D
Acq On : 10 Apr 2024 10:48
Operator : SY/MD
Sample : P2007-11
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 11 05:55:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 11 05:54:50 2024
Response via : Initial Calibration

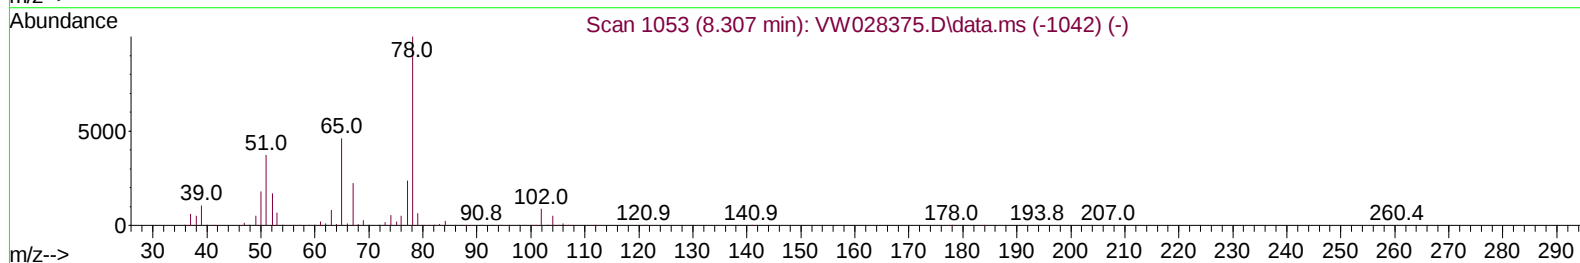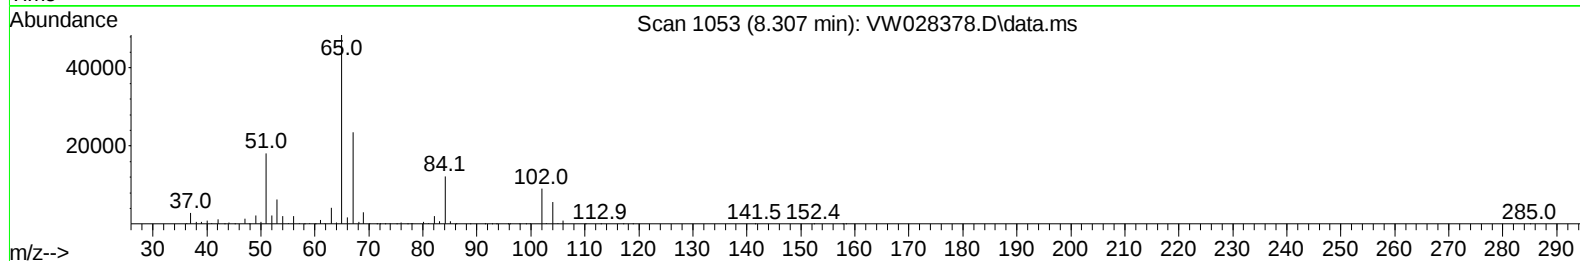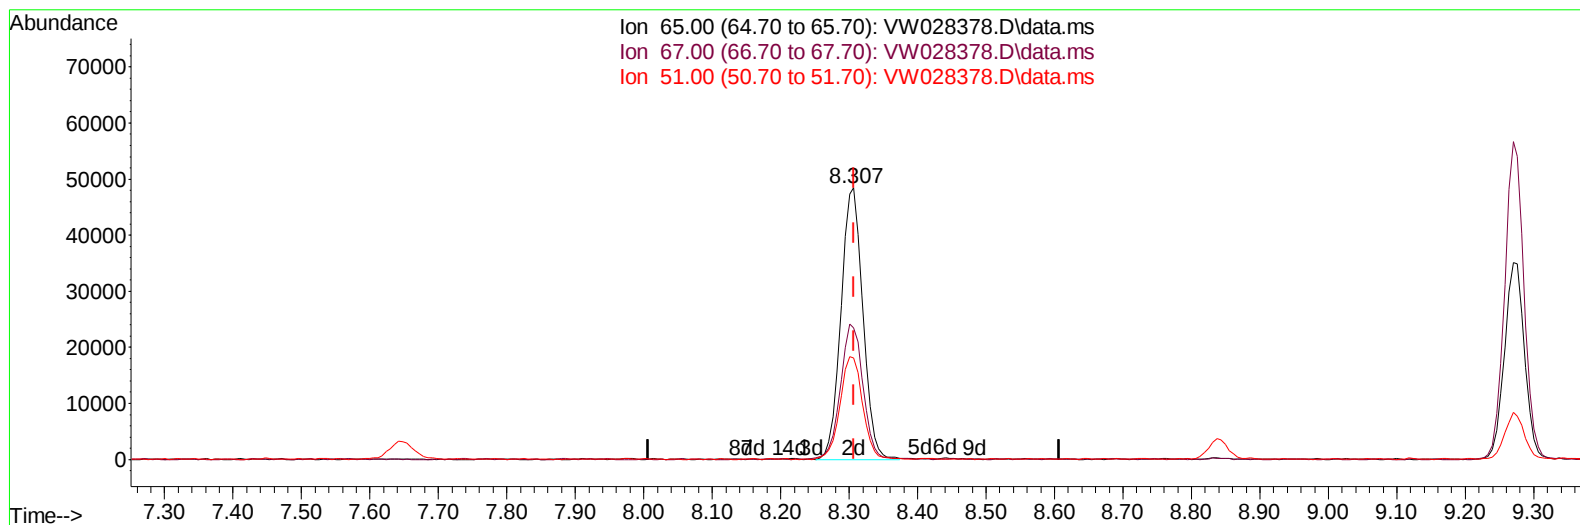

TIC: VW028378.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 27.10 ug/L m

response 107896

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.07#
51.00	108.40	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028378.D
 Acq On : 10 Apr 2024 10:48
 Operator : SY/MD
 Sample : P2007-11
 Misc : 5.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 11 05:55:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		293648	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		272063	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		128014	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		101074	21.470	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	85.880%		
7) Chloroethane-d5	2.899	69		81221	22.763	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	91.040%		
11) 1,1-Dichloroethene-d2	4.027	65		42890	21.514	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	86.040%		
21) 2-Butanone-d5	7.075	46		54245	61.577	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	123.160%		
24) Chloroform-d	7.648	84		184297	24.052	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	96.200%		
26) 1,2-Dichloroethane-d4	8.307	65		107896m	27.095	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	108.400%		
32) Benzene-d6	8.270	84		366679	24.671	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	98.680%		
36) 1,2-Dichloropropane-d6	9.270	67		111360	25.207	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	100.840%		
41) Toluene-d8	10.325	98		331719	24.545	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	98.160%		
43) trans-1,3-Dichloroprop...	10.575	79		44747	25.473	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	101.880%		
47) 2-Hexanone-d5	10.922	63		37464	61.220	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	122.440%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		91655	29.405	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	117.640%		
66) 1,2-Dichlorobenzene-d4	13.848	152		106929	26.412	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	105.640%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
Data File : VW028378.D
Acq On : 10 Apr 2024 10:48
Operator : SY/MD
Sample : P2007-11
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 11 05:55:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 11 05:54:50 2024
Response via : Initial Calibration

