




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028386.D
 Acq On : 10 Apr 2024 17:29
 Operator : SY/MD
 Sample : P2052-03
 Misc : 5.51g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 05:58:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

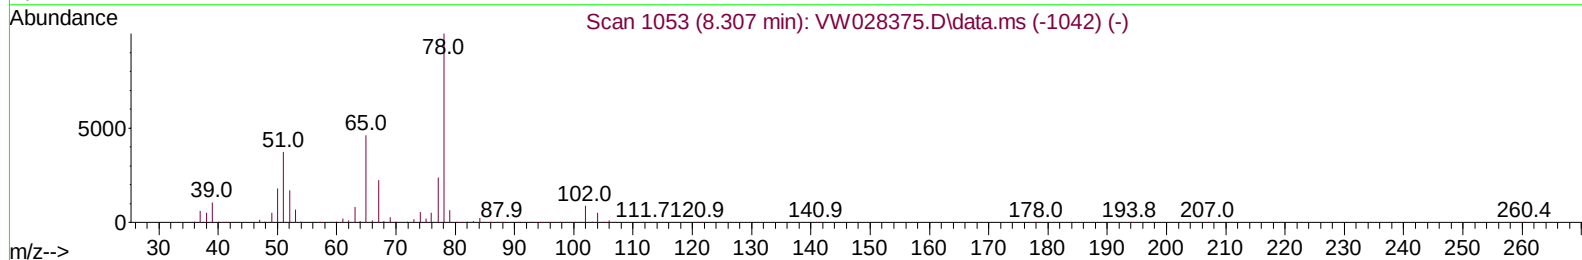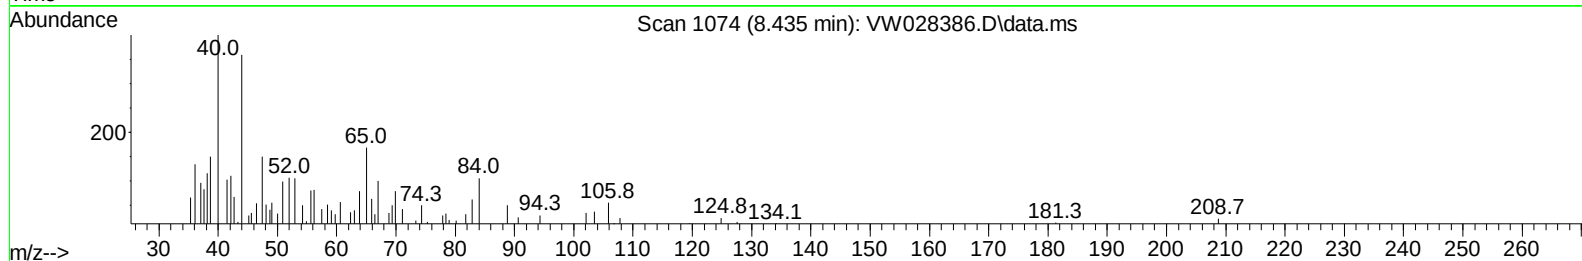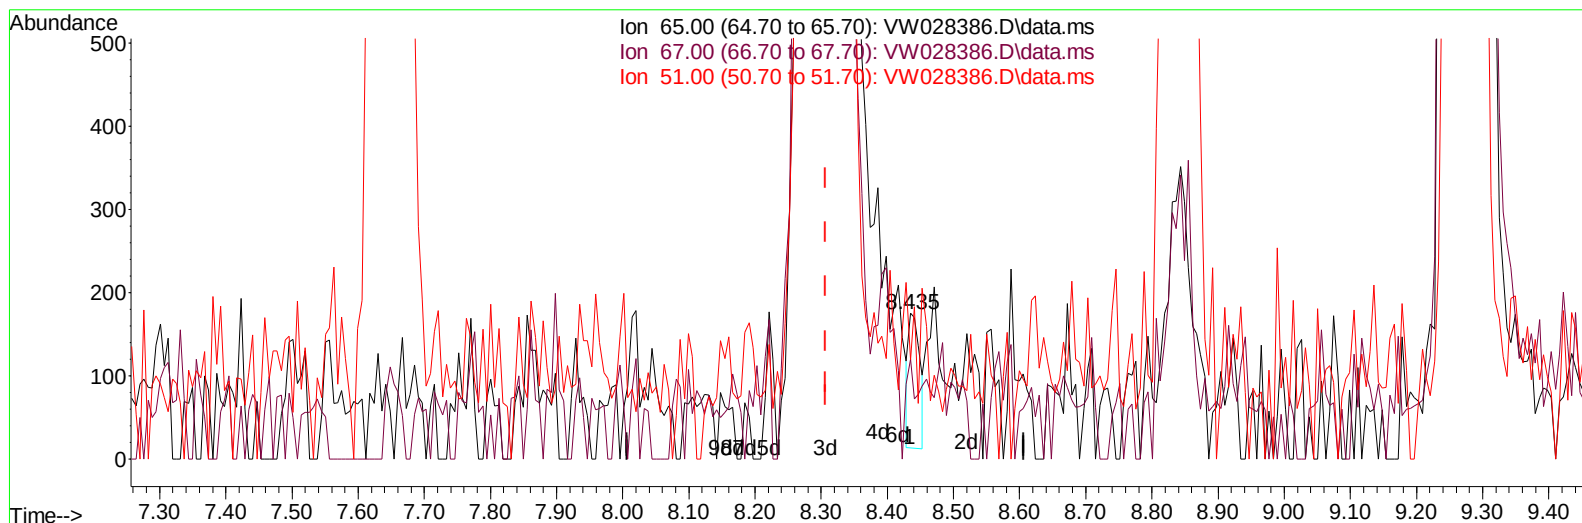

TIC: VW028386.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.435min (+ 0.128) 0.03 ug/L

response 194

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	53.09
51.00	108.40	138.66
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028386.D
 Acq On : 10 Apr 2024 17:29
 Operator : SY/MD
 Sample : P2052-03
 Misc : 5.51g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 05:58:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

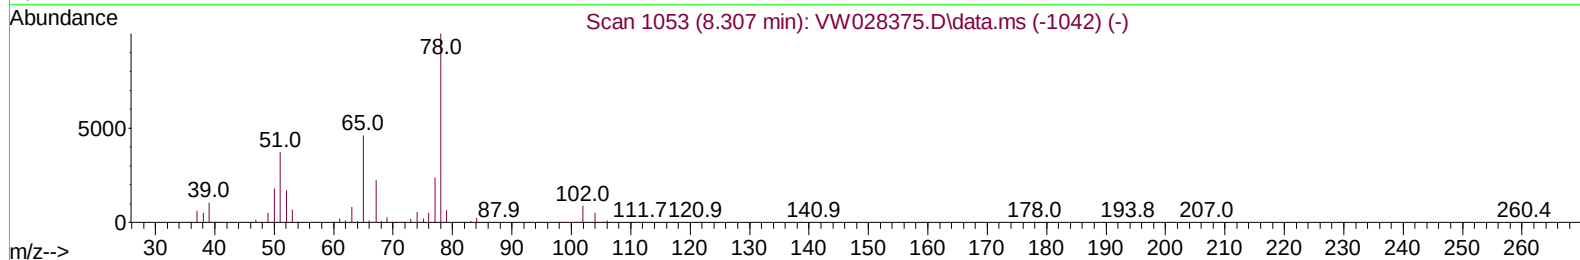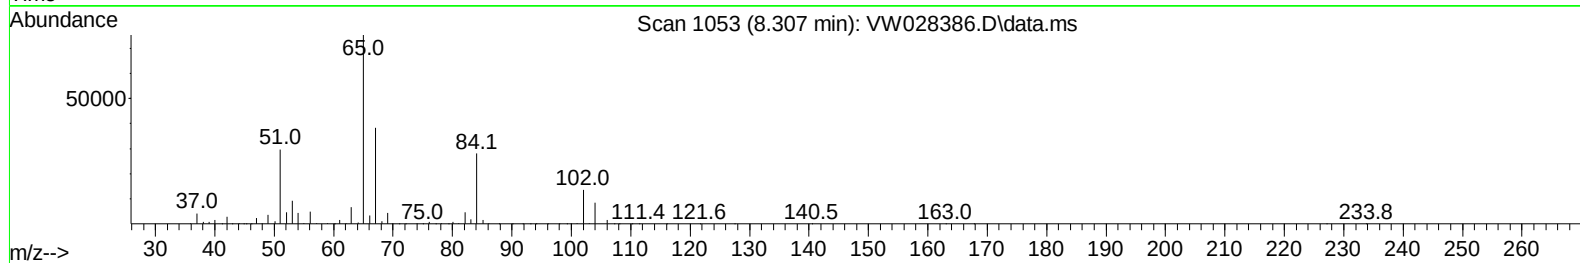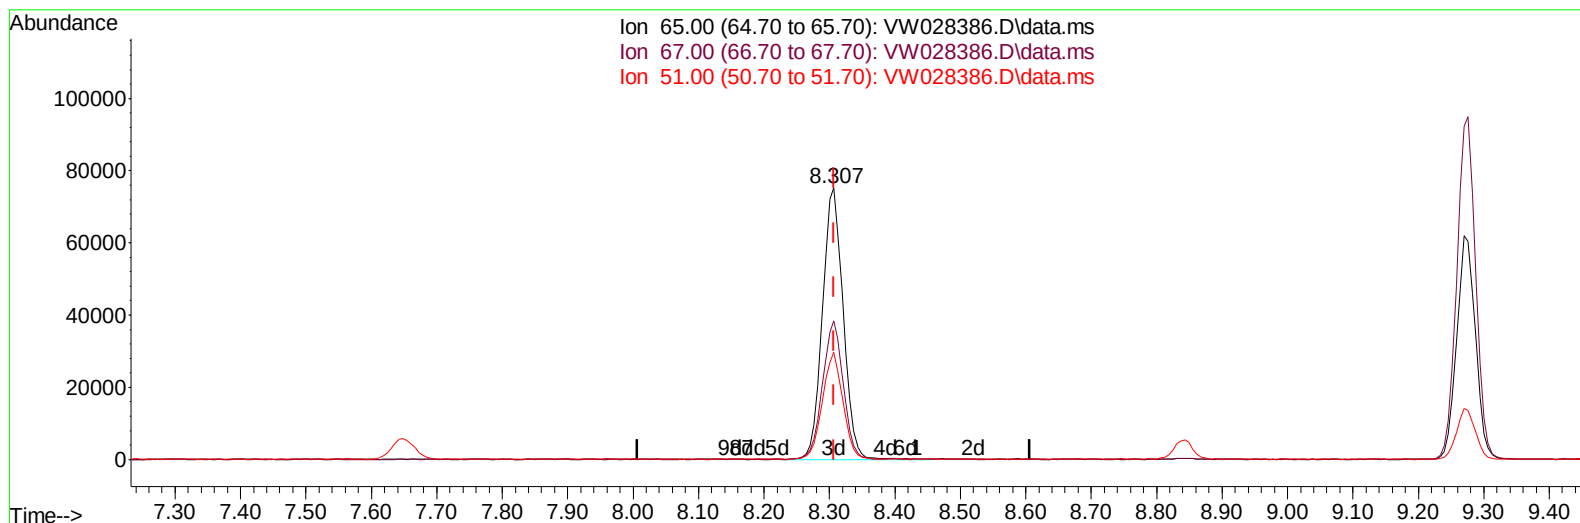

TIC: VW028386.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 27.36 ug/L m

response 165216

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.06#
51.00	108.40	0.16#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028386.D
 Acq On : 10 Apr 2024 17:29
 Operator : SY/MD
 Sample : P2052-03
 Misc : 5.51g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 05:58:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		445321	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		299058	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		54507	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		203116	28.451	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	113.800%	
7) Chloroethane-d5	2.905	69		157001	29.015	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	116.080%	
11) 1,1-Dichloroethene-d2	4.021	65		78564	25.986	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	103.960%	
21) 2-Butanone-d5	7.075	46		72843	54.526	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	109.060%	
24) Chloroform-d	7.648	84		315637	27.162	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	108.640%	
26) 1,2-Dichloroethane-d4	8.307	65		165216m	27.359	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	109.440%	
32) Benzene-d6	8.276	84		645840	39.531	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	158.120%#	
36) 1,2-Dichloropropane-d6	9.276	67		189952	39.116	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	156.480%#	
41) Toluene-d8	10.325	98		493856	33.243	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	132.960%#	
43) trans-1,3-Dichloroprop...	10.575	79		50147	25.970	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	103.880%	
47) 2-Hexanone-d5	10.922	63		47314	70.337	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	140.680%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		118118	34.474	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	137.880%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		74280	43.091	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	172.360%#	
Target Compounds							
13) Acetone	4.131	43		6470	3.944	ug/L	Qvalue 67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
Data File : VW028386.D
Acq On : 10 Apr 2024 17:29
Operator : SY/MD
Sample : P2052-03
Misc : 5.51g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AB2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 11 05:58:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 11 05:54:50 2024
Response via : Initial Calibration

