




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028387.D
 Acq On : 10 Apr 2024 17:53
 Operator : SY/MD
 Sample : P2052-04
 Misc : 5.93g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB3

Manual IntegrationsAPPROVED

Quant Time: Apr 11 05:59:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

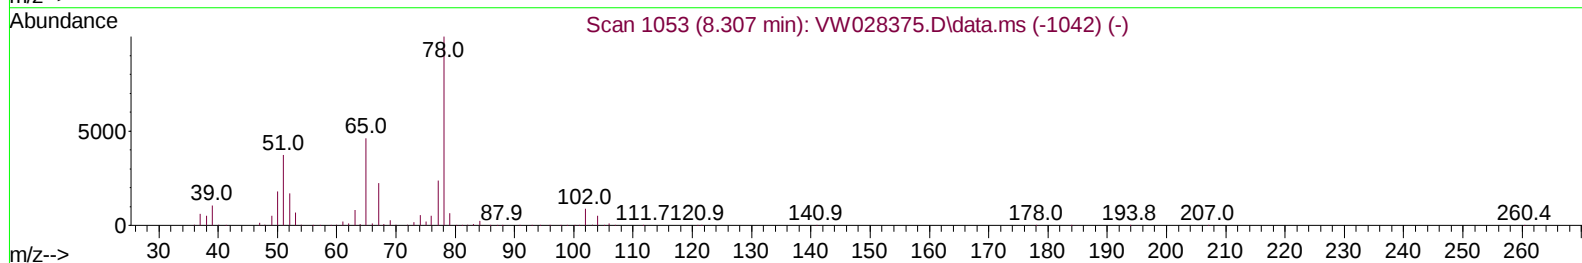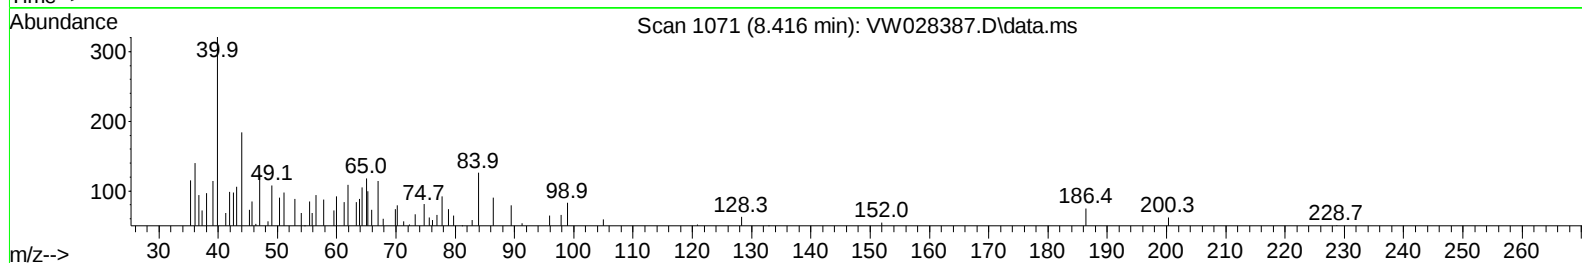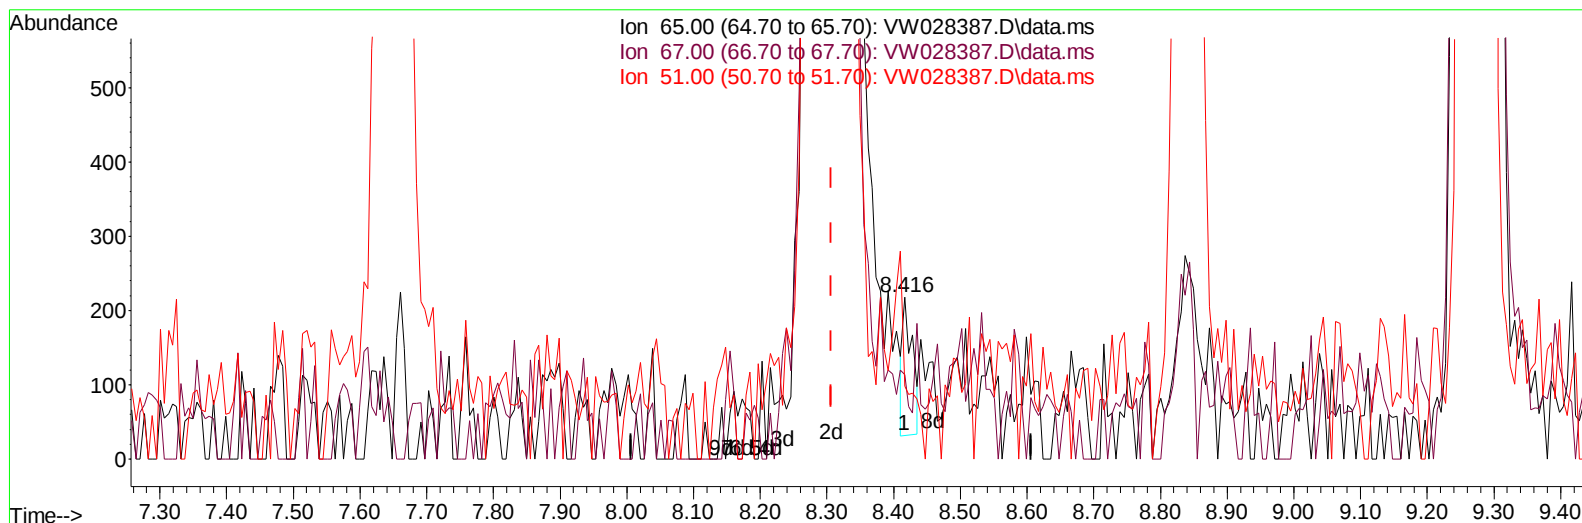

TIC: VW028387.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.416min (+ 0.110) 0.05 ug/L

response 181

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	44.75
51.00	108.40	86.74
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028387.D
 Acq On : 10 Apr 2024 17:53
 Operator : SY/MD
 Sample : P2052-04
 Misc : 5.93g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 11 05:59:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

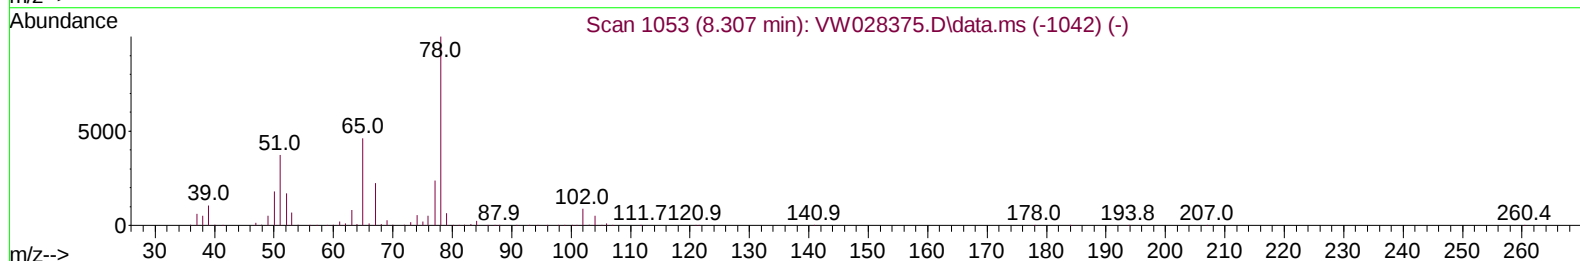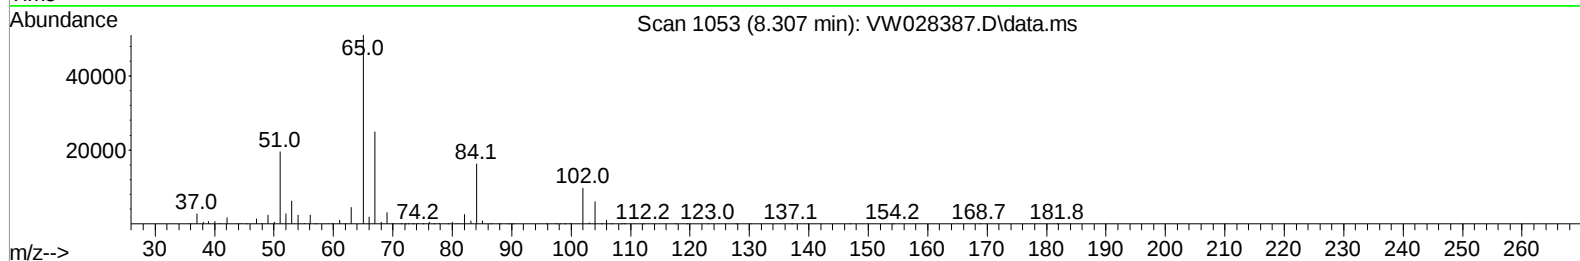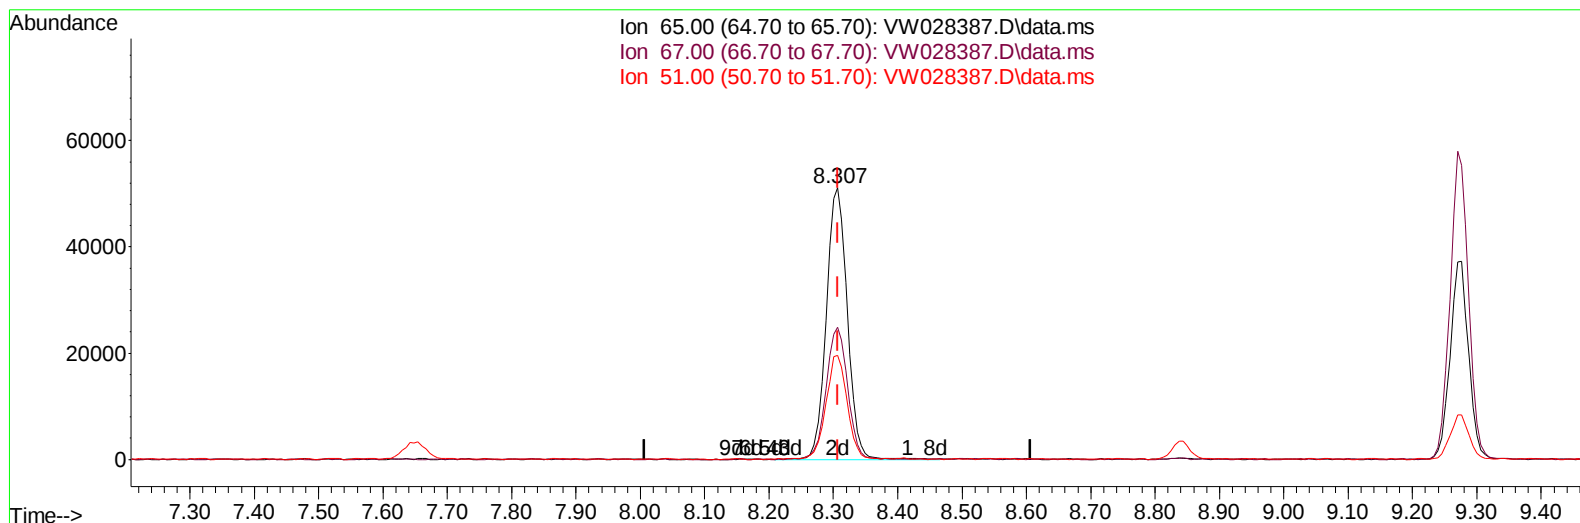

TIC: VW028387.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 30.60 ug/L m

response 115323

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.07#
51.00	108.40	0.14#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028387.D
 Acq On : 10 Apr 2024 17:53
 Operator : SY/MD
 Sample : P2052-04
 Misc : 5.93g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB3

Manual IntegrationsAPPROVED

Quant Time: Apr 11 05:59:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		277918	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		252710	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		110750	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		108548	24.363	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	97.440%		
7) Chloroethane-d5	2.905	69		85771	25.399	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	101.600%		
11) 1,1-Dichloroethene-d2	4.027	65		46904	24.859	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	99.440%		
21) 2-Butanone-d5	7.075	46		52796	63.325	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	126.640%		
24) Chloroform-d	7.648	84		186101	25.662	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	102.640%		
26) 1,2-Dichloroethane-d4	8.307	65		115323m	30.600	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	122.400%		
32) Benzene-d6	8.276	84		371137	26.883	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	107.520%		
36) 1,2-Dichloropropane-d6	9.270	67		116003	28.269	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	113.080%		
41) Toluene-d8	10.325	98		332491	26.486	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	105.960%		
43) trans-1,3-Dichloroprop...	10.575	79		45859	28.105	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	112.440%		
47) 2-Hexanone-d5	10.922	63		37872	66.627	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	133.260%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		92466	31.937	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	127.760%#		
66) 1,2-Dichlorobenzene-d4	13.848	152		99891	28.520	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	114.080%		
Target Compounds							
13) Acetone	4.125	43		4138	4.042	ug/L	Qvalue 61

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
Data File : VW028387.D
Acq On : 10 Apr 2024 17:53
Operator : SY/MD
Sample : P2052-04
Misc : 5.93g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AB3

Manual IntegrationsAPPROVED

Quant Time: Apr 11 05:59:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 11 05:54:50 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/11/2024
Supervised By :Mahesh Dadoda 04/13/2024

