

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028386.D
 Acq On : 10 Apr 2024 17:29
 Operator : SY/MD
 Sample : P2052-03
 Misc : 5.51g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 11 05:58:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	445321	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	299058	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	54507	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	203116	28.451	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 113.800%			
7) Chloroethane-d5	2.905	69	157001	29.015	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 116.080%			
11) 1,1-Dichloroethene-d2	4.021	65	78564	25.986	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 103.960%			
21) 2-Butanone-d5	7.075	46	72843	54.526	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 109.060%			
24) Chloroform-d	7.648	84	315637	27.162	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 108.640%			
26) 1,2-Dichloroethane-d4	8.307	65	165216m	27.359	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 109.440%			
32) Benzene-d6	8.276	84	645840	39.531	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 158.120%#			
36) 1,2-Dichloropropane-d6	9.276	67	189952	39.116	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 156.480%#			
41) Toluene-d8	10.325	98	493856	33.243	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 132.960%#			
43) trans-1,3-Dichloroprop...	10.575	79	50147	25.970	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 103.880%			
47) 2-Hexanone-d5	10.922	63	47314	70.337	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 140.680%#			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	118118	34.474	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 137.880%#			
66) 1,2-Dichlorobenzene-d4	13.848	152	74280	43.091	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 172.360%#			
Target Compounds					Qvalue	
13) Acetone	4.131	43	6470	3.944	ug/L	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
Data File : VW028386.D
Acq On : 10 Apr 2024 17:29
Operator : SY/MD
Sample : P2052-03
Misc : 5.51g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AB2

Quant Time: Apr 11 05:58:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 11 05:54:50 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 04/11/2024
Supervised By : Mahesh Dadoda 04/13/2024

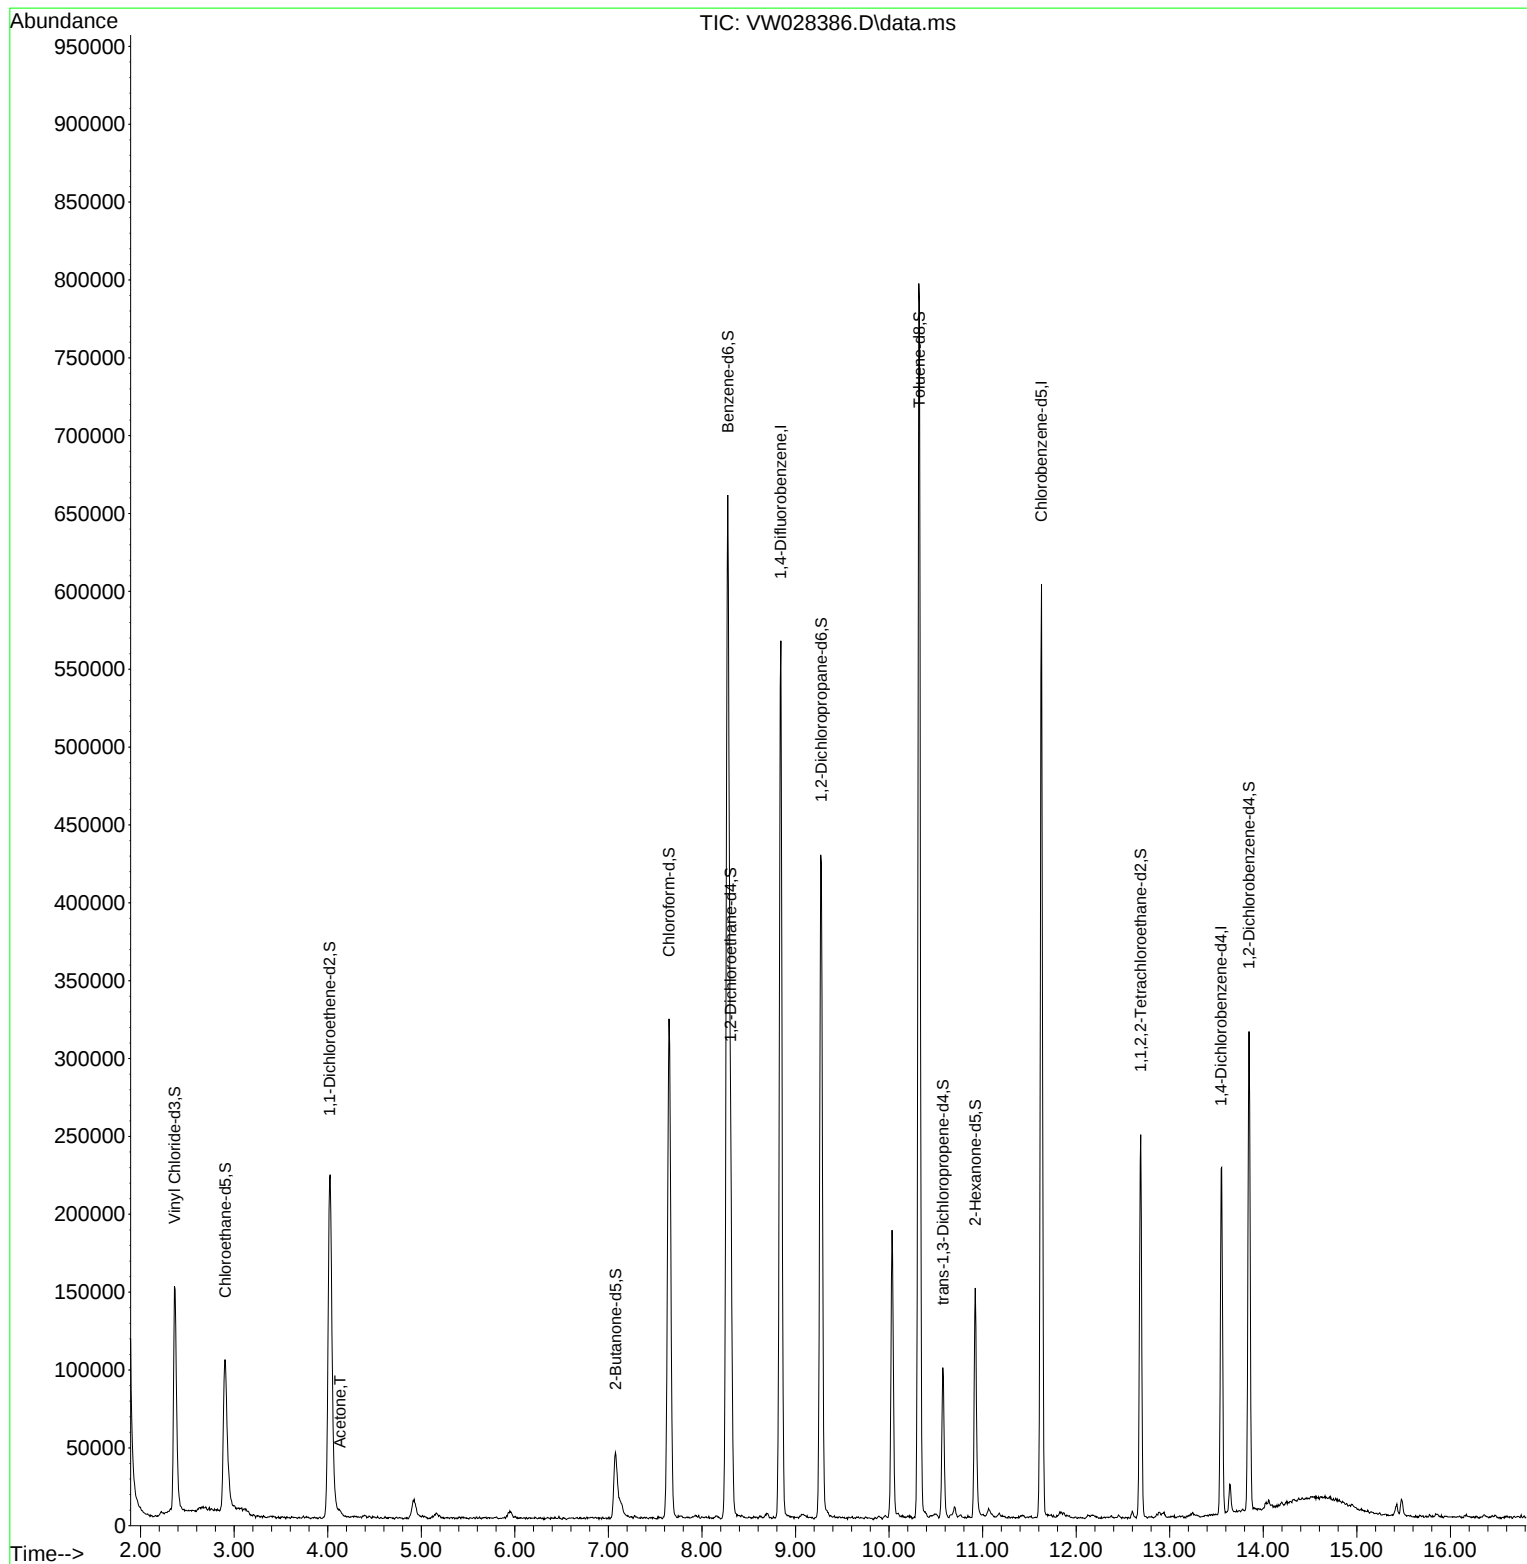

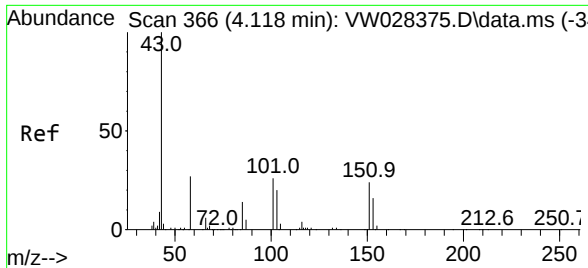

#13

Acetone

Concen: 3.944 ug/L

RT: 4.131 min Scan# 30

Delta R.T. 0.012 min

Lab File: VW028386.D

Acq: 10 Apr 2024 17:29

Instrument :

MSVOA_W

ClientSampleId :

C0AB2

Tgt Ion: 43 Resp: 6470

Ion Ratio Lower Upper

43 100

58 9.9 0.0 53.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024

Supervised By :Mahesh Dadoda 04/13/2024

