

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
 Data File : VW028387.D
 Acq On : 10 Apr 2024 17:53
 Operator : SY/MD
 Sample : P2052-04
 Misc : 5.93g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 11 05:59:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 11 05:54:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	277918	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	252710	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	110750	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	108548	24.363	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 97.440%			
7) Chloroethane-d5	2.905	69	85771	25.399	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 101.600%			
11) 1,1-Dichloroethene-d2	4.027	65	46904	24.859	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 99.440%			
21) 2-Butanone-d5	7.075	46	52796	63.325	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 126.640%			
24) Chloroform-d	7.648	84	186101	25.662	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 102.640%			
26) 1,2-Dichloroethane-d4	8.307	65	115323m	30.600	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 122.400%			
32) Benzene-d6	8.276	84	371137	26.883	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 107.520%			
36) 1,2-Dichloropropane-d6	9.270	67	116003	28.269	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 113.080%			
41) Toluene-d8	10.325	98	332491	26.486	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 105.960%			
43) trans-1,3-Dichloroprop...	10.575	79	45859	28.105	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 112.440%			
47) 2-Hexanone-d5	10.922	63	37872	66.627	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 133.260%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	92466	31.937	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 127.760%#			
66) 1,2-Dichlorobenzene-d4	13.848	152	99891	28.520	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 114.080%			
Target Compounds					Qvalue	
13) Acetone	4.125	43	4138	4.042	ug/L	61

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041024\
Data File : VW028387.D
Acq On : 10 Apr 2024 17:53
Operator : SY/MD
Sample : P2052-04
Misc : 5.93g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AB3

Quant Time: Apr 11 05:59:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 11 05:54:50 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024
Supervised By :Mahesh Dadoda 04/13/2024

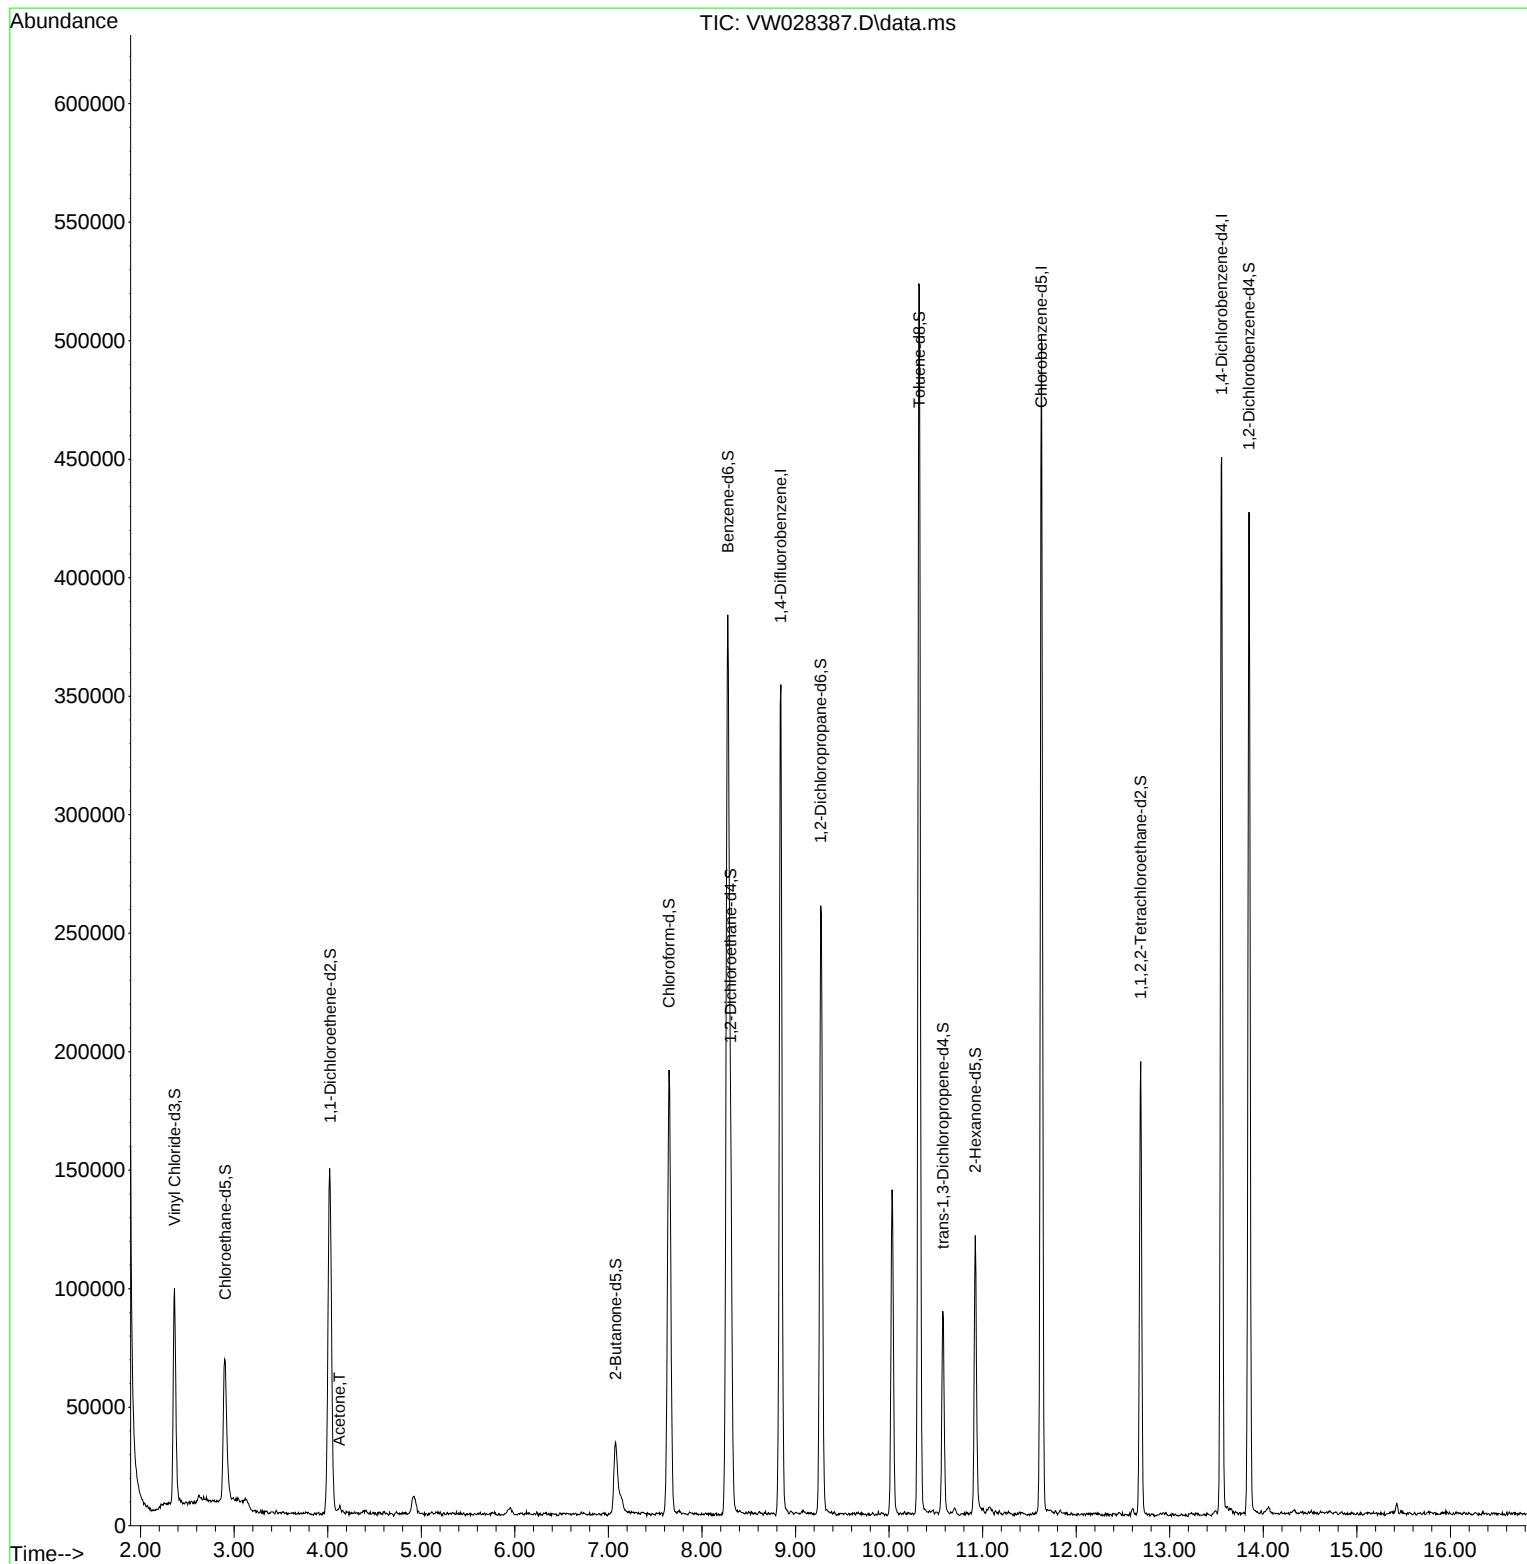

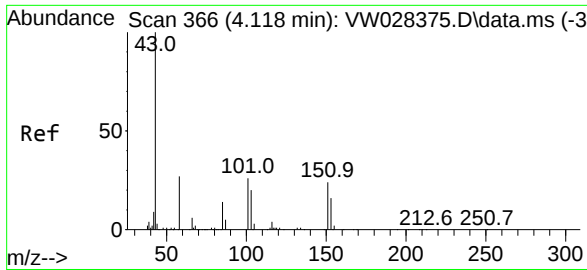

#13

Acetone

Concen: 4.042 ug/L

RT: 4.125 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW028387.D

Acq: 10 Apr 2024 17:53

Instrument :

MSVOA_W

ClientSampleId :

C0AB3

Tgt Ion: 43 Resp: 4138

Ion Ratio Lower Upper

43 100

58 6.7 0.0 53.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 04/11/2024

Supervised By :Mahesh Dadoda 04/13/2024

