

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041119\
Quantitation Report (QT Reviewed)


Data File : VW009910.D
Acq On : 11 Apr 2019 13:06
Operator : SY/VA
Sample : K2304-06
Misc : 4.65G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF891

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:24 AM

Quant Time: Apr 12 06:43:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 05:38:57 2019
Response via : Initial Calibration

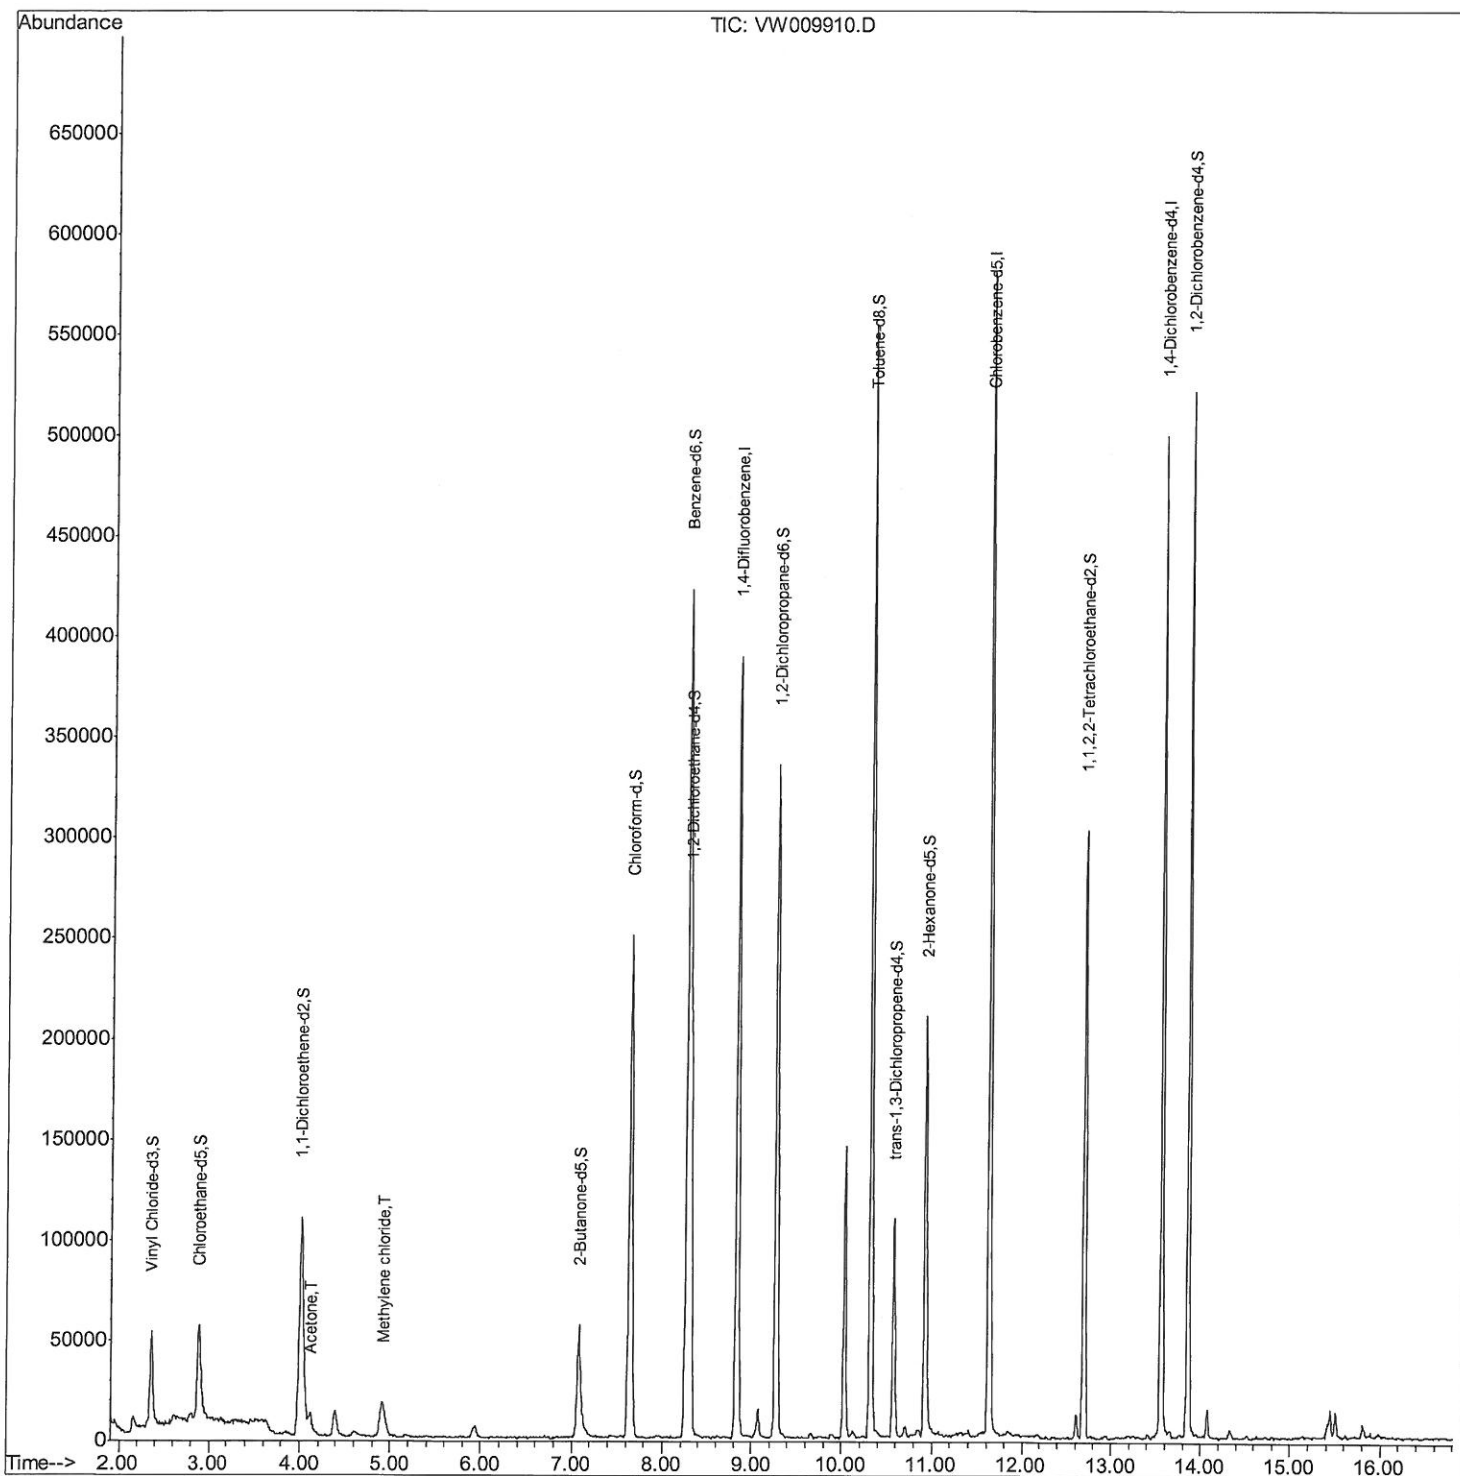

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041119\
Quantitation Report (Qedit)




Data File : VW009910.D
Acq On : 11 Apr 2019 13:06
Operator : SY/VA
Sample : K2304-06
Misc : 4.65G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF891

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:24 AM

Quant Time: Apr 12 06:41:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 05:38:57 2019
Response via : Initial Calibration

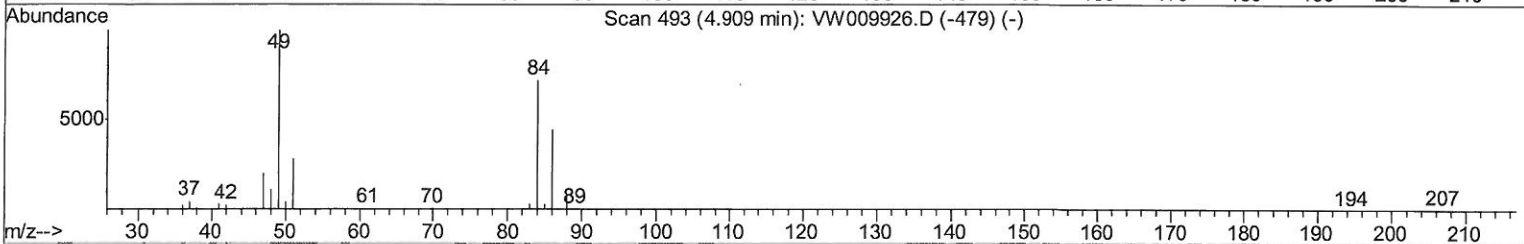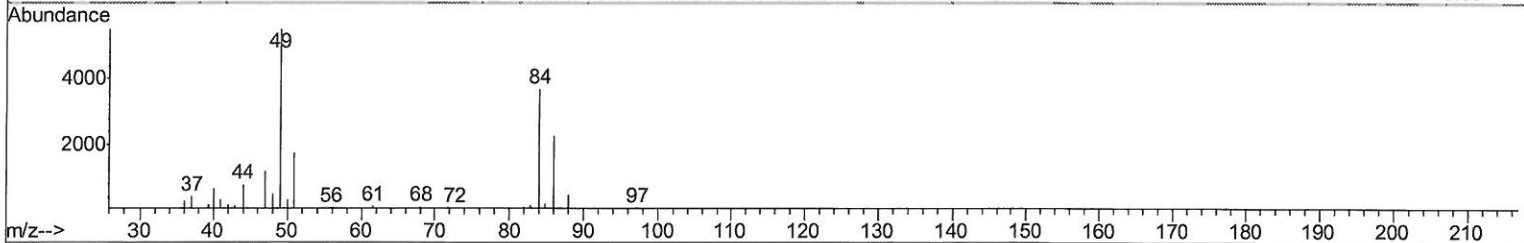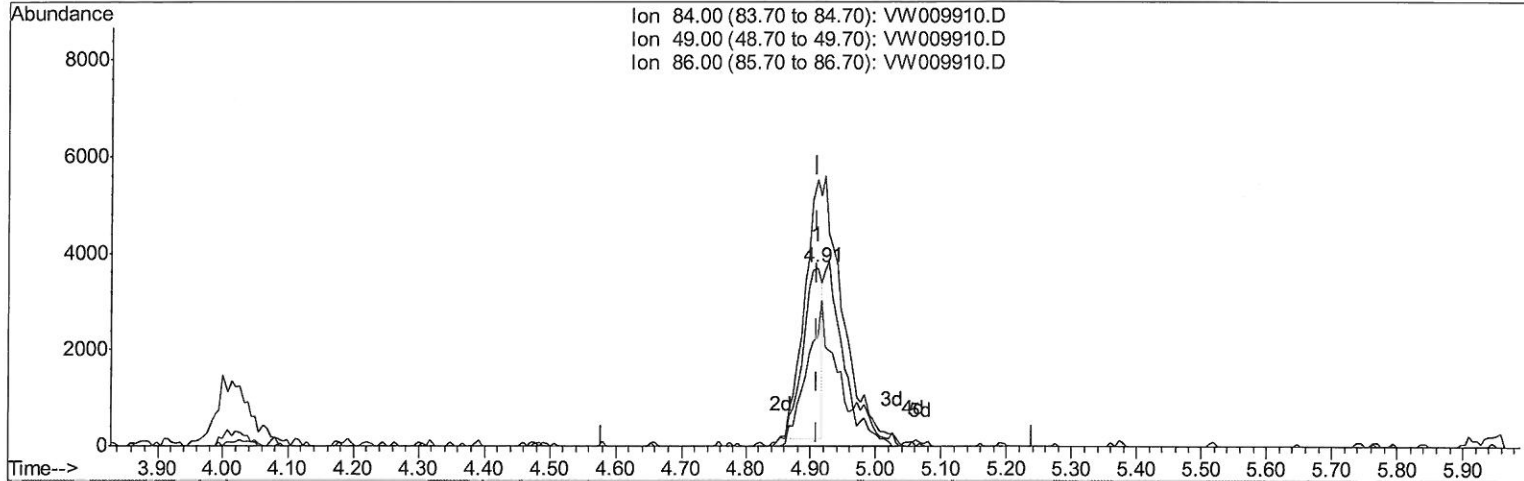

TIC: VW009910.D

(16) Methylene chloride (T)

4.910min (+0.000) 1.36ug/L

response 7079

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	149.53
86.00	66.30	61.68
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041119\
Quantitation Report (Qedit)




Data File : VW009910.D
Acq On : 11 Apr 2019 13:06
Operator : SY/VA
Sample : K2304-06
Misc : 4.65G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF891

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:24 AM

Quant Time: Apr 12 06:41:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 05:38:57 2019
Response via : Initial Calibration

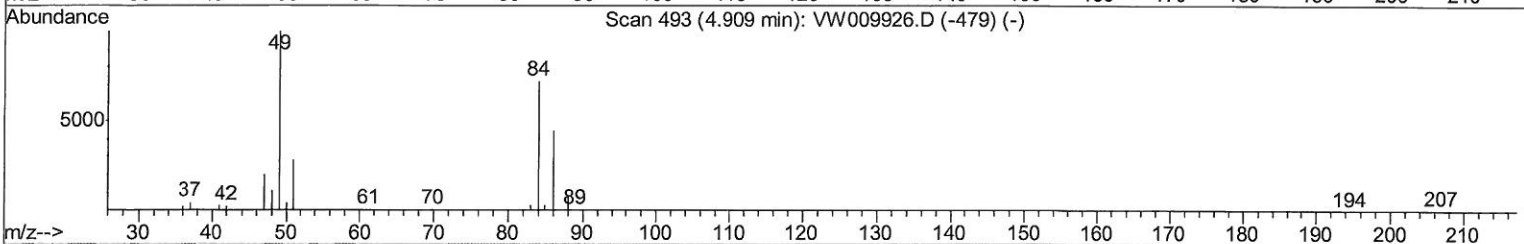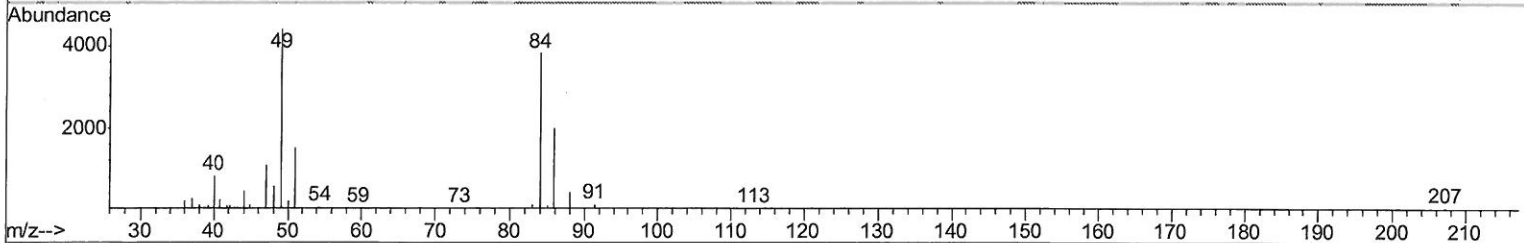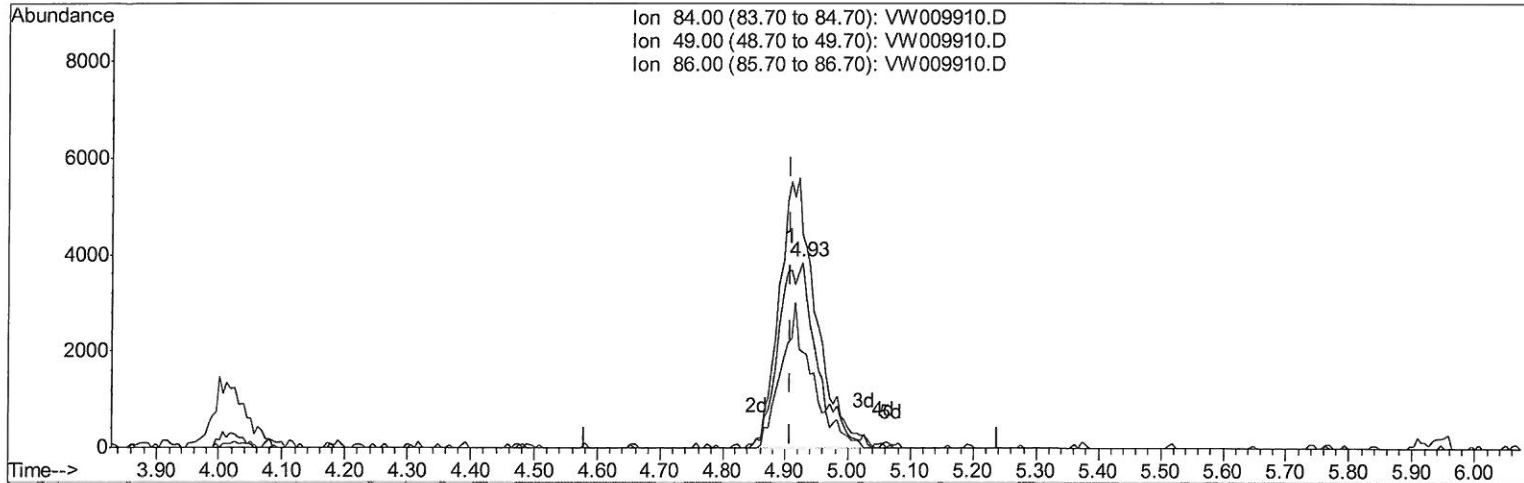

TIC: VW009910.D

(16) Methylene chloride (T)

4.928min (+0.018) 3.18ug/L m

response 16536

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	114.55
86.00	66.30	51.76
0.00	0.00	0.00

7MD
4/16/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041119\
Quantitation Report (QT Reviewed)

Data File : VW009910.D
Acq On : 11 Apr 2019 13:06
Operator : SY/VA
Sample : K2304-06
Misc : 4.65G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF891

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:24 AM

Quant Time: Apr 12 06:43:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 05:38:57 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	294563	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	302910	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	118217	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	63439	16.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.84%
7) Chloroethane-d5	2.90	69	66976	18.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.88%
10) 1,1-Dichloroethene-d2	4.01	63	133798	16.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.56%
20) 2-Butanone-d5	7.08	46	94030	75.13	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	150.26%#
24) Chloroform-d	7.65	84	230075	28.62	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	114.48%
26) 1,2-Dichloroethane-d4	8.31	65	162409	32.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	131.64%#
29) Benzene-d6	8.27	84	396830	24.96	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.84%
33) 1,2-Dichloropropane-d6	9.27	67	140871	28.68	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.72%
37) Toluene-d8	10.32	98	340302	23.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.60%
38) trans-1,3-Dichloropropene-	10.58	79	54865	23.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.68%
39) 2-Hexanone-d5	10.93	63	56003	60.50	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.00%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	139906	30.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	122.56%#
61) 1,2-Dichlorobenzene-d4	13.86	152	125803	30.33	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	121.32%#

Target Compounds

					Qvalue
13) Acetone	4.12	43	16159	12.050	ug/L
16) Methylene chloride	4.93	84	16536m	3.183	ug/L

95 MD
4/18/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed