

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041119\
Quantitation Report (QT Reviewed)


Data File : VW009930.D
Acq On : 11 Apr 2019 23:50
Operator : SY/VA
Sample : K2278-18
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB6Z0

Quant Time: Apr 12 04:57:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 04:36:14 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:38 AM

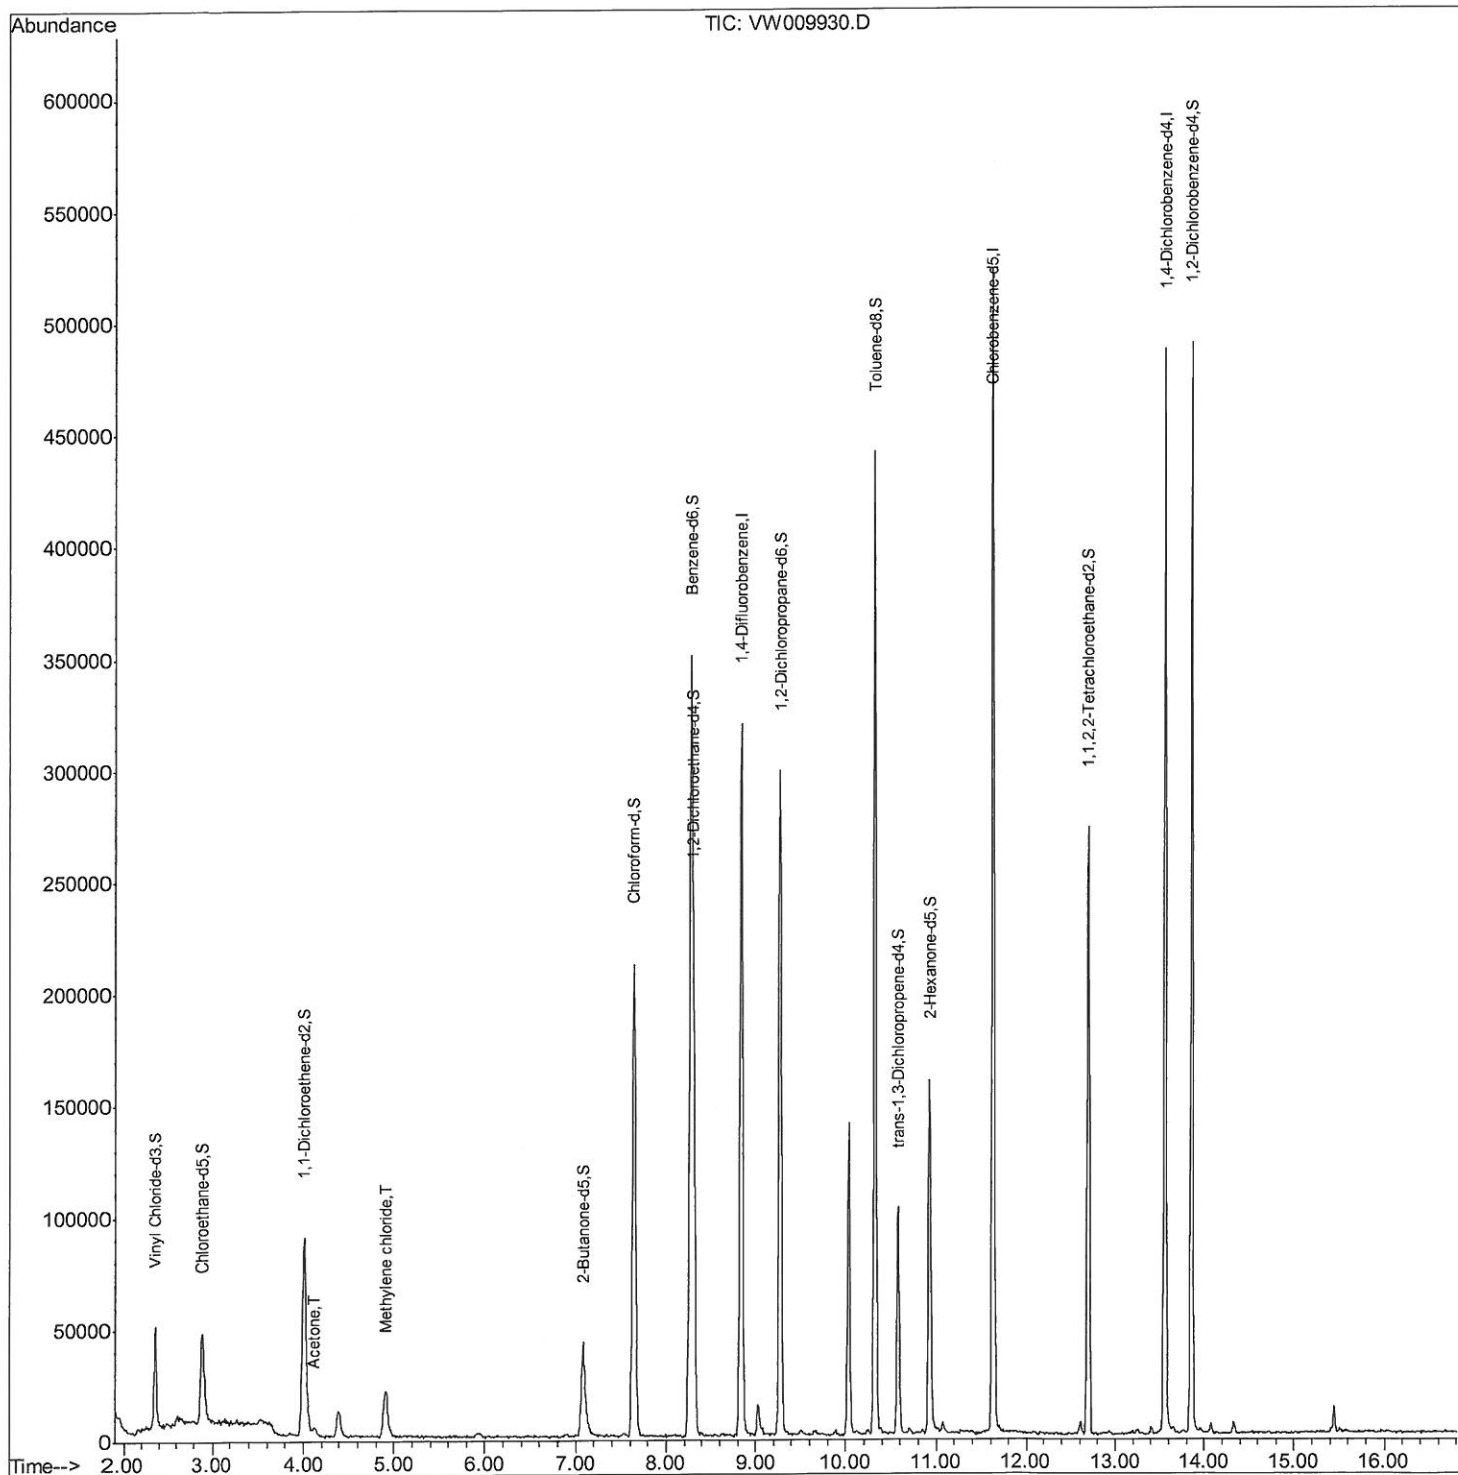

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041119\
Quantitation Report (Qedit)




Data File : VW009930.D
Acq On : 11 Apr 2019 23:50
Operator : SY/VA
Sample : K2278-18
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
DB6Z0

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:38 AM

Quant Time: Apr 12 04:56:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 04:36:14 2019
Response via : Initial Calibration

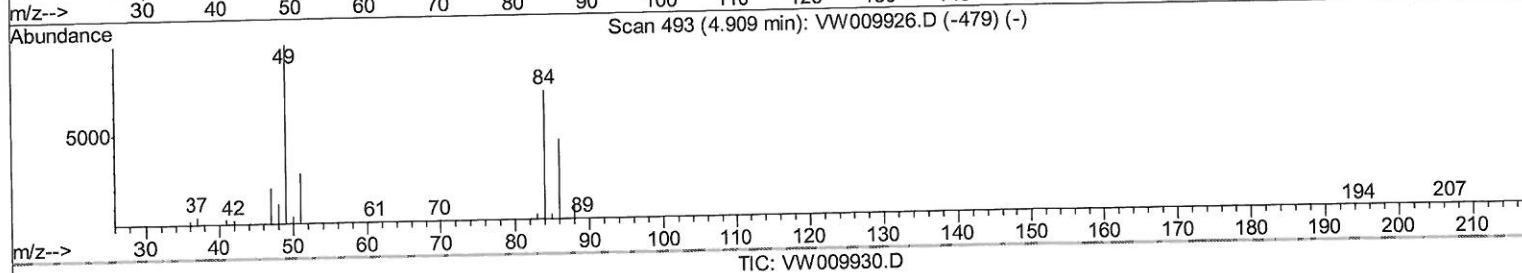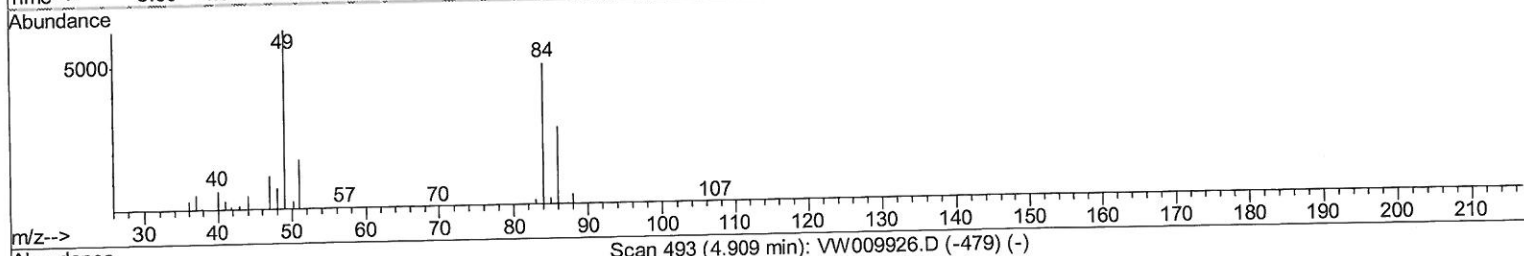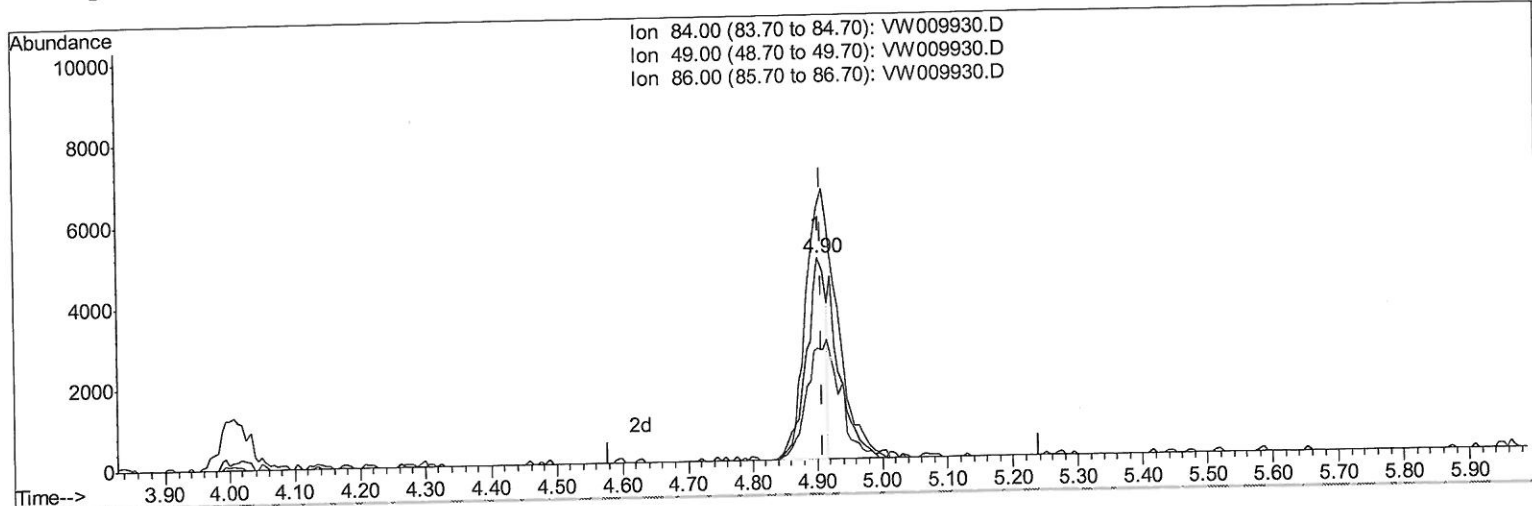

(16) Methylene chloride (T)

4.903min (-0.006) 2.37ug/L

response 10057

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	126.14
86.00	66.30	55.04
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041119\
Quantitation Report (Qedit)




Data File : VW009930.D
Acq On : 11 Apr 2019 23:50
Operator : SY/VA
Sample : K2278-18
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DB6Z0

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:38 AM

Quant Time: Apr 12 04:56:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 04:36:14 2019
Response via : Initial Calibration

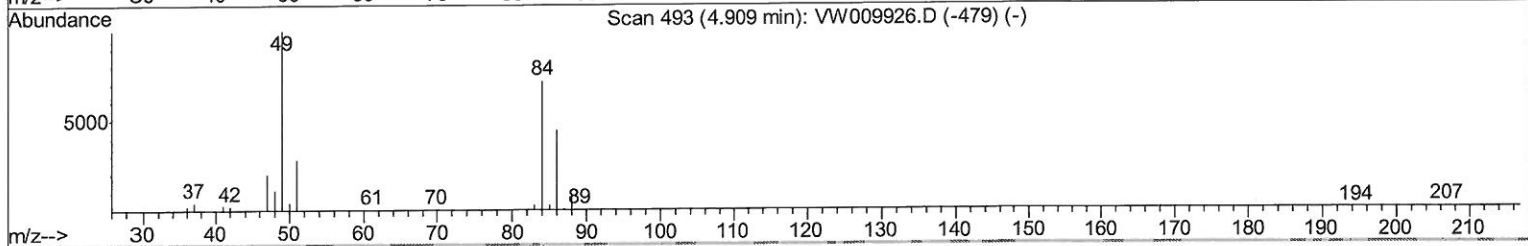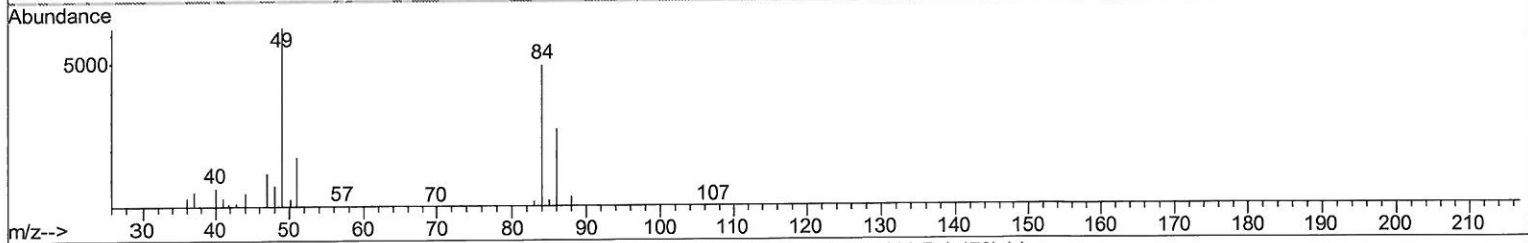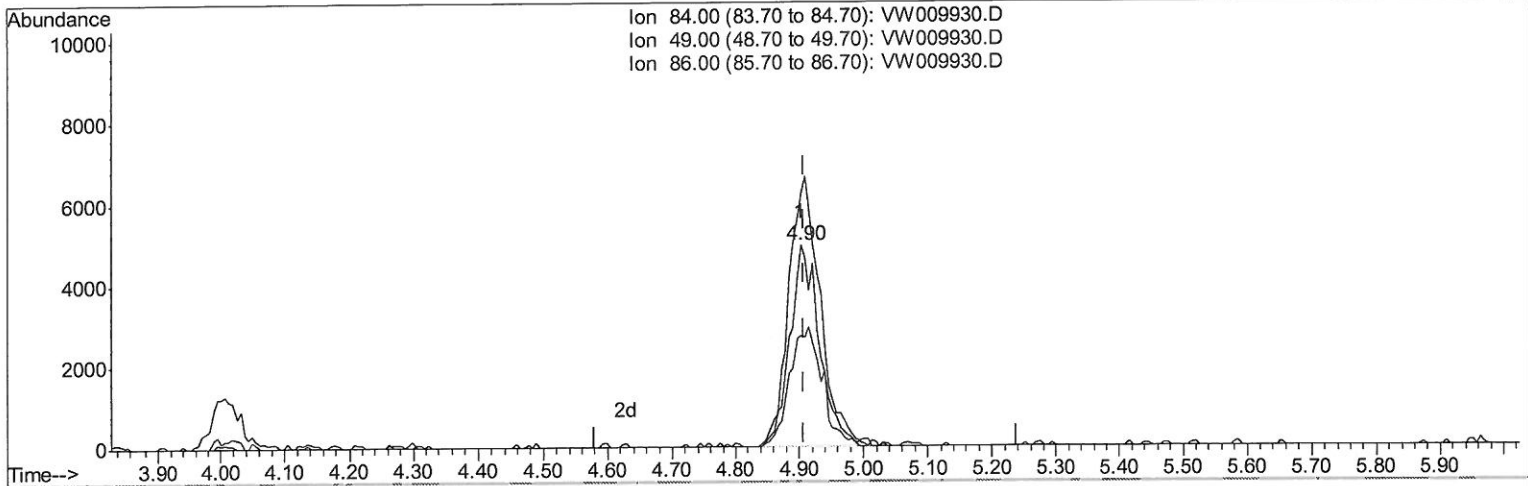

TIC: VW009930.D

(16) Methylene chloride (T)

4.903min (-0.006) 3.71ug/L m

response 15762

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	126.14
86.00	66.30	55.04
0.00	0.00	0.00

Handwritten: MMD
4/16/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW041119\
Quantitation Report (QT Reviewed)

Data File : VW009930.D
Acq On : 11 Apr 2019 23:50
Operator : SY/VA
Sample : K2278-18
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
DB6Z0

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:38 AM

Quant Time: Apr 12 04:57:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 04:36:14 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	241006	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	272762	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	116819	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	49140	15.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.32%
7) Chloroethane-d5	2.89	69	52458	18.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.64%
10) 1,1-Dichloroethene-d2	4.01	63	97707	14.41	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.64%
20) 2-Butanone-d5	7.08	46	70068	68.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	136.86%#
24) Chloroform-d	7.65	84	197244	29.99	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	119.96%
26) 1,2-Dichloroethane-d4	8.31	65	141151	34.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	139.84%#
29) Benzene-d6	8.27	84	326588	22.81	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.24%
33) 1,2-Dichloropropane-d6	9.27	67	122868	27.78	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.12%
37) Toluene-d8	10.32	98	273996	20.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.80%
38) trans-1,3-Dichloropropene-	10.58	79	51409	24.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.48%
39) 2-Hexanone-d5	10.93	63	43928	52.70	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	123492	30.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	120.12%#
61) 1,2-Dichlorobenzene-d4	13.86	152	121748	29.70	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	118.80%

Target Compounds

					Qvalue	
13) Acetone	4.12	43	4129	3.763	ug/L	75
16) Methylene chloride	4.90	84	15762m	3.708	ug/L	75

75 MLO
4/16/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed