

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\

Data File : VW009953.D

Acq On : 12 Apr 2019 12:21

Operator : SY/VA

Sample : K2255-18RE

Misc : 5.41G/10ML/MSVOA W/SOIL

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 13 00:27:33 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 12 23:54:39 2019

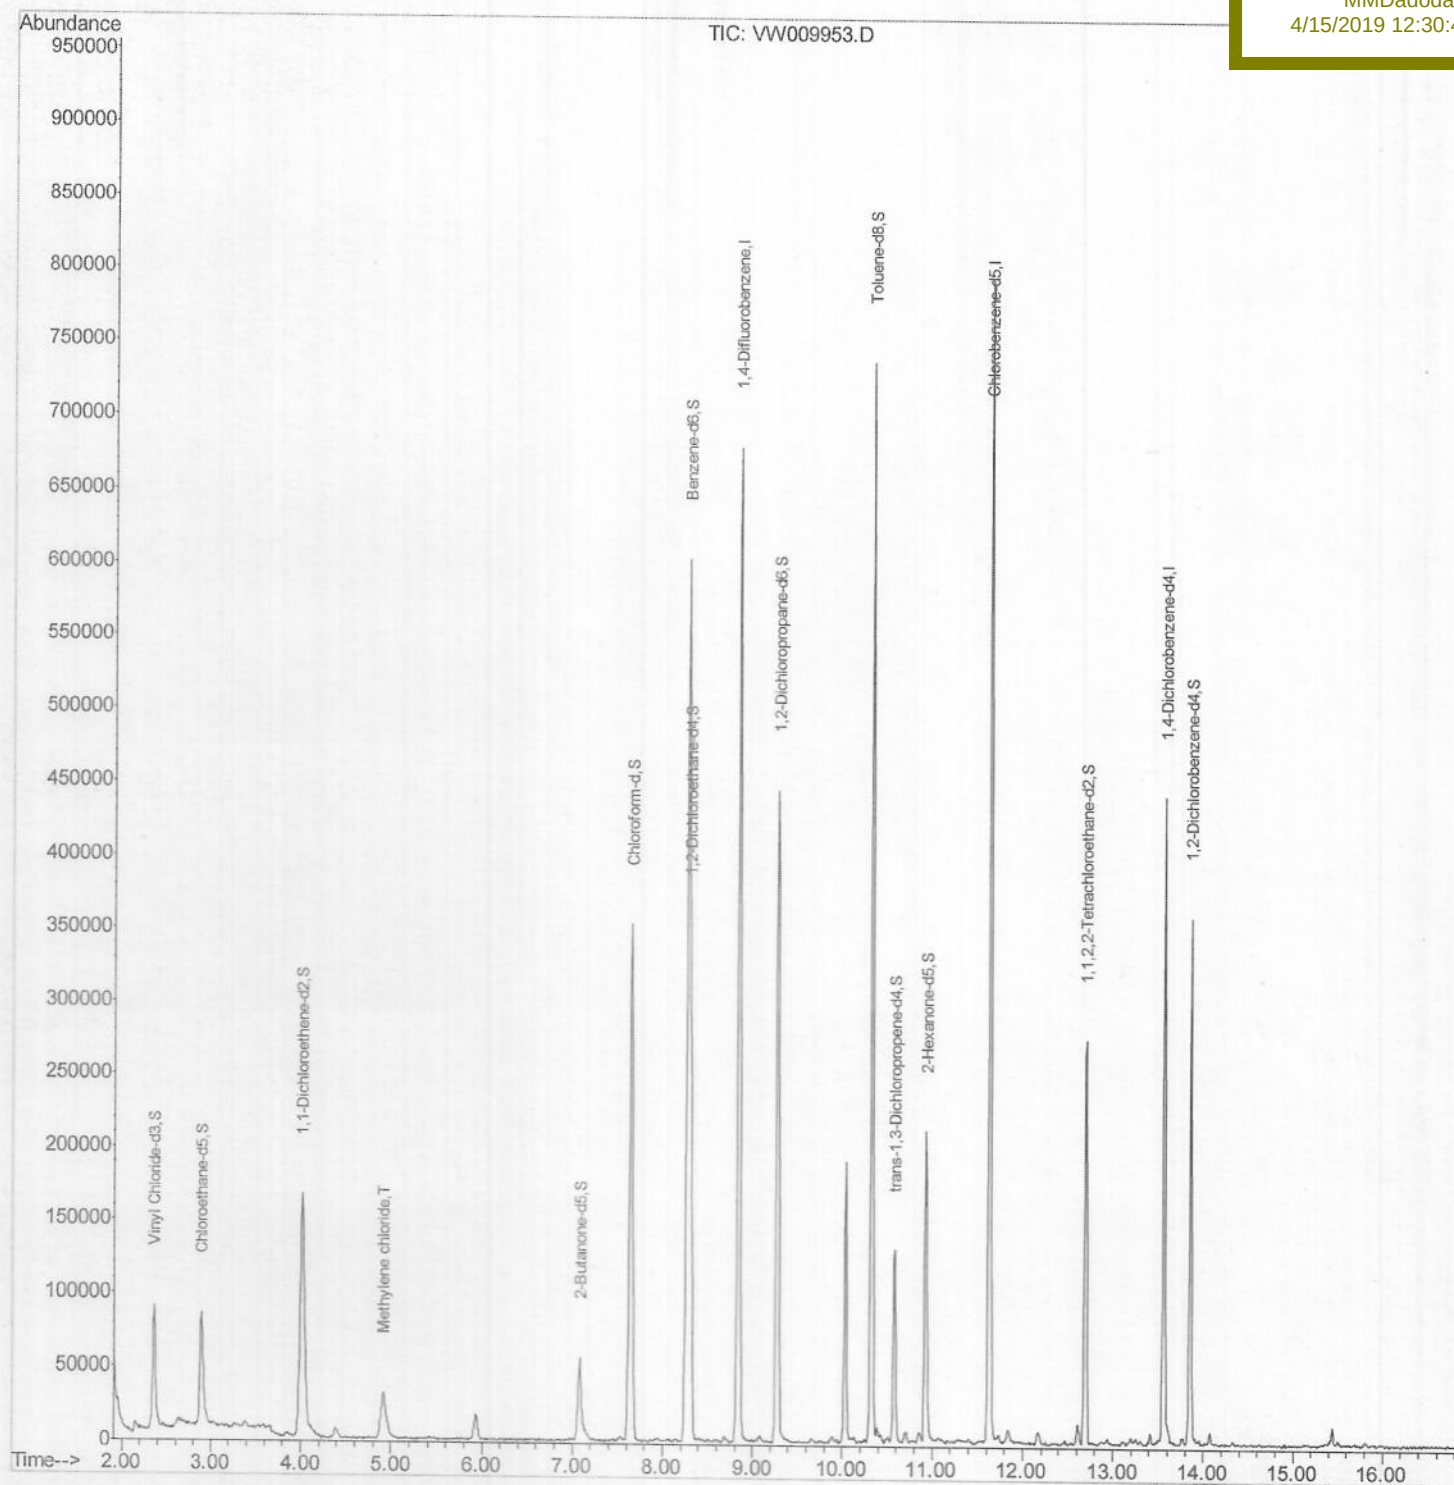
Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :

BFC19RE

Manual Integrations
APPROVEDMMDadoda
4/15/2019 12:30:43 AM

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\

Data File : VW009953.D

Acq On : 12 Apr 2019 12:21

Operator : SY/VA

Sample : K2255-18RE

Misc : 5.41G/10ML/MSVOA W/SOIL

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 13 00:25:34 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 12 23:54:39 2019

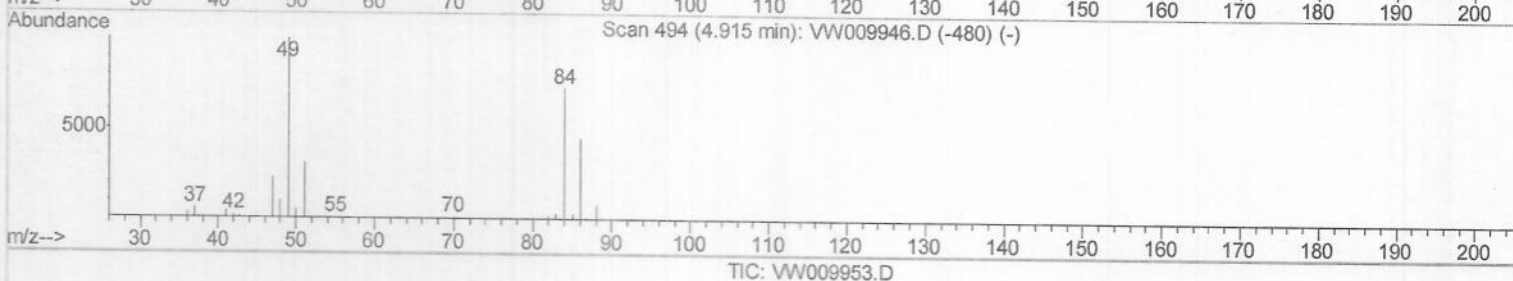
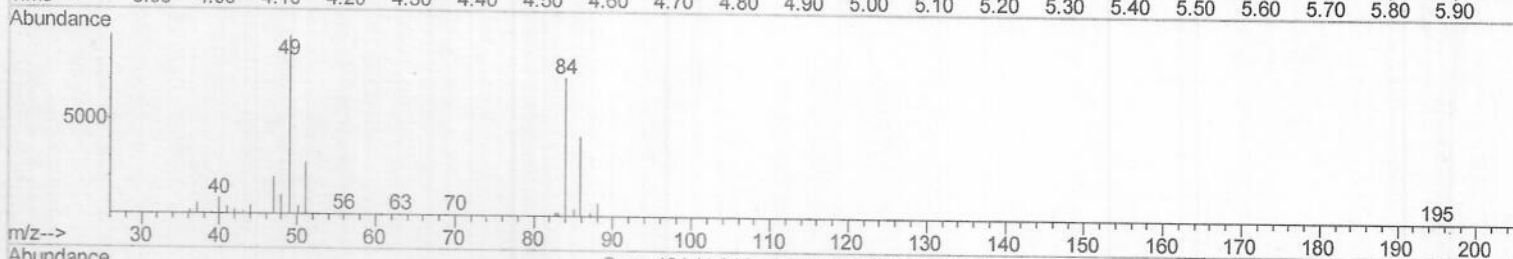
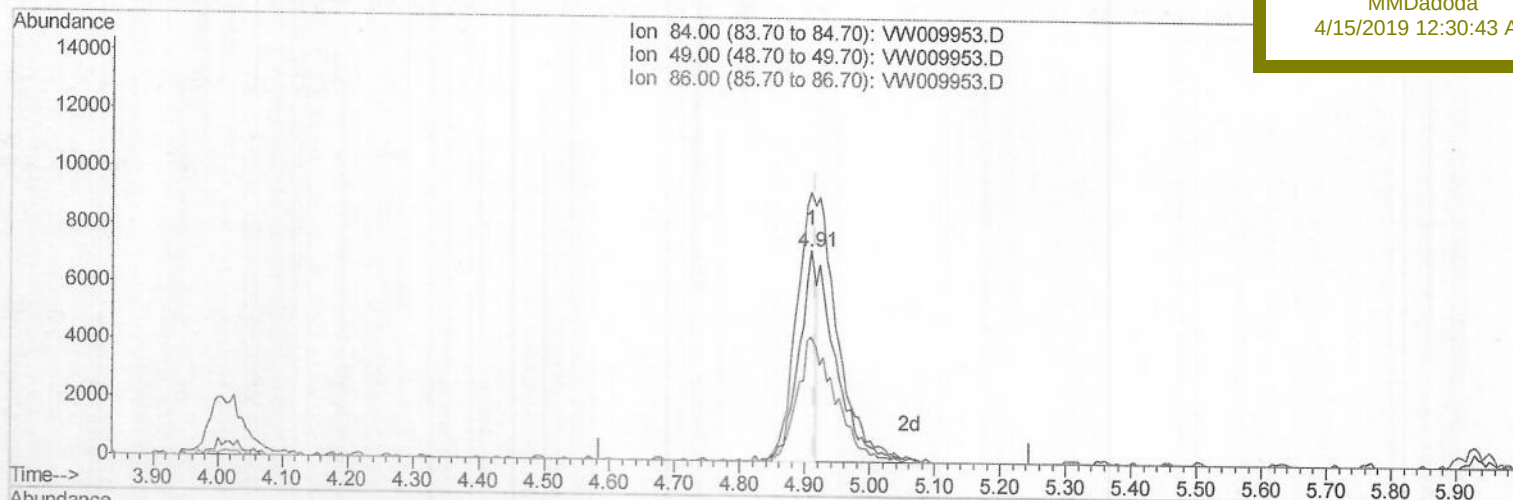
Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :

BFC19RE

Manual Integrations
APPROVEDMMDadoda
4/15/2019 12:30:43 AM

(16) Methylene chloride (T)

4.909min (-0.006) 1.43ug/L

response 13007

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	128.15
86.00	66.30	58.85
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\

Data File : VW009953.D

Acq On : 12 Apr 2019 12:21

Operator : SY/VA

Sample : K2255-18RE

Misc : 5.41G/10ML/MSVOA W/SOIL

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 13 00:25:34 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 12 23:54:39 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :

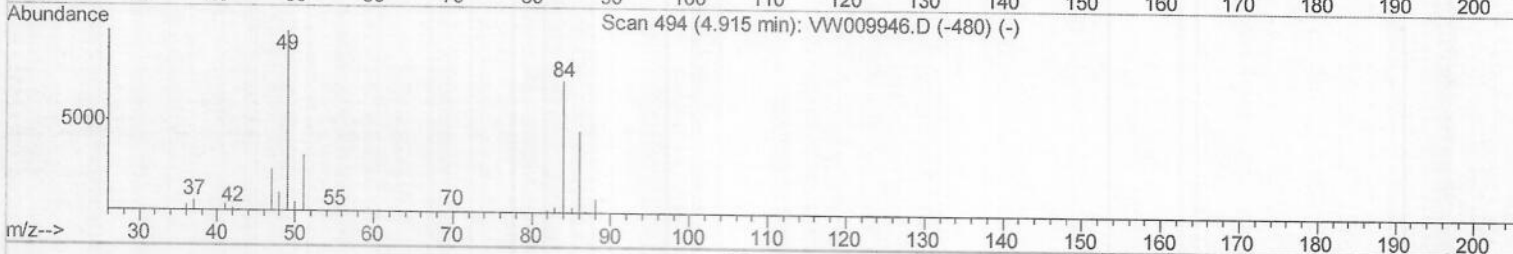
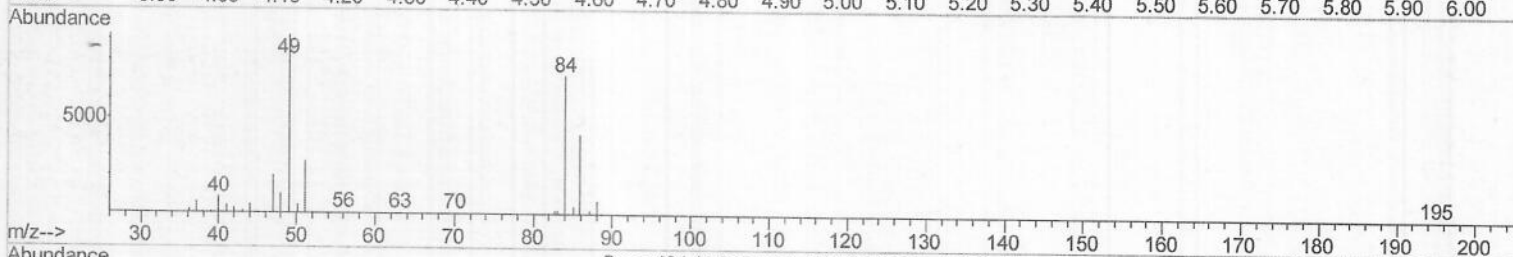
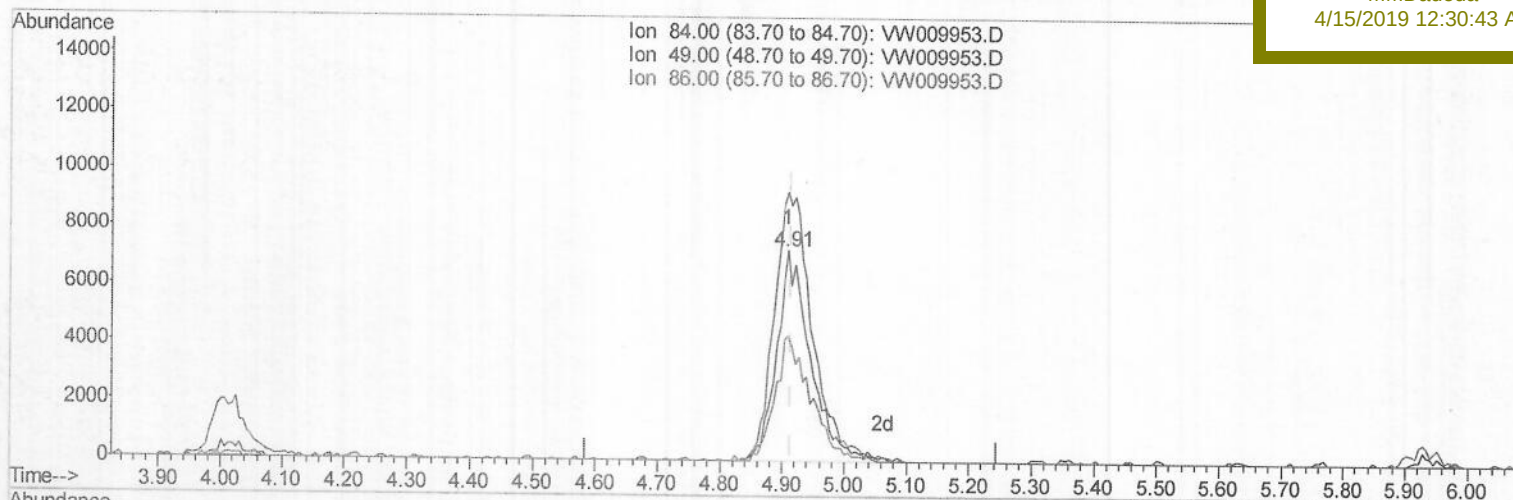
BFC19RE

Manual Integrations

APPROVED

MMDadoda

4/15/2019 12:30:43 AM



TIC: VW009953.D

(16) Methylene chloride (T)

4.909min (-0.006) 3.04ug/L m

response 27732

M.D
4/22/19

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	128.15
86.00	66.30	58.85
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\

Data File : VW009953.D

Acq On : 12 Apr 2019 12:21

Operator : SY/VA

Sample : K2255-18RE

Misc : 5.41G/10ML/MSVOA W/SOIL

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 13 00:25:34 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 12 23:54:39 2019

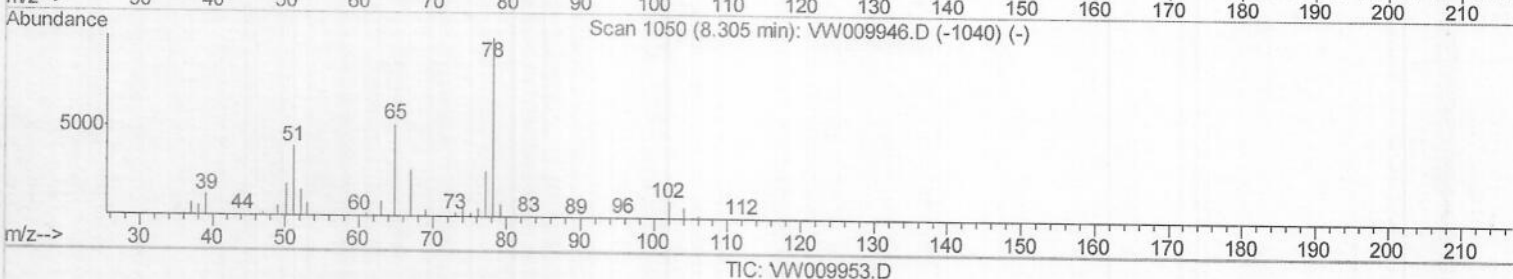
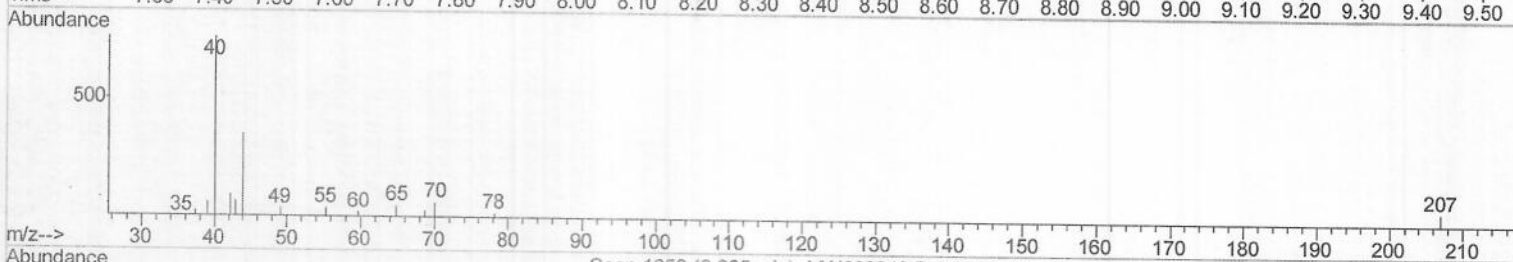
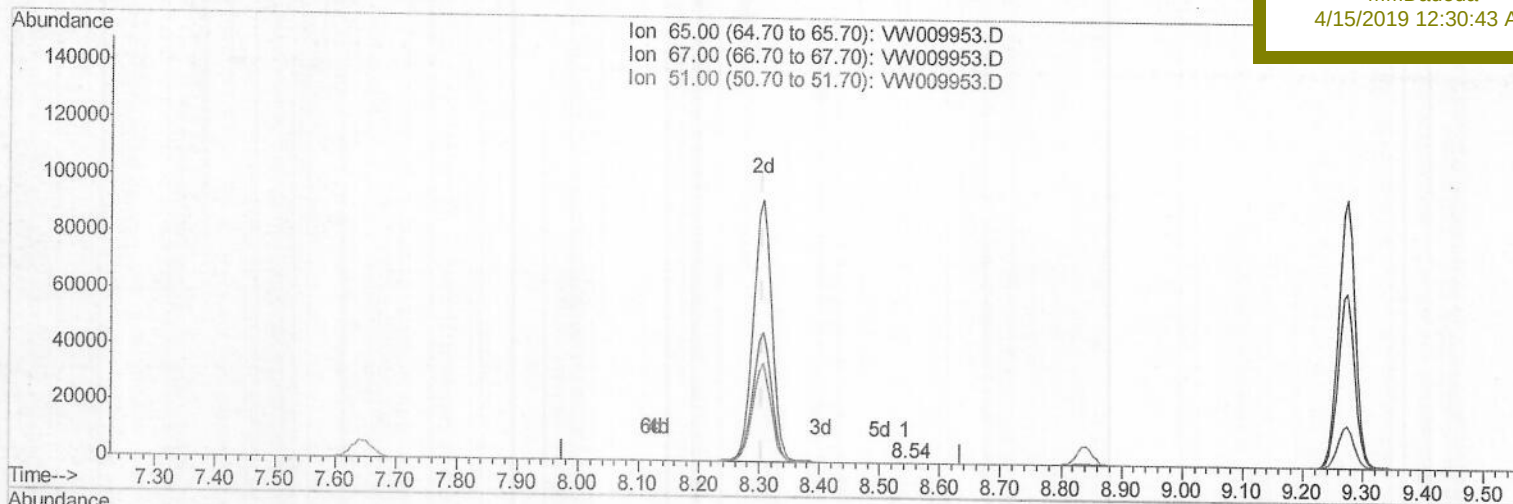
Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :

BFC19RE

Manual Integrations
APPROVEDMMDadoda
4/15/2019 12:30:43 AM

(26) 1,2-Dichloroethane-d4 (S)

8.543min (+0.238) 0.01ug/L

response 63

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	39.68
51.00	109.90	95.24
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\

Data File : VW009953.D

Acq On : 12 Apr 2019 12:21

Operator : SY/VA

Sample : K2255-18RE

Misc : 5.41G/10ML/MSVOA W/SOIL

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 13 00:25:34 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 12 23:54:39 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :

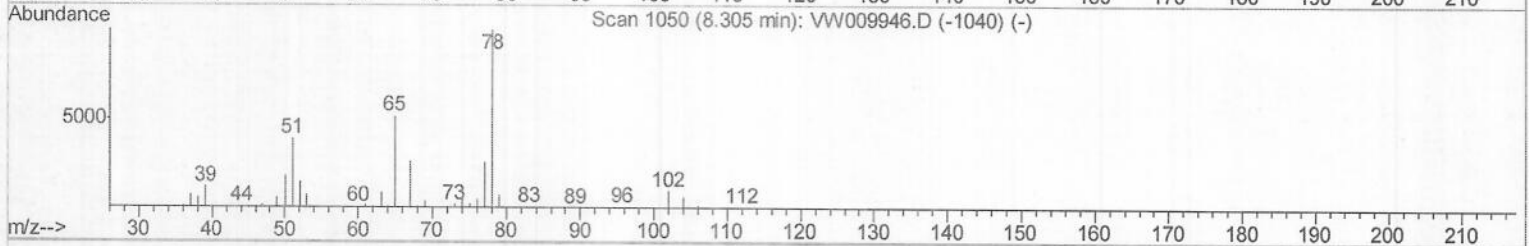
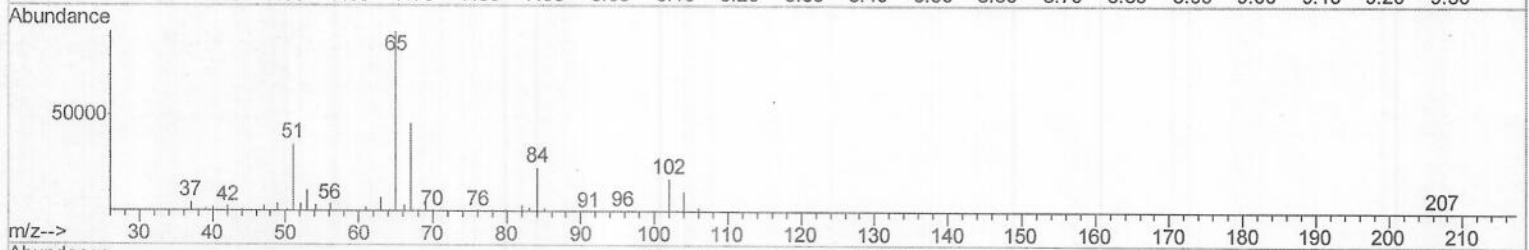
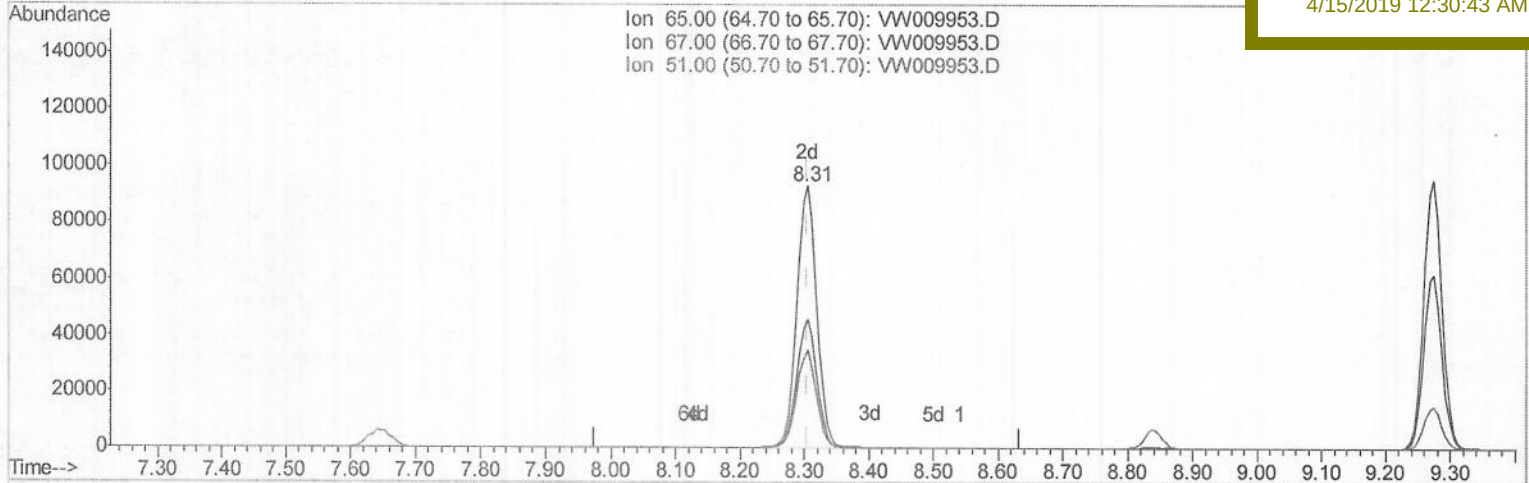
BFC19RE

Manual Integrations

APPROVED

MMDadoda

4/15/2019 12:30:43 AM



(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.000) 23.01ug/L m

response 199102

Ion Exp% Act%

65.00 100 100

67.00 50.90 0.01#

51.00 109.90 0.03#

0.00 0.00 0.00

M.D
4/22/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\

Data File : VW009953.D

Acq On : 12 Apr 2019 12:21

Operator : SY/VA

Sample : K2255-18RE

Misc : 5.41G/10ML/MSVOA W/SOIL

ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 13 00:27:33 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Fri Apr 12 23:54:39 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

Client Sampled :

BFC19RE

Manual Integrations
APPROVEDMMDadoda
4/15/2019 12:30:43 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	516559	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	409451	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	105258	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	111730	16.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.12%
7) Chloroethane-d5	2.89	69	107629	17.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.52%
10) 1,1-Dichloroethene-d2	4.01	63	213786	14.71	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.84%
20) 2-Butanone-d5	7.08	46	94054	42.85	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.70%
24) Chloroform-d	7.65	84	326872	23.19	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.76%
26) 1,2-Dichloroethane-d4	8.31	65	199102m	23.01	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.04%
29) Benzene-d6	8.27	84	568765	26.46	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.84%
33) 1,2-Dichloropropane-d6	9.27	67	186751	28.13	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	112.52%
37) Toluene-d8	10.32	98	449964	22.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.56%
38) trans-1,3-Dichloropropene-	10.58	79	66460	20.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.96%
39) 2-Hexanone-d5	10.93	63	60606	48.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.86%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	128847	20.88	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.52%
61) 1,2-Dichlorobenzene-d4	13.86	152	88051	23.84	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.36%

Target Compounds

16) Methylene chloride	4.91	84	27732m	3.044	ug/L	Ovalue
------------------------	------	----	--------	-------	------	--------

(#)=qualifier out of range (m)=manual integration (+)=signals summed

Mr D
4/22/19