

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\
 Data File : VW009962.D
 Acq On : 12 Apr 2019 16:49
 Operator : SY/VA
 Sample : K2303-07
 Misc : 5.71G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BF8A2

Manual Integrations
APPROVED

MMDadoda
 4/15/2019 12:30:46 AM

Quant Time: Apr 13 01:13:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 12 23:54:39 2019
 Response via : Initial Calibration

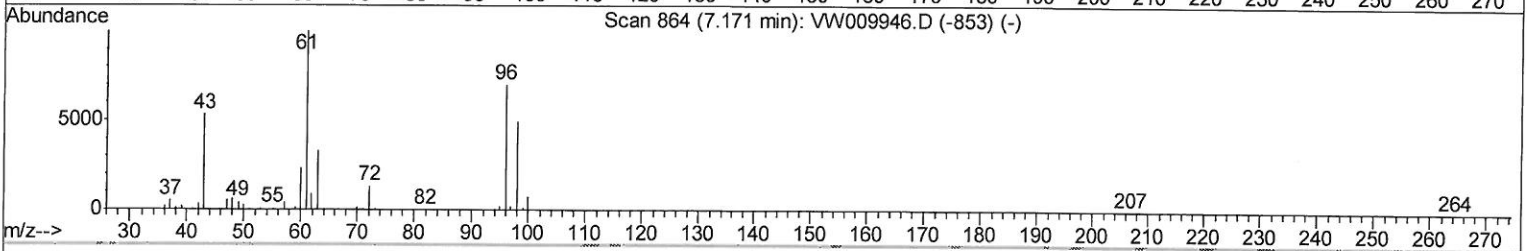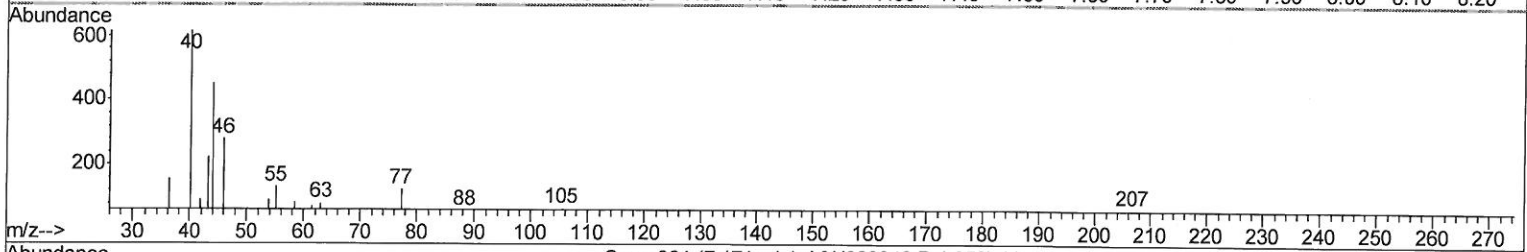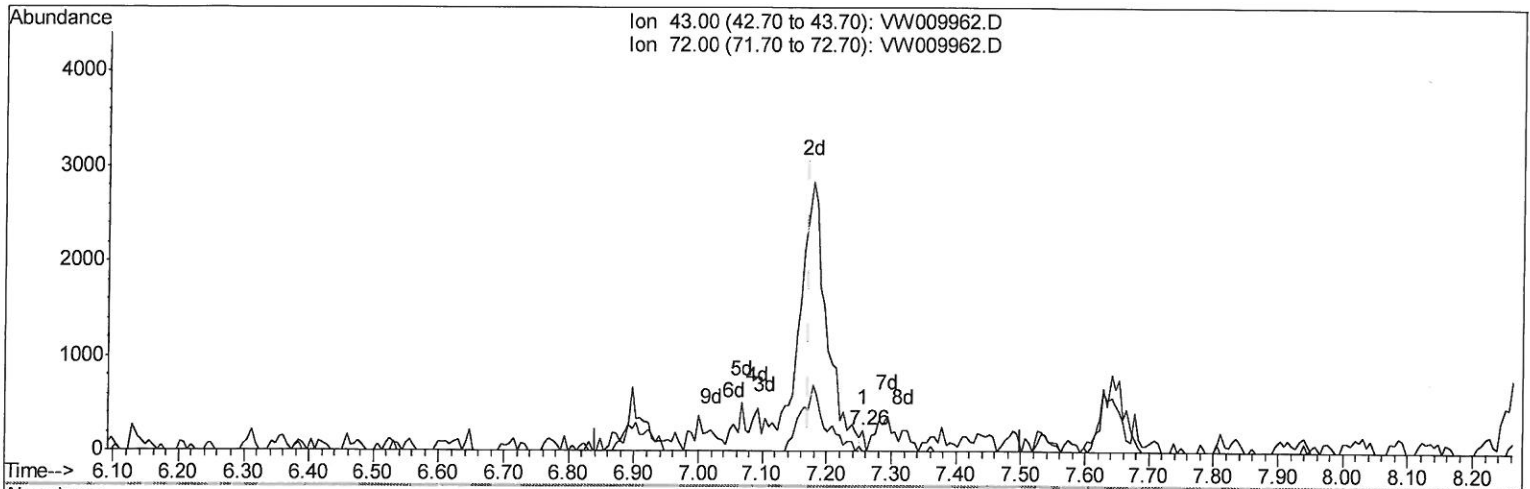

TIC: VW009962.D

(21) 2-Butanone

7.257min (+0.086) 0.03ug/L

response 81

Ion	Exp%	Act%
43.00	100	100
72.00	24.10	24.69
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\
 Data File : VW009962.D
 Acq On : 12 Apr 2019 16:49
 Operator : SY/VA
 Sample : K2303-07
 Misc : 5.71G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF8A2

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:30:46 AM

Quant Time: Apr 13 01:13:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 12 23:54:39 2019
 Response via : Initial Calibration

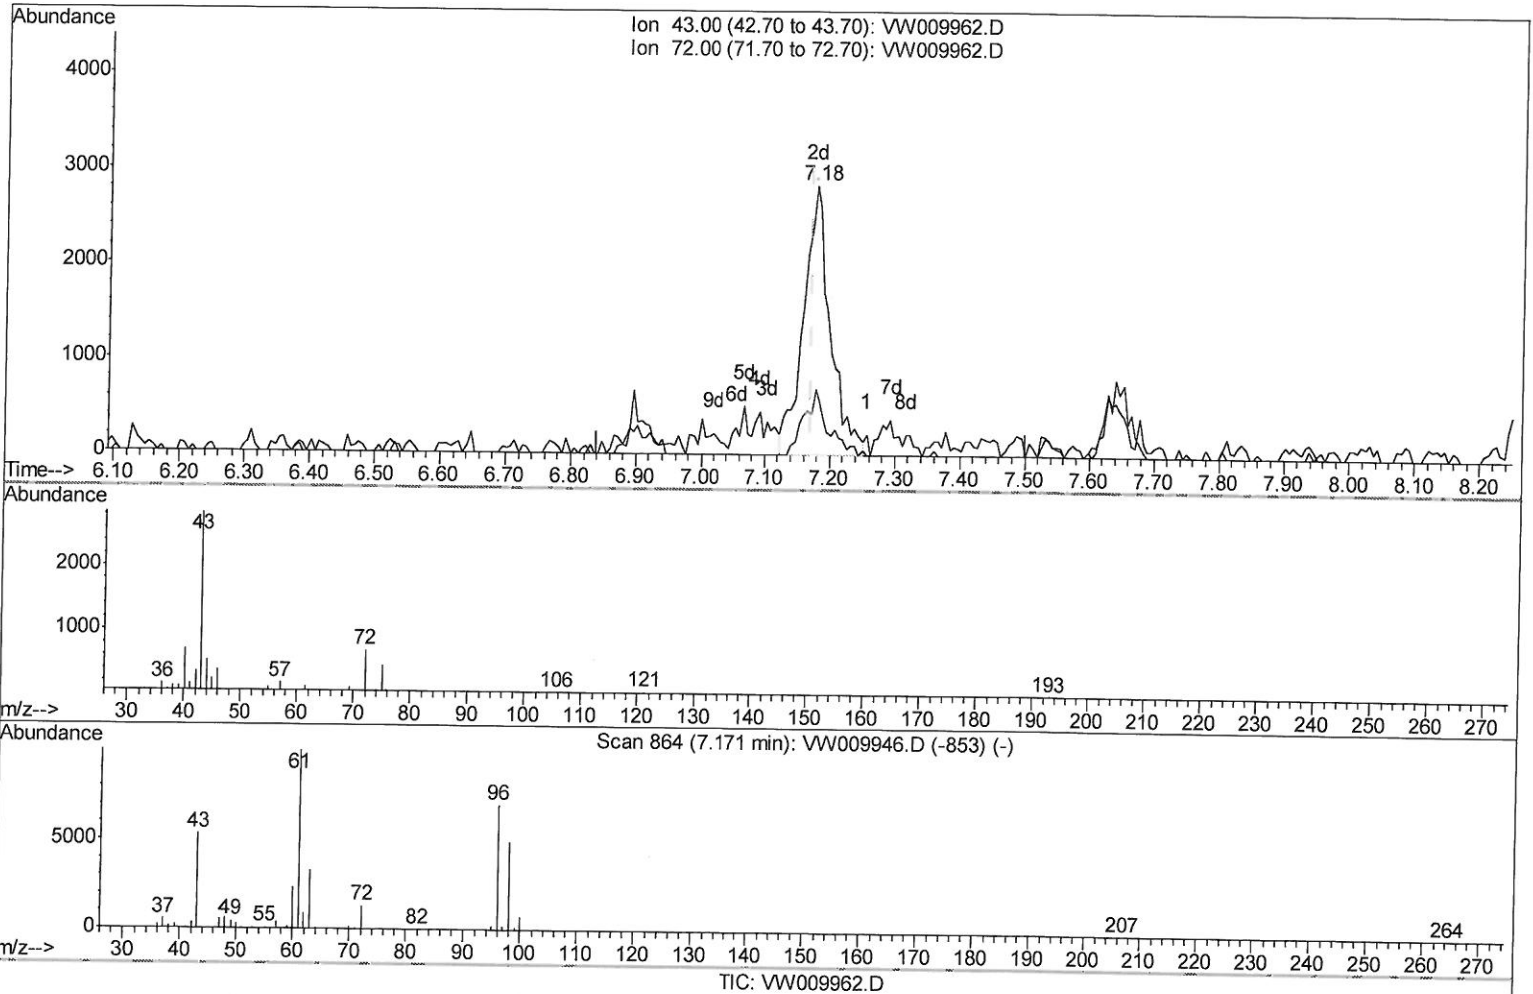

(21) 2-Butanone

7.177min (+0.006) 3.03ug/L m 204/187/19 54

response 8212

Ion	Exp%	Act%
43.00	100	100
72.00	24.10	0.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\
 Data File : VW009962.D
 Acq On : 12 Apr 2019 16:49
 Operator : SY/VA
 Sample : K2303-07
 Misc : 5.71G/10ML/MSVOA W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF8A2

Manual Integrations
 APPROVED

MMDadoda
 4/15/2019 12:30:46 AM

Quant Time: Apr 13 01:14:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 12 23:54:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	467634	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	445484	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	182945	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	91498	14.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.80%
7) Chloroethane-d5	2.90	69	86752	15.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.88%
10) 1,1-Dichloroethene-d2	4.01	63	181080	13.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.04%
20) 2-Butanone-d5	7.07	46	101839	51.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.52%
24) Chloroform-d	7.65	84	283584	22.22	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.88%
26) 1,2-Dichloroethane-d4	8.31	65	177430	22.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.60%
29) Benzene-d6	8.27	84	488425	20.89	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.56%
33) 1,2-Dichloropropane-d6	9.27	67	164847	22.82	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.28%
37) Toluene-d8	10.32	98	407496	18.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.40%
38) trans-1,3-Dichloropropene-	10.58	79	65673	19.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.24%
39) 2-Hexanone-d5	10.93	63	69873	51.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.64%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	153361	22.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.36%
61) 1,2-Dichlorobenzene-d4	13.86	152	152912	23.82	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.28%

Target Compounds

				Ovalue
13) Acetone	4.12	43	31469	14.782 ug/L 96
16) Methylene chloride	4.92	84	41979	5.090 ug/L 92
21) 2-Butanone	7.18	43	8212m	3.033 ug/L 04/18/19 by

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW041119\
Data File : VW009962.D
Acq On : 12 Apr 2019 16:49
Operator : SY/VA
Sample : K2303-07
Misc : 5.71G/10ML/MSVOA W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF8A2

Manual Integrations
APPROVED

MMDadoda
4/15/2019 12:30:46 AM

Quant Time: Apr 13 01:14:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 23:54:39 2019
Response via : Initial Calibration

