

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022493.D
 Acq On : 11 Apr 2022 19:21
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 12 00:00:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	384630	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	369158	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	191604	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	139888	16.452	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.800%
7) Chloroethane-d5	2.885	69	92413	17.342	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.360%
11) 1,1-Dichloroethene-d2	4.013	63	143033	12.969	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.880%
21) 2-Butanone-d5	7.080	46	78759	53.054	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.100%
24) Chloroform-d	7.653	84	270352	22.488	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.960%
26) 1,2-Dichloroethane-d4	8.305	65	160468	23.361	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.440%
32) Benzene-d6	8.275	84	493056	21.861	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.440%
36) 1,2-Dichloropropane-d6	9.275	67	153073	23.453	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.800%
41) Toluene-d8	10.323	98	468416	21.206	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.840%
43) trans-1,3-Dichloroprop...	10.579	79	64663	20.992	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.960%
47) 2-Hexanone-d5	10.927	63	65224	53.711	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.420%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	140891	25.387	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	167827	24.729	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.920%
Target Compounds						Qvalue
68) 1,2-Dibromo-3-chloropr...	14.822	75	2659	2.813	ug/L	# 14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
Data File : VW022493.D
Acq On : 11 Apr 2022 19:21
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 12 00:00:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Apr 11 23:55:29 2022
Response via : Initial Calibration

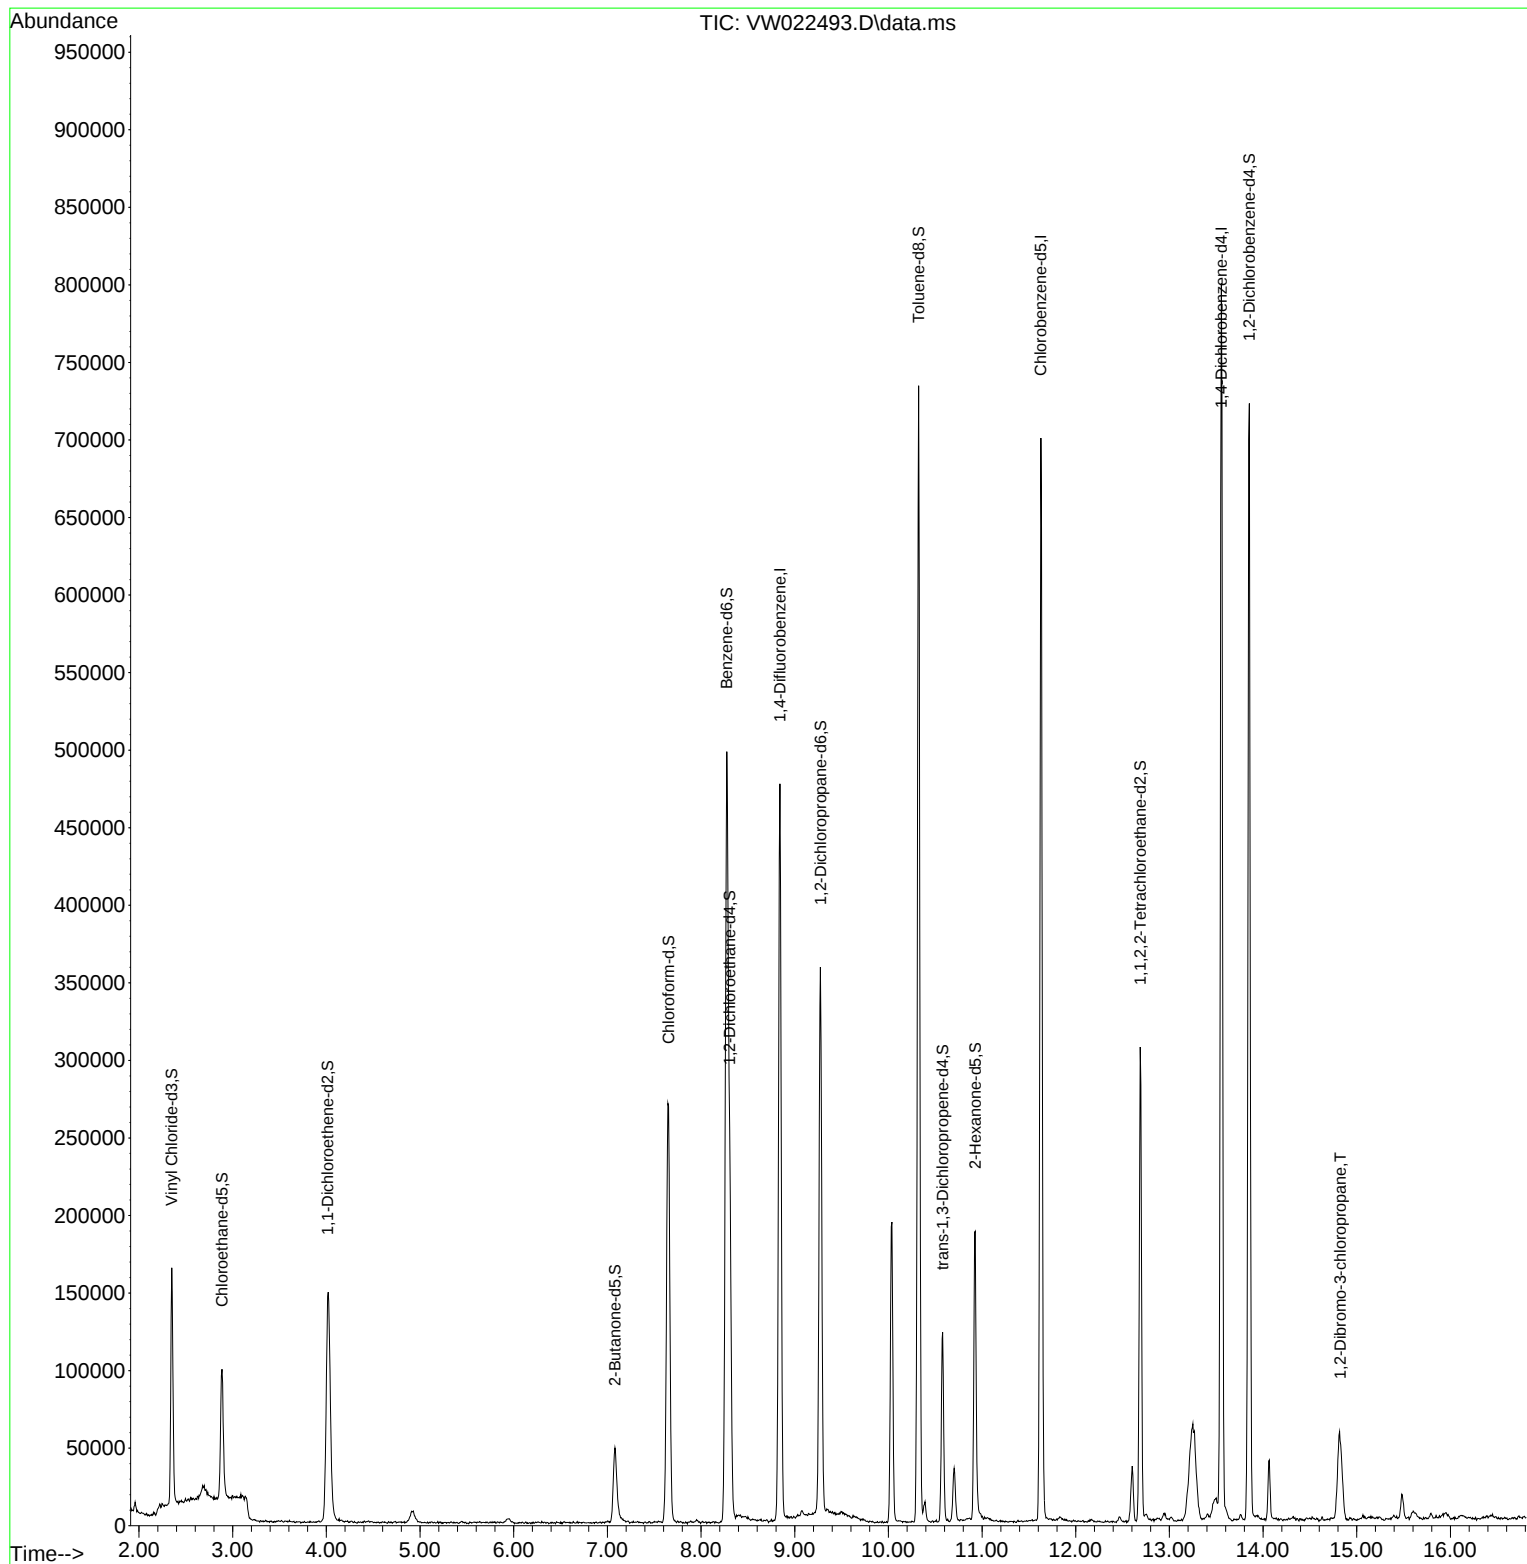

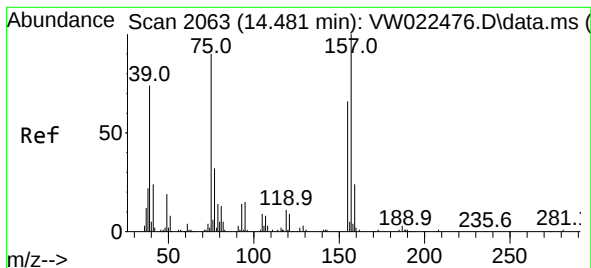

#68
 1,2-Dibromo-3-chloropropane
 Concen: 2.813 ug/L
 RT: 14.822 min Scan# 2119
 Delta R.T. 0.342 min
 Lab File: VW022493.D
 Acq: 11 Apr 2022 19:21

Instrument :
 MSVOA_W
 ClientSampleId :

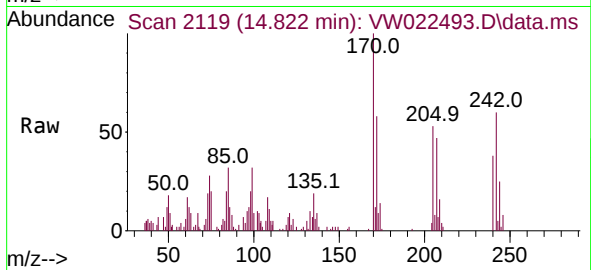

Tgt Ion: 75 Resp: 2659
 Ion Ratio Lower Upper
 75 100
 155 7.5 55.6 83.4#
 157 0.0 69.8 104.6#

