




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022483.D
 Acq On : 11 Apr 2022 15:21
 Operator : SY/VA
 Sample : N2316-04
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:58:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

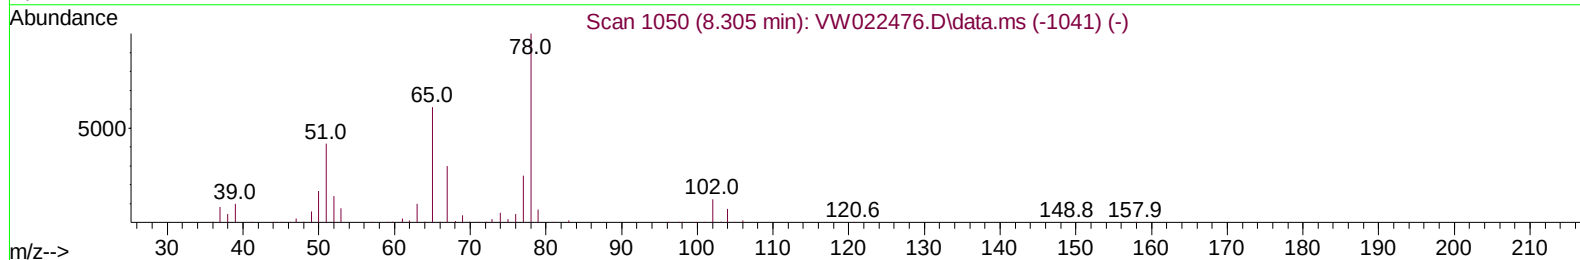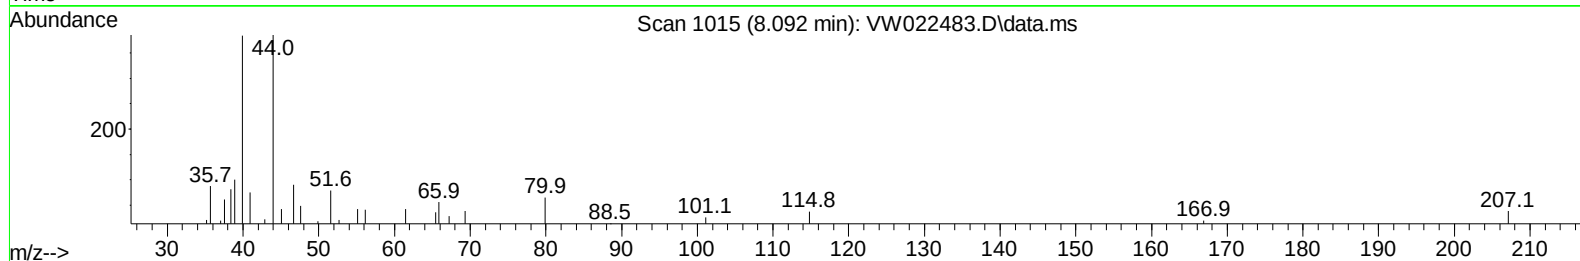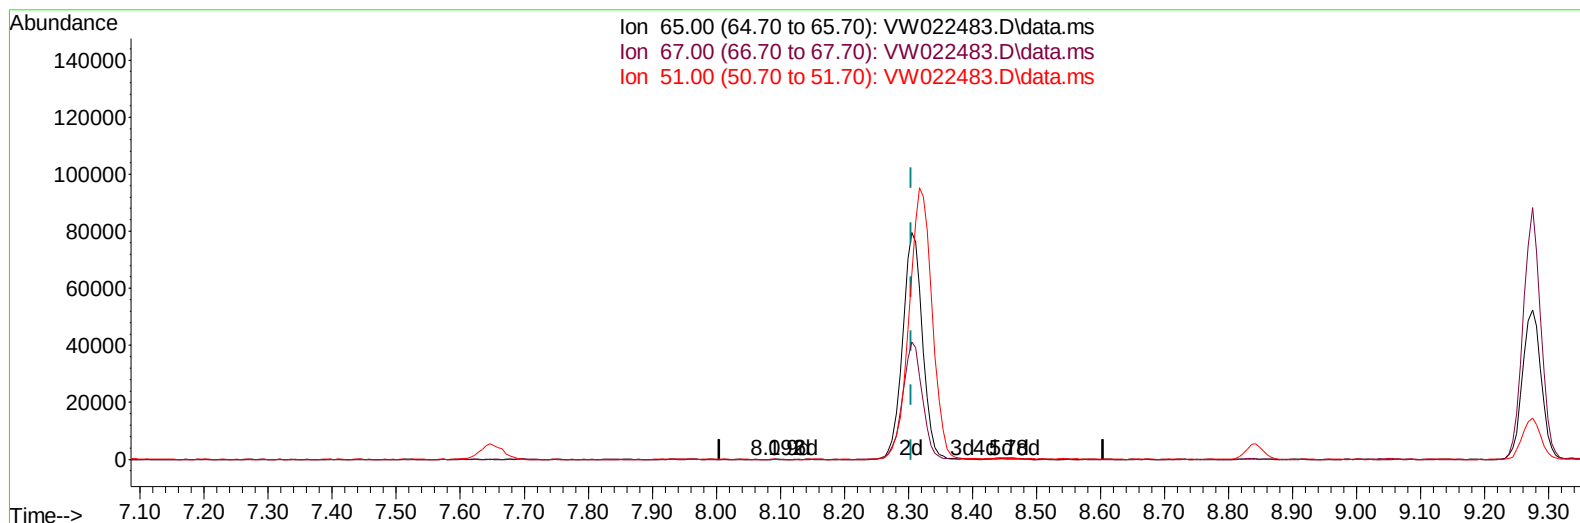

TIC: VW022483.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.092min (-0.213) 0.01 ug/L

response 50

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	46.00
51.00	99.30	112.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022483.D
 Acq On : 11 Apr 2022 15:21
 Operator : SY/VA
 Sample : N2316-04
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:58:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

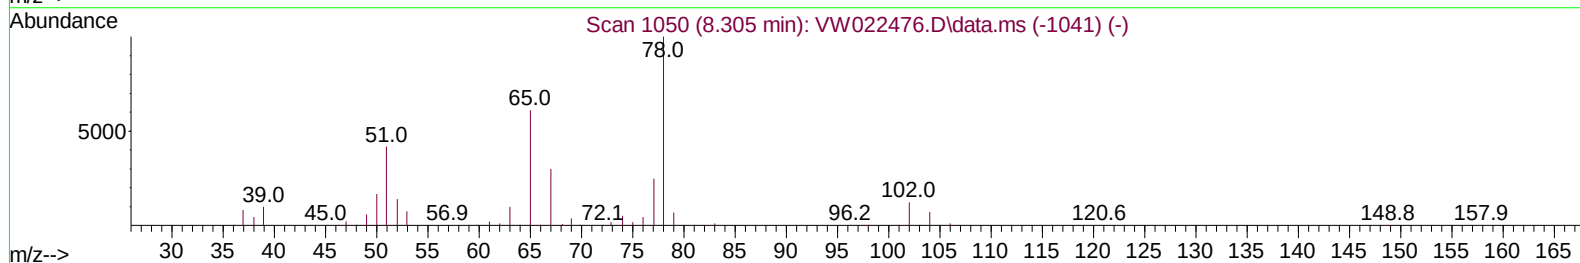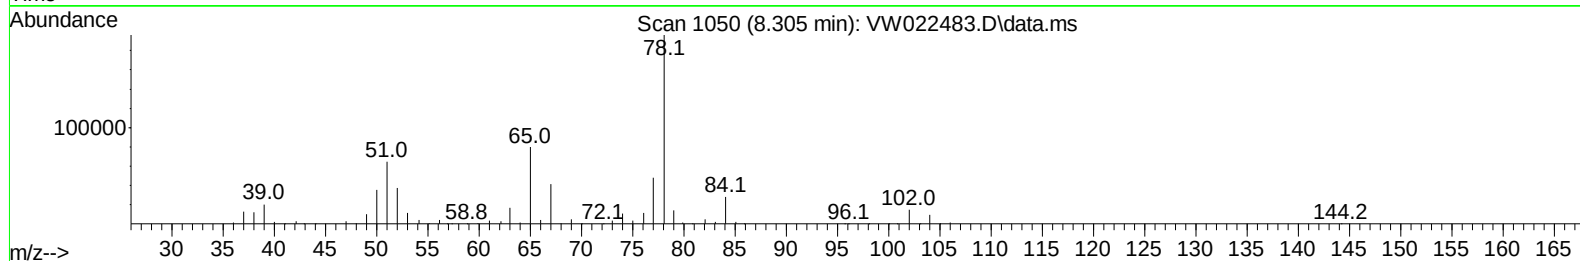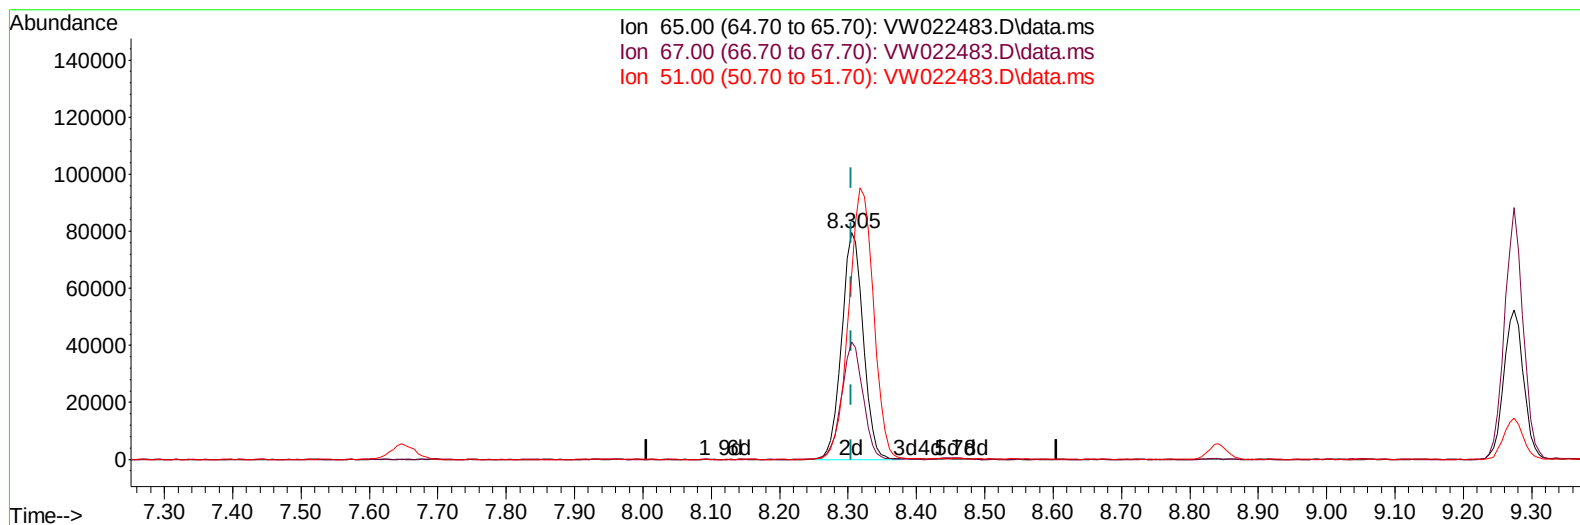

TIC: VW022483.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 22.42 ug/L m

response 172259

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.01#
51.00	99.30	0.03#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022483.D
 Acq On : 11 Apr 2022 15:21
 Operator : SY/VA
 Sample : N2316-04
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:58:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

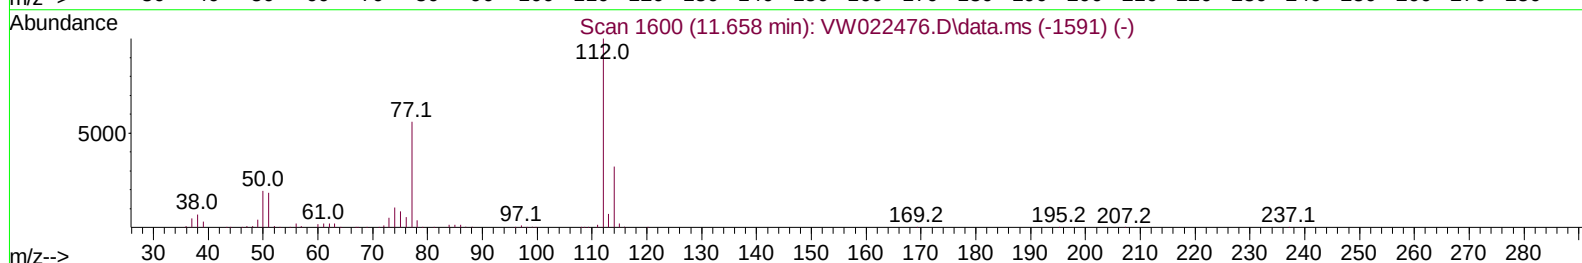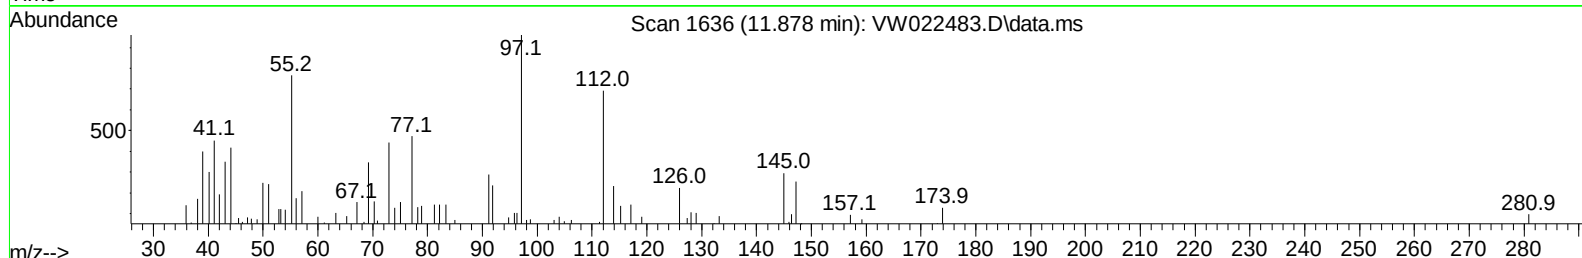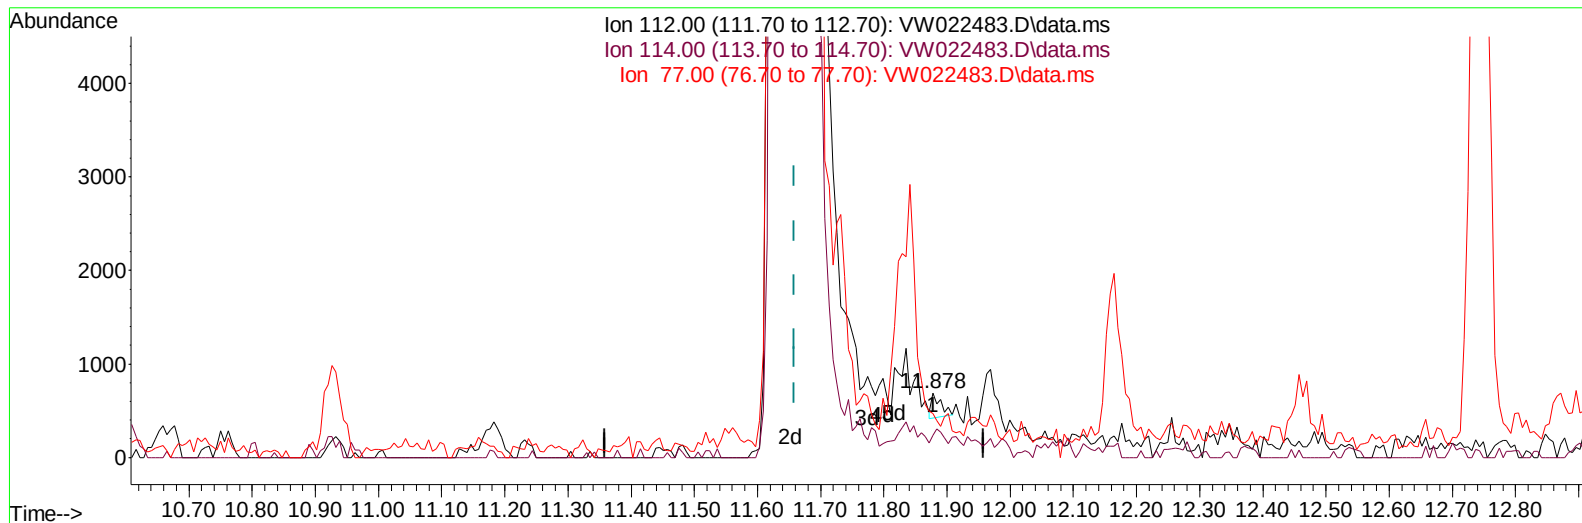

TIC: VW022483.D\data.ms

(51) Chlorobenzene (T)

11.878min (+ 0.220) 0.01 ug/L

response 276

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	29.30	33.82
77.00	60.10	68.35
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022483.D
 Acq On : 11 Apr 2022 15:21
 Operator : SY/VA
 Sample : N2316-04
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:58:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

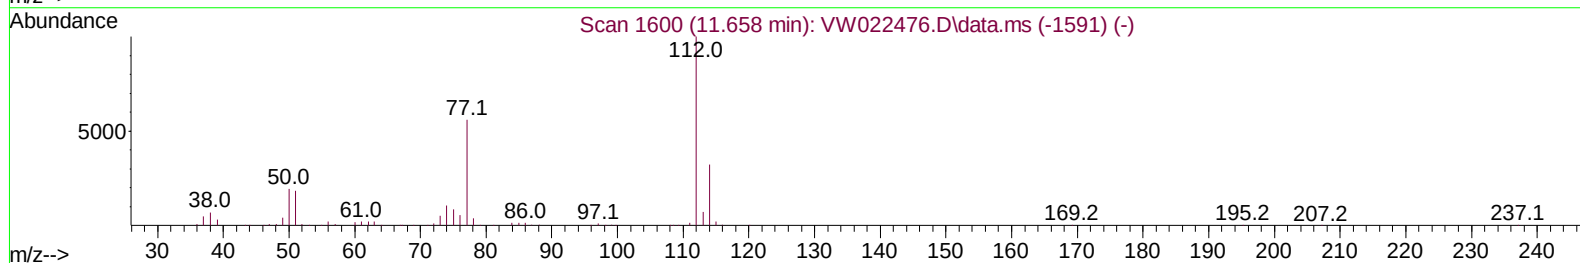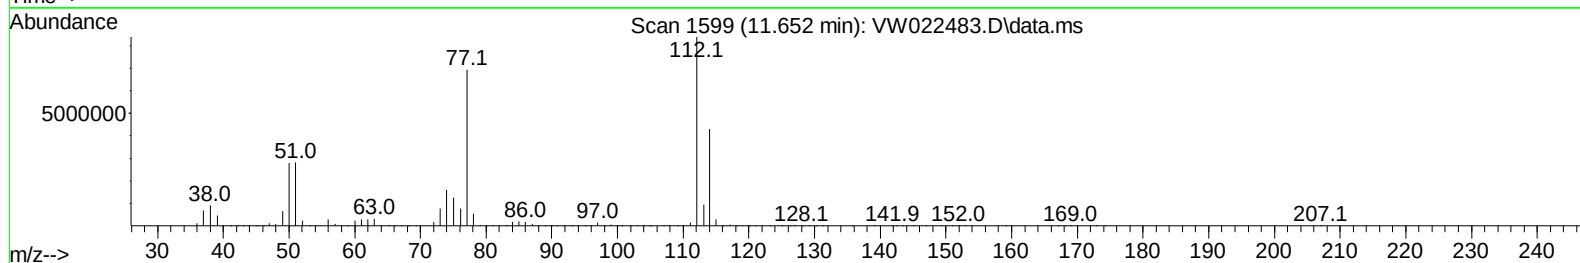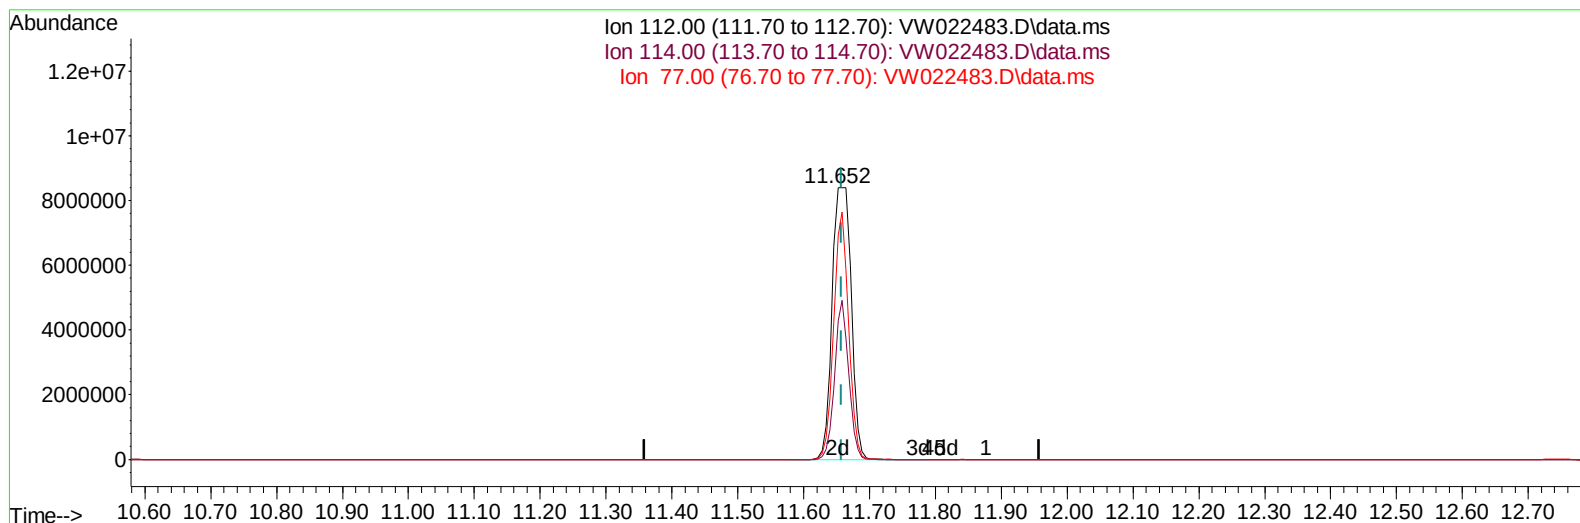

TIC: VW022483.D\data.ms

(51) Chlorobenzene (T)

11.652min (-0.006) 801.53 ug/L m

response 16789610

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	29.30	51.04#
77.00	60.10	82.66#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022483.D
 Acq On : 11 Apr 2022 15:21
 Operator : SY/VA
 Sample : N2316-04
 Misc : 6.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ2

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:58:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	430178	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	440600	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	208235	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	151154	15.894	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.560%	
7) Chloroethane-d5	2.885	69	106972	17.948	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	71.800%	
11) 1,1-Dichloroethene-d2	4.019	63	170272	13.804	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	55.200%	
21) 2-Butanone-d5	7.074	46	89938	54.169	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.340%	
24) Chloroform-d	7.653	84	295670	21.990	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	87.960%	
26) 1,2-Dichloroethane-d4	8.305	65	172259m	22.422	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	89.680%	
32) Benzene-d6	8.275	84	534701	19.863	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	79.440%	
36) 1,2-Dichloropropane-d6	9.274	67	166751	21.406	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	85.640%	
41) Toluene-d8	10.323	98	503938	19.114	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	76.440%	
43) trans-1,3-Dichloroprop...	10.579	79	74566	20.282	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	81.120%	
47) 2-Hexanone-d5	10.921	63	77973	53.798	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	107.600%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	154621	23.343	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	93.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	183354	24.859	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.440%	
Target Compounds						
					Qvalue	
13) Acetone	4.129	43	14940	13.216	ug/L	88
14) Carbon disulfide	4.391	76	26760	1.404	ug/L	100
33) Benzene	8.323	78	1005178	33.602	ug/L	100
42) Toluene	10.384	91	114900	3.352	ug/L	97
51) Chlorobenzene	11.652	112	16789610m	801.530	ug/L	
52) Ethylbenzene	11.731	91	21461	0.559	ug/L	99
53) m,p-Xylene	11.835	106	14159	0.969	ug/L	100
54) o-Xylene	12.164	106	10275	0.736	ug/L	89
63) 1,2,4-Trimethylbenzene	13.249	105	15710	0.543	ug/L	96
65) 1,4-Dichlorobenzene	13.579	146	16081	1.149	ug/L	96
67) 1,2-Dichlorobenzene	13.865	146	17474	1.392	ug/L #	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
Data File : VW022483.D
Acq On : 11 Apr 2022 15:21
Operator : SY/VA
Sample : N2316-04
Misc : 6.57g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNQ2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:58:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Apr 11 23:55:29 2022
Response via : Initial Calibration

