




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022484.D
 Acq On : 11 Apr 2022 15:45
 Operator : SY/VA
 Sample : N2316-05
 Misc : 6.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:58:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

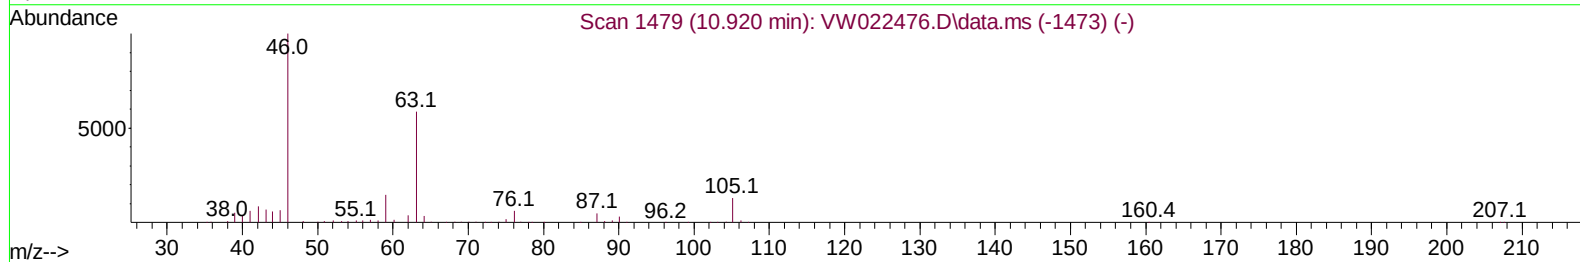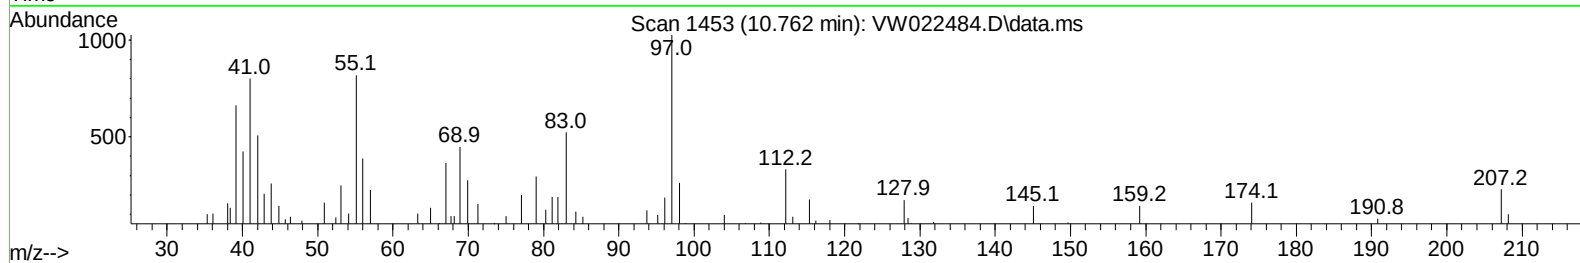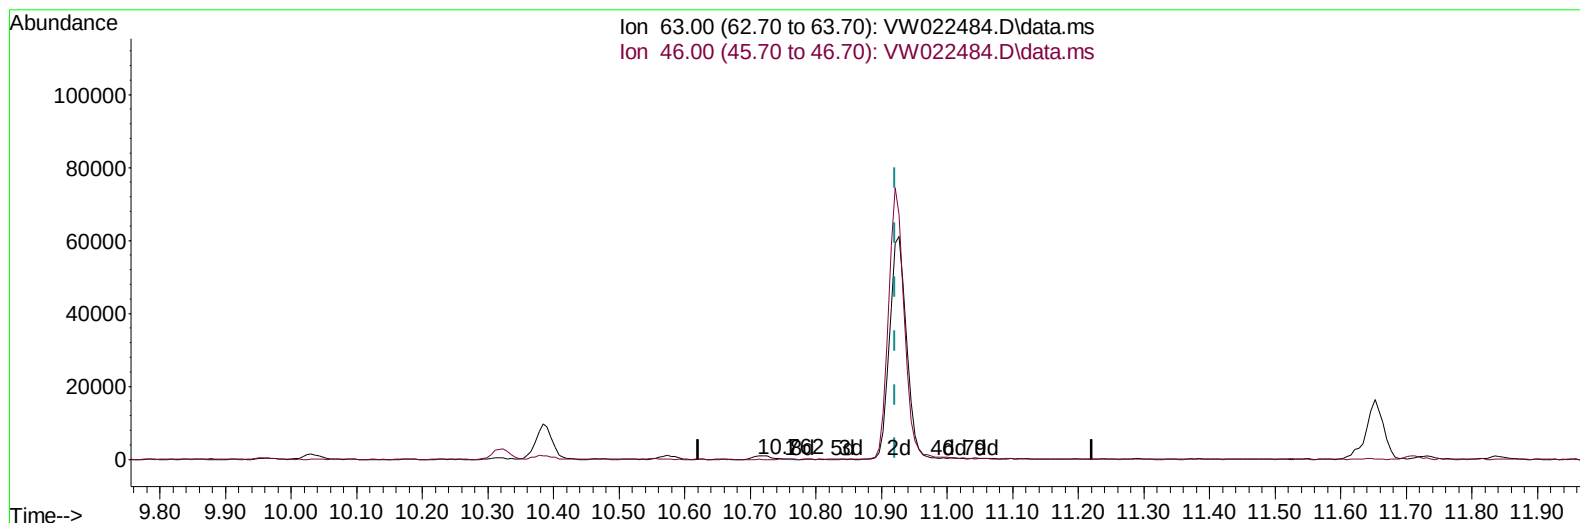

TIC: VW022484.D\data.ms

(47) 2-Hexanone-d5 (S)

10.762min (-0.158) 0.05 ug/L

response 75

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	177.60	205.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022484.D
 Acq On : 11 Apr 2022 15:45
 Operator : SY/VA
 Sample : N2316-05
 Misc : 6.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:58:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

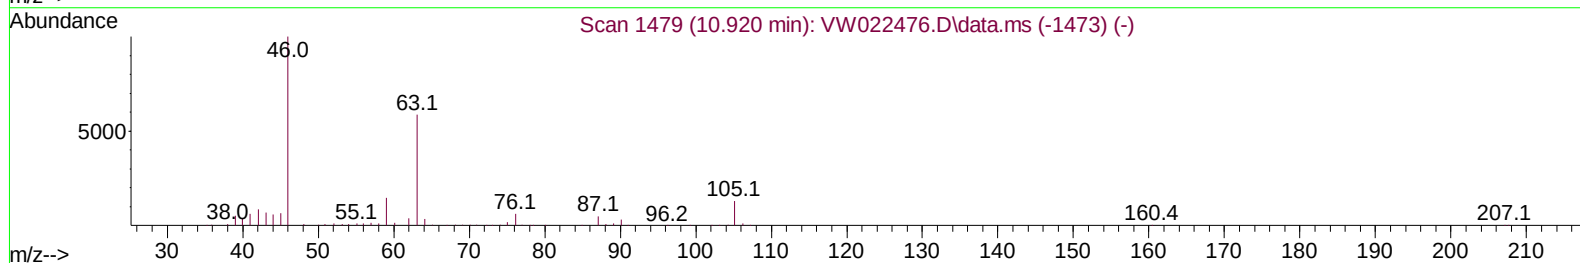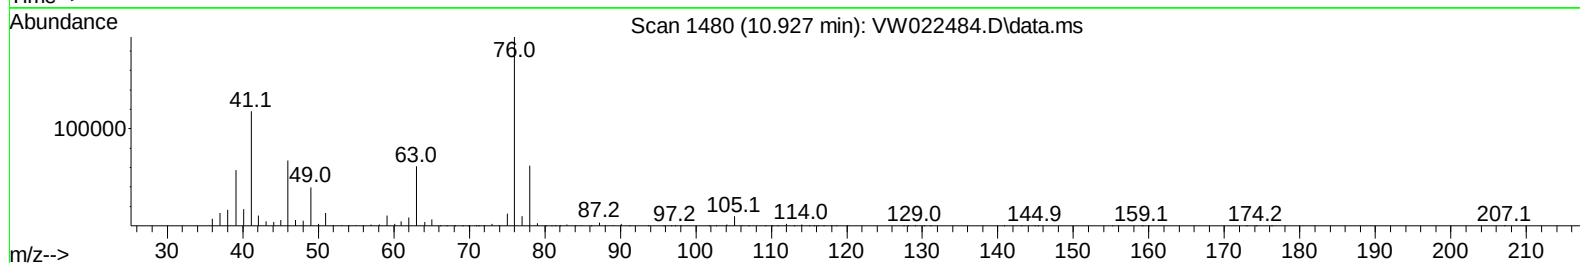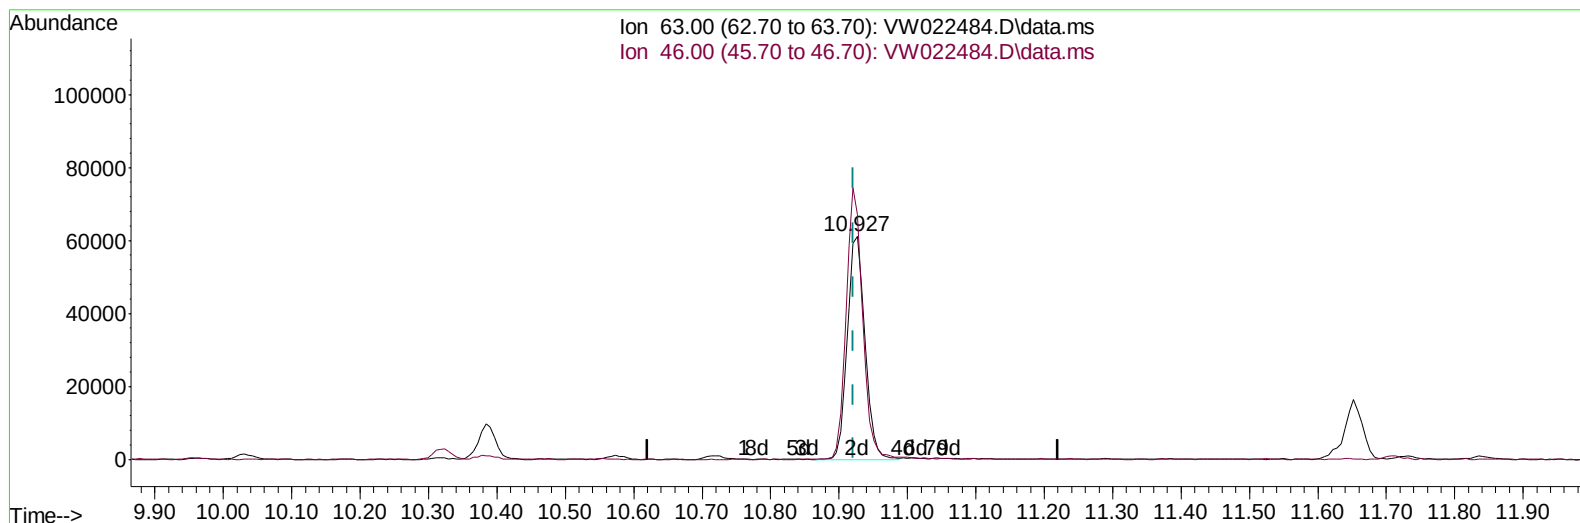

TIC: VW022484.D\data.ms

(47) 2-Hexanone-d5 (S)

10.927min (+ 0.006) 80.56 ug/L m

response 110135

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	177.60	0.14#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022484.D
 Acq On : 11 Apr 2022 15:45
 Operator : SY/VA
 Sample : N2316-05
 Misc : 6.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ3

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:58:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	432021	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	415601	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	213406	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	157793	16.522	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	66.080%	
7) Chloroethane-d5	2.885	69	120116	20.067	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.280%	
11) 1,1-Dichloroethene-d2	4.019	63	174769	14.109	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.440%	
21) 2-Butanone-d5	7.080	46	80501	48.279	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.560%	
24) Chloroform-d	7.647	84	300685	22.267	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	89.080%	
26) 1,2-Dichloroethane-d4	8.305	65	176251	22.844	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	91.360%	
32) Benzene-d6	8.275	84	556285	21.908	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	87.640%	
36) 1,2-Dichloropropane-d6	9.275	67	171532	23.344	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	93.360%	
41) Toluene-d8	10.323	98	522507	21.011	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	84.040%	
43) trans-1,3-Dichloroprop...	10.573	79	74673	21.533	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	86.120%	
47) 2-Hexanone-d5	10.927	63	110135m	80.560	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	161.120%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	156051	24.976	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	99.920%	
66) 1,2-Dichlorobenzene-d4	13.853	152	193369	25.582	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	102.320%	
Target Compounds						
						Qvalue
13) Acetone	4.129	43	103768	91.403	ug/L	94
22) 2-Butanone	7.177	43	17864	10.418	ug/L	81
33) Benzene	8.323	78	2163596	76.678	ug/L	100
35) Methylcyclohexane	9.335	83	16486	1.216	ug/L	95
42) Toluene	10.384	91	169621	5.246	ug/L	96
51) Chlorobenzene	11.652	112	1228794	62.191	ug/L	97
52) Ethylbenzene	11.731	91	34084	0.940	ug/L	99
53) m,p-Xylene	11.835	106	9638	0.699	ug/L	85
54) o-Xylene	12.164	106	8638	0.656	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
Data File : VW022484.D
Acq On : 11 Apr 2022 15:45
Operator : SY/VA
Sample : N2316-05
Misc : 6.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNQ3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:58:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Apr 11 23:55:29 2022
Response via : Initial Calibration

