




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
Data File : VW022487.D
Acq On : 11 Apr 2022 16:57
Operator : SY/VA
Sample : N2316-08
Misc : 6.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNQ7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:59:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Apr 11 23:55:29 2022
Response via : Initial Calibration

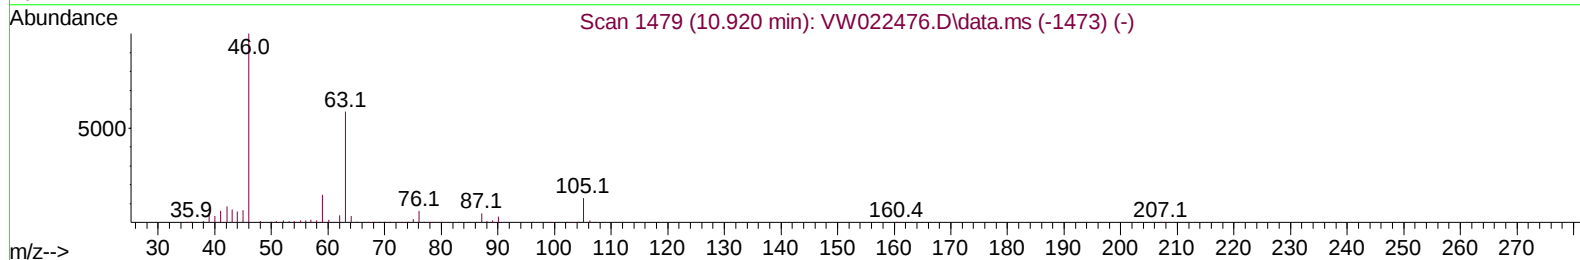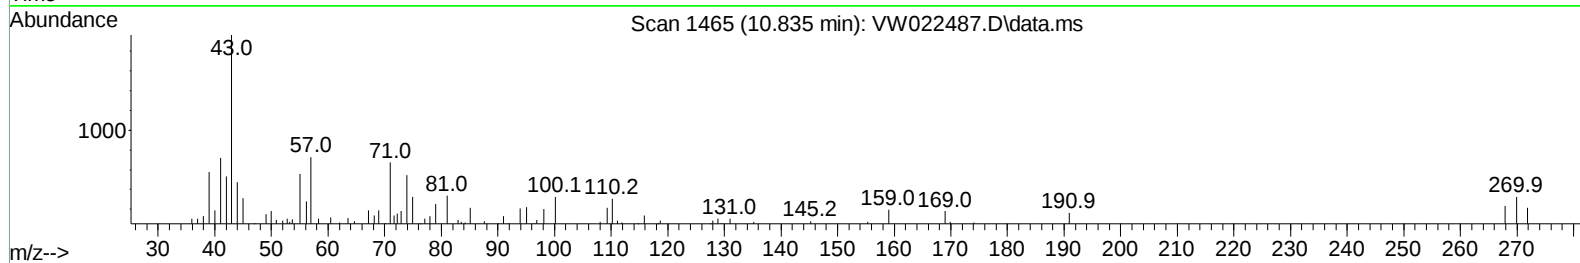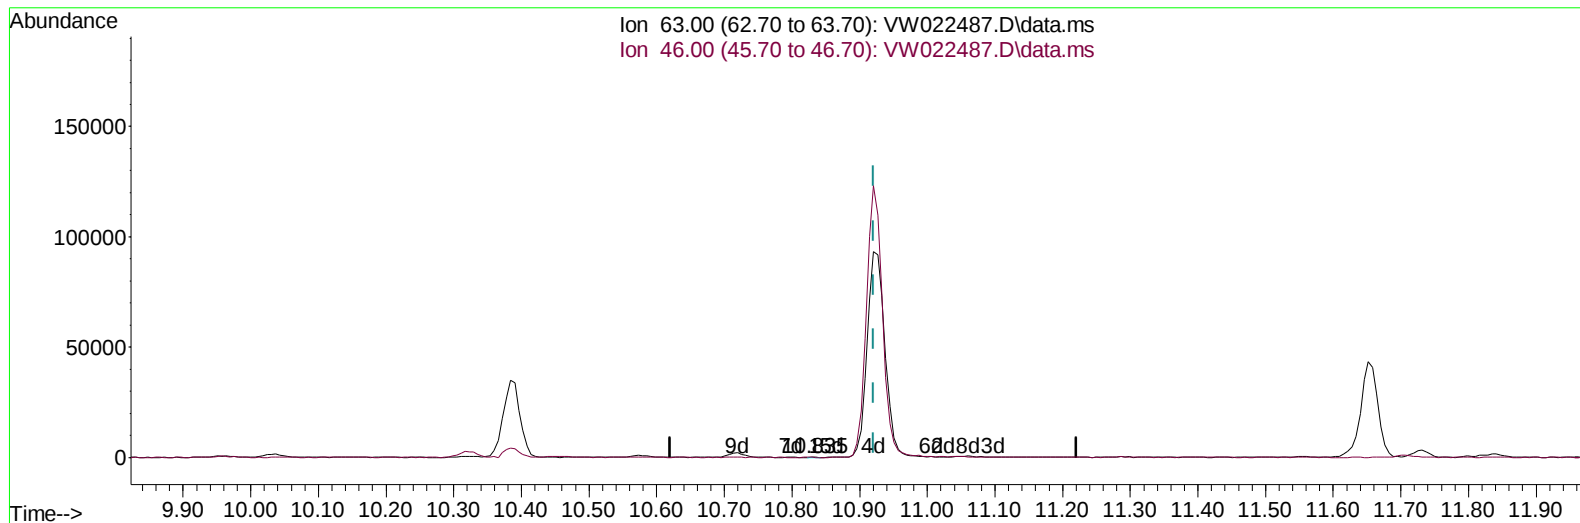

TIC: VW022487.D\data.ms

(47) 2-Hexanone-d5 (S)

10.835min (-0.085) 0.05 ug/L

response 71

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	177.60	166.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
Data File : VW022487.D
Acq On : 11 Apr 2022 16:57
Operator : SY/VA
Sample : N2316-08
Misc : 6.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNQ7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:59:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Apr 11 23:55:29 2022
Response via : Initial Calibration

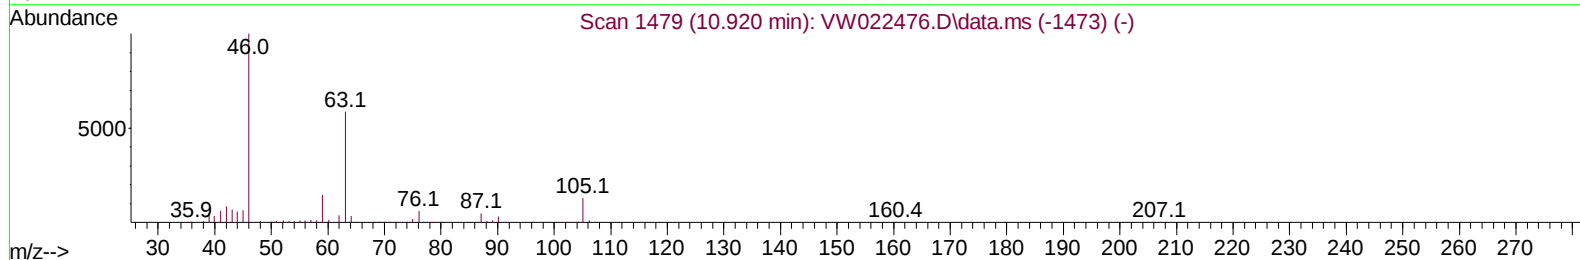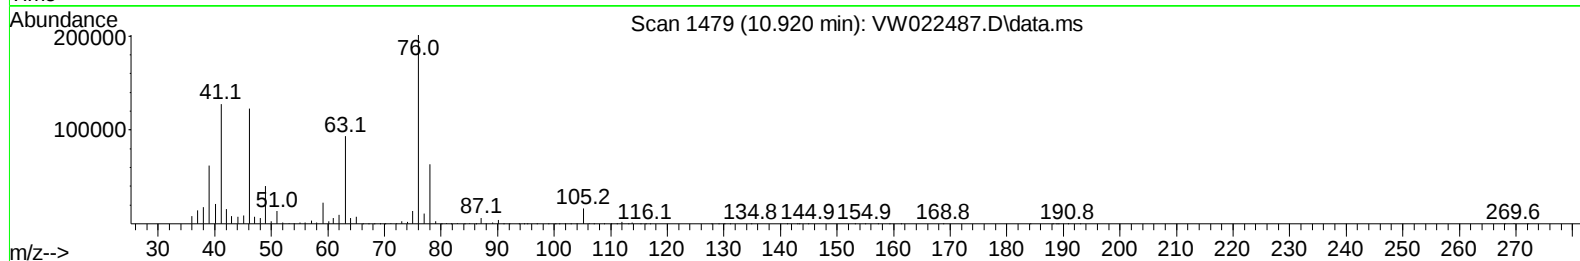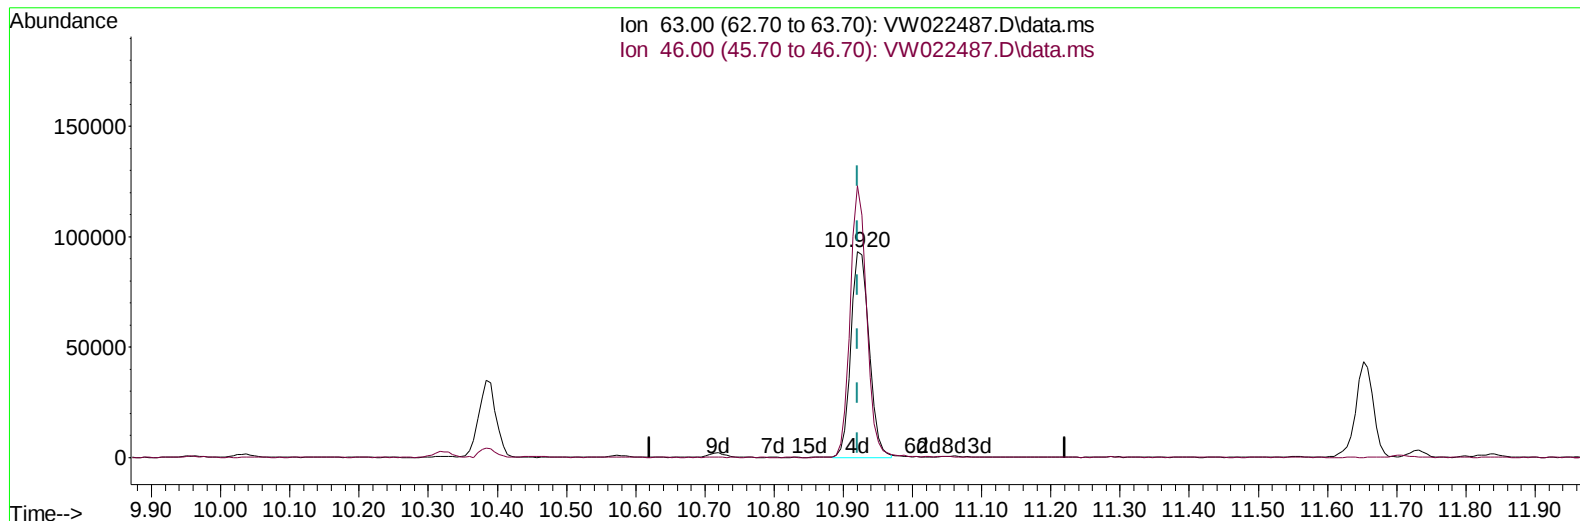

TIC: VW022487.D\data.ms

(47) 2-Hexanone-d5 (S)

10.920min (+ 0.000) 117.50 ug/L m

response 170636

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	177.60	0.07#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022487.D
 Acq On : 11 Apr 2022 16:57
 Operator : SY/VA
 Sample : N2316-08
 Misc : 6.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ7

Manual IntegrationsAPPROVED

Quant Time: Apr 11 23:59:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	450522	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	441460	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	214413	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	156674	15.731	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	62.920%	
7) Chloroethane-d5	2.885	69	108433	17.372	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	69.480%	
11) 1,1-Dichloroethene-d2	4.019	63	159996	12.386	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	49.560%	
21) 2-Butanone-d5	7.074	46	137379	79.007	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	158.020%#	
24) Chloroform-d	7.647	84	311035	22.088	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.360%	
26) 1,2-Dichloroethane-d4	8.311	65	200350	24.901	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	99.600%	
32) Benzene-d6	8.275	84	560172	20.769	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.080%	
36) 1,2-Dichloropropane-d6	9.274	67	184073	23.583	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	94.320%	
41) Toluene-d8	10.323	98	522499	19.780	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.120%	
43) trans-1,3-Dichloroprop...	10.579	79	84704	22.995	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.960%	
47) 2-Hexanone-d5	10.920	63	170636m	117.503	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	235.000%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	211892	31.927	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	127.720%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	191286	25.187	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.760%	
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	229745	194.058	ug/L	96
19) 1,1-Dichloroethane	6.214	63	7039	0.543	ug/L #	88
22) 2-Butanone	7.171	43	30569	17.096	ug/L	97
29) Cyclohexane	7.958	56	20661	1.635	ug/L	96
33) Benzene	8.323	78	5779119	192.815	ug/L	100
35) Methylcyclohexane	9.329	83	67283	4.673	ug/L	98
42) Toluene	10.384	91	644733	18.772	ug/L	92
48) 2-Hexanone	10.969	43	11966	3.871	ug/L #	87
51) Chlorobenzene	11.658	112	3340397	159.159	ug/L	93
52) Ethylbenzene	11.731	91	101280	2.631	ug/L	94
53) m,p-Xylene	11.841	106	22155	1.514	ug/L	99
54) o-Xylene	12.164	106	19227	1.375	ug/L	98
60) Isopropylbenzene	12.457	105	33244	0.933	ug/L	98
63) 1,2,4-Trimethylbenzene	13.249	105	15598	0.524	ug/L	94
65) 1,4-Dichlorobenzene	13.572	146	7947	0.551	ug/L	88
67) 1,2-Dichlorobenzene	13.865	146	14904	1.153	ug/L	87

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw041122\
 Data File : VW022487.D
 Acq On : 11 Apr 2022 16:57
 Operator : SY/VA
 Sample : N2316-08
 Misc : 6.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETNQ7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
 Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:59:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev	(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed								

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
Data File : VW022487.D
Acq On : 11 Apr 2022 16:57
Operator : SY/VA
Sample : N2316-08
Misc : 6.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETNQ7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2022
Supervised By :Mahesh Dadoda 04/12/2022

Quant Time: Apr 11 23:59:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Apr 11 23:55:29 2022
Response via : Initial Calibration

