

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
 Data File : VW022481.D
 Acq On : 11 Apr 2022 14:26
 Operator : SY/VA
 Sample : VIBLK417
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK417

Quant Time: Apr 11 23:58:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Apr 11 23:55:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	412797	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	385210	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	196319	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	149307	16.361	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	65.440%		
7) Chloroethane-d5	2.885	69	99065	17.321	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.280%		
11) 1,1-Dichloroethene-d2	4.019	63	169116	14.288	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.160%		
21) 2-Butanone-d5	7.073	46	81329	51.047	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.100%		
24) Chloroform-d	7.646	84	284940	22.084	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.320%		
26) 1,2-Dichloroethane-d4	8.305	65	161756	21.942	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.760%		
32) Benzene-d6	8.274	84	516564	21.949	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	87.800%		
36) 1,2-Dichloropropane-d6	9.274	67	157309	23.097	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	92.400%		
41) Toluene-d8	10.323	98	492124	21.350	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.400%		
43) trans-1,3-Dichloroprop...	10.579	79	67554	21.017	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	84.080%		
47) 2-Hexanone-d5	10.920	63	64995	51.292	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.580%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	146438	25.287	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.160%		
66) 1,2-Dichlorobenzene-d4	13.853	152	183464	26.384	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.520%		
Target Compounds					Qvalue	
51) Chlorobenzene	11.658	112	9441	0.516	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041122\
Data File : VW022481.D
Acq On : 11 Apr 2022 14:26
Operator : SY/VA
Sample : VIBLK417
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK417


Quant Time: Apr 11 23:58:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Apr 11 23:55:29 2022
Response via : Initial Calibration

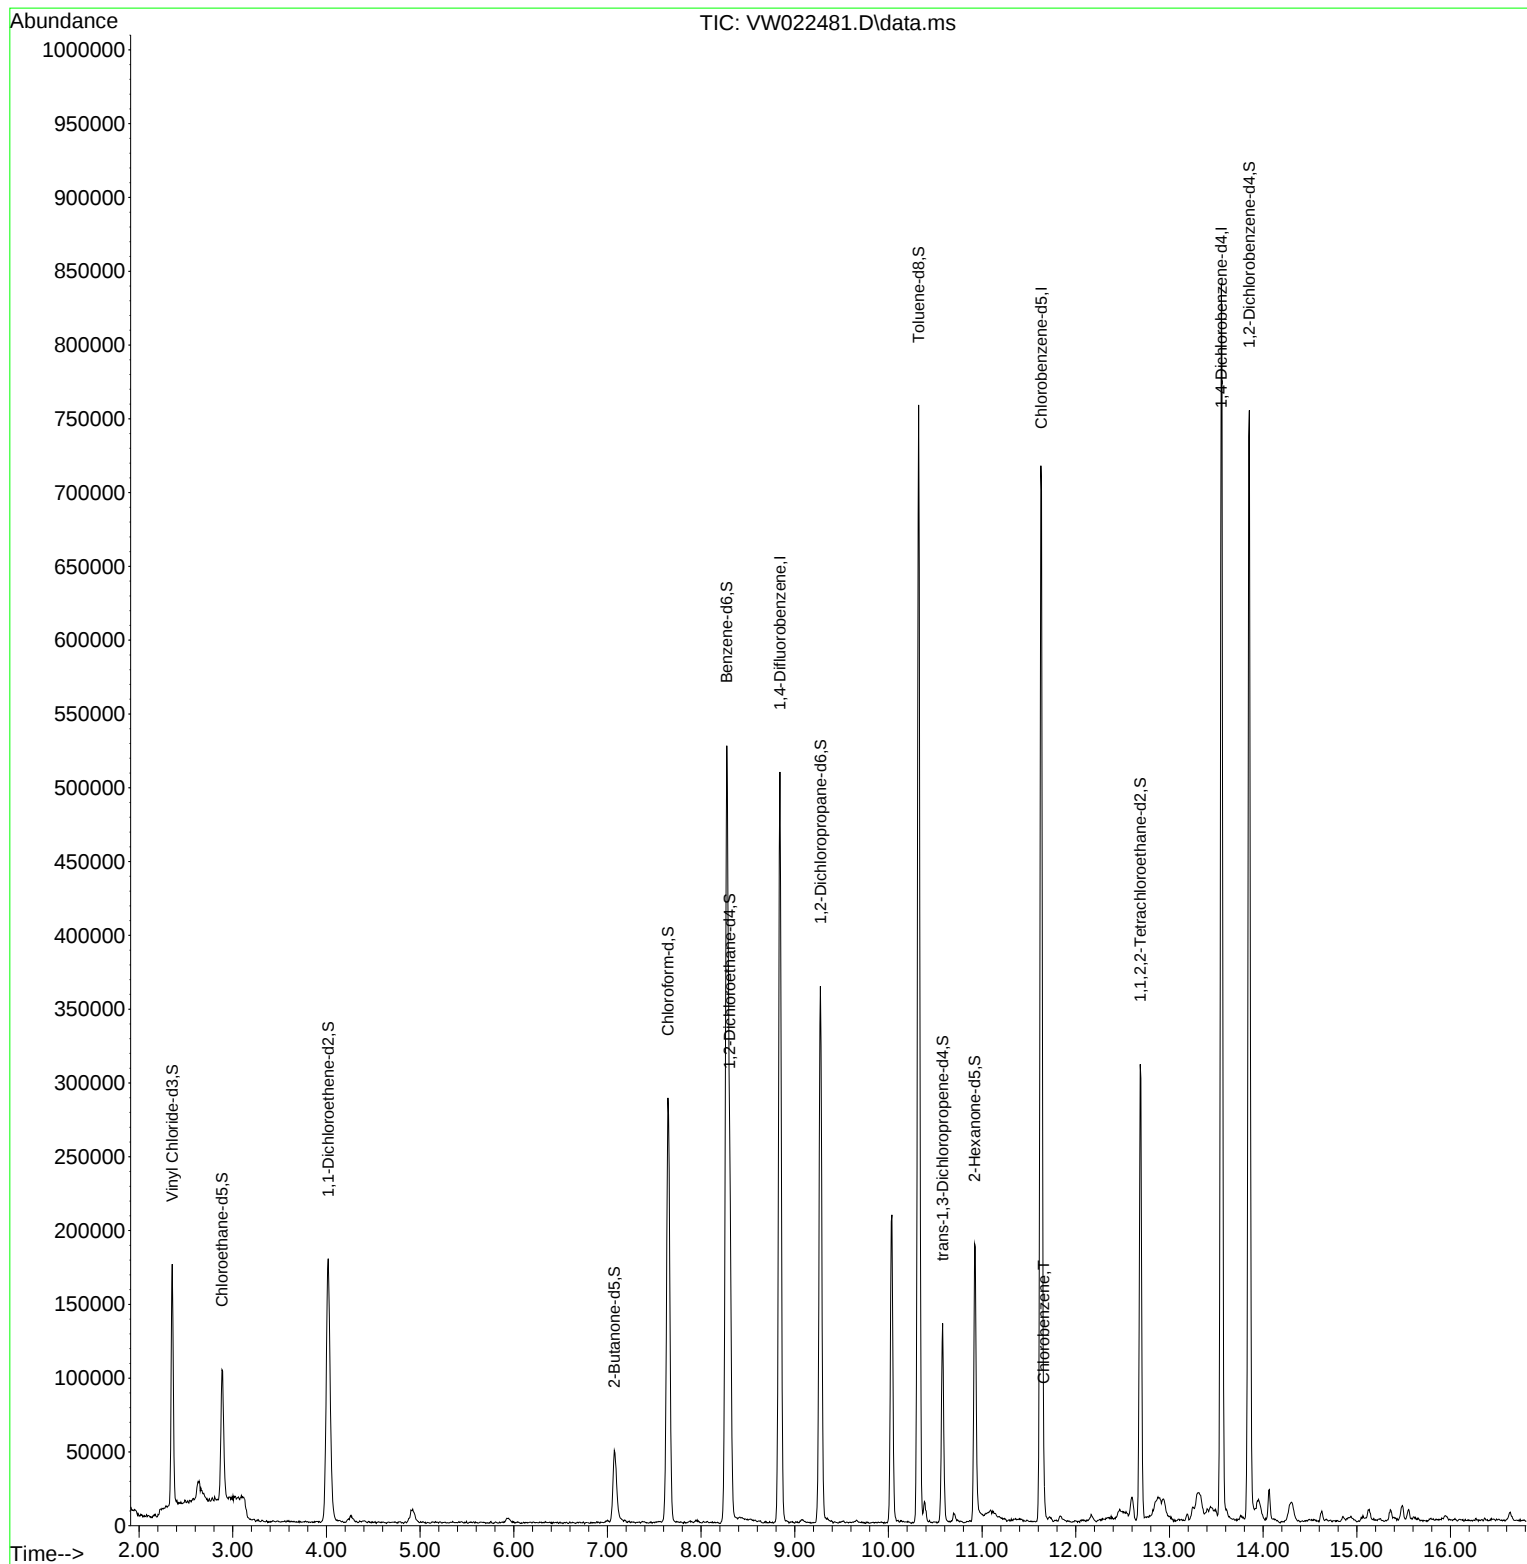

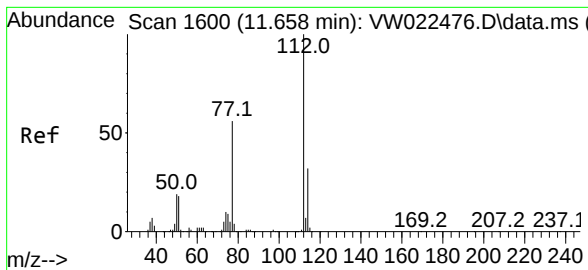

#51
 Chlorobenzene
 Concen: 0.516 ug/L
 RT: 11.658 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VW022481.D
 Acq: 11 Apr 2022 14:26

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK417

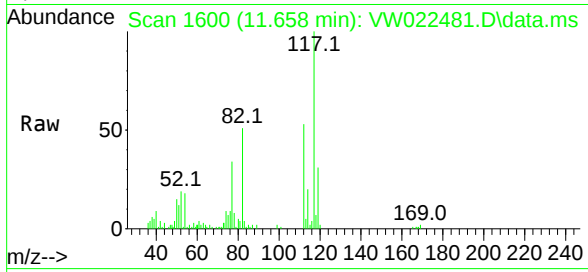

Tgt Ion:	112	Resp:	9441
Ion	Ratio	Lower	Upper
112	100		
114	37.1	20.5	38.1
77	64.5	48.1	72.1

