

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041221\
 Data File : VW018629.D
 Acq On : 12 Apr 2021 17:46
 Operator : SY/VA
 Sample : M2011-04
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG784

Quant Time: Apr 17 04:28:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM033121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 17 04:26:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	315094	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	250888	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	71593	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	95614	18.88	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.52%		
7) Chloroethane-d5	2.897	69	75761	18.70	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.80%		
11) 1,1-Dichloroethene-d2	4.019	63	107511	13.65	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	54.60%		
21) 2-Butanone-d5	7.073	46	80908	76.62	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	153.24%#		
24) Chloroform-d	7.653	84	173310	20.93	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	83.72%		
26) 1,2-Dichloroethane-d4	8.305	65	114269	22.96	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.84%		
32) Benzene-d6	8.274	84	327299	24.88	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	99.52%		
36) 1,2-Dichloropropane-d6	9.274	67	100504	26.22	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	104.88%		
41) Toluene-d8	10.323	98	289366	22.40	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	89.60%		
43) trans-1,3-Dichloroprop...	10.579	79	38980	20.42	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.68%		
47) 2-Hexanone-d5	10.926	63	60444	80.54	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	161.08%#		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	104475	28.50	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	114.00%		
66) 1,2-Dichlorobenzene-d4	13.853	152	55540	22.93	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.72%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	18078	24.28	ug/L	98
14) Carbon disulfide	4.391	76	18720	1.47	ug/L	99
16) Methylene chloride	4.927	84	10529	2.23	ug/L	82
42) Toluene	10.384	91	5989	0.35	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041221\
Data File : VW018629.D
Acq On : 12 Apr 2021 17:46
Operator : SY/VA
Sample : M2011-04
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG784

Quant Time: Apr 17 04:28:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM033121SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 17 04:26:19 2021
Response via : Initial Calibration




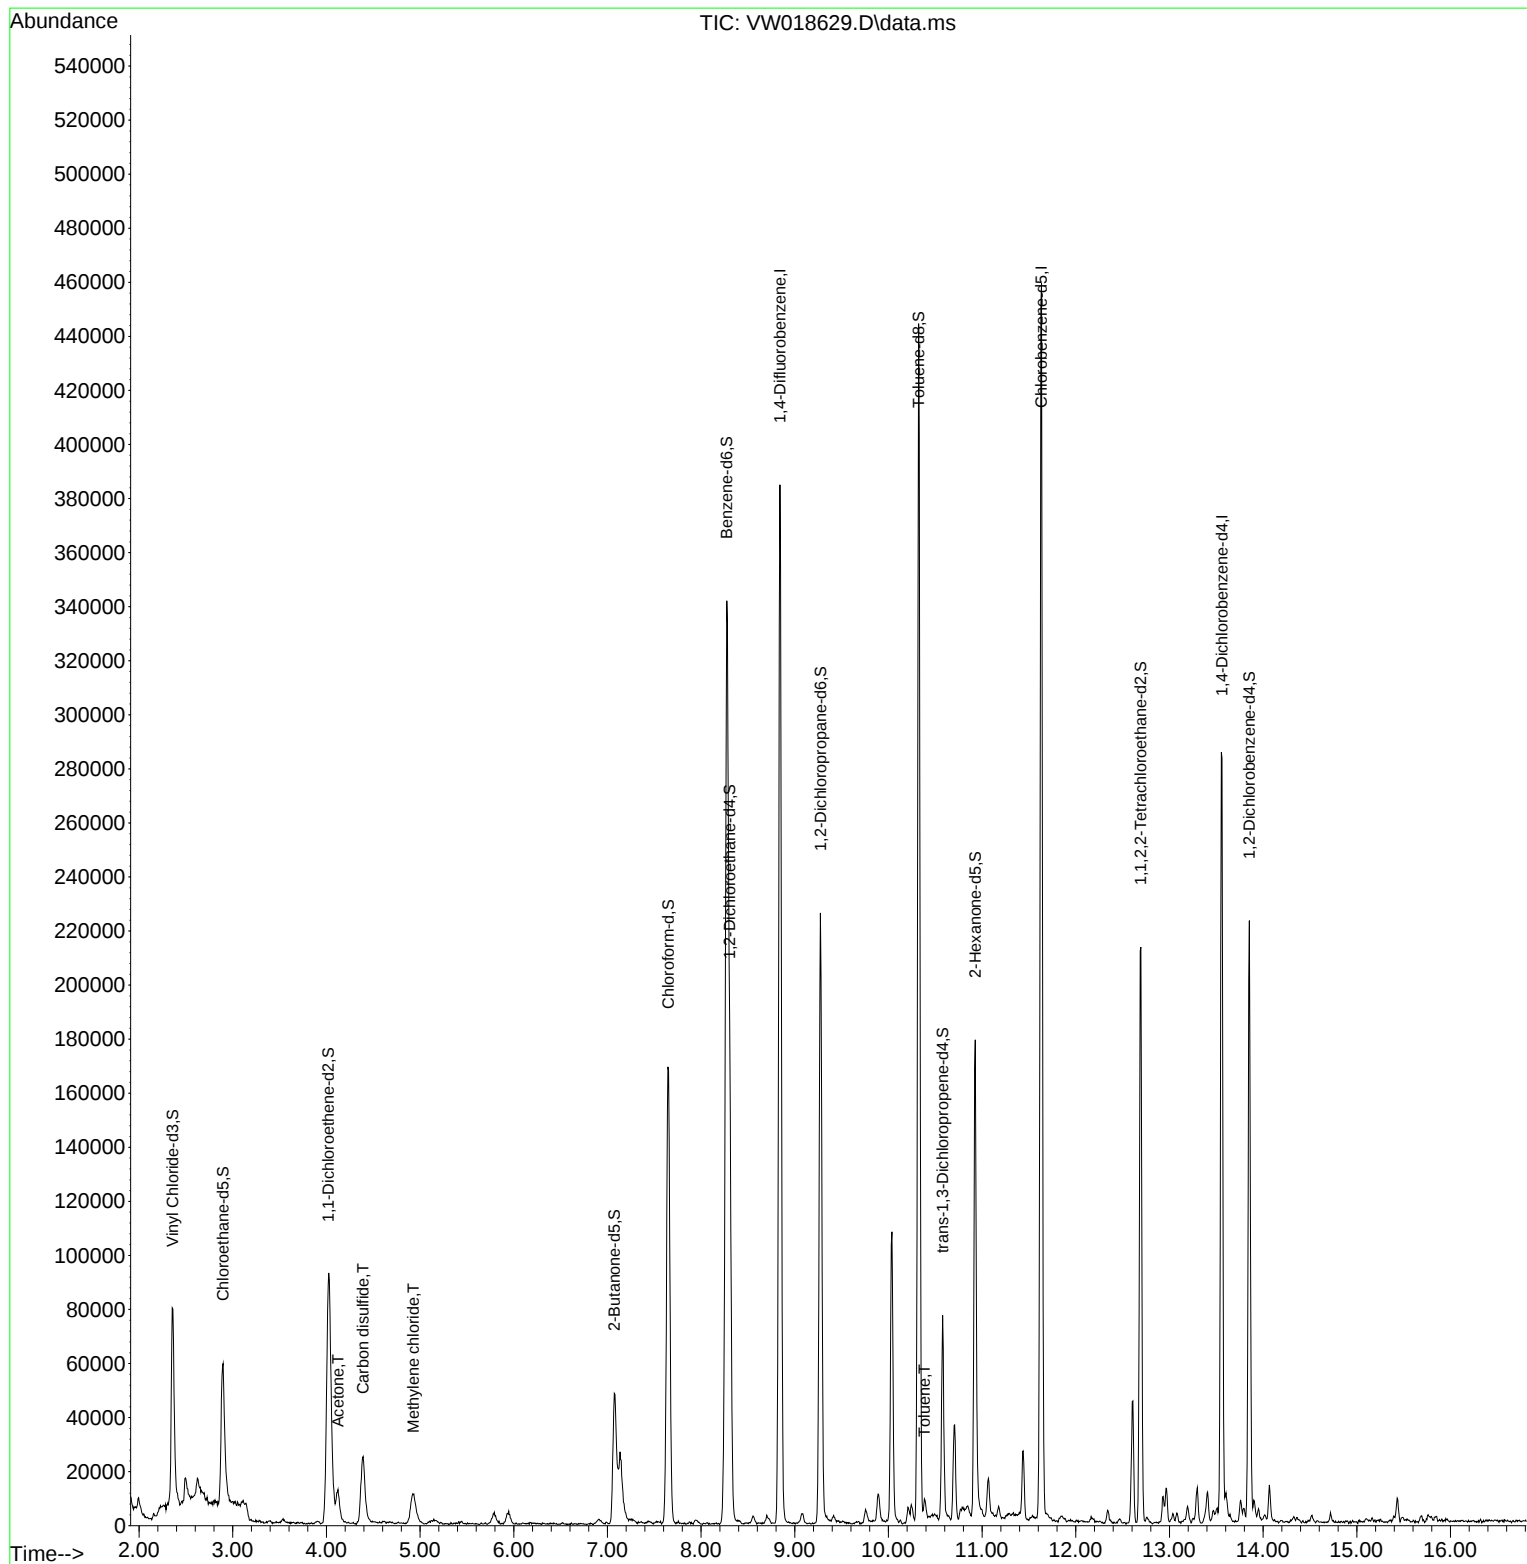


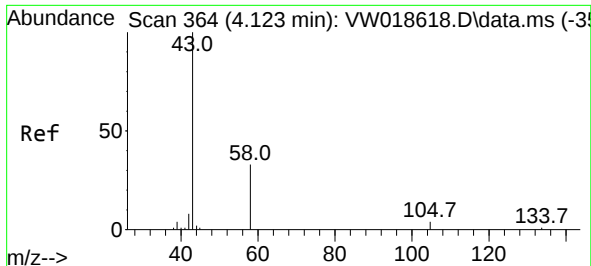

#13
Acetone
Concen: 24.28 ug/L
RT: 4.123 min Scan# 364
Delta R.T. -0.000 min
Lab File: VW018629.D
Acq: 12 Apr 2021 17:46




Instrument :
MSVOA_W
ClientSampleId :
BG784


Tgt Ion: 43 Resp: 18078
Ion Ratio Lower Upper
43 100
58 28.2 0.0 53.8

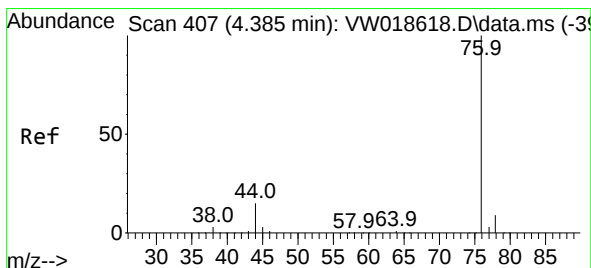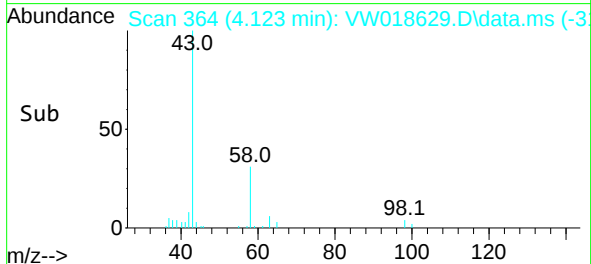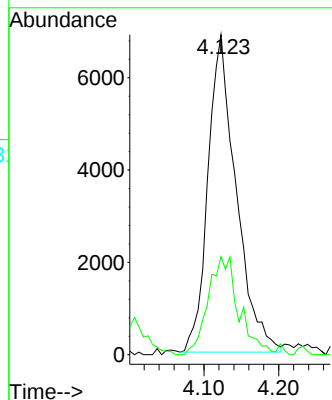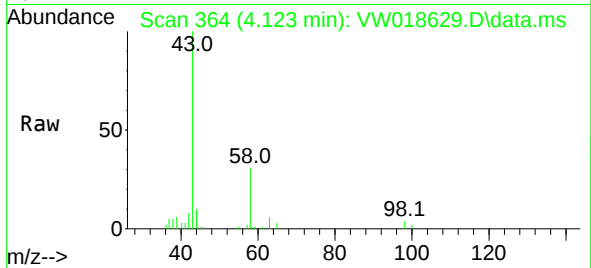

#14
Carbon disulfide
Concen: 1.47 ug/L
RT: 4.391 min Scan# 408
Delta R.T. 0.006 min
Lab File: VW018629.D
Acq: 12 Apr 2021 17:46

Tgt Ion: 76 Resp: 18720
Ion Ratio Lower Upper
76 100
78 8.7 7.4 11.0


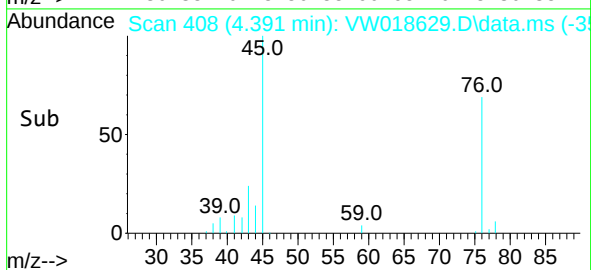
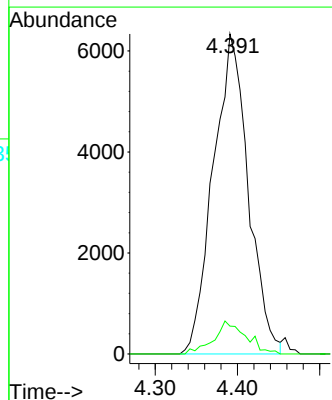
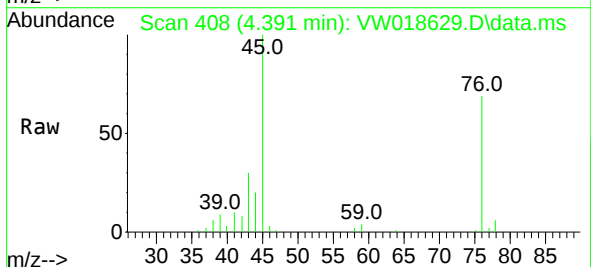


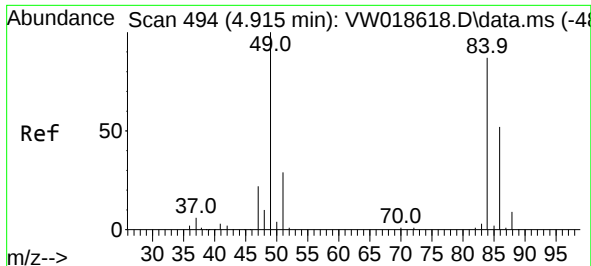

#16
Methylene chloride
Concen: 2.23 ug/L
RT: 4.927 min Scan# 496
Delta R.T. 0.012 min
Lab File: VW018629.D
Acq: 12 Apr 2021 17:46

Instrument :
MSVOA_W
ClientSampled :
BG784

Tgt Ion: 84 Resp: 10529
Ion Ratio Lower Upper
84 100
86 53.1 45.3 84.1
49 100.7 86.6 160.8

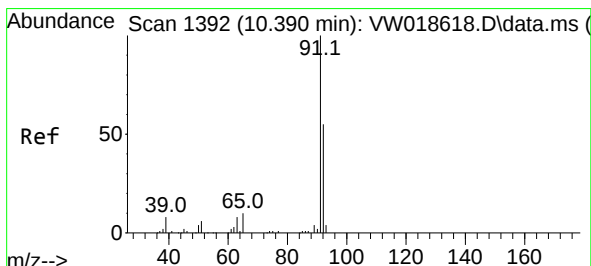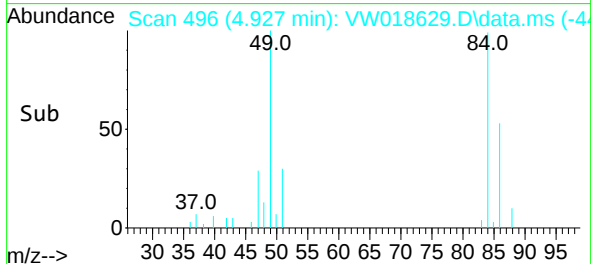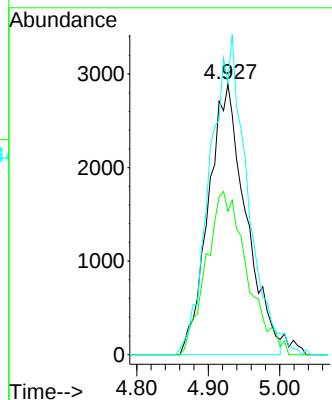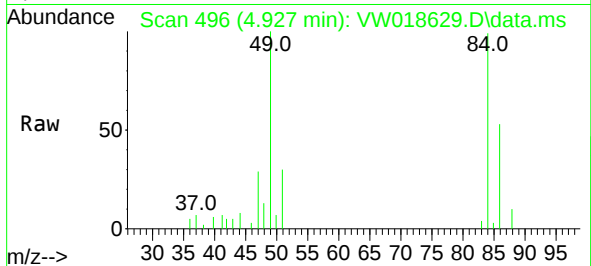

#42
Toluene
Concen: 0.35 ug/L
RT: 10.384 min Scan# 1391
Delta R.T. -0.006 min
Lab File: VW018629.D
Acq: 12 Apr 2021 17:46

Tgt Ion: 91 Resp: 5989
Ion Ratio Lower Upper
91 100
92 54.6 39.5 73.3

