

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041221\
 Data File : VW018631.D
 Acq On : 12 Apr 2021 18:34
 Operator : SY/VA
 Sample : M2011-07
 Misc : 5.47G/10ML/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG787

Manual Integrations
 APPROVED

MMDadoda
 4/19/2021 11:48:31 AM

Quant Time: Apr 17 04:29:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM033121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 17 04:26:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	478242	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	441039	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	199057	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	135900	17.68	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.72%		
7) Chloroethane-d5	2.891	69	108898	17.71	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.84%		
11) 1,1-Dichloroethene-d2	4.019	63	160767	13.45	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	53.80%		
21) 2-Butanone-d5	7.074	46	71388	44.54	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	89.08%		
24) Chloroform-d	7.647	84	258427	20.56	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.24%		
26) 1,2-Dichloroethane-d4	8.305	65	158135	20.94	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.76%		
32) Benzene-d6	8.275	84	498923	21.57	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.28%		
36) 1,2-Dichloropropane-d6	9.274	67	149160	22.13	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.52%		
41) Toluene-d8	10.323	98	476225	20.98	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	83.92%		
43) trans-1,3-Dichloroprop...	10.579	79	60481	18.03	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	72.12%		
47) 2-Hexanone-d5	10.927	63	57458	43.55	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.10%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	135282	21.00	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	84.00%		
66) 1,2-Dichlorobenzene-d4	13.853	152	147437	21.89	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.56%		
Target Compounds						Qvalue
13) Acetone	4.117	43	36838	32.59	ug/L	95
16) Methylene chloride	4.922	84	14611m	2.04	ug/L	
22) 2-Butanone	7.183	43	9642	5.30	ug/L	99
42) Toluene	10.390	91	9723	0.33	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041221\
Data File : VW018631.D
Acq On : 12 Apr 2021 18:34
Operator : SY/VA
Sample : M2011-07
Misc : 5.47G/10ML/MSVOA_W/SOIL
ALS Vial : 16 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BG787

Quant Time: Apr 17 04:29:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM033121SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 17 04:26:19 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
4/19/2021 11:48:31 AM

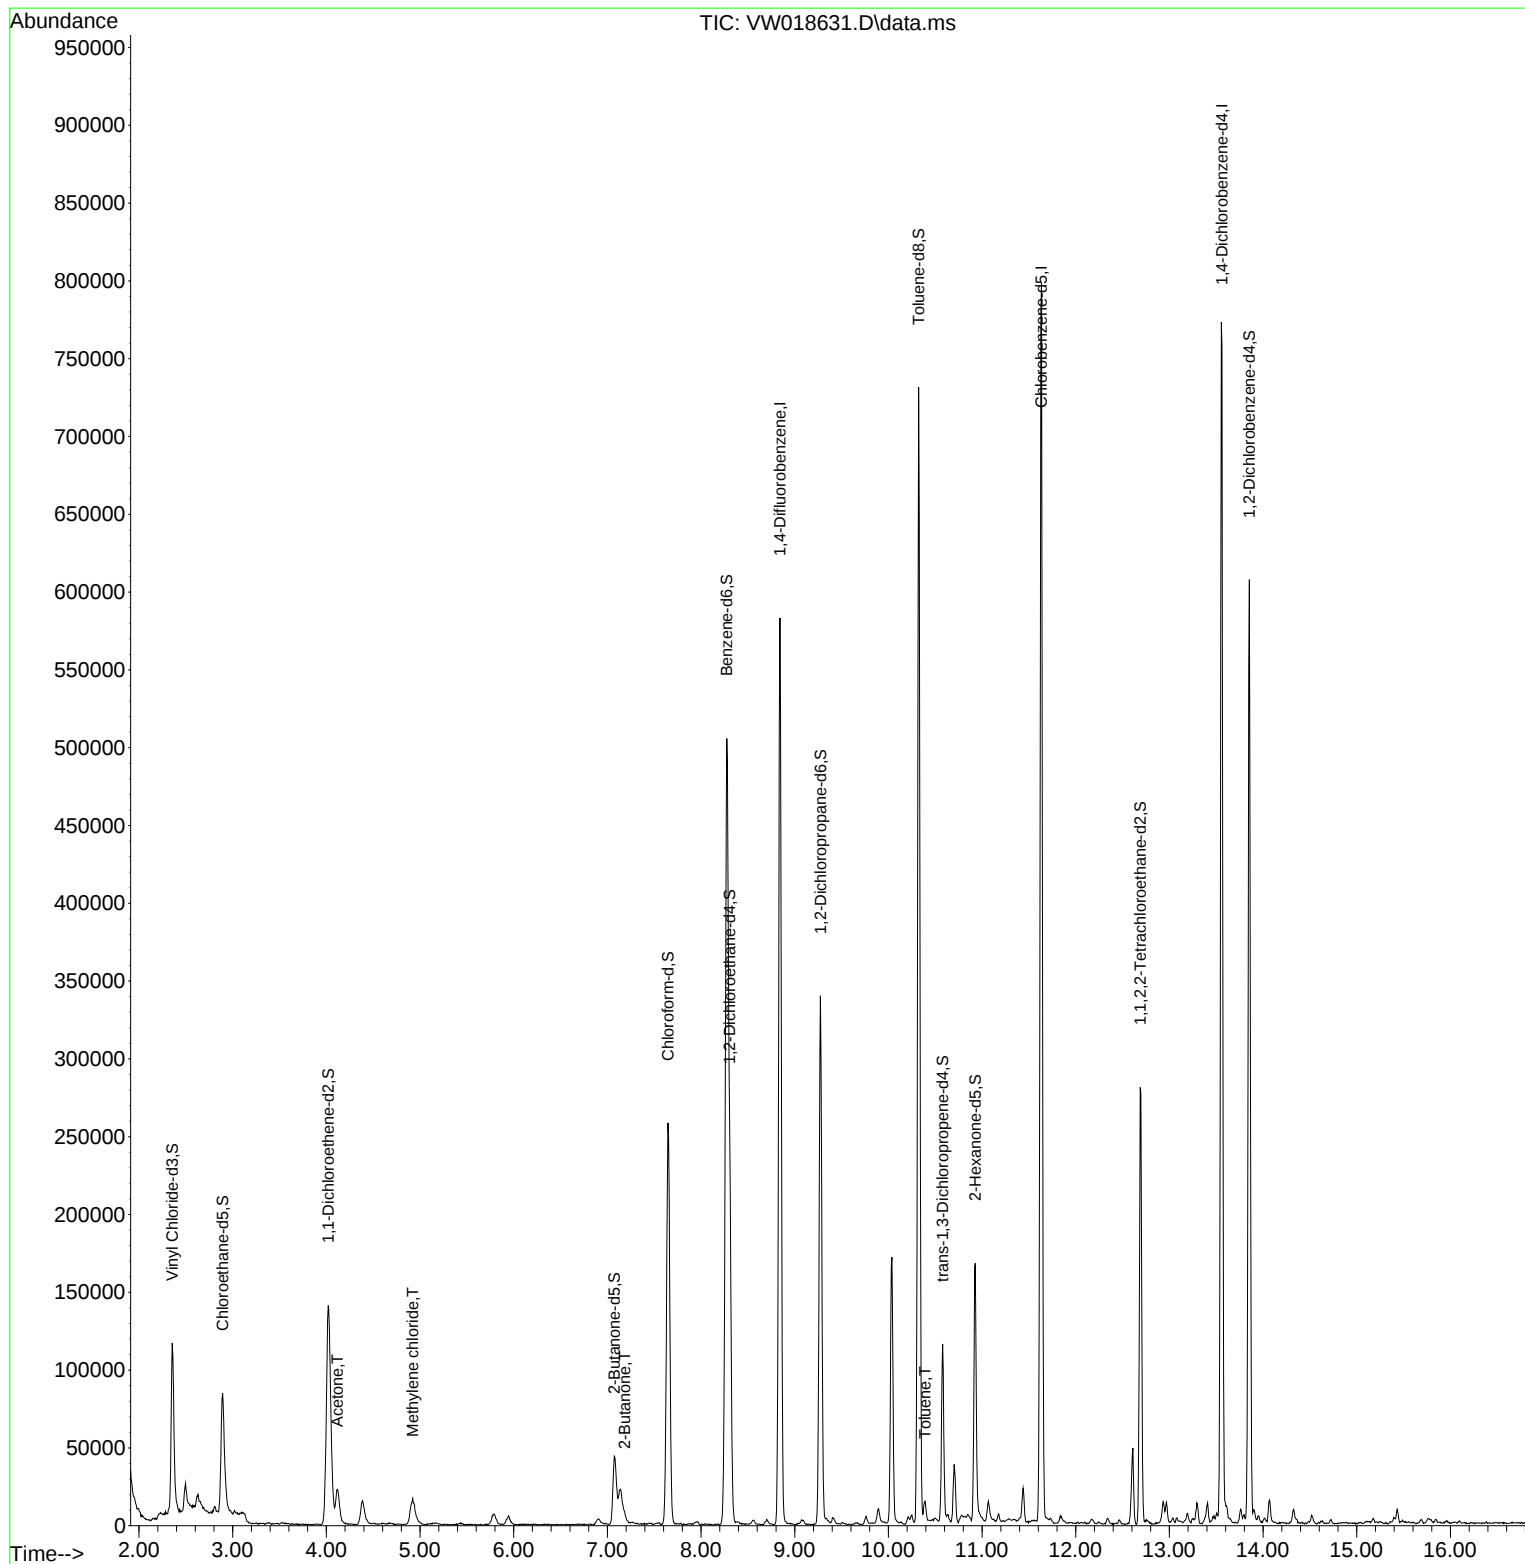

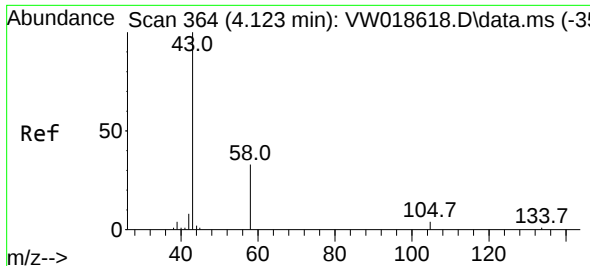





#13
Acetone
Concen: 32.59 ug/L
RT: 4.117 min Scan# 363
Delta R.T. -0.006 min
Lab File: VW018631.D
Acq: 12 Apr 2021 18:34

Tgt Ion: 43 Resp: 36838
Ion Ratio Lower Upper
43 100
58 29.7 0.0 53.8

Instrument :
MSVOA_W
ClientSampled :
BG787




Manual Integrations
APPROVED


MMDadoda
4/19/2021 11:48:31 AM

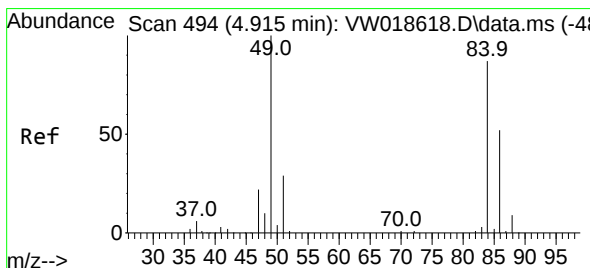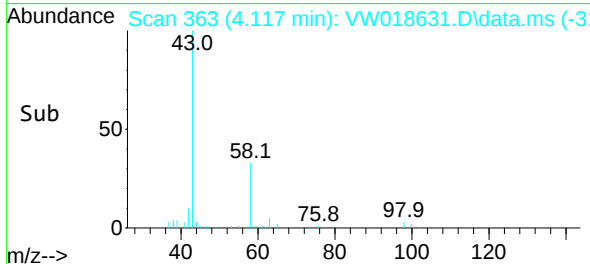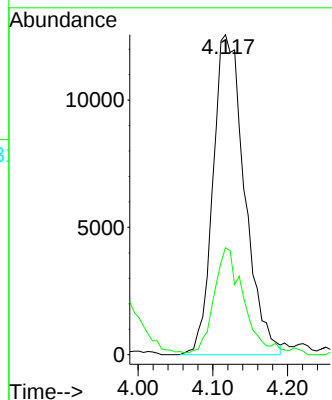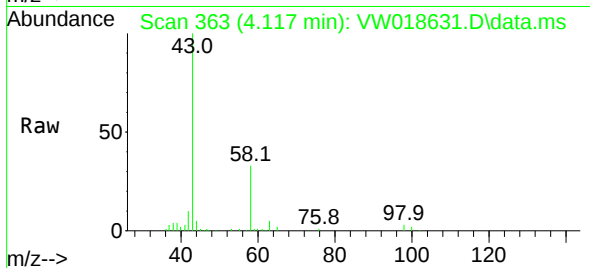

#16
Methylene chloride
Concen: 2.04 ug/L m
RT: 4.922 min Scan# 495
Delta R.T. 0.006 min
Lab File: VW018631.D
Acq: 12 Apr 2021 18:34

Tgt Ion: 84 Resp: 14611
Ion Ratio Lower Upper
84 100
86 60.4 45.3 84.1
49 102.7 86.6 160.8

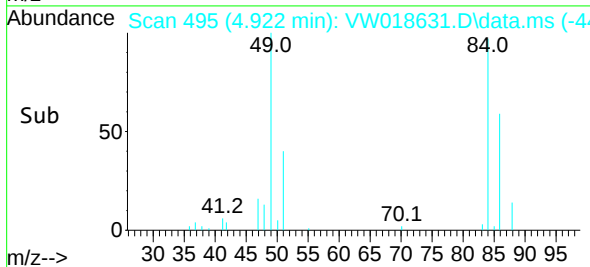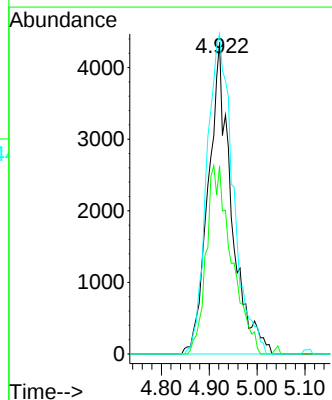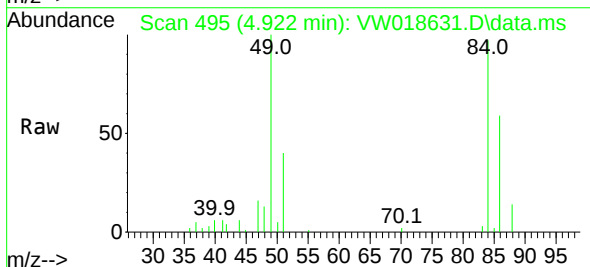

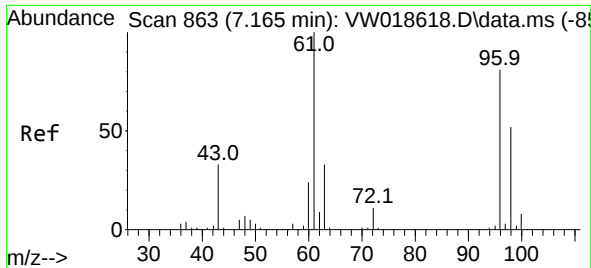





#22
2-Butanone
Concen: 5.30 ug/L
RT: 7.183 min Scan# 866
Delta R.T. 0.018 min
Lab File: VW018631.D
Acq: 12 Apr 2021 18:34

Tgt Ion: 43 Resp: 9642
Ion Ratio Lower Upper
43 100
72 29.3 14.9 44.7

Instrument :
MSVOA_W
ClientSampled :
BG787

Manual Integrations
APPROVED

MMDadoda
4/19/2021 11:48:31 AM

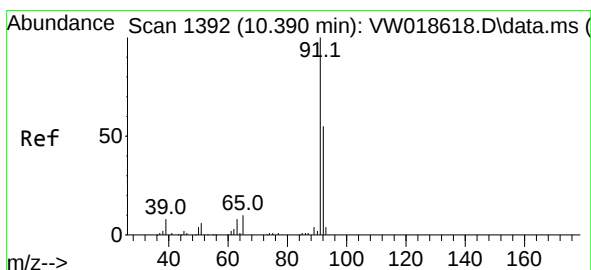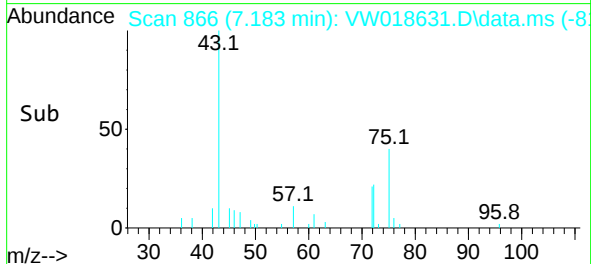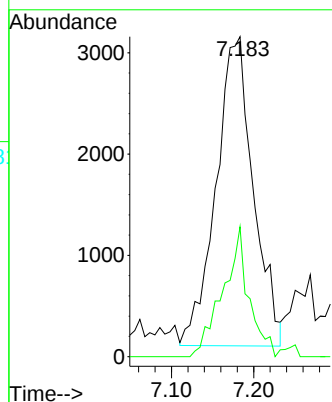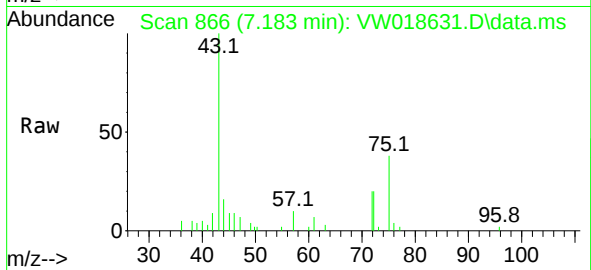

#42
Toluene
Concen: 0.33 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.000 min
Lab File: VW018631.D
Acq: 12 Apr 2021 18:34

Tgt Ion: 91 Resp: 9723
Ion Ratio Lower Upper
91 100
92 55.0 39.5 73.3

