
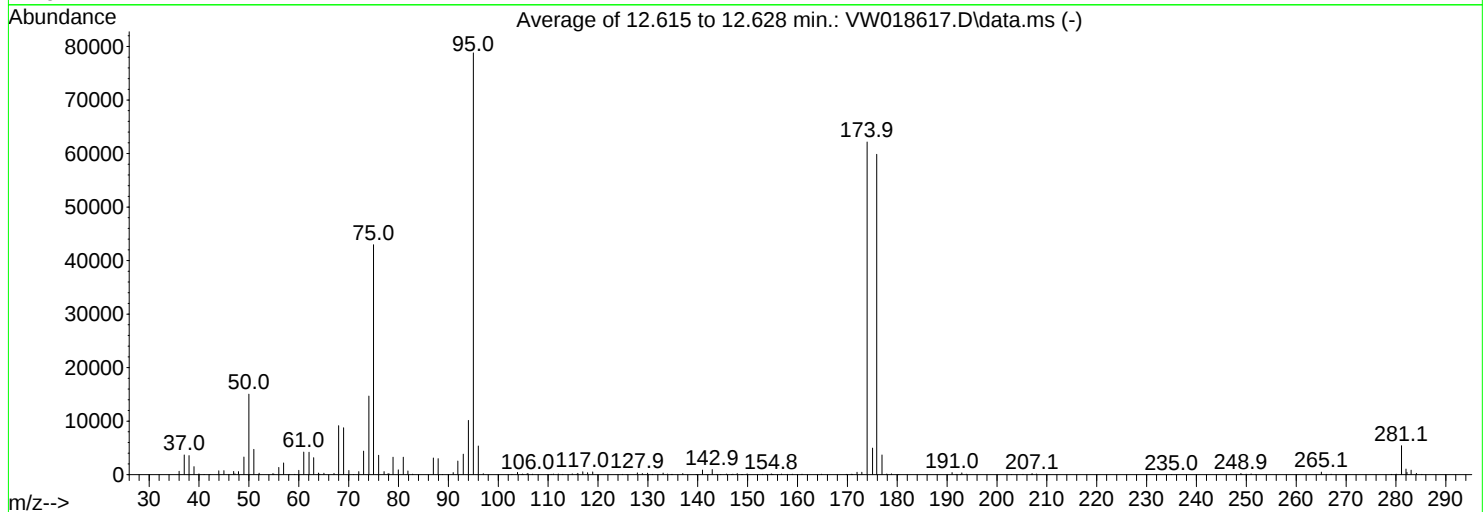


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041221\
 Data File : VW018617.D
 Acq On : 12 Apr 2021 12:13
 Operator : SY/VA
 Sample : BFB03
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB103

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM033121SMA.M
 Title : SFAM01.0
 Last Update : Sat Apr 17 04:26:19 2021

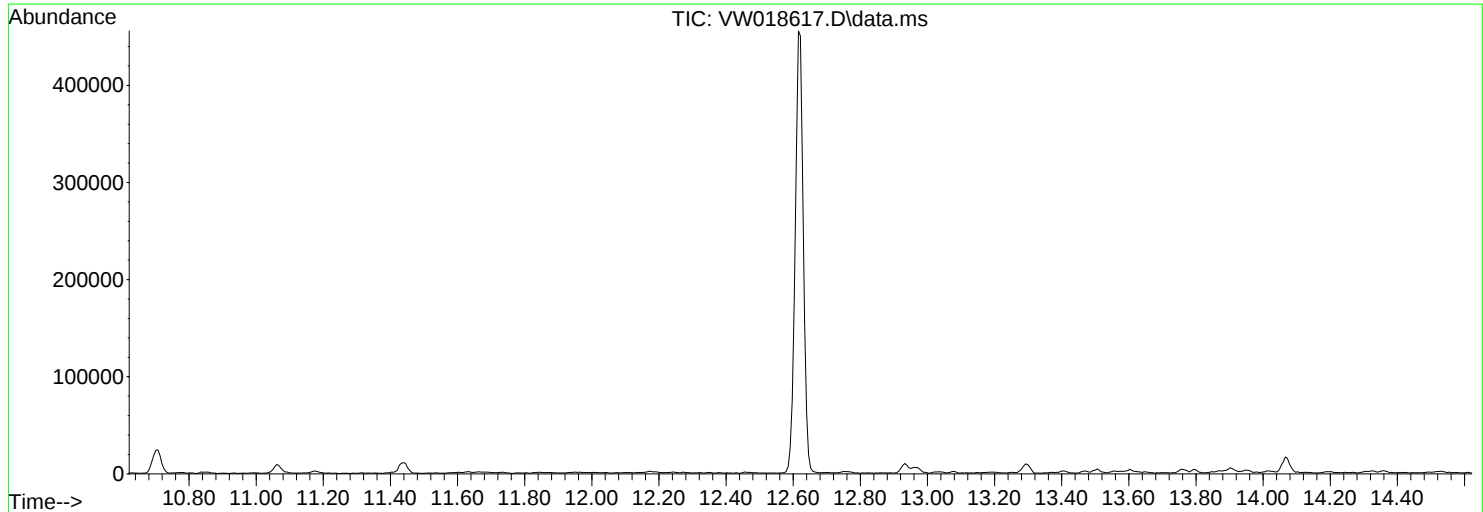

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	15045	PASS
75	95	30	80	54.5	42963	PASS
95	95	100	100	100.0	78813	PASS
96	95	5	9	6.8	5359	PASS
173	174	0.00	2	0.7	466	PASS
174	95	50	120	78.9	62163	PASS
175	174	5	9	8.0	4968	PASS
176	174	95	105	96.3	59840	PASS
177	176	5	10	6.2	3685	PASS

m/z	Abundance
39.00	62.0
40.00	197.0
43.00	107.0
43.70	128.0
44.10	263.0
56.10	61.0
56.80	102.0
57.40	82.0
69.00	52.0
73.00	100.0
169.00	90.0
281.40	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

m/z	Abundance
36.00	720.0
37.10	4537.0
38.00	4322.0
39.00	1968.0
39.90	334.0
42.20	88.0
43.10	83.0
44.00	939.0
45.10	891.0
46.00	107.0
47.00	1000.0
47.90	688.0
49.00	3913.0
50.00	16920.0
51.00	5410.0
52.10	313.0
54.80	254.0
56.00	1307.0
57.00	2664.0
58.00	111.0
59.20	113.0
60.10	935.0
61.00	5102.0
62.10	4895.0
63.00	4126.0
63.90	465.0
65.00	370.0
67.00	322.0
68.00	10353.0
69.00	11004.0
70.00	865.0
71.00	102.0
72.10	621.0
73.00	5370.0
74.10	17400.0
75.00	50528.0
76.00	3991.0
77.20	543.0
77.90	529.0
78.90	3938.0
79.90	907.0
81.00	3437.0
81.90	806.0
82.90	94.0
87.00	3725.0
87.90	3034.0
88.80	91.0
91.00	472.0
91.90	3219.0
93.00	4254.0
94.00	11434.0
95.00	88592.0
96.00	6211.0
97.00	244.0
102.70	146.0
103.80	438.0
104.60	100.0
105.10	103.0
105.80	420.0
106.80	55.0
110.60	185.0
111.10	95.0
112.00	127.0
113.00	104.0
114.90	153.0
115.80	305.0
117.00	506.0
117.90	363.0
118.90	488.0
124.90	162.0
125.80	72.0
127.90	411.0
128.90	175.0
130.00	304.0
130.90	108.0
133.10	562.0
134.00	215.0
134.70	182.0
137.00	198.0
139.70	54.0
140.90	1108.0
142.20	89.0
142.90	1016.0
143.90	96.0
144.60	104.0
145.80	148.0
147.10	237.0
147.90	401.0
148.80	92.0
149.00	98.0
149.80	70.0
153.00	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

153.80	51.0
154.70	183.0
155.10	109.0
156.90	141.0
159.00	107.0
160.90	166.0
164.90	137.0
168.80	68.0
169.80	72.0
170.80	89.0
171.90	422.0
172.90	1398.0
173.90	60960.0
175.00	5318.0
175.90	58936.0
177.00	4200.0
178.00	237.0
178.80	159.0
180.30	67.0
191.00	585.0
191.80	145.0
193.00	733.0
193.80	154.0
202.90	86.0
205.20	114.0
206.90	354.0
208.00	103.0
235.00	63.0
248.90	437.0
250.00	195.0
251.00	267.0
251.90	50.0
265.10	767.0
266.10	160.0
267.00	104.0
279.10	143.0
281.10	9950.0
282.00	2569.0
283.10	1390.0
284.10	382.0
285.20	166.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

m/z	Abundance
36.00	746.0
37.00	3856.0
38.00	3751.0
39.10	1602.0
40.00	396.0
43.10	105.0
44.00	1065.0
45.00	840.0
46.00	118.0
46.90	824.0
47.90	578.0
49.00	3488.0
50.00	17376.0
51.00	5405.0
52.00	230.0
55.00	393.0
56.00	1489.0
57.00	2544.0
58.10	83.0
59.90	717.0
61.00	4796.0
62.00	4583.0
63.00	3182.0
64.00	439.0
65.10	277.0
67.10	228.0
68.00	10021.0
69.00	9436.0
70.10	694.0
72.00	600.0
73.00	5037.0
74.00	15721.0
75.00	46432.0
76.00	4136.0
77.10	598.0
78.10	490.0
78.90	3453.0
79.90	935.0
80.90	3807.0
81.90	803.0
82.80	143.0
87.00	3375.0
87.90	3298.0
91.00	312.0
91.90	2650.0
93.00	4265.0
94.00	11313.0
95.00	89112.0
96.00	5492.0
97.00	248.0
102.80	57.0
103.90	470.0
104.80	243.0
106.00	391.0
106.90	101.0
110.00	74.0
111.00	108.0
112.10	78.0
112.90	91.0
114.80	224.0
116.00	368.0
117.00	700.0
117.90	494.0
119.00	569.0
125.80	57.0
127.90	418.0
128.90	282.0
129.90	236.0
130.90	82.0
132.90	205.0
133.90	97.0
134.90	208.0
137.00	277.0
141.00	768.0
141.70	69.0
142.90	1183.0
143.80	112.0
145.80	198.0
146.80	103.0
147.90	144.0
149.90	247.0
153.00	109.0
153.80	117.0
154.80	233.0
156.70	201.0
157.90	126.0
158.90	122.0
160.90	52.0
164.80	96.0
169.80	78.0
171.00	176.0
172.00	515.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

174.00	70048.0
175.00	5375.0
175.90	70336.0
176.90	3730.0
177.80	169.0
178.90	308.0
190.90	331.0
192.00	100.0
192.80	307.0
193.90	91.0
205.20	68.0
207.10	393.0
207.80	110.0
248.90	234.0
249.80	102.0
250.90	154.0
265.00	468.0
267.00	142.0
280.00	105.0
281.10	4189.0
282.20	1232.0
283.00	660.0
284.20	203.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

m/z	Abundance
35.90	429.0
37.00	2627.0
38.00	2651.0
39.00	1107.0
40.10	272.0
41.00	117.0
42.90	65.0
43.90	969.0
44.90	507.0
47.20	486.0
47.90	441.0
49.10	2447.0
50.00	10838.0
51.00	3369.0
52.00	227.0
54.80	302.0
56.00	1393.0
57.00	1685.0
59.20	57.0
60.00	766.0
61.00	2770.0
62.00	3088.0
63.00	2228.0
64.20	288.0
65.10	192.0
67.10	171.0
68.00	7088.0
69.00	6028.0
70.00	748.0
72.00	506.0
73.00	3057.0
74.10	10963.0
75.00	31928.0
76.00	2757.0
77.00	552.0
78.90	2427.0
80.00	853.0
80.90	2512.0
81.90	454.0
82.80	61.0
86.90	2245.0
88.00	2637.0
90.90	388.0
92.00	1809.0
93.00	3005.0
94.00	7670.0
95.00	58736.0
96.00	4374.0
97.00	73.0
103.90	366.0
104.90	96.0
105.90	240.0
106.90	89.0
111.00	157.0
112.00	201.0
114.90	92.0
115.90	387.0
116.90	456.0
118.00	248.0
118.90	464.0
127.90	151.0
128.90	141.0
130.00	241.0
133.00	107.0
133.90	52.0
137.10	156.0
140.90	751.0
142.90	686.0
147.00	81.0
148.00	89.0
149.90	100.0
154.90	182.0
156.80	52.0
158.00	56.0
160.90	73.0
169.80	57.0
170.80	178.0
171.90	428.0
173.90	55480.0
175.10	4212.0
175.90	50248.0
176.90	3124.0
191.10	257.0
192.70	191.0
207.00	67.0
207.90	123.0
249.10	251.0
265.20	201.0
280.10	125.0
281.10	2066.0
282.00	599.0
283.00	479.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103

284.00

139.0

Instrument :
MSVOA_W
ClientSampleId :
BFB103